

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020407.D
 Acq On : 24 Jun 2022 21:31
 Operator : CG/JU
 Sample : N3359-13
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4S8

Quant Time: Jun 25 00:55:39 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.749	152	3306	0.400	ng/ul	0.00
4) Naphthalene-d8	10.535	136	11216	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.377	164	7231	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188	16397	0.400	ng/ul	0.00
17) Chrysene-d12	21.308	240	15546	0.400	ng/ul	0.00
23) Perylene-d12	23.585	264	14892	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	13541	3.535	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.129	152	4153	0.226	ng/ul	0.00
18) Fluoranthene-d10	19.151	212	12529	0.244	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.235	88	1166	0.298	ng/ul#	1
5) Naphthalene	10.584	128	810	0.023	ng/ul#	78
15) Phenanthrene	17.158	178	1491	0.026	ng/ul#	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

EW4S8

TIC: BN020407.D\data.ms

Abundance

Time-->

1,4-Dichlorobenzene-d4, I

1,4-Dichlorobenzene-d4, I

1-Naphthalene-d8, I

2-Methylnaphthalene-d10, SURR


Acenaphthene-d10, I

Phenanthrene-d10, I

Fluoranthene-d10, SURR

Chrysene-d12





Perylene-d12, I

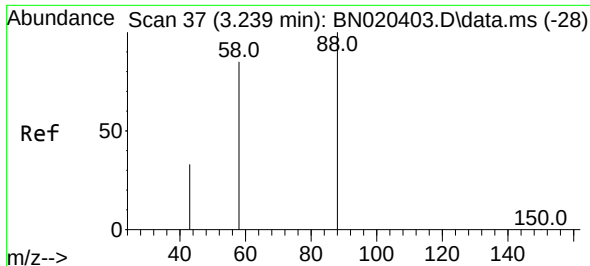

#2
1,4-Dioxane
Concen: 0.298 ng/ul
RT: 3.235 min Scan# 30
Delta R.T. -0.004 min
Lab File: BN020407.D
Acq: 24 Jun 2022 21:31




Instrument :
BNA_N
ClientSampleId :
EW4S8


Tgt Ion: 88 Resp: 1166
Ion Ratio Lower Upper
88 100
43 204.7 32.5 48.7#
58 59.8 46.2 69.2

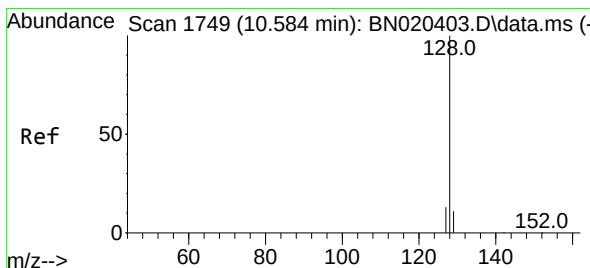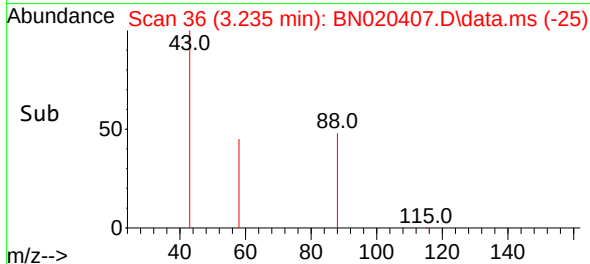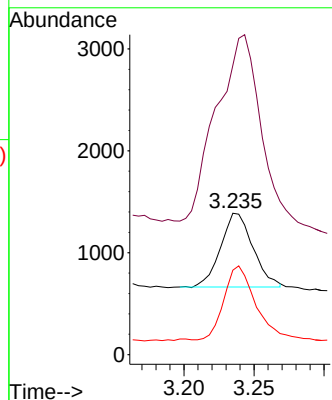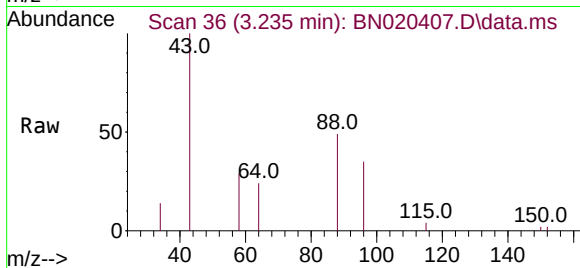

#5
Naphthalene
Concen: 0.023 ng/ul
RT: 10.584 min Scan# 1749
Delta R.T. 0.001 min
Lab File: BN020407.D
Acq: 24 Jun 2022 21:31


Tgt Ion: 128 Resp: 810
Ion Ratio Lower Upper
128 100
129 21.1 9.5 14.3#
127 22.8 11.3 16.9#

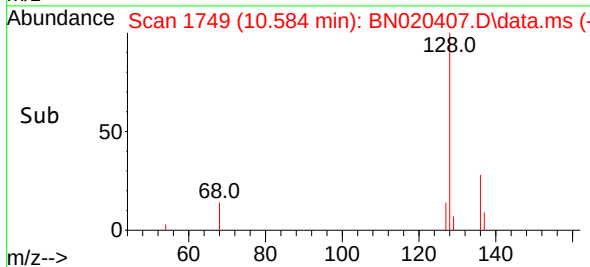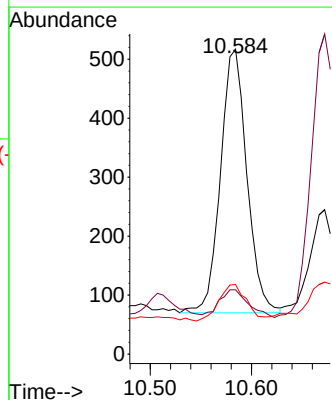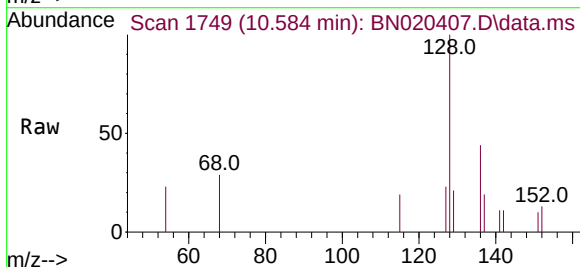

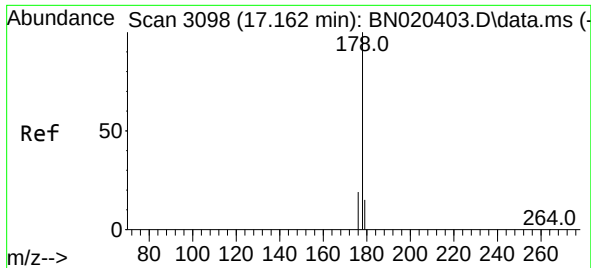

#15
 Phenanthrene
 Concen: 0.026 ng/ul
 RT: 17.158 min Scan# 3097
 Delta R.T. -0.003 min
 Lab File: BN020407.D
 Acq: 24 Jun 2022 21:31

Instrument :
 BNA_N
 ClientSampleId :
 EW4S8

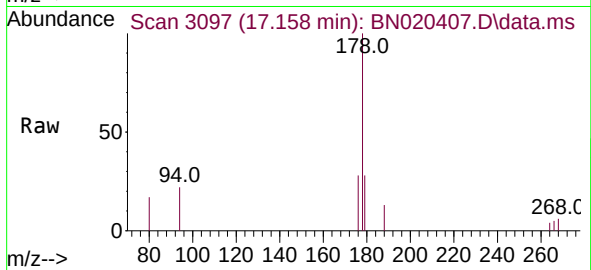

Tgt Ion:	178	Resp:	1491
Ion	Ratio	Lower	Upper
178	100		
179	27.8	12.6	18.8#
176	27.7	15.8	23.6#

