

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020408.D
 Acq On : 24 Jun 2022 22:07
 Operator : CG/JU
 Sample : N3313-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YB7L6

Quant Time: Jun 25 00:55:42 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.749	152	4244	0.400	ng/ul	0.00
4) Naphthalene-d8	10.533	136	15432	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.380	164	10407	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.118	188	23874	0.400	ng/ul	0.00
17) Chrysene-d12	21.306	240	22382	0.400	ng/ul	0.00
23) Perylene-d12	23.586	264	21511	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	22780	4.633	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.128	152	8593	0.339	ng/ul	0.00
18) Fluoranthene-d10	19.149	212	26788	0.363	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.239	88	4805	0.957	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020408.D
Acq On : 24 Jun 2022 22:07
Operator : CG/JU
Sample : N3313-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YB7L6


Quant Time: Jun 25 00:55:42 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration

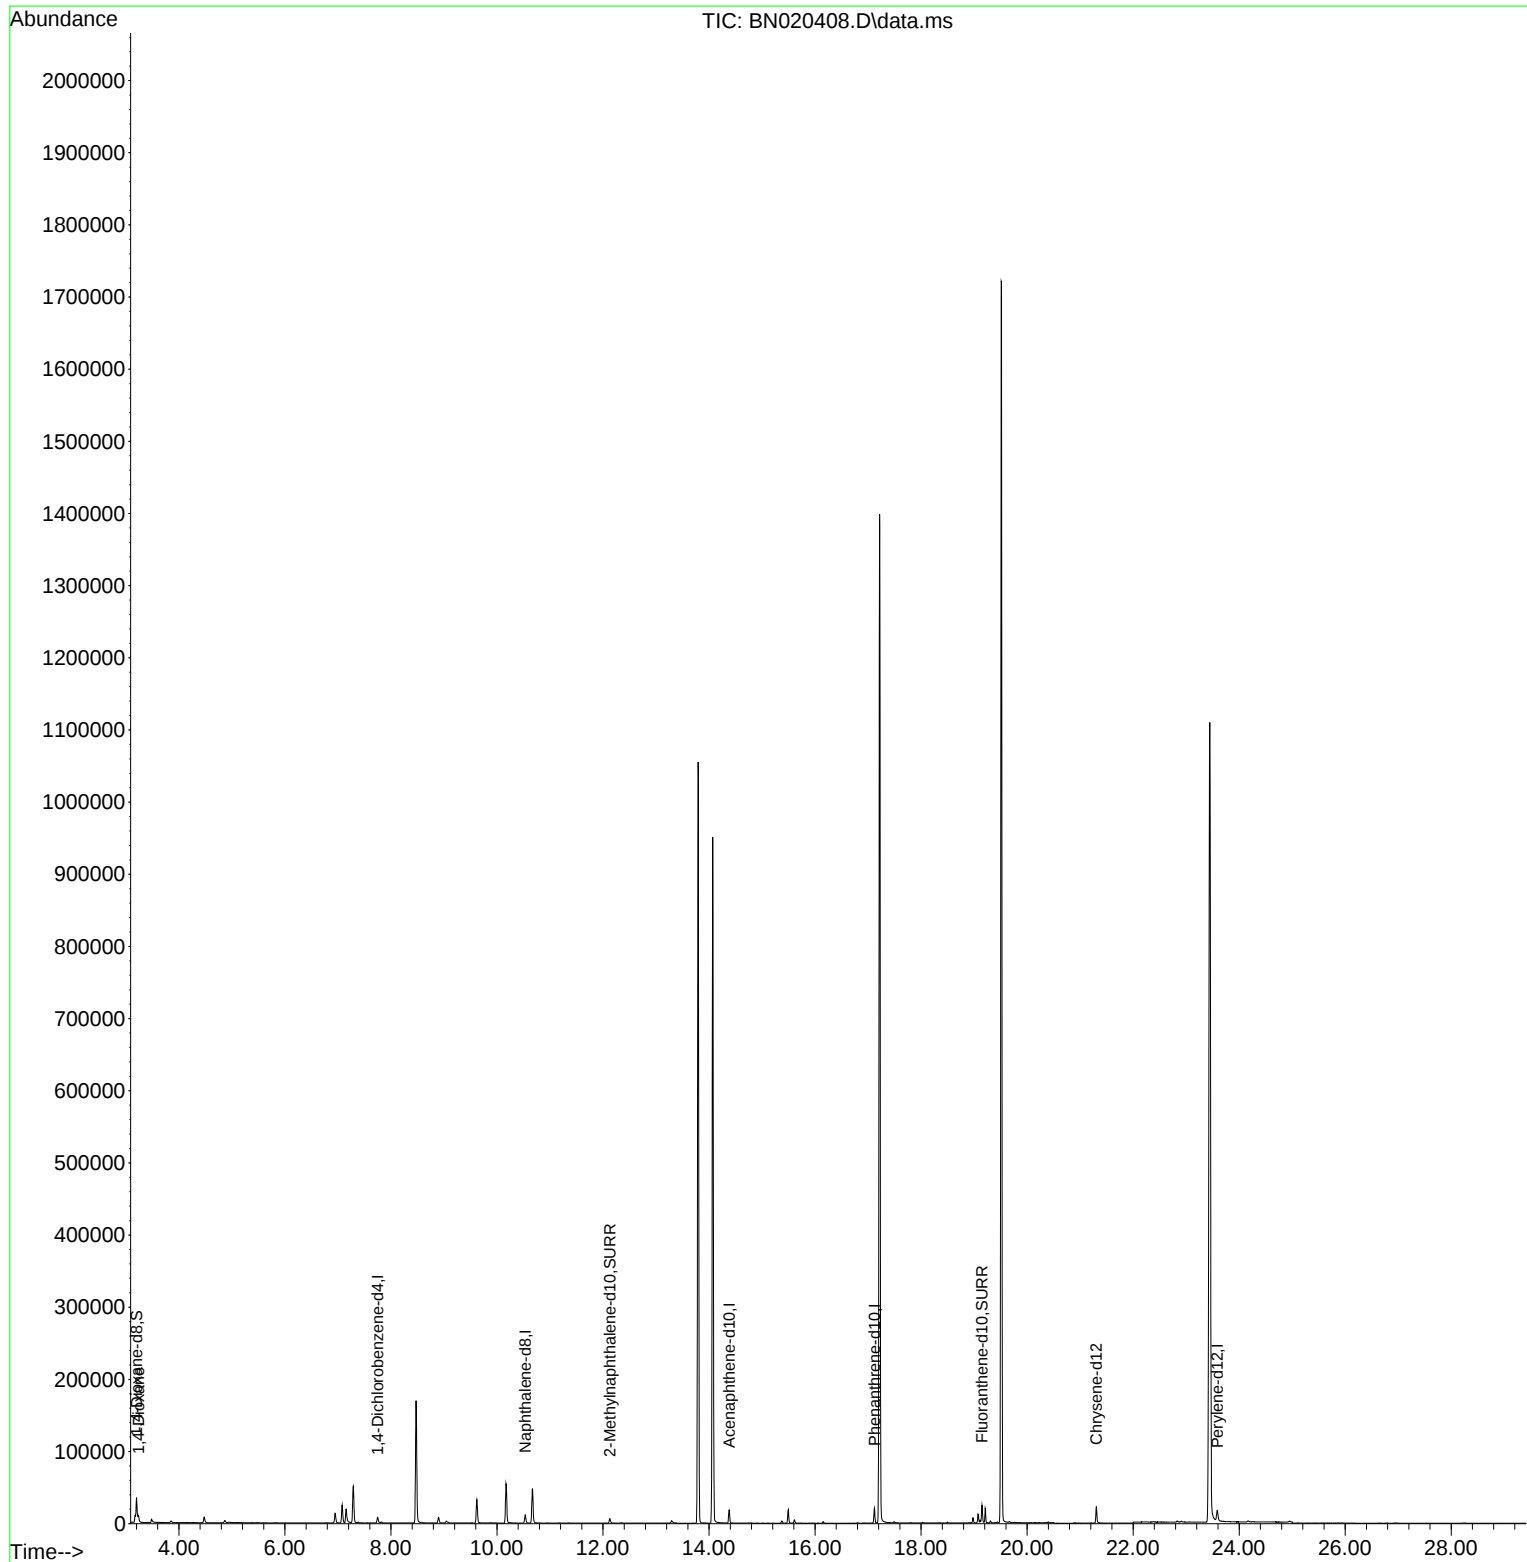

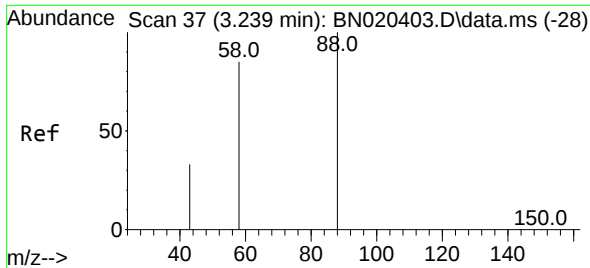

#2
 1,4-Dioxane
 Concen: 0.957 ng/ul
 RT: 3.239 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN020408.D
 Acq: 24 Jun 2022 22:07

Instrument :
 BNA_N
 ClientSampleId :
 YB7L6

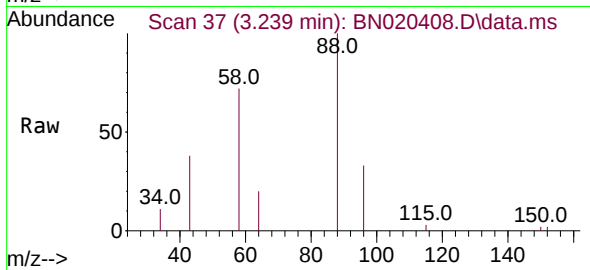

Tgt Ion: 88 Resp: 4805
 Ion Ratio Lower Upper
 88 100
 43 38.4 32.5 48.7
 58 72.3 46.2 69.2#

