

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020418.D
 Acq On : 25 Jun 2022 04:11
 Operator : CG/JU
 Sample : N3359-19
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EW4T4

Quant Time: Jun 25 06:32:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.750	152	2555	0.400	ng/ul	0.00
4) Naphthalene-d8	10.535	136	9060	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.377	164	6124	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.120	188	13772	0.400	ng/ul	0.00
17) Chrysene-d12	21.306	240	12618	0.400	ng/ul	0.00
23) Perylene-d12	23.589	264	12724	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	13945	4.711	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.130	152	5627	0.378	ng/ul	0.00
18) Fluoranthene-d10	19.151	212	16397	0.394	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.579	128	1546	0.055	ng/ul#	90
7) 2-Methylnaphthalene	12.201	142	866	0.046	ng/ul	96
8) 1-Methylnaphthalene	12.421	142	471	0.027	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020418.D
Acq On : 25 Jun 2022 04:11
Operator : CG/JU
Sample : N3359-19
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EW4T4

Quant Time: Jun 25 06:32:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration




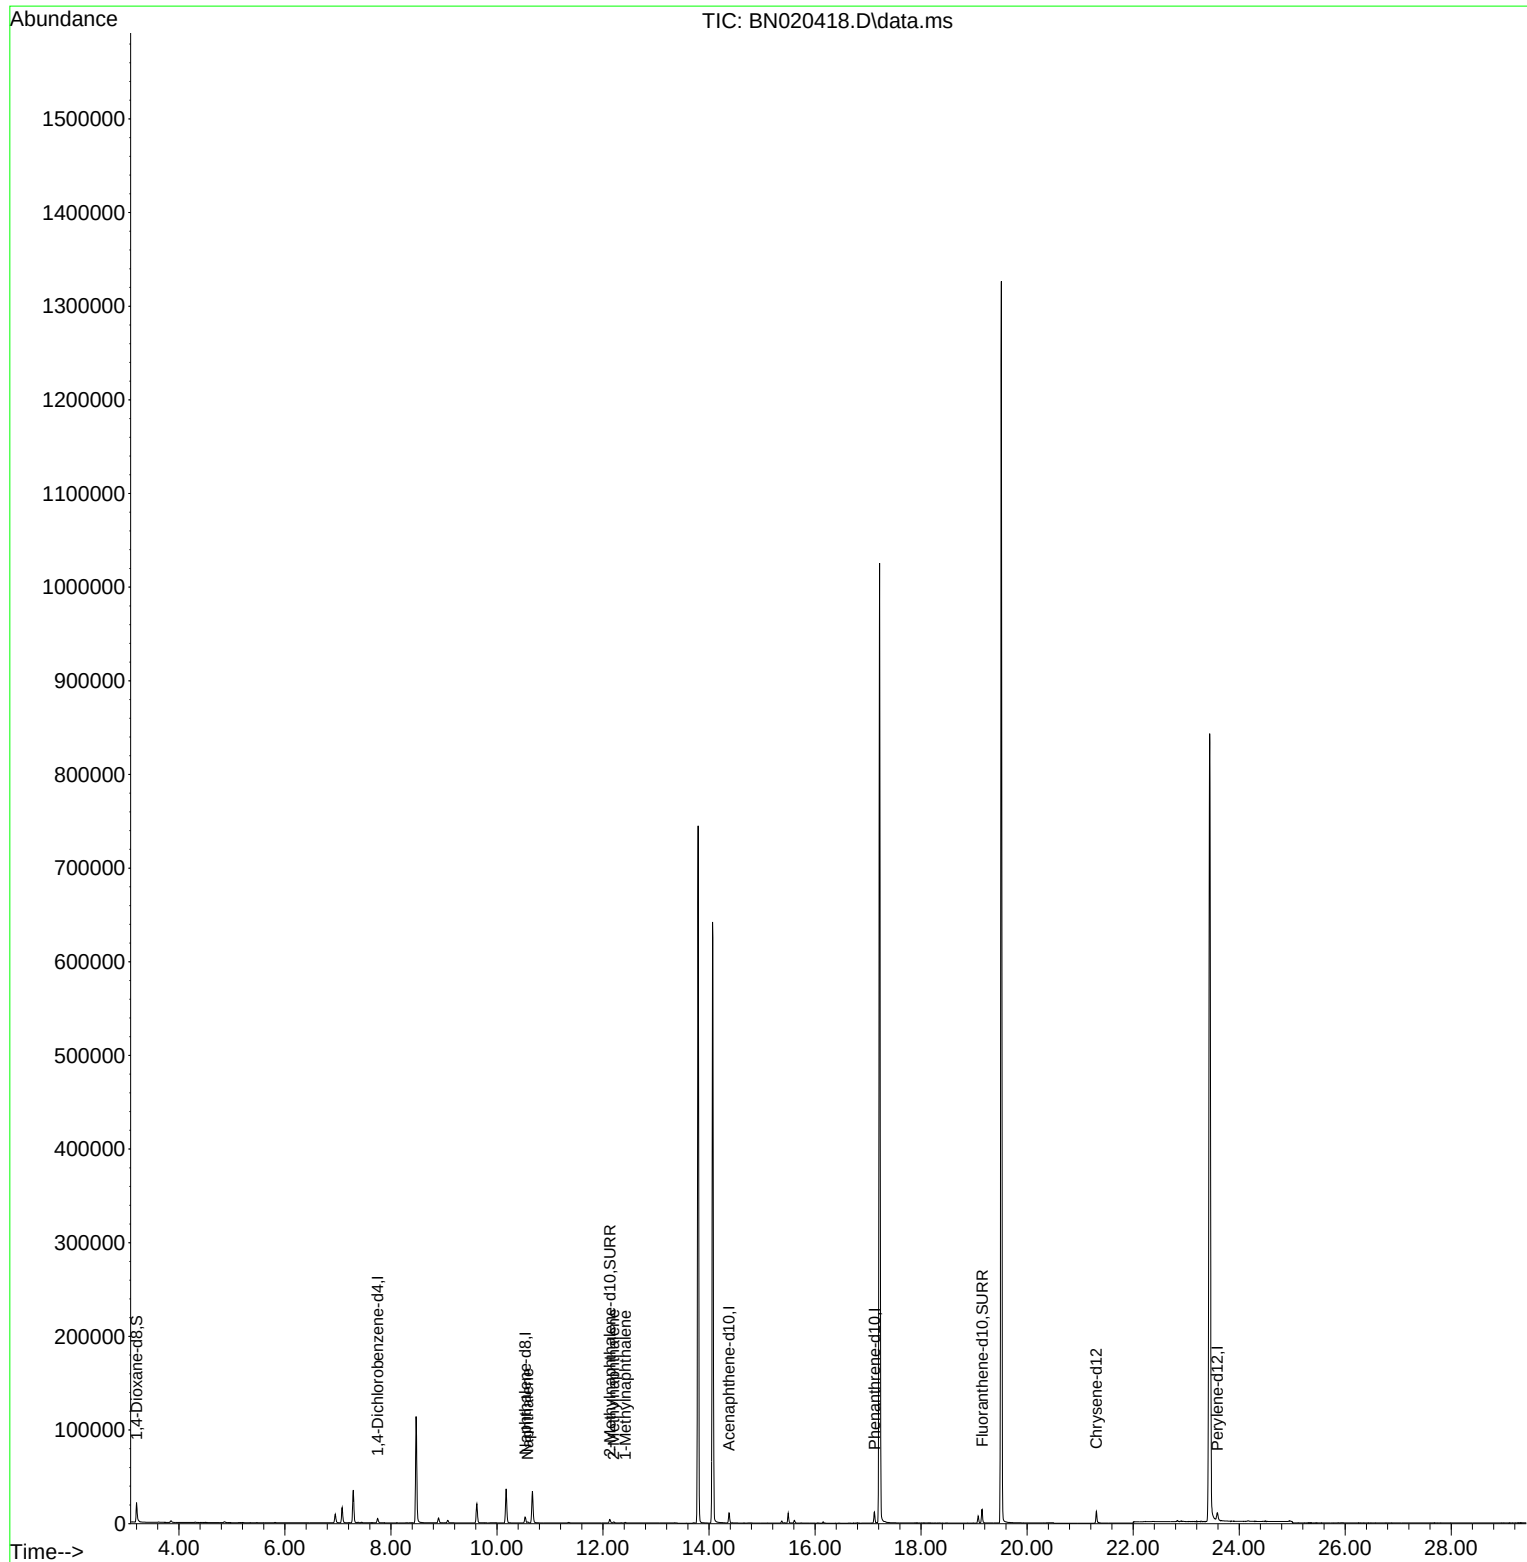


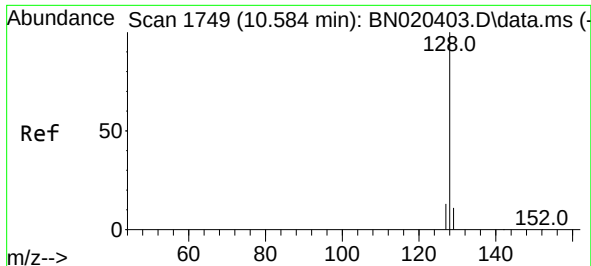

#5
Naphthalene
Concen: 0.055 ng/ul
RT: 10.579 min Scan# 1748
Delta R.T. -0.004 min
Lab File: BN020418.D
Acq: 25 Jun 2022 04:11




Instrument :
BNA_N
ClientSampleId :
EW4T4


Tgt Ion:128 Resp: 1546
Ion Ratio Lower Upper
128 100
129 16.5 9.5 14.3#
127 17.3 11.3 16.9#

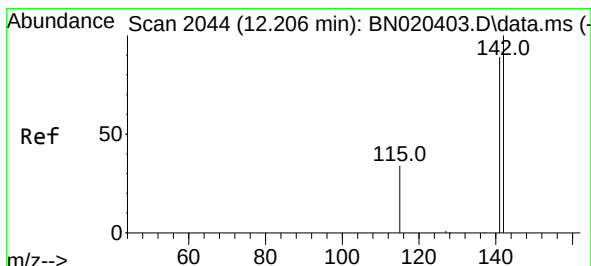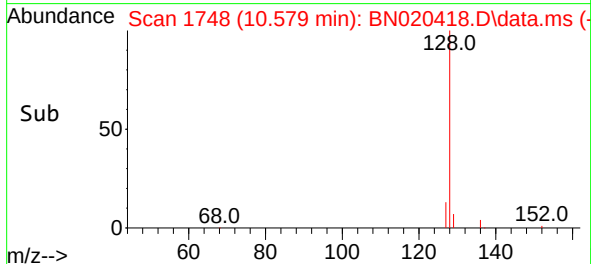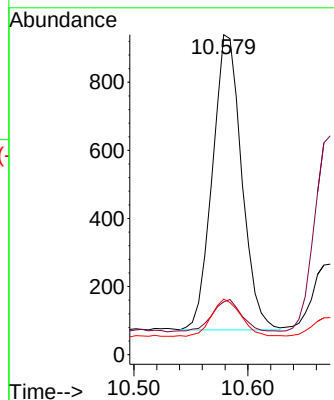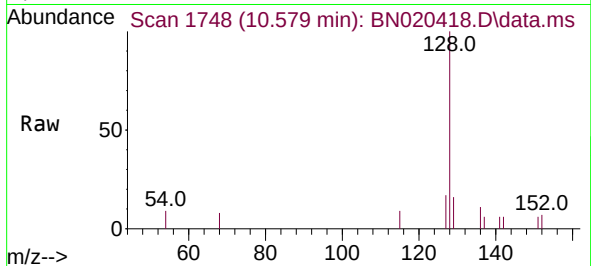

#7
2-Methylnaphthalene
Concen: 0.046 ng/ul
RT: 12.201 min Scan# 2043
Delta R.T. -0.004 min
Lab File: BN020418.D
Acq: 25 Jun 2022 04:11

Tgt Ion:142 Resp: 866
Ion Ratio Lower Upper
142 100
141 86.6 72.1 108.1

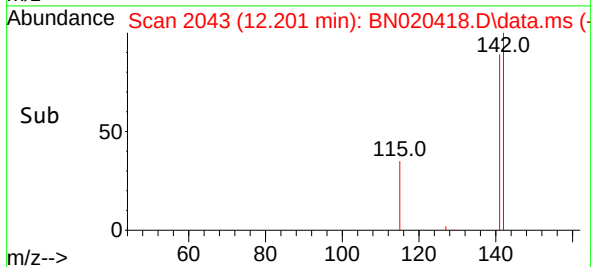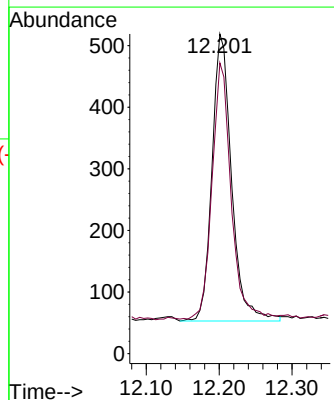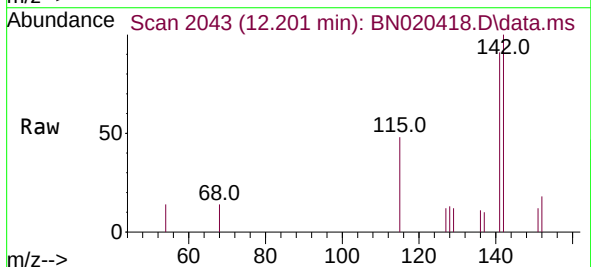

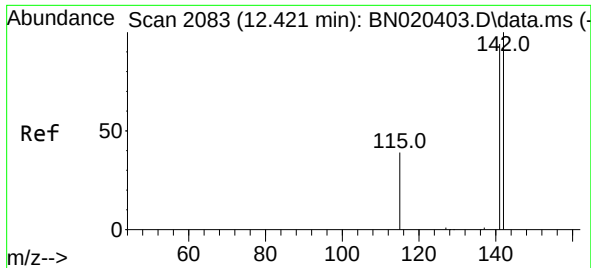

#8

1-Methylnaphthalene

Concen: 0.027 ng/ul

RT: 12.421 min Scan# 20

Delta R.T. 0.001 min

Lab File: BN020418.D


Acq: 25 Jun 2022 04:11

Instrument :

BNA_N

ClientSampleId :

EW4T4

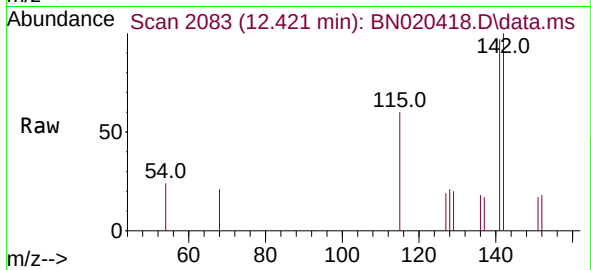

Tgt Ion:142 Resp: 471

Ion Ratio Lower Upper

142 100

141 92.6 73.7 110.5

