

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
 Data File : BN020456.D
 Acq On : 26 Jun 2022 04:21
 Operator : CG/JU
 Sample : N3400-12
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AD9

Quant Time: Jun 27 03:44:13 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.745	152	2895	0.400	ng/ul	0.00
4) Naphthalene-d8	10.529	136	10181	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.377	164	7028	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.116	188	15161	0.400	ng/ul	0.00
17) Chrysene-d12	21.306	240	13404	0.400	ng/ul	0.00
23) Perylene-d12	23.589	264	12555	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.201	96	14481	4.318	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.124	152	6330	0.379	ng/ul	0.00
18) Fluoranthene-d10	19.146	212	16356	0.370	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.235	88	906	0.265	ng/ul#	85
5) Naphthalene	10.579	128	2891	0.092	ng/ul#	92
7) 2-Methylnaphthalene	12.196	142	590	0.028	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062422\
Data File : BN020456.D
Acq On : 26 Jun 2022 04:21
Operator : CG/JU
Sample : N3400-12
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AD9

Quant Time: Jun 27 03:44:13 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration




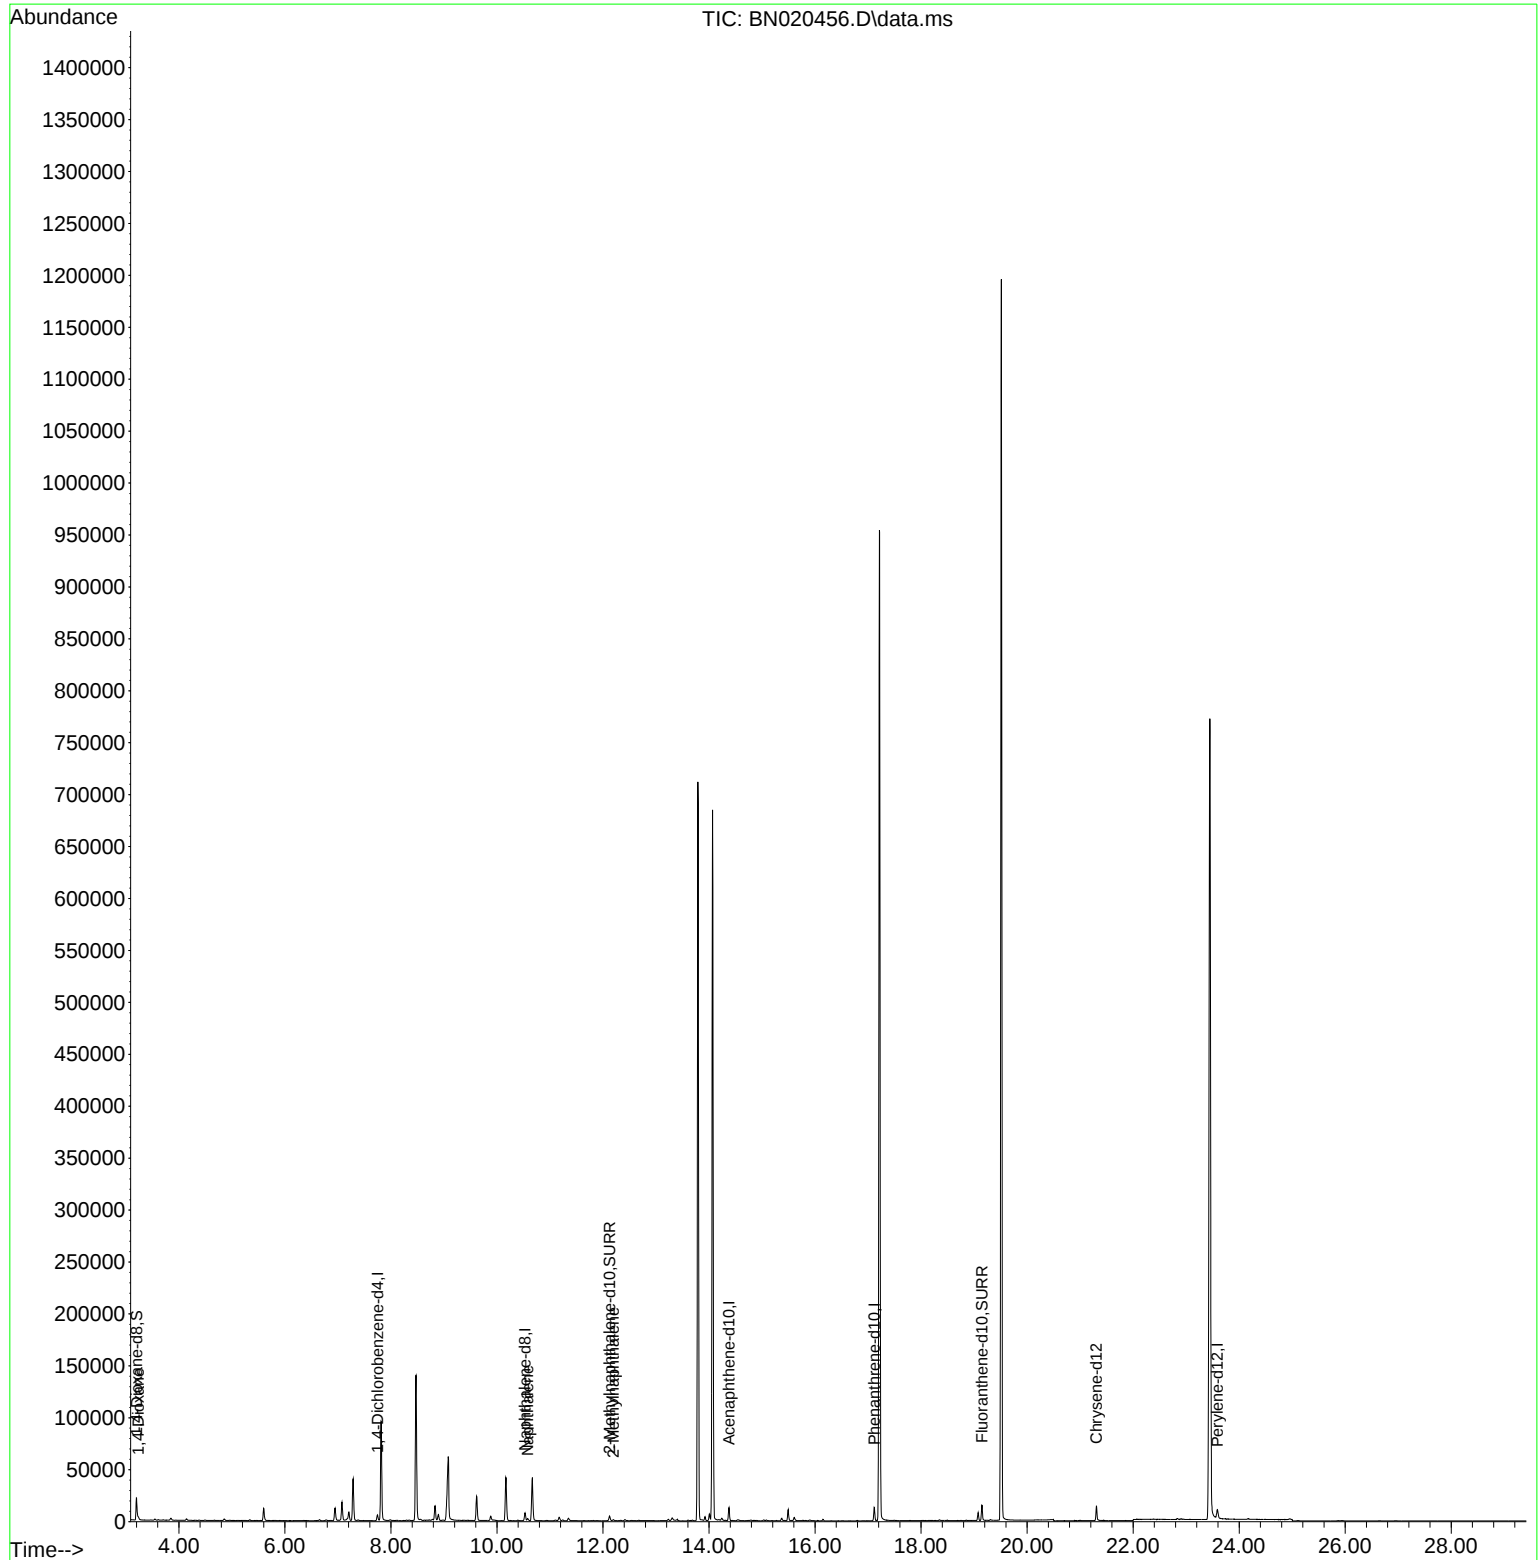


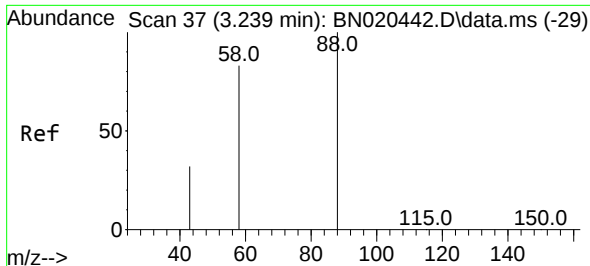

#2
 1,4-Dioxane
 Concen: 0.265 ng/ul
 RT: 3.235 min Scan# 30
 Delta R.T. -0.004 min
 Lab File: BN020456.D
 Acq: 26 Jun 2022 04:21




Instrument :
 BNA_N
 ClientSampleId :
 C0AD9


Tgt Ion: 88 Resp: 906
 Ion Ratio Lower Upper
 88 100
 43 61.4 32.5 48.7#
 58 59.3 46.2 69.2

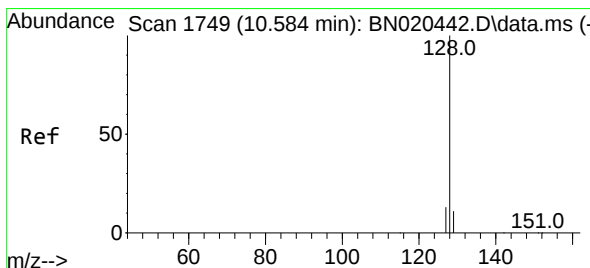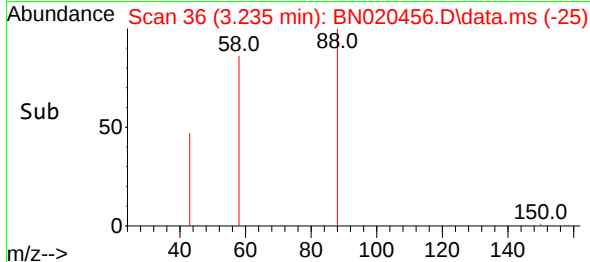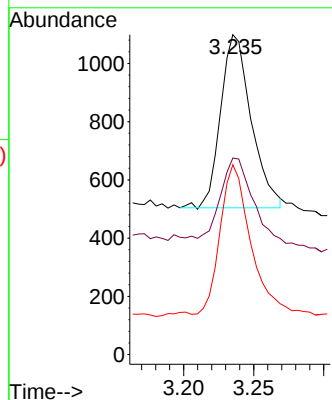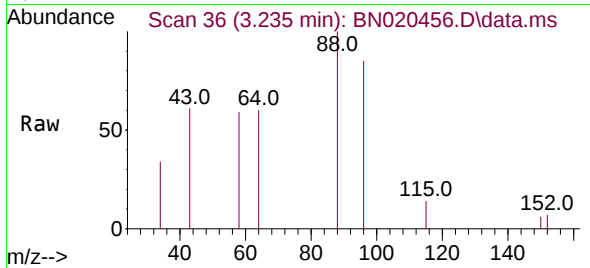

#5
 Naphthalene
 Concen: 0.092 ng/ul
 RT: 10.579 min Scan# 1748
 Delta R.T. -0.004 min
 Lab File: BN020456.D
 Acq: 26 Jun 2022 04:21

Tgt Ion: 128 Resp: 2891
 Ion Ratio Lower Upper
 128 100
 129 14.9 9.5 14.3#
 127 17.2 11.3 16.9#

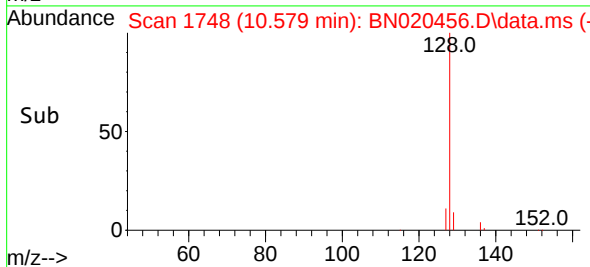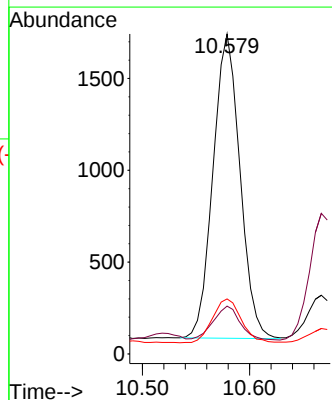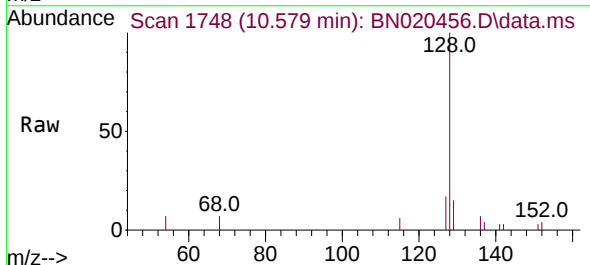

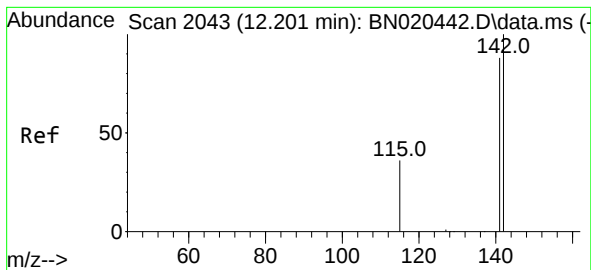

#7
 2-Methylnaphthalene
 Concen: 0.028 ng/ul
 RT: 12.196 min Scan# 2042
 Delta R.T. -0.009 min
 Lab File: BN020456.D
 Acq: 26 Jun 2022 04:21

Instrument :
 BNA_N
 ClientSampleId :
 C0AD9

Tgt Ion:142 Resp: 590
 Ion Ratio Lower Upper
 142 100
 141 92.7 72.1 108.1

