

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
 Data File : BN032212.D
 Acq On : 24 Jun 2024 17:41
 Operator : MA/JU
 Sample : P2856-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0SH1

Quant Time: Jun 24 18:21:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	255276	20.000	ng/ul	0.00
20) Naphthalene-d8	10.410	136	967605	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.275	164	585646	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.028	188	1192416	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.263	240	1158907	20.000	ng/ul	0.00
88) Perylene-d12	24.174	264	1339353	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.169	96	28813	4.669	ng/uL	0.00
4) Pyridine-d5	3.569	84	382947	22.047	ng/ul	0.00
7) Phenol-d5	6.810	99	515660	23.563	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	274949	21.479	ng/ul	0.00
11) 2-Chlorophenol-d4	7.163	132	451103	27.015	ng/ul	0.00
15) 4-Methylphenol-d8	8.340	113	425853	23.872	ng/ul	0.00
21) Nitrobenzene-d5	8.787	128	216698	29.290	ng/ul	0.00
24) 2-Nitrophenol-d4	9.504	143	230842	30.206	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.040	165	397076	27.831	ng/ul	0.00
31) 4-Chloroaniline-d4	10.557	131	586748	27.698	ng/ul	0.00
46) Dimethylphthalate-d6	13.692	166	1197755	29.357	ng/ul	0.00
49) Acenaphthylene-d8	13.969	160	1376160	29.334	ng/ul	0.00
54) 4-Nitrophenol-d4	14.510	143	183527	22.466	ng/ul	0.00
60) Fluorene-d10	15.269	176	1014067	29.375	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.410	200	120687	20.136	ng/ul	0.00
73) Anthracene-d10	17.128	188	1598548	31.313	ng/ul	0.00
81) Pyrene-d10	19.427	212	1806056	29.123	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.980	264	1942903	30.379	ng/ul	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.457	128	119602	2.388	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
Data File : BN032212.D
Acq On : 24 Jun 2024 17:41
Operator : MA/JU
Sample : P2856-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0SH1

Quant Time: Jun 24 18:21:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

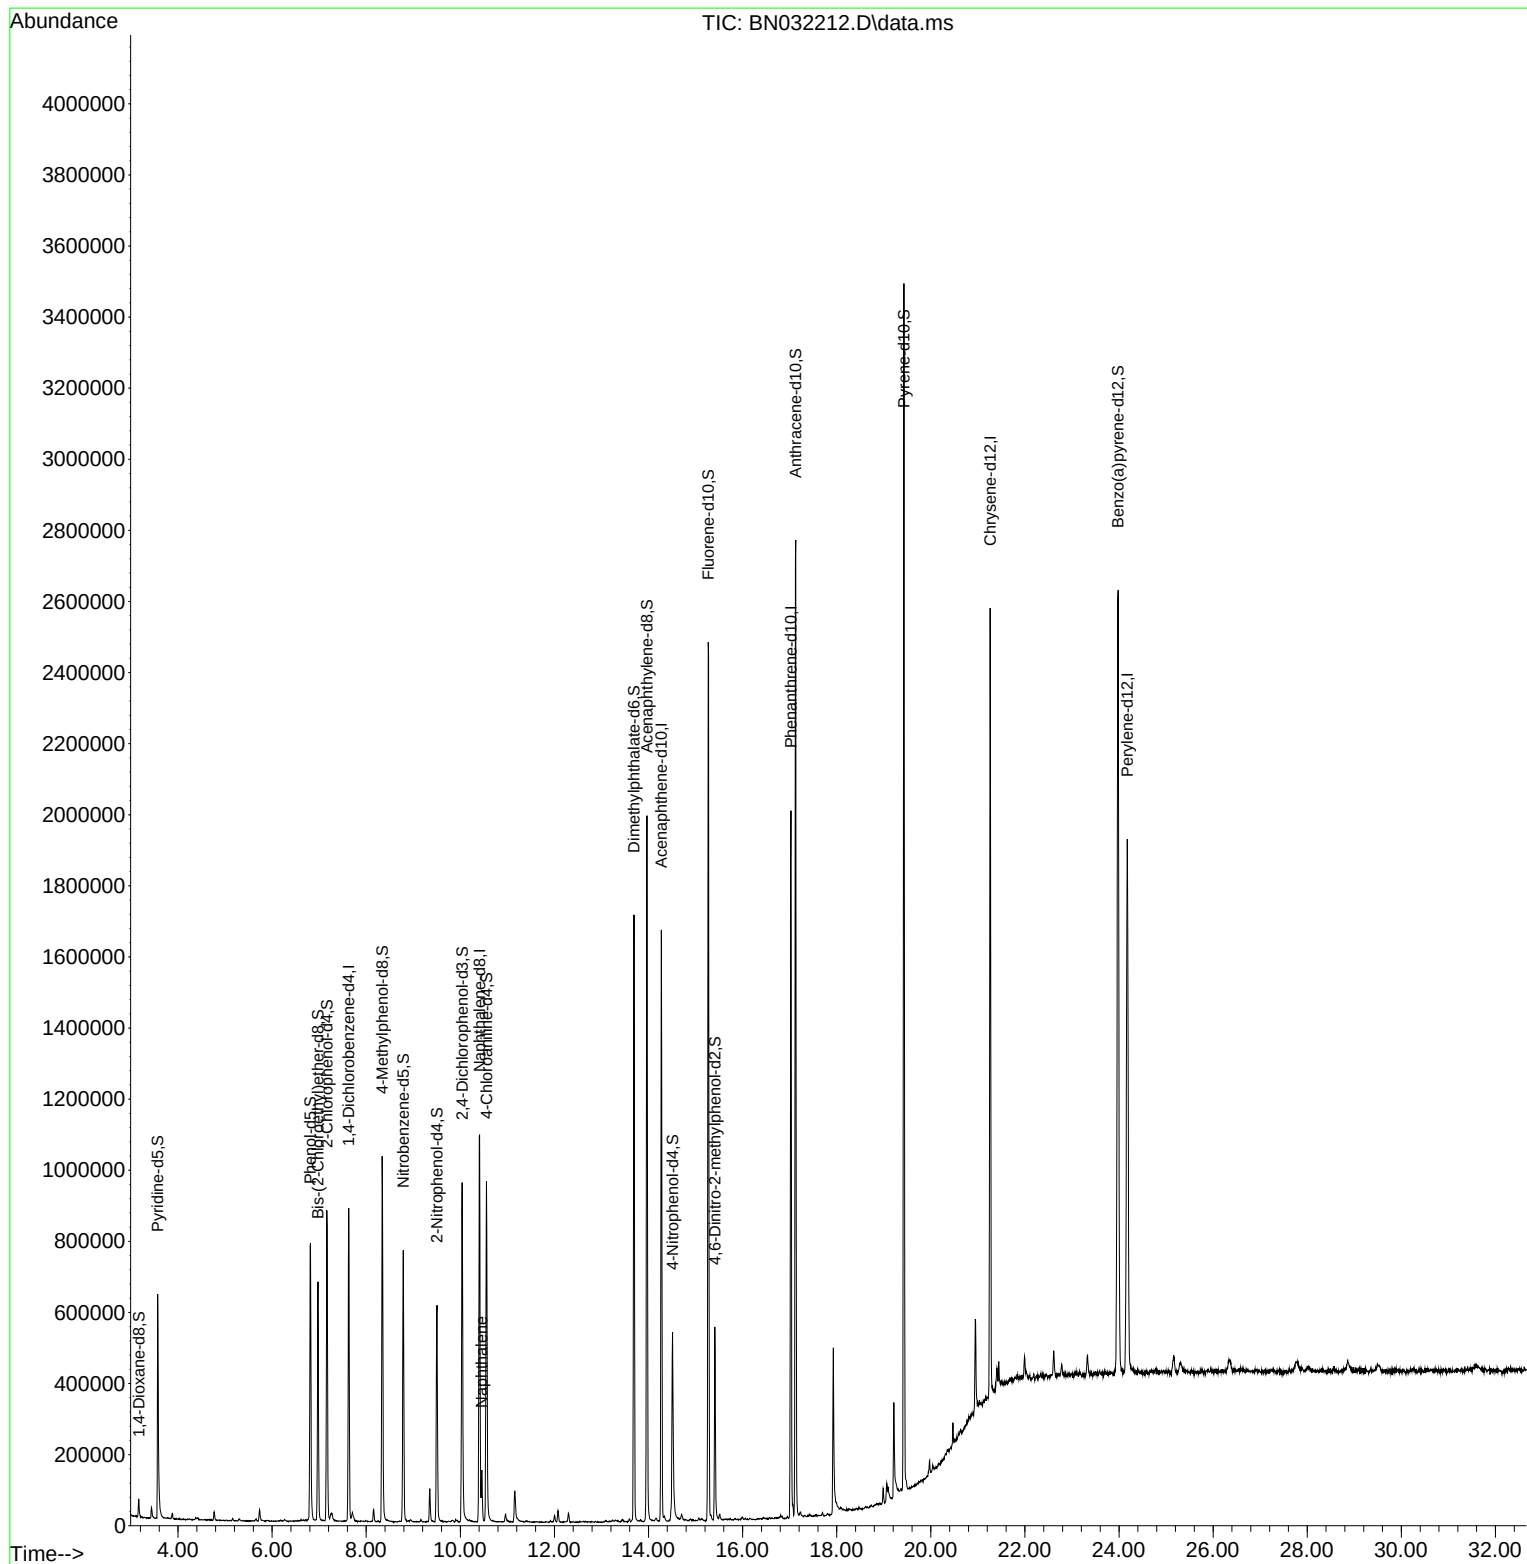

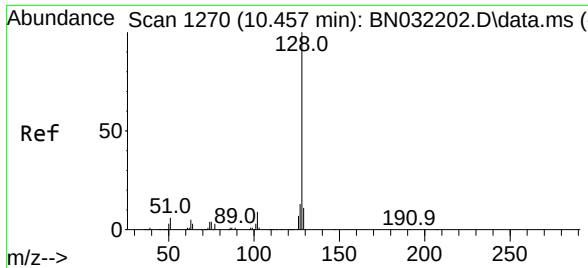

#30
Naphthalene
Concen: 2.388 ng/ul
RT: 10.457 min Scan# 11
Delta R.T. -0.012 min
Lab File: BN032212.D
Acq: 24 Jun 2024 17:41

Instrument :
BNA_N
ClientSampleId :
C0SH1

Tgt Ion:128 Resp: 119602
Ion Ratio Lower Upper
128 100
129 11.1 8.5 12.7
127 12.7 10.3 15.5

