

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
 Data File : BN032223.D
 Acq On : 25 Jun 2024 01:34
 Operator : MA/JU
 Sample : P2873-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0S32

Quant Time: Jun 25 02:14:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 10:49:40 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	311710	20.000	ng/u1	0.00
20) Naphthalene-d8	10.404	136	1179997	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.269	164	705860	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.022	188	1423829	20.000	ng/u1	-0.01
79) Chrysene-d12	21.257	240	1384291	20.000	ng/u1	-0.01
88) Perylene-d12	24.174	264	1629405	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	35396	4.698	ng/uL	0.00
4) Pyridine-d5	3.575	84	140002	6.601	ng/u1	0.00
7) Phenol-d5	6.811	99	185622	6.946	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	449795	28.777	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.163	132	572625	28.084	ng/u1	0.00
15) 4-Methylphenol-d8	8.340	113	348363	15.993	ng/u1	0.00
21) Nitrobenzene-d5	8.787	128	345483	38.292	ng/u1	0.00
24) 2-Nitrophenol-d4	9.499	143	258920	27.781	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.034	165	544476	31.293	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.552	131	761649	29.483	ng/u1	-0.01
46) Dimethylphthalate-d6	13.693	166	1868648	38.000	ng/u1	0.00
49) Acenaphthylene-d8	13.963	160	2138929	37.828	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.516	143	44022	4.471	ng/u1	0.01
60) Fluorene-d10	15.269	176	1601976	38.502	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.410	200	71154	9.942	ng/u1	0.00
73) Anthracene-d10	17.122	188	2637658	43.270	ng/u1	0.00
81) Pyrene-d10	19.428	212	2957271	39.922	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.974	264	3304621	42.473	ng/u1	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.787	77	13014	1.038	ng/u1	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
Data File : BN032223.D
Acq On : 25 Jun 2024 01:34
Operator : MA/JU
Sample : P2873-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0S32


Quant Time: Jun 25 02:14:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 10:49:40 2024
Response via : Initial Calibration

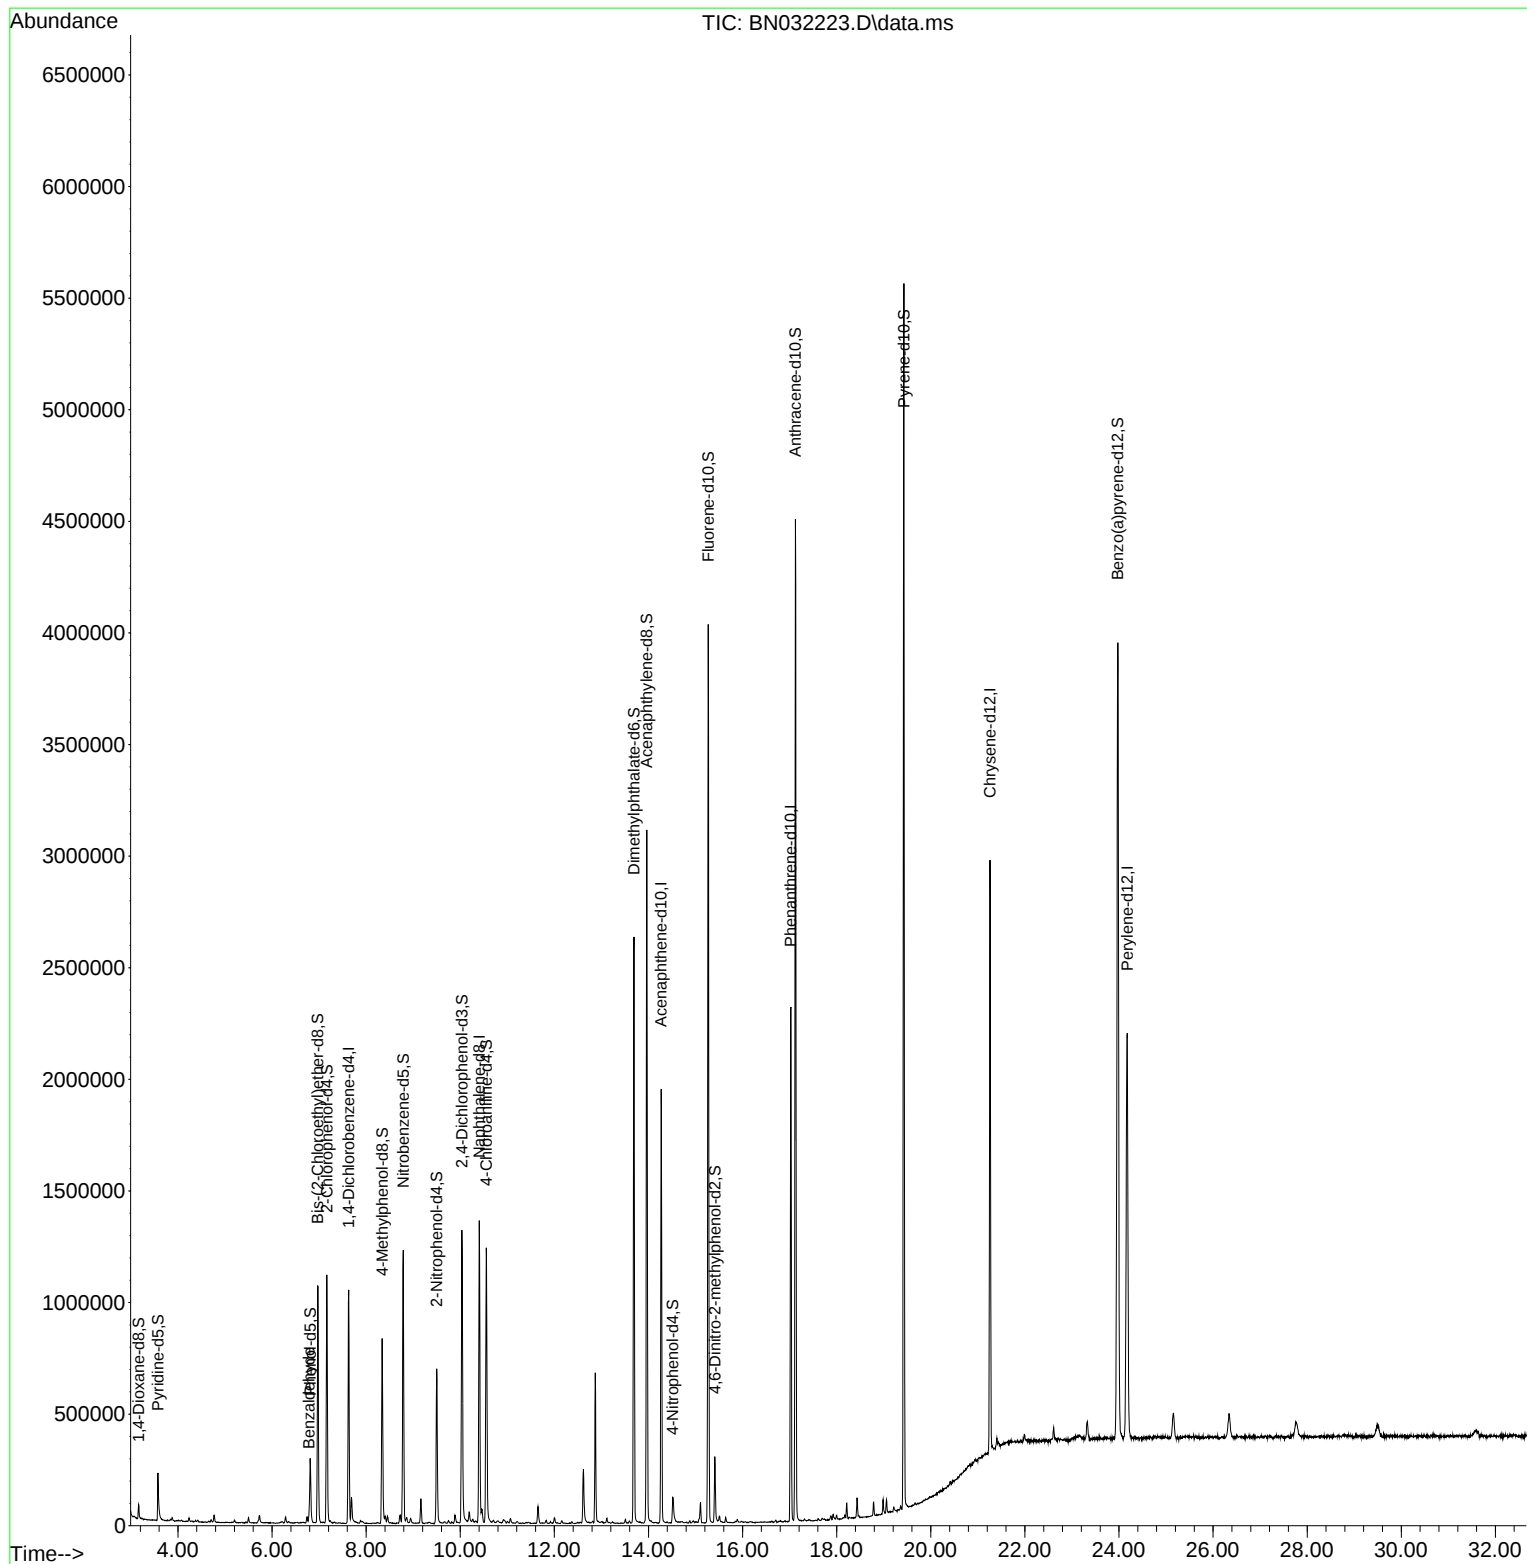

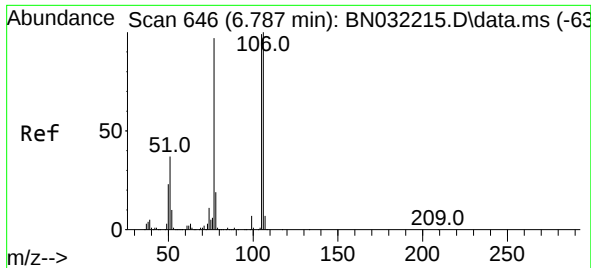

#6
Benzaldehyde
Concen: 1.038 ng/ul
RT: 6.787 min Scan# 64
Delta R.T. -0.006 min
Lab File: BN032223.D
Acq: 25 Jun 2024 01:34

Instrument :
BNA_N
ClientSampleId :
C0S32

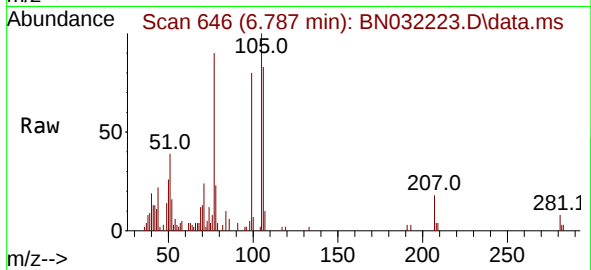

Tgt Ion:	77	Resp:	13014
Ion	Ratio	Lower	Upper
77	100		
105	111.6	80.2	120.4
106	92.3	76.8	115.2

