

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
 Data File : BN032217.D
 Acq On : 24 Jun 2024 21:38
 Operator : MA/JU
 Sample : PB161672BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK672

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	26	30	39	rVB	70757	109159	1.65%	0.167%
2	3.569	95	99	116	rBV	760402	1243001	18.78%	1.898%
3	3.875	146	151	159	rVB	15691	26058	0.39%	0.040%
4	6.810	643	650	665	rBV	1050300	1741738	26.31%	2.660%
5	6.975	671	678	689	rBV	868005	1384584	20.92%	2.115%
6	7.163	703	710	729	rBV	1127873	1856093	28.04%	2.835%
7	7.628	780	789	800	rBV	1011494	1622463	24.51%	2.478%
8	8.340	902	910	934	rBV	1293655	2213411	33.44%	3.380%
9	8.787	978	986	997	rBV	964865	1625131	24.55%	2.482%
10	9.498	1100	1107	1118	rBV	781532	1361127	20.56%	2.079%
11	9.751	1146	1150	1153	rBV4	3591	6899	0.10%	0.011%
12	10.034	1191	1198	1221	rBV	1155960	2177832	32.90%	3.326%
13	10.404	1254	1261	1274	rBV	1264052	2187390	33.04%	3.341%
14	10.557	1279	1287	1300	rBV	947450	1787294	27.00%	2.730%
15	12.004	1527	1533	1538	rBV3	17108	29980	0.45%	0.046%
16	13.234	1738	1742	1750	rVB9	3668	7243	0.11%	0.011%
17	13.686	1812	1819	1835	rBV	2032972	2950289	44.57%	4.506%
18	13.963	1859	1866	1881	rBV	2414558	3780084	57.10%	5.773%
19	14.275	1911	1919	1930	rBV	1891216	2795787	42.23%	4.270%
20	14.510	1952	1959	1978	rBV	722651	1413634	21.35%	2.159%
21	14.686	1986	1989	2000	rVB	5061	12048	0.18%	0.018%
22	15.269	2081	2088	2106	rBV	3166507	4634996	70.02%	7.079%
23	15.410	2106	2112	2125	rVV	817416	1219973	18.43%	1.863%
24	15.510	2125	2129	2135	rVB2	17726	28978	0.44%	0.044%
25	15.780	2170	2175	2179	rVB3	8199	10149	0.15%	0.015%
26	16.051	2215	2221	2226	rVB5	10115	15737	0.24%	0.024%
27	16.704	2329	2332	2336	rVB6	5944	6807	0.10%	0.010%
28	16.822	2348	2352	2357	rVB5	4856	7482	0.11%	0.011%
29	17.022	2380	2386	2396	rBV	2188848	3256405	49.19%	4.973%
30	17.122	2396	2403	2416	rBV2	3343139	5054342	76.35%	7.719%
31	17.692	2497	2500	2504	rBV6	10376	11873	0.18%	0.018%
32	17.922	2535	2539	2546	rBV6	16820	33051	0.50%	0.050%
33	18.986	2716	2720	2727	rBV2	49009	70813	1.07%	0.108%
34	19.063	2729	2733	2737	rVV	37105	51974	0.79%	0.079%
35	19.427	2789	2795	2810	rBV	4374954	6016696	90.89%	9.189%
36	21.257	3101	3106	3116	rBV	2473745	3731138	56.36%	5.698%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
Data File : BN032217.D
Acq On : 24 Jun 2024 21:38
Operator : MA/JU
Sample : PB161672BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK672

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	23.974	3559	3568	3578	rBV2	2681480	6619708	100.00%	10.110%
38	24.168	3593	3601	3615	rVB	1727896	4377523	66.13%	6.685%




Sum of corrected areas: 65478890

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
Data File : BN032217.D
Acq On : 24 Jun 2024 21:38
Operator : MA/JU
Sample : PB161672BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK672

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

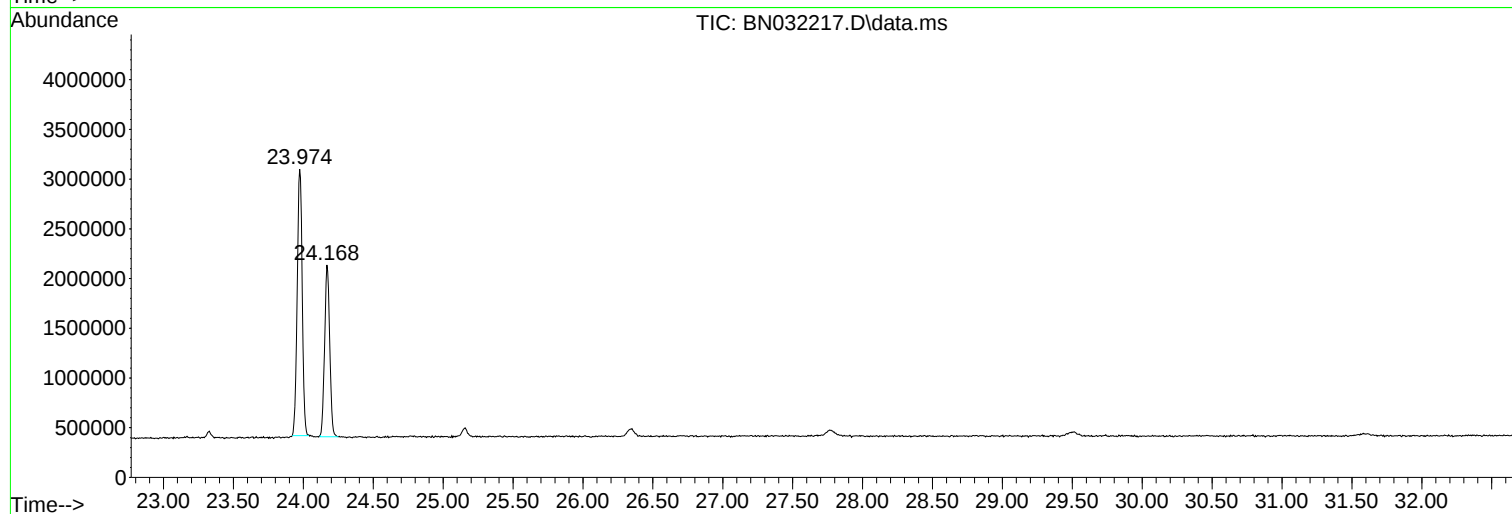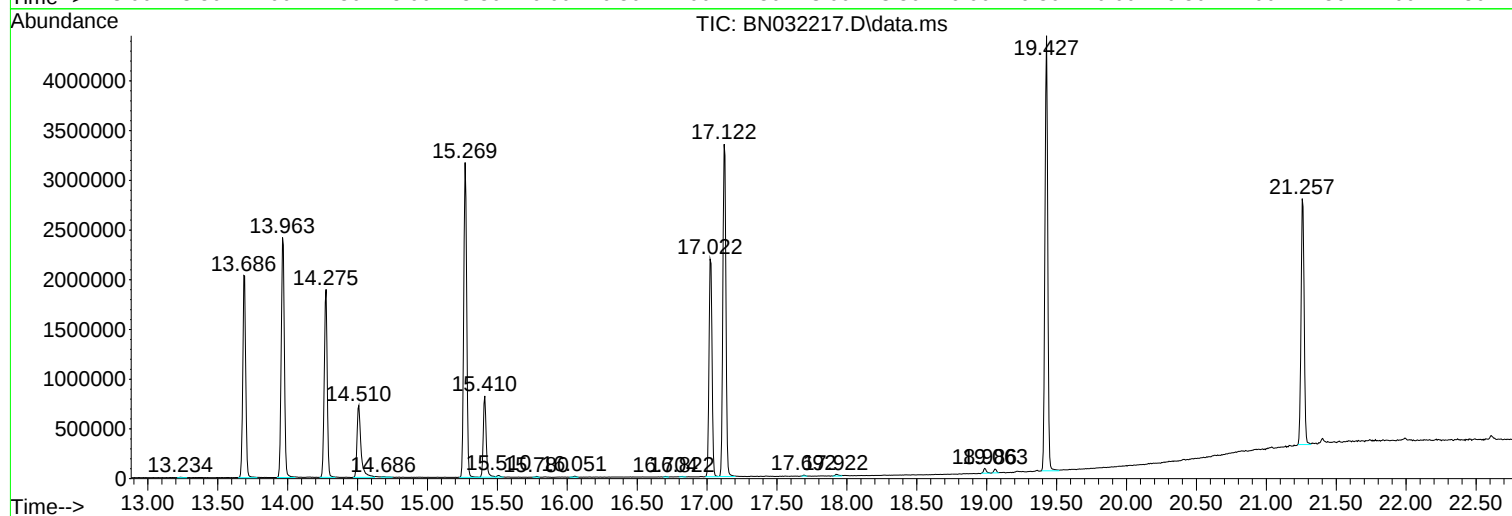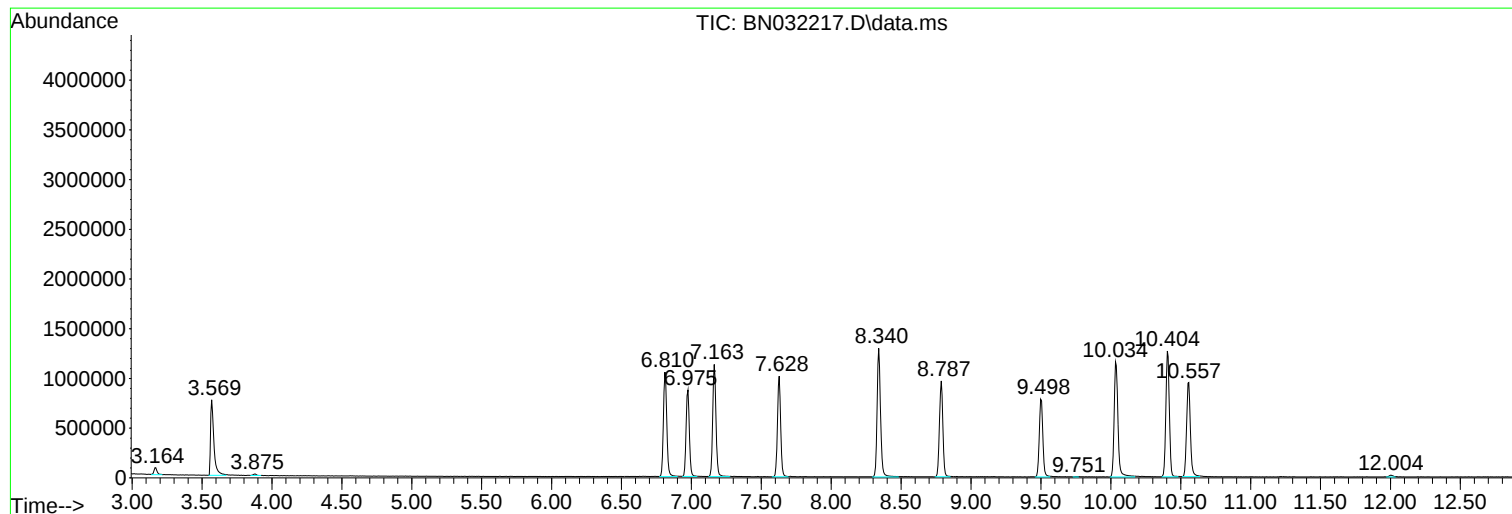

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
Data File : BN032217.D
Acq On : 24 Jun 2024 21:38
Operator : MA/JU
Sample : PB161672BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK672

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
Data File : BN032217.D
Acq On : 24 Jun 2024 21:38
Operator : MA/JU
Sample : PB161672BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK672

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------