

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
 Data File : BN032226.D
 Acq On : 25 Jun 2024 03:31
 Operator : MA/JU
 Sample : P2961-17
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E1G72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.163	26	30	41	rVB	74641	109956	1.08%	0.127%
2	3.446	75	78	84	rVB3	7653	10861	0.11%	0.013%
3	3.575	97	100	118	rBV	161578	284207	2.79%	0.330%
4	3.875	147	151	162	rVB	64490	103666	1.02%	0.120%
5	4.651	279	283	288	rBV7	6340	12868	0.13%	0.015%
6	4.769	297	303	310	rVB	25675	38782	0.38%	0.045%
7	6.651	619	623	632	rVB	5257	11780	0.12%	0.014%
8	6.810	643	650	660	rBV	422213	699831	6.87%	0.811%
9	6.975	671	678	689	rBV	1292976	2095420	20.58%	2.430%
10	7.163	702	710	720	rBV	1549920	2540895	24.95%	2.946%
11	7.628	782	789	797	rBV	1117016	1849841	18.16%	2.145%
12	7.681	797	798	805	rVB4	10122	16014	0.16%	0.019%
13	8.339	901	910	923	rBV	1211576	2099896	20.62%	2.435%
14	8.787	978	986	1001	rBV	1487468	2530035	24.84%	2.933%
15	9.498	1098	1107	1119	rBV	1254825	2123933	20.86%	2.463%
16	9.686	1129	1139	1145	rBV7	8750	24225	0.24%	0.028%
17	10.034	1191	1198	1222	rBV	1855094	3315791	32.56%	3.844%
18	10.404	1253	1261	1271	rBV	1477038	2561329	25.15%	2.970%
19	10.551	1279	1286	1302	rBV	553323	1048905	10.30%	1.216%
20	11.163	1384	1390	1395	rBV2	18527	42512	0.42%	0.049%
21	11.998	1526	1532	1539	rBV2	27678	46465	0.46%	0.054%
22	13.686	1812	1819	1833	rBV	3090256	4615842	45.33%	5.352%
23	13.963	1854	1866	1880	rBV2	3760583	5837350	57.32%	6.768%
24	14.269	1911	1918	1933	rBV	2150089	3356550	32.96%	3.892%
25	14.510	1953	1959	1977	rBV	286502	594278	5.84%	0.689%
26	14.639	1977	1981	1985	rVV6	5902	11190	0.11%	0.013%
27	14.704	1985	1992	1999	rVB6	7986	21809	0.21%	0.025%
28	15.069	2050	2054	2058	rBV	11725	17653	0.17%	0.020%
29	15.269	2081	2088	2096	rBV	4707522	7047852	69.21%	8.172%
30	15.327	2096	2098	2103	rVV3	21008	26790	0.26%	0.031%
31	15.410	2105	2112	2124	rVV	1488364	2132051	20.94%	2.472%
32	15.510	2124	2129	2137	rVB3	27914	54430	0.53%	0.063%
33	15.845	2180	2186	2188	rBV6	6078	10387	0.10%	0.012%
34	16.810	2348	2350	2357	rVB4	7728	11736	0.12%	0.014%
35	16.951	2369	2374	2377	rBV6	9114	14052	0.14%	0.016%
36	17.021	2380	2386	2397	rVV	2663551	3920741	38.50%	4.546%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
Data File : BN032226.D
Acq On : 25 Jun 2024 03:31
Operator : MA/JU
Sample : P2961-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Title : SVOA CALIBRATION

37	17.121	2397	2403	2418	rVV2	5215808	7838359	76.97%	9.088%
38	17.310	2432	2435	2440	rBV	8009	10998	0.11%	0.013%
39	17.421	2449	2454	2460	rVB4	8149	13668	0.13%	0.016%
40	17.698	2497	2501	2506	rVB6	8670	13656	0.13%	0.016%
41	17.921	2534	2539	2548	rBV	120073	198482	1.95%	0.230%
42	17.992	2549	2551	2556	rVB	12599	18011	0.18%	0.021%
43	18.986	2715	2720	2725	rBV	78209	113923	1.12%	0.132%
44	19.057	2728	2732	2737	rBV	68367	104267	1.02%	0.121%
45	19.209	2754	2758	2765	rBV	84109	129684	1.27%	0.150%
46	19.357	2781	2783	2788	rVB5	20435	21230	0.21%	0.025%
47	19.427	2788	2795	2808	rBV	6515321	9032721	88.70%	10.473%
48	21.256	3101	3106	3113	rBV	2922889	4313557	42.36%	5.001%
49	23.974	3559	3568	3581	rVB2	4087955	10183813	100.00%	11.807%
50	24.174	3593	3602	3612	rVB	2034289	5016464	49.26%	5.816%




Sum of corrected areas: 86248756

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
Data File : BN032226.D
Acq On : 25 Jun 2024 03:31
Operator : MA/JU
Sample : P2961-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

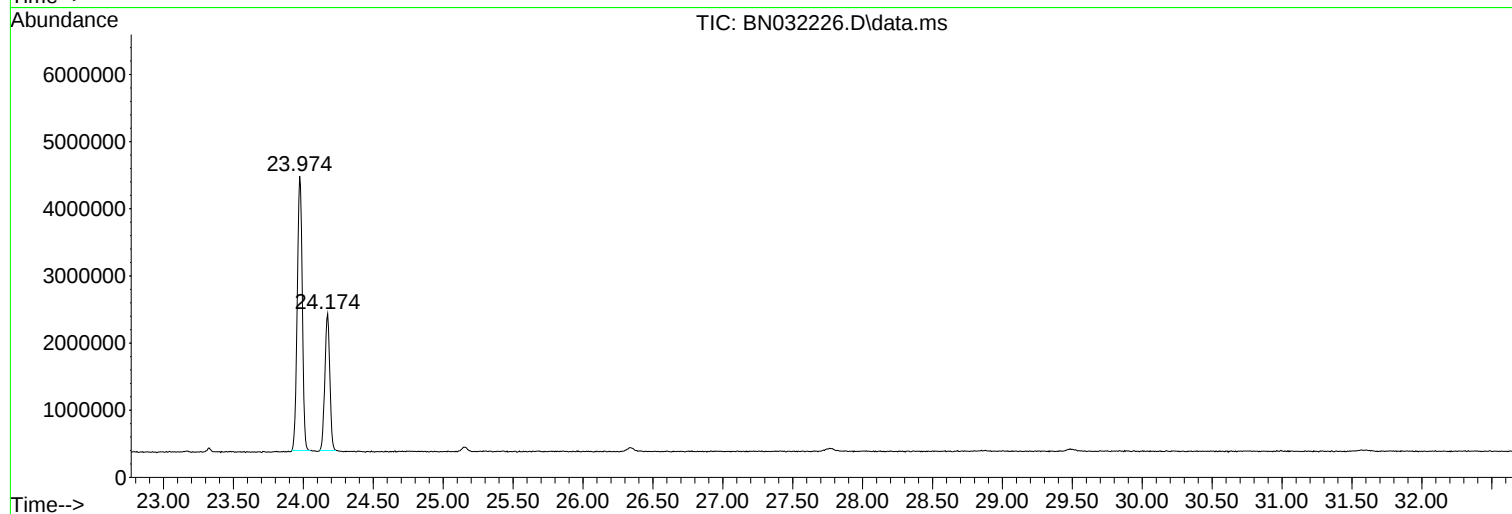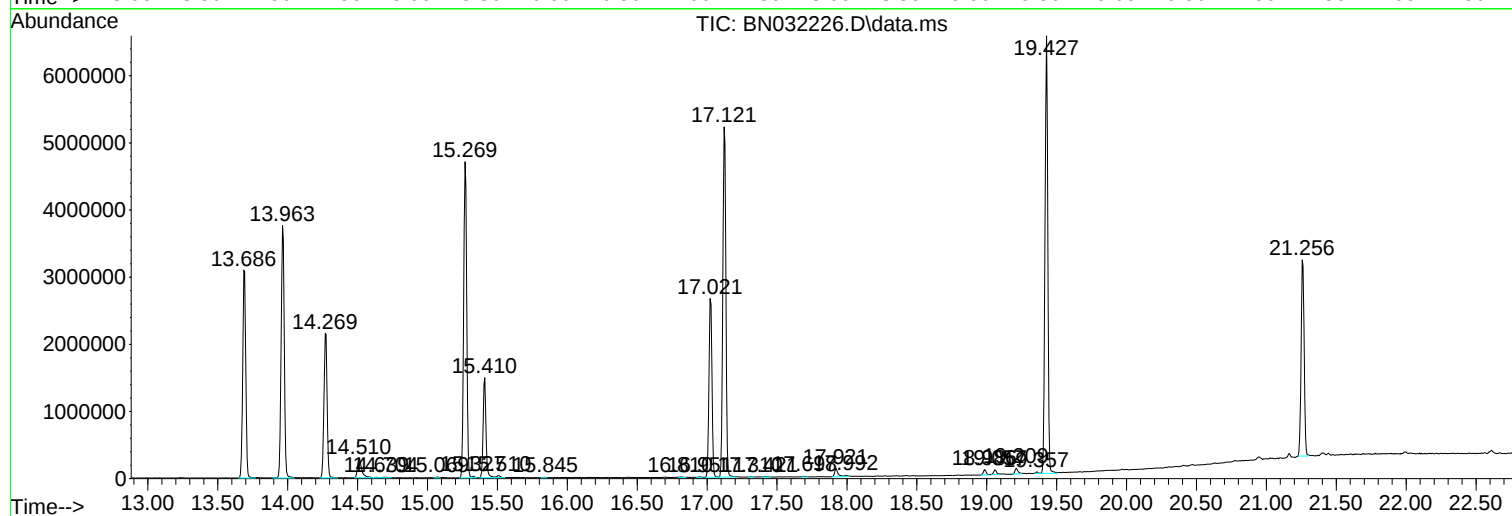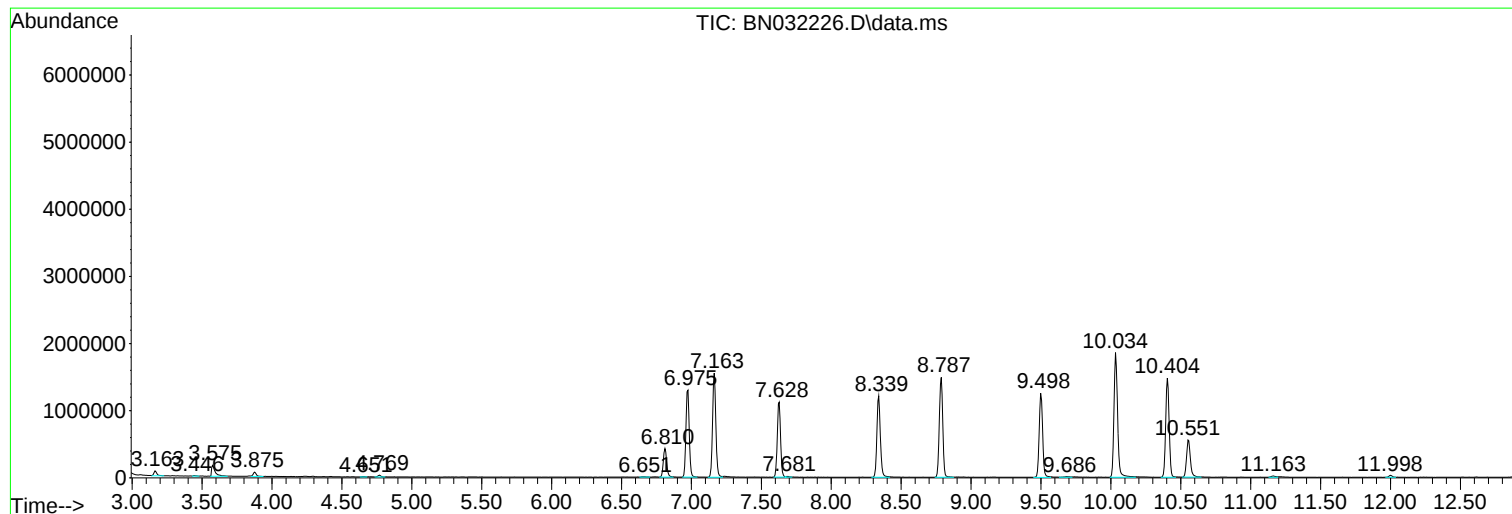

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
Data File : BN032226.D
Acq On : 25 Jun 2024 03:31
Operator : MA/JU
Sample : P2961-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
Data File : BN032226.D
Acq On : 25 Jun 2024 03:31
Operator : MA/JU
Sample : P2961-17
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E1G72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc