

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
 Data File : BN032232.D
 Acq On : 25 Jun 2024 08:06
 Operator : MA/JU
 Sample : PB161513BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK513

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN032232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	26	30	36	rBV	70657	93090	1.54%	0.152%
2	3.564	96	98	122	rBV	785897	1272586	21.12%	2.082%
3	3.875	146	151	157	rBV2	19343	29002	0.48%	0.047%
4	6.811	643	650	663	rBV	963561	1627570	27.01%	2.663%
5	6.969	670	677	687	rBV	826878	1305348	21.66%	2.136%
6	7.163	701	710	723	rBV	1072139	1765989	29.30%	2.890%
7	7.622	781	788	805	rVB	932978	1556461	25.83%	2.547%
8	8.340	902	910	930	rBV	1179086	2072887	34.39%	3.392%
9	8.781	977	985	997	rBV	911376	1557615	25.84%	2.549%
10	9.499	1099	1107	1120	rBV	754781	1294637	21.48%	2.118%
11	10.034	1191	1198	1216	rBV	1120599	2028590	33.66%	3.319%
12	10.404	1253	1261	1272	rBV	1214270	2065853	34.28%	3.380%
13	10.551	1277	1286	1314	rVB	1156482	2086213	34.62%	3.414%
14	12.004	1527	1533	1541	rBV2	14176	29482	0.49%	0.048%
15	13.687	1812	1819	1833	rBV	1965577	2785467	46.22%	4.558%
16	13.963	1857	1866	1888	rBV	2282811	3550222	58.91%	5.809%
17	14.269	1911	1918	1928	rBV	1713834	2570873	42.66%	4.207%
18	14.504	1951	1958	1979	rBV	666912	1317885	21.87%	2.156%
19	15.269	2080	2088	2105	rBV	2911291	4317384	71.64%	7.064%
20	15.404	2105	2111	2124	rVV	687518	1053884	17.49%	1.724%
21	15.510	2124	2129	2133	rVB4	13810	25719	0.43%	0.042%
22	16.051	2218	2221	2225	rVB4	6785	10318	0.17%	0.017%
23	16.810	2346	2350	2356	rVB5	4514	8150	0.14%	0.013%
24	17.022	2379	2386	2396	rBV	2147628	3015185	50.03%	4.934%
25	17.122	2396	2403	2414	rVV	3302199	4710053	78.15%	7.707%
26	17.692	2496	2500	2505	rBV8	5091	7867	0.13%	0.013%
27	17.922	2536	2539	2543	rBV6	7466	10714	0.18%	0.018%
28	18.986	2716	2720	2728	rBV3	42589	64513	1.07%	0.106%
29	19.057	2728	2732	2738	rBV	39659	64515	1.07%	0.106%
30	19.427	2788	2795	2807	rBV	3854120	5508560	91.40%	9.013%
31	21.257	3101	3106	3114	rBV	2328918	3365559	55.84%	5.507%
32	23.974	3559	3568	3583	rVB	2483223	6026879	100.00%	9.861%
33	24.168	3593	3601	3615	rVB	1565847	3916649	64.99%	6.409%




Sum of corrected areas: 61115719

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
Data File : BN032232.D
Acq On : 25 Jun 2024 08:06
Operator : MA/JU
Sample : PB161513BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

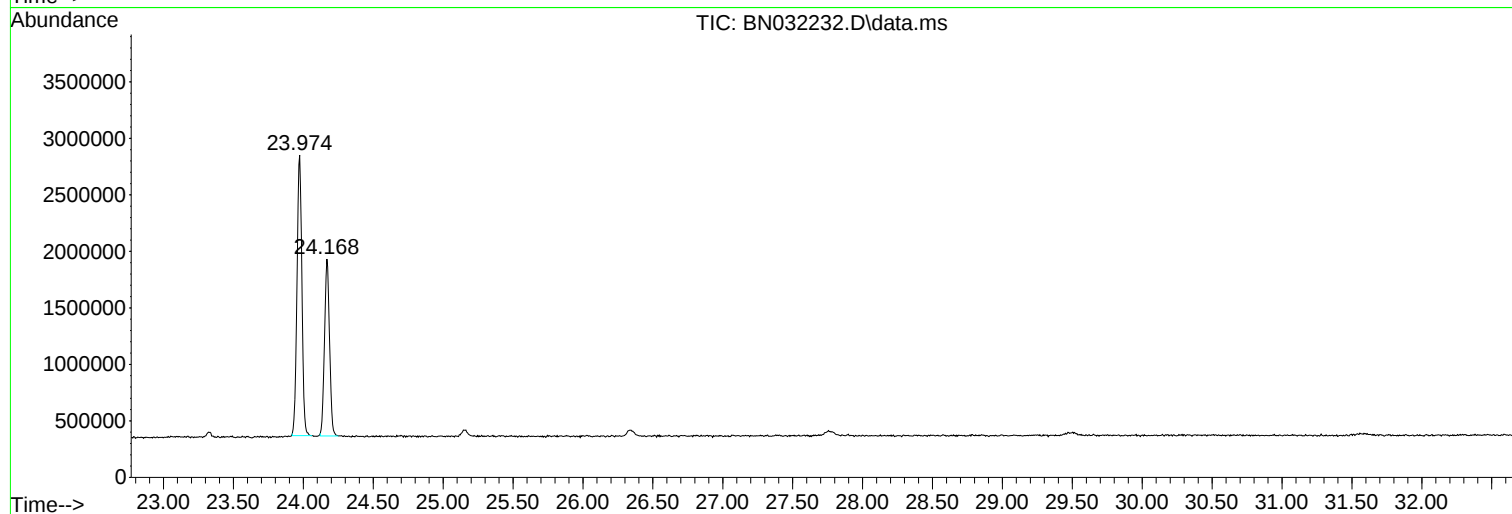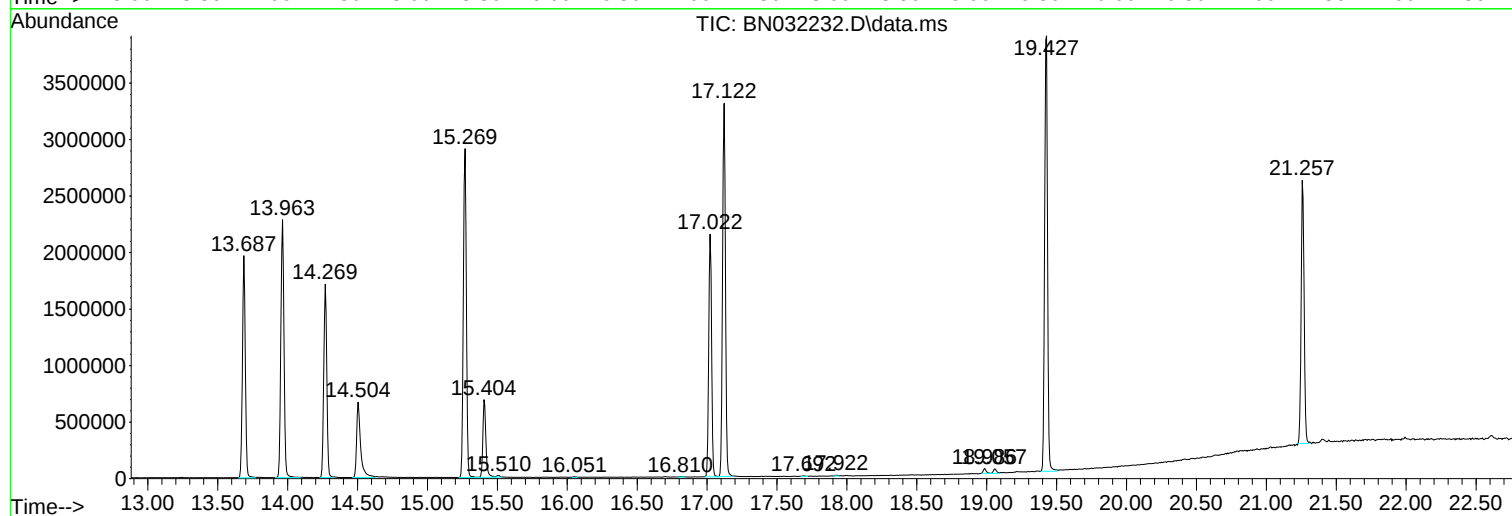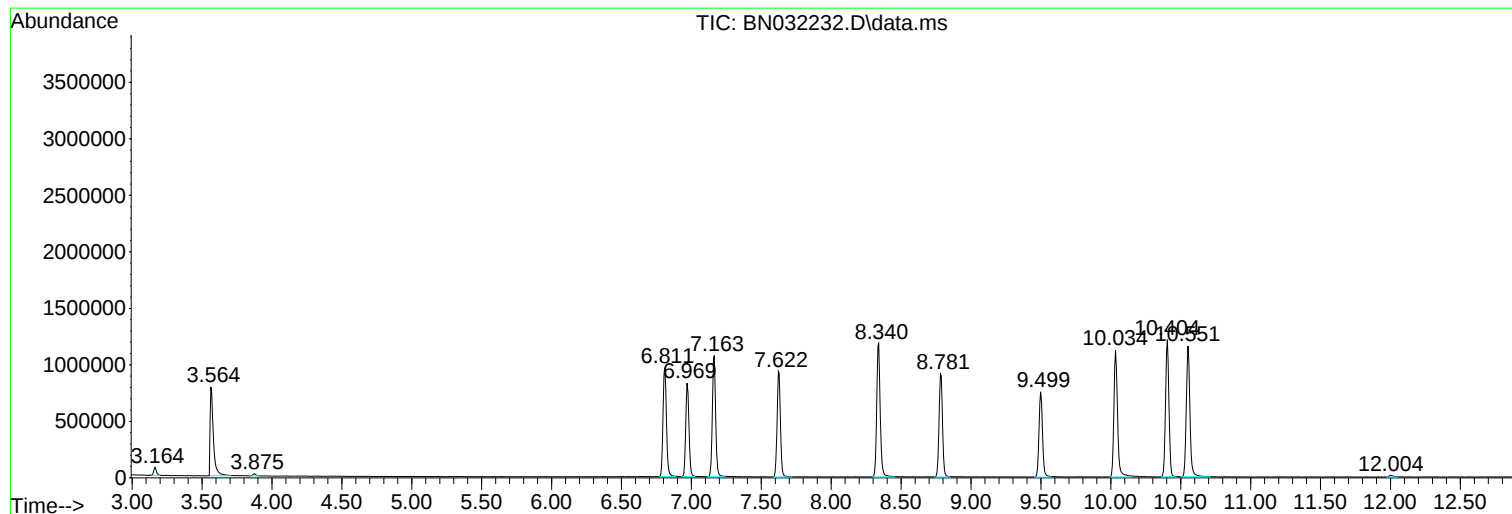

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
Data File : BN032232.D
Acq On : 25 Jun 2024 08:06
Operator : MA/JU
Sample : PB161513BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062424\
Data File : BN032232.D
Acq On : 25 Jun 2024 08:06
Operator : MA/JU
Sample : PB161513BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK513

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN052924.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------