


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062425\
Data File : BN037366.D
Acq On : 24 Jun 2025 09:17
Operator : RC/JU
Sample : DFTPP378
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP378

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
Title : SVOA CALIBRATION
Last Update : Thu Jun 19 14:59:41 2025

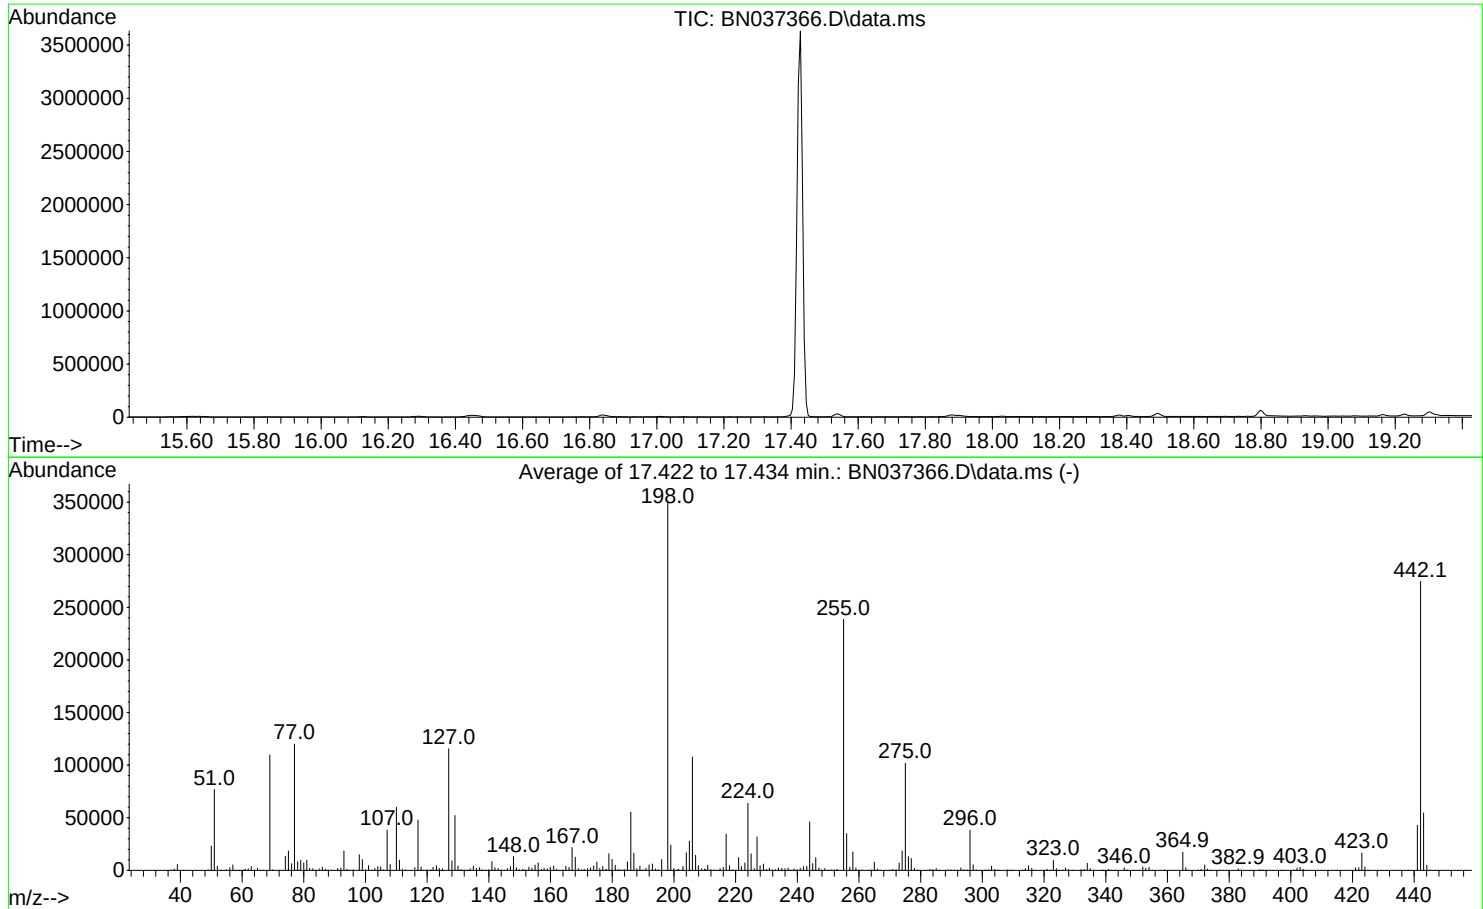

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.0	76925	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.4	109667	PASS
70	69	0.00	2	0.6	617	PASS
127	198	10	80	33.1	115568	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	349632	PASS
199	198	5	9	6.9	23981	PASS
275	198	10	60	29.1	101755	PASS
365	198	1	100	4.9	17236	PASS
441	198	0.01	100	12.2	42749	PASS
442	198	50	100	78.5	274624	PASS
443	442	15	24	19.9	54539	PASS