

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
 Data File : BN015041.D
 Acq On : 24 Jun 2021 15:30
 Operator : CG/JU
 Sample : M2682-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGDB0

Quant Time: Jun 24 16:06:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 24 14:43:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	175215	20.000	ng/u1	0.00
20) Naphthalene-d8	10.499	136	688418	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.351	164	401323	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.098	188	796176	20.000	ng/u1	0.00
79) Chrysene-d12	21.298	240	741599	20.000	ng/u1	0.00
88) Perylene-d12	23.539	264	772954	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	5578	1.239	ng/uL	0.00
4) Pyridine-d5	3.687	84	29189	2.404	ng/u1	0.01
7) Phenol-d5	6.893	99	96635	6.354	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.064	67	63123	7.068	ng/u1	0.00
11) 2-Chlorophenol-d4	7.258	132	82133	7.123	ng/u1	0.00
15) 4-Methylphenol-d8	8.416	113	75757	6.455	ng/u1	0.00
21) Nitrobenzene-d5	8.869	128	33261	7.063	ng/u1	0.00
24) 2-Nitrophenol-d4	9.587	143	28915	6.893	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.116	165	66322	6.699	ng/u1	0.00
31) 4-Chloroaniline-d4	10.628	131	85324	5.561	ng/u1	0.00
46) Dimethylphthalate-d6	13.763	166	222040	8.057	ng/u1	0.00
49) Acenaphthylene-d8	14.040	160	259304	7.248	ng/u1	0.00
54) 4-Nitrophenol-d4	14.540	143	3885	0.808	ng/u1	0.00
60) Fluorene-d10	15.345	176	195282	8.145	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.451	200	2568	0.781	ng/u1	-0.01
73) Anthracene-d10	17.192	188	320285	8.789	ng/u1	0.00
81) Pyrene-d10	19.498	212	359878	9.258	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.398	264	303213	7.946	ng/u1	0.00
Target Compounds						
					Qvalue	
80) Fluoranthene	19.163	202	53049	1.131	ng/u1	98
86) Bis(2-ethylhexyl)phtha...	21.227	149	38869	1.392	ng/u1	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
Data File : BN015041.D
Acq On : 24 Jun 2021 15:30
Operator : CG/JU
Sample : M2682-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGDB0

Quant Time: Jun 24 16:06:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 24 14:43:13 2021
Response via : Initial Calibration




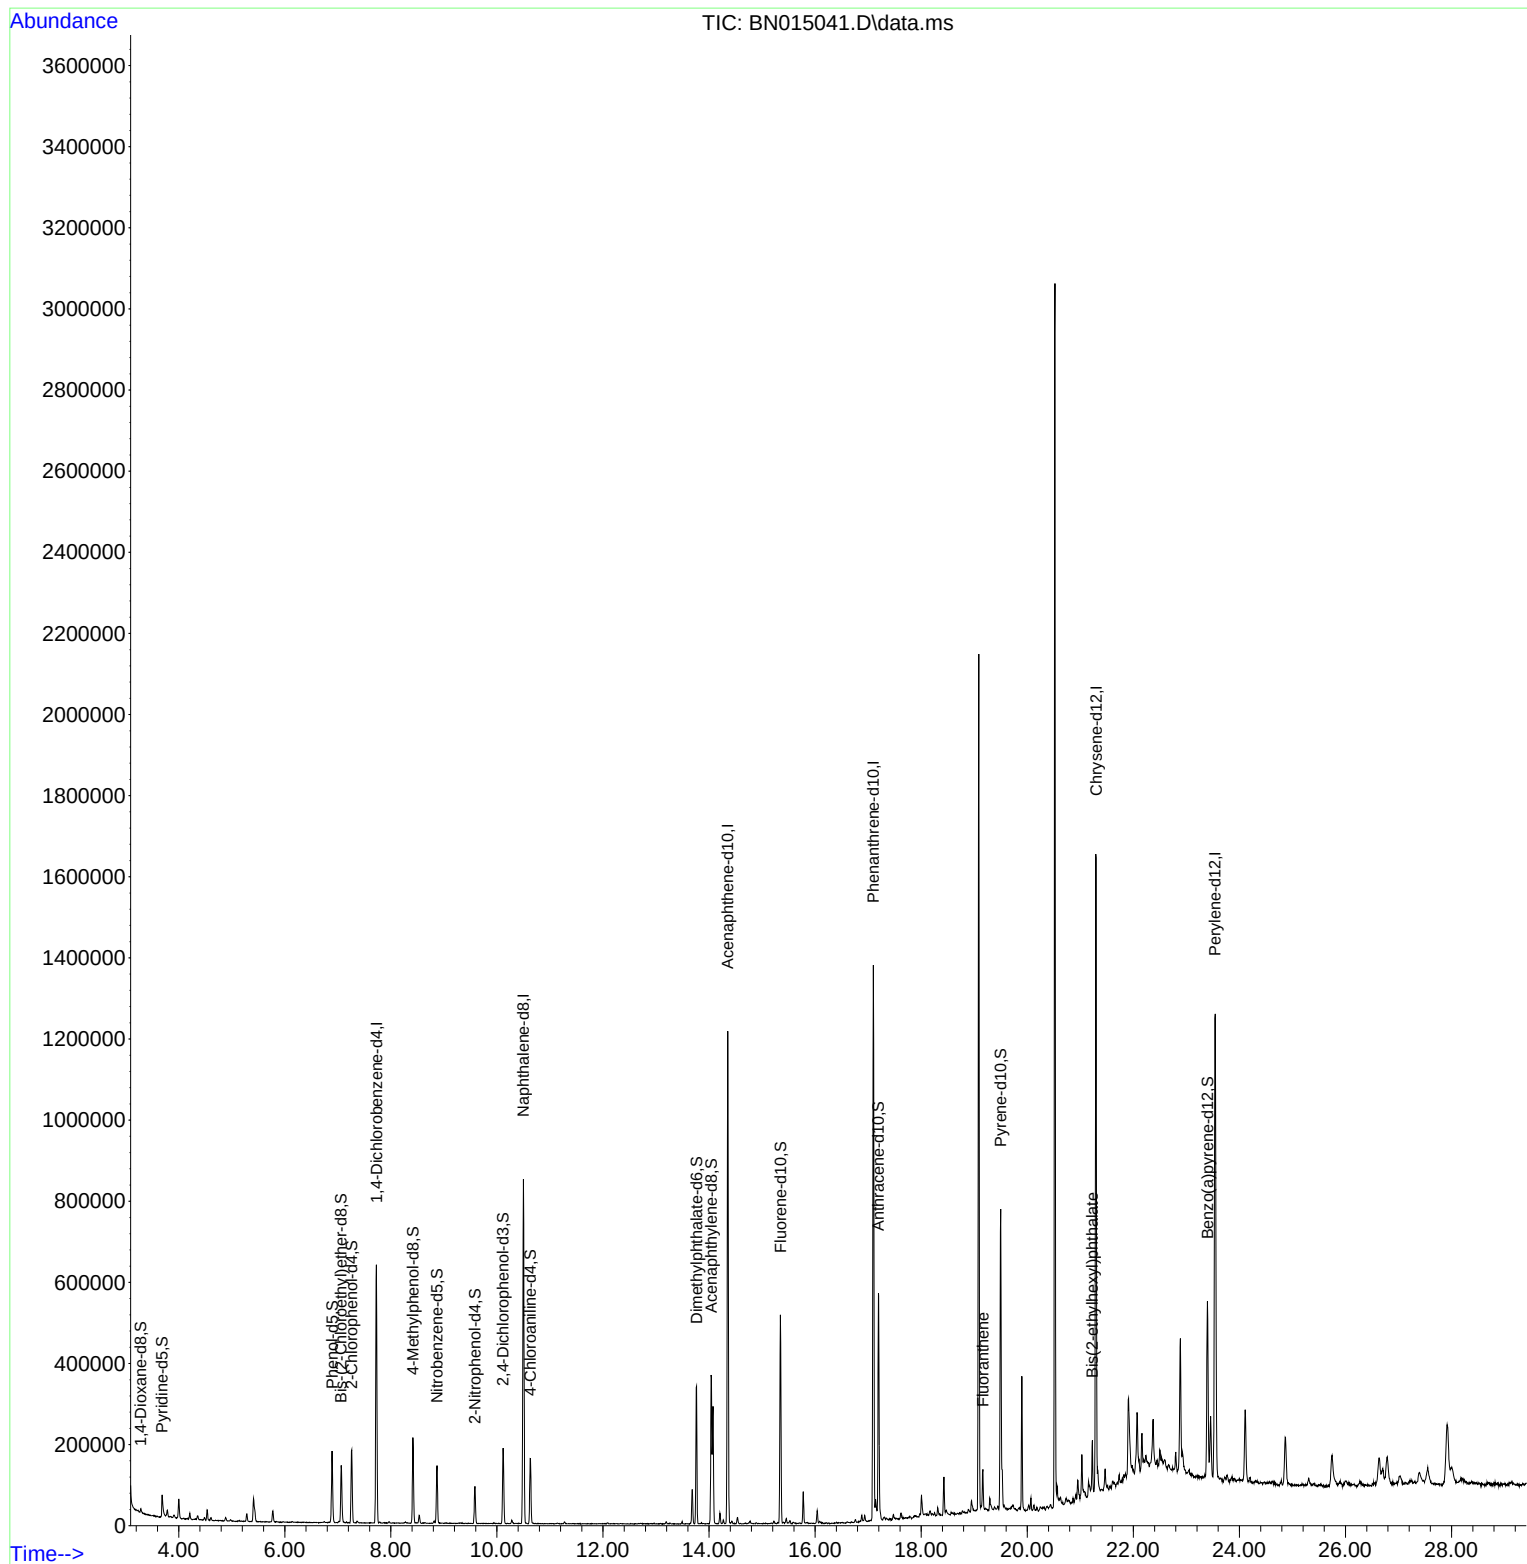


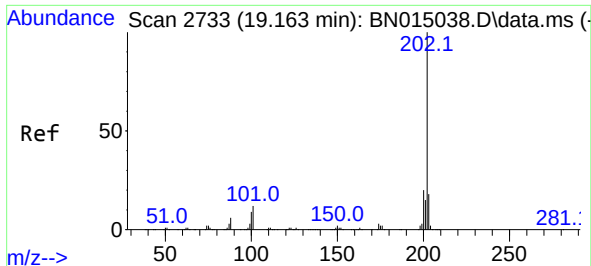

#80
Fluoranthene
Concen: 1.131 ng/u1
RT: 19.163 min Scan# 2733
Delta R.T. 0.000 min
Lab File: BN015041.D
Acq: 24 Jun 2021 15:30

Instrument :
BNA_N
ClientSampled :
BGDB0

Tgt Ion:202 Resp: 53049
Ion Ratio Lower Upper
202 100
101 12.9 9.5 14.3
100 9.6 7.4 11.2

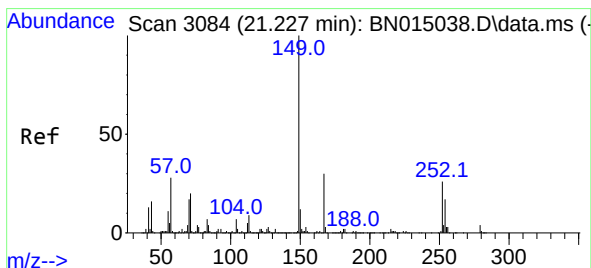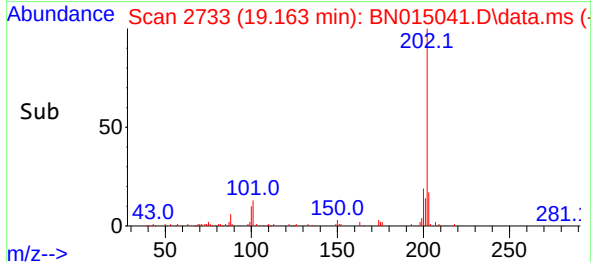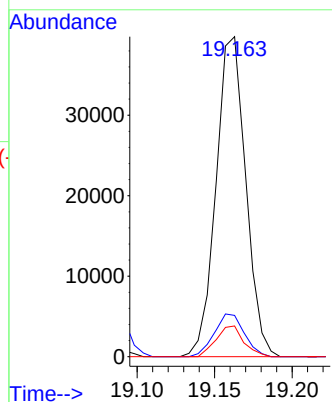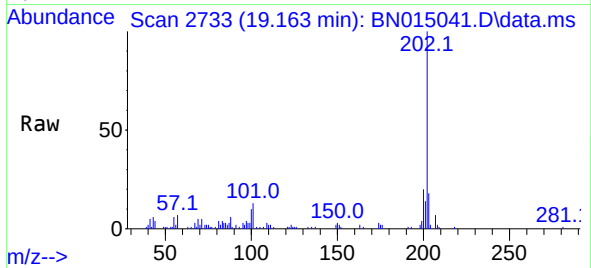

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.392 ng/u1
RT: 21.227 min Scan# 3084
Delta R.T. 0.000 min
Lab File: BN015041.D
Acq: 24 Jun 2021 15:30

Tgt Ion:149 Resp: 38869
Ion Ratio Lower Upper
149 100
167 27.1 23.4 35.0
279 3.7 3.4 5.2

