

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
 Data File : BN015044.D
 Acq On : 24 Jun 2021 17:18
 Operator : CG/JU
 Sample : M2682-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGD76

Quant Time: Jun 25 01:22:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 24 14:43:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	157290	20.000	ng/ul	0.00
20) Naphthalene-d8	10.498	136	639518	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.351	164	381914	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.098	188	756712	20.000	ng/ul	0.00
79) Chrysene-d12	21.298	240	735728	20.000	ng/ul	0.00
88) Perylene-d12	23.545	264	740858	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	10478	2.592	ng/uL	0.00
4) Pyridine-d5	3.681	84	95254	8.741	ng/ul	0.00
7) Phenol-d5	6.893	99	190279	13.938	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	113985	14.217	ng/ul	0.00
11) 2-Chlorophenol-d4	7.263	132	152160	14.699	ng/ul	0.00
15) 4-Methylphenol-d8	8.416	113	113040	10.729	ng/ul	0.00
21) Nitrobenzene-d5	8.869	128	68360	15.626	ng/ul	0.00
24) 2-Nitrophenol-d4	9.586	143	66420	17.045	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.116	165	132261	14.380	ng/ul	0.00
31) 4-Chloroaniline-d4	10.634	131	175111	12.285	ng/ul	0.00
46) Dimethylphthalate-d6	13.763	166	414276	15.797	ng/ul	0.00
49) Acenaphthylene-d8	14.045	160	529280	15.547	ng/ul	0.00
54) 4-Nitrophenol-d4	14.539	143	52937	11.573	ng/ul	0.00
60) Fluorene-d10	15.345	176	375061	16.439	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	29831	9.545	ng/ul	0.00
73) Anthracene-d10	17.198	188	557021	16.083	ng/ul	0.00
81) Pyrene-d10	19.498	212	541440	14.040	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.398	264	393835	10.768	ng/ul	0.00
Target Compounds						
					Qvalue	
80) Fluoranthene	19.162	202	77365	1.662	ng/ul	99
82) Pyrene	19.527	202	57199	1.179	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.227	149	36741	1.327	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
Data File : BN015044.D
Acq On : 24 Jun 2021 17:18
Operator : CG/JU
Sample : M2682-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGD76

Quant Time: Jun 25 01:22:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 24 14:43:13 2021
Response via : Initial Calibration




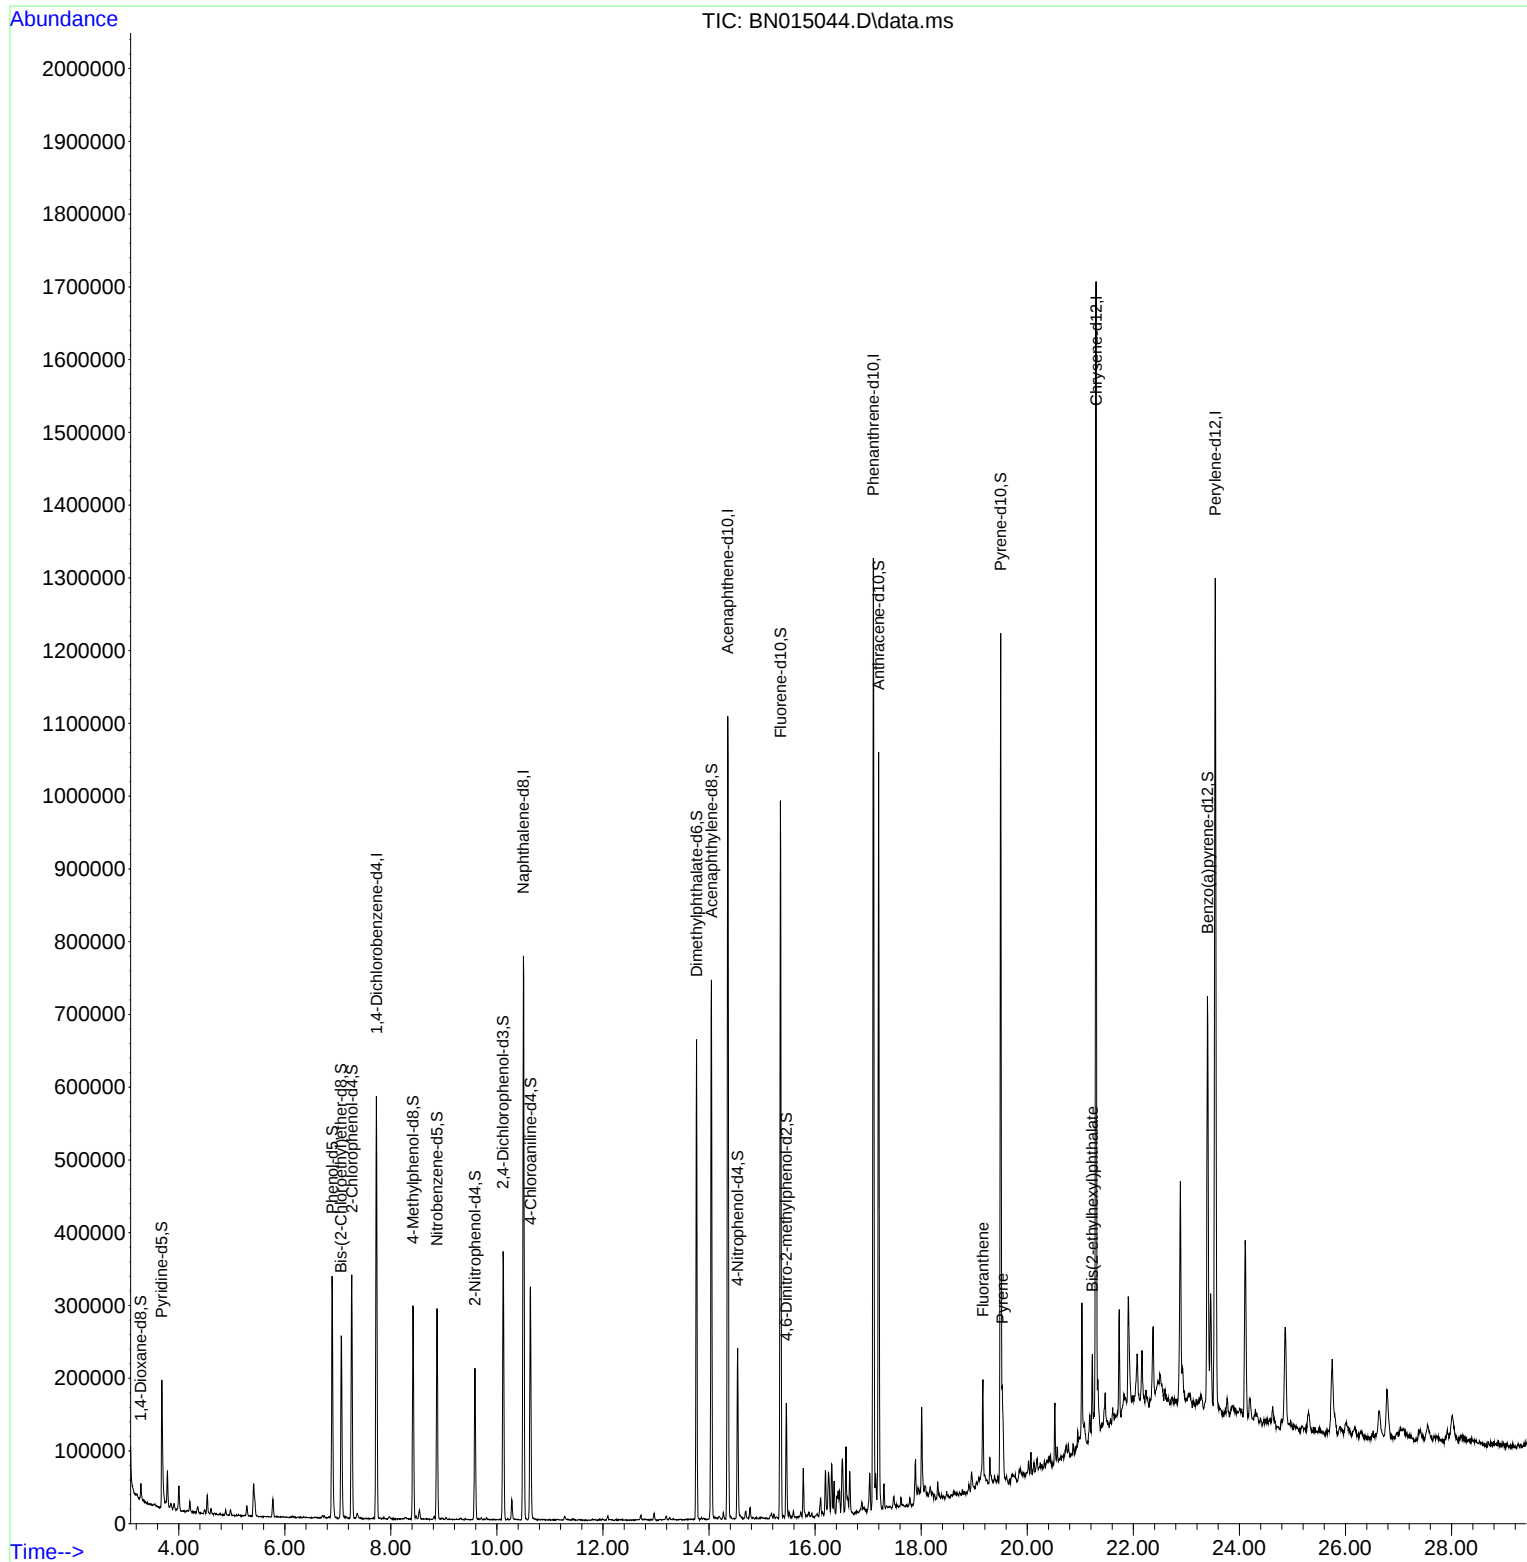


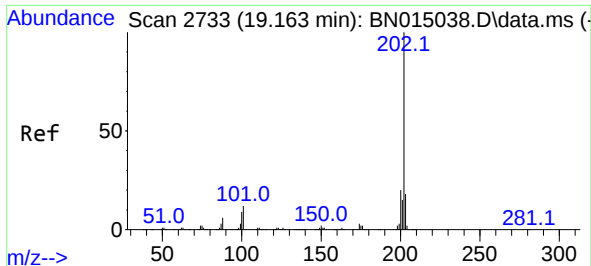

#80
Fluoranthene
Concen: 1.662 ng/u1
RT: 19.162 min Scan# 2733
Delta R.T. -0.000 min
Lab File: BN015044.D
Acq: 24 Jun 2021 17:18




Instrument :
BNA_N
ClientSampleId :
BGD76


Tgt Ion:202 Resp: 77365
Ion Ratio Lower Upper
202 100
101 12.4 9.5 14.3
100 8.7 7.4 11.2

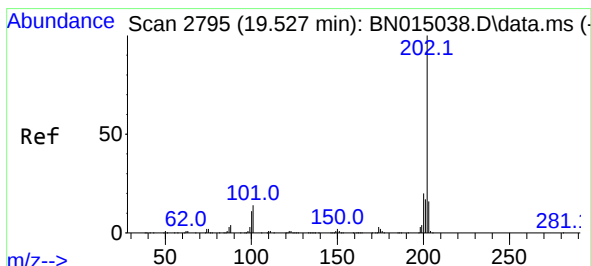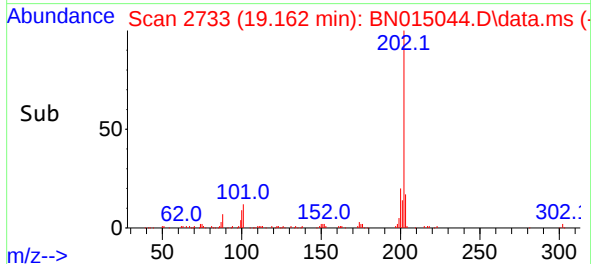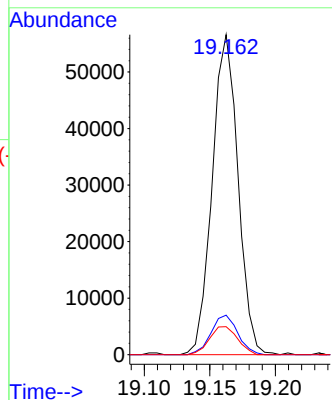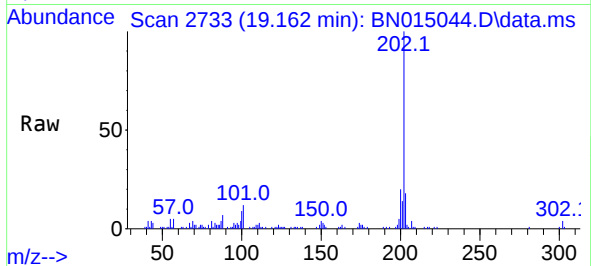

#82
Pyrene
Concen: 1.179 ng/u1
RT: 19.527 min Scan# 2795
Delta R.T. -0.000 min
Lab File: BN015044.D
Acq: 24 Jun 2021 17:18

Tgt Ion:202 Resp: 57199
Ion Ratio Lower Upper
202 100
101 15.1 11.6 17.4
100 10.4 9.2 13.8

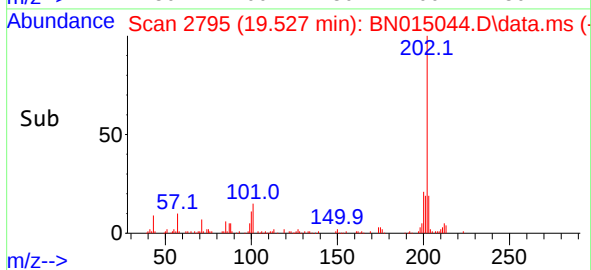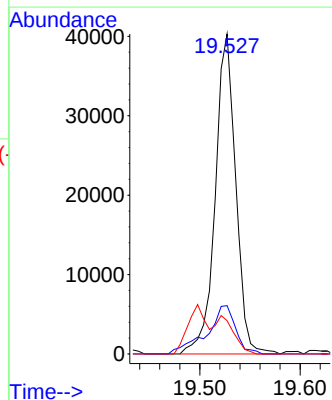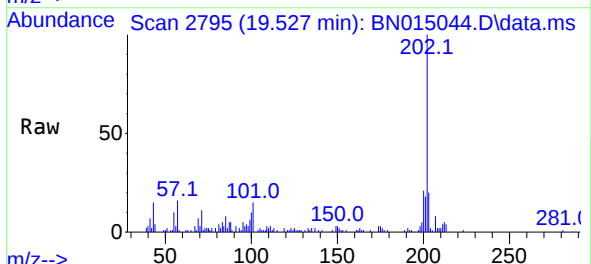

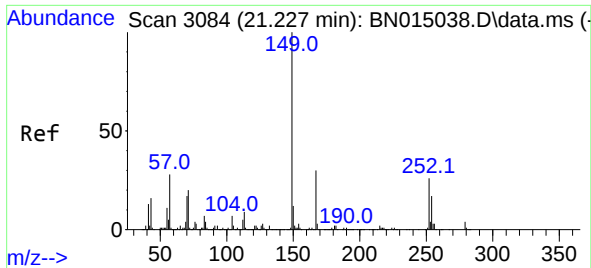

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.327 ng/ul
 RT: 21.227 min Scan# 3084
 Delta R.T. -0.000 min
 Lab File: BN015044.D
 Acq: 24 Jun 2021 17:18

Instrument :
 BNA_N
 ClientSampleId :
 BGD76

Tgt Ion:149 Resp: 36741

Ion	Ratio	Lower	Upper
149	100		
167	28.4	23.4	35.0
279	4.0	3.4	5.2

