

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
 Data File : BN015048.D
 Acq On : 24 Jun 2021 19:41
 Operator : CG/JU
 Sample : M2682-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGD62

Quant Time: Jun 25 01:22:53 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 24 14:43:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	165401	20.000	ng/ul	0.00
20) Naphthalene-d8	10.498	136	662117	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.351	164	395871	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.098	188	779860	20.000	ng/ul	0.00
79) Chrysene-d12	21.292	240	774656	20.000	ng/ul	0.00
88) Perylene-d12	23.539	264	782881	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	8747	2.058	ng/uL	0.00
4) Pyridine-d5	3.687	84	46328	4.043	ng/ul	0.01
7) Phenol-d5	6.893	99	156532	10.904	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	95104	11.281	ng/ul	0.00
11) 2-Chlorophenol-d4	7.263	132	127546	11.717	ng/ul	0.00
15) 4-Methylphenol-d8	8.416	113	117075	10.567	ng/ul	0.00
21) Nitrobenzene-d5	8.869	128	56010	12.366	ng/ul	0.00
24) 2-Nitrophenol-d4	9.587	143	51298	12.715	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.116	165	108012	11.343	ng/ul	0.00
31) 4-Chloroaniline-d4	10.628	131	156128	10.579	ng/ul	0.00
46) Dimethylphthalate-d6	13.763	166	333741	12.277	ng/ul	0.00
49) Acenaphthylene-d8	14.045	160	422058	11.960	ng/ul	0.00
54) 4-Nitrophenol-d4	14.539	143	38352	8.089	ng/ul	0.00
60) Fluorene-d10	15.345	176	292037	12.349	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	21307	6.615	ng/ul	0.00
73) Anthracene-d10	17.198	188	449617	12.596	ng/ul	0.00
81) Pyrene-d10	19.498	212	517321	12.741	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.398	264	477898	12.365	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.221	149	51283	1.759	ng/ul#	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
Data File : BN015048.D
Acq On : 24 Jun 2021 19:41
Operator : CG/JU
Sample : M2682-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGD62

Quant Time: Jun 25 01:22:53 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 24 14:43:13 2021
Response via : Initial Calibration

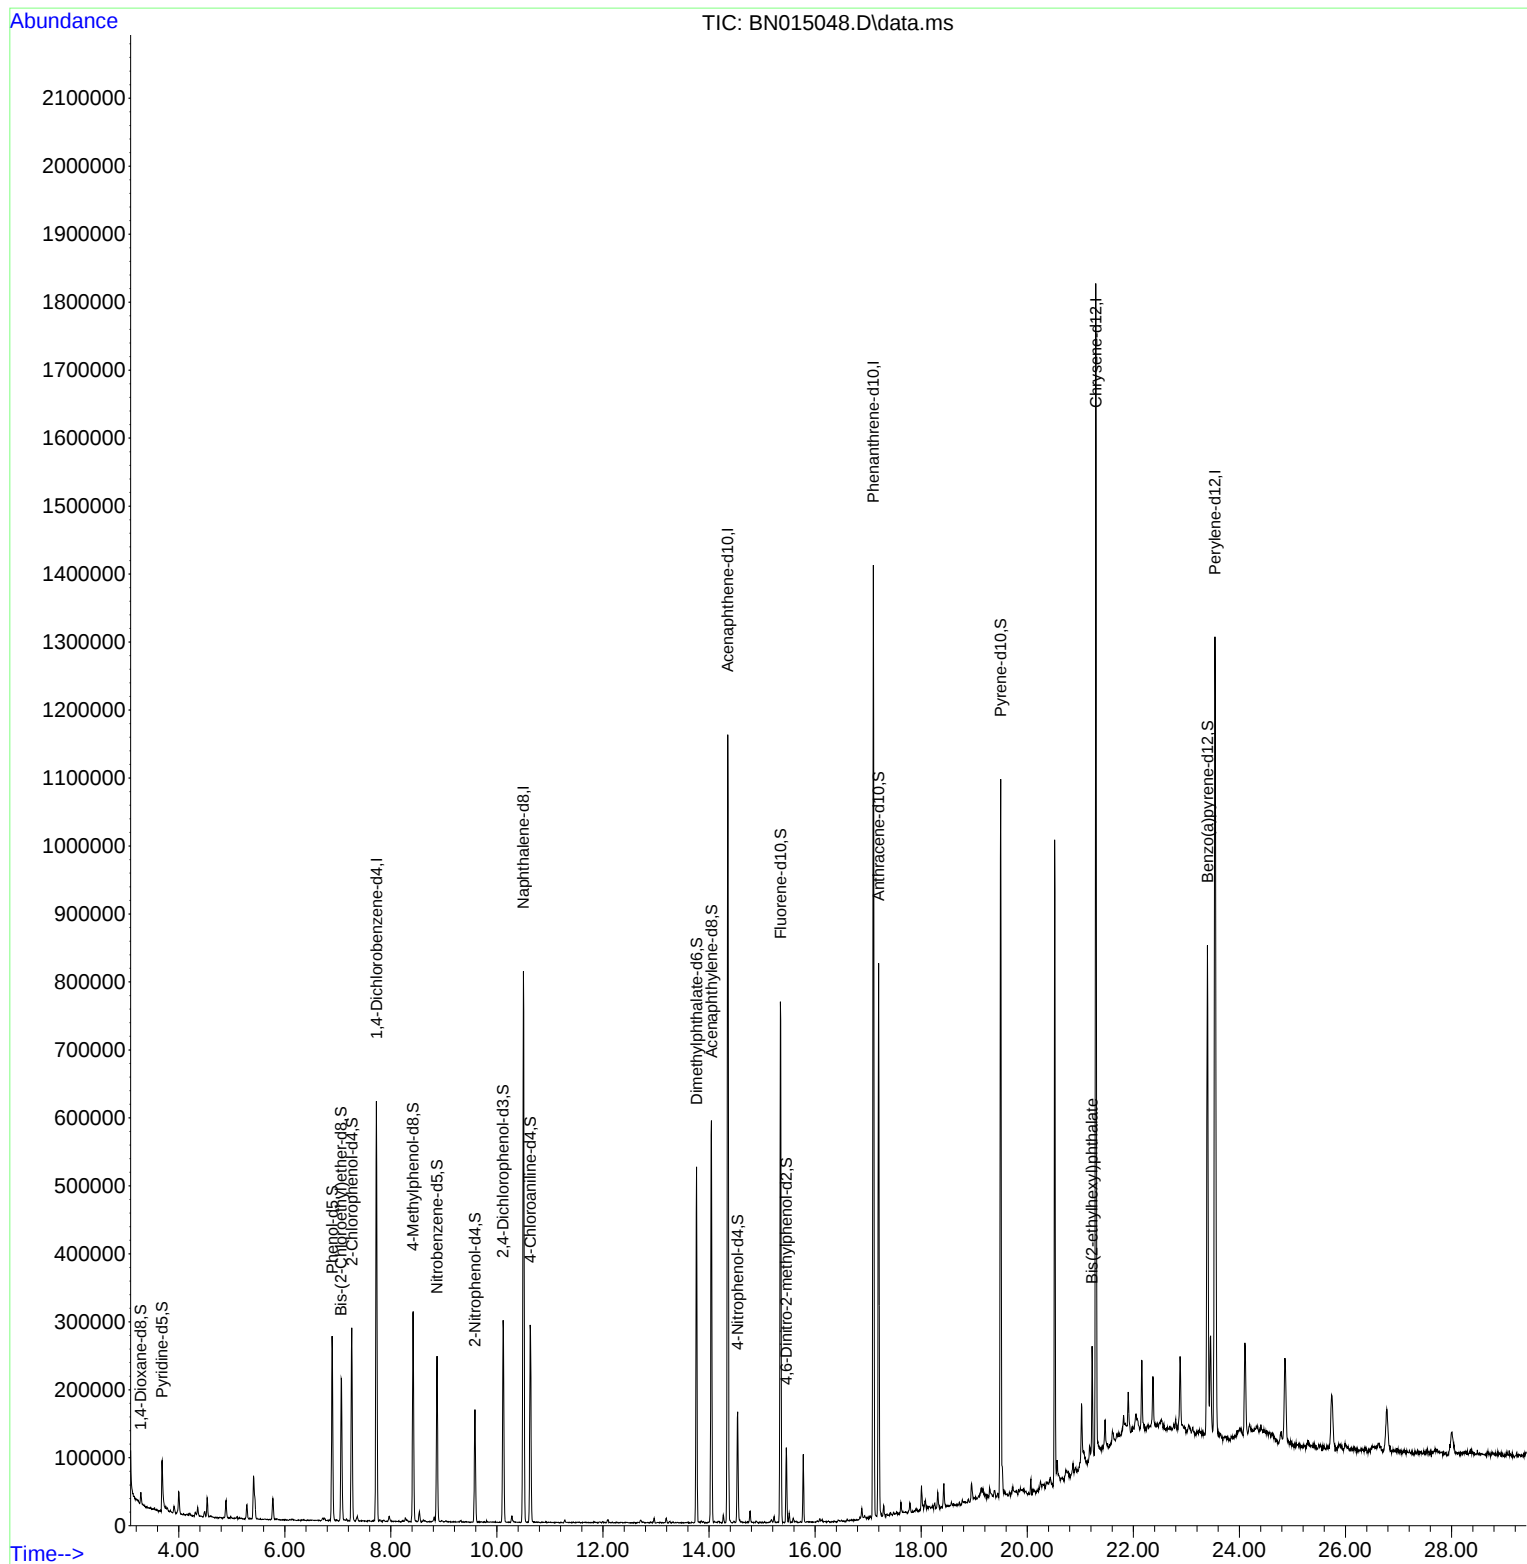

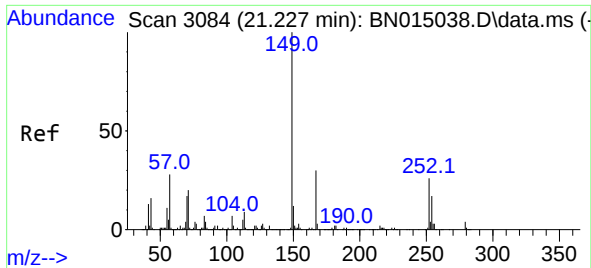

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.759 ng/ul
RT: 21.221 min Scan# 3083
Delta R.T. -0.006 min
Lab File: BN015048.D
Acq: 24 Jun 2021 19:41

Instrument :
BNA_N
ClientSampleId :
BGD62

Tgt Ion:149 Resp: 51283
Ion Ratio Lower Upper
149 100
167 29.3 23.4 35.0
279 3.4 3.4 5.2#

