

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
 Data File : BN015059.D
 Acq On : 25 Jun 2021 02:48
 Operator : CG/JU
 Sample : M2682-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGD43

Quant Time: Jun 25 03:20:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 24 14:43:13 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.728	152	140380	20.000	ng/ul	0.00
20) Naphthalene-d8	10.499	136	561542	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.351	164	334291	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.098	188	679622	20.000	ng/ul	0.00
79) Chrysene-d12	21.292	240	664096	20.000	ng/ul	0.00
88) Perylene-d12	23.539	264	699268	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	9534	2.643	ng/uL	0.00
4) Pyridine-d5	3.681	84	46433	4.774	ng/ul	0.00
7) Phenol-d5	6.893	99	166802	13.690	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.064	67	97090	13.569	ng/ul	0.00
11) 2-Chlorophenol-d4	7.264	132	134202	14.526	ng/ul	0.00
15) 4-Methylphenol-d8	8.416	113	108137	11.500	ng/ul	0.00
21) Nitrobenzene-d5	8.869	128	58234	15.160	ng/ul	0.00
24) 2-Nitrophenol-d4	9.587	143	55208	16.135	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.116	165	111544	13.812	ng/ul	0.00
31) 4-Chloroaniline-d4	10.628	131	159891	12.775	ng/ul	0.00
46) Dimethylphthalate-d6	13.763	166	330288	14.388	ng/ul	0.00
49) Acenaphthylene-d8	14.040	160	431208	14.471	ng/ul	0.00
54) 4-Nitrophenol-d4	14.540	143	32332	8.075	ng/ul	0.00
60) Fluorene-d10	15.345	176	299596	15.002	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	16152	5.754	ng/ul	0.00
73) Anthracene-d10	17.198	188	473846	15.233	ng/ul	0.00
81) Pyrene-d10	19.498	212	543117	15.603	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.398	264	512952	14.859	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.222	149	48276	1.931	ng/ul	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
Data File : BN015059.D
Acq On : 25 Jun 2021 02:48
Operator : CG/JU
Sample : M2682-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGD43


Quant Time: Jun 25 03:20:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 24 14:43:13 2021
Response via : Initial Calibration

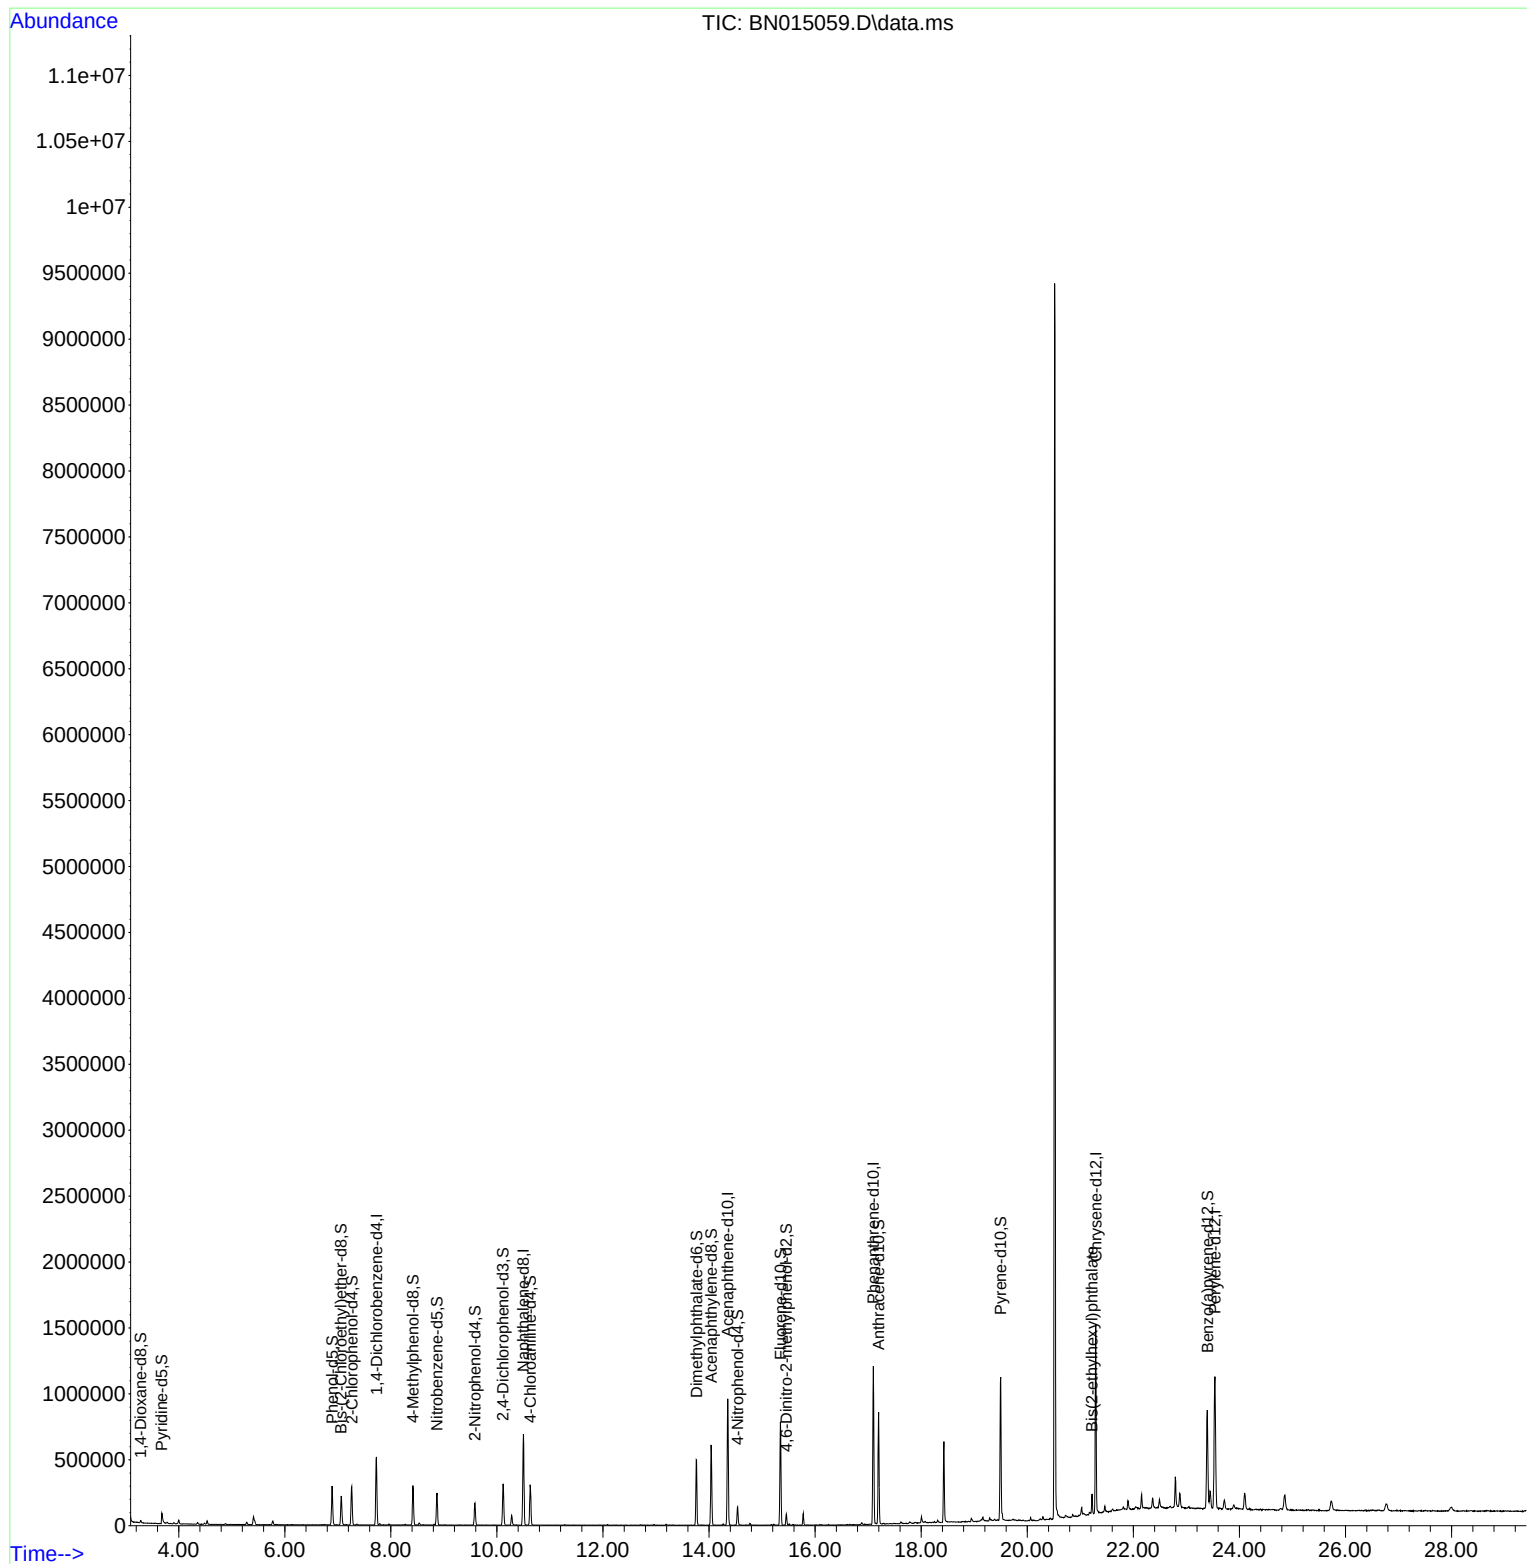

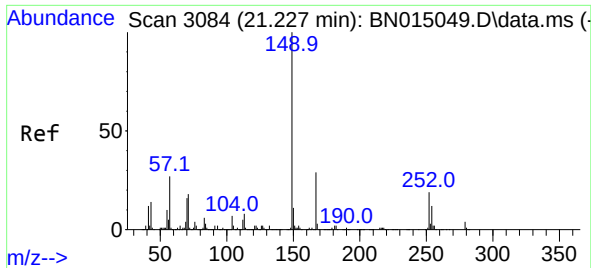

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.931 ng/ul
RT: 21.222 min Scan# 3083
Delta R.T. -0.006 min
Lab File: BN015059.D
Acq: 25 Jun 2021 02:48

Instrument :
BNA_N
ClientSampleId :
BGD43

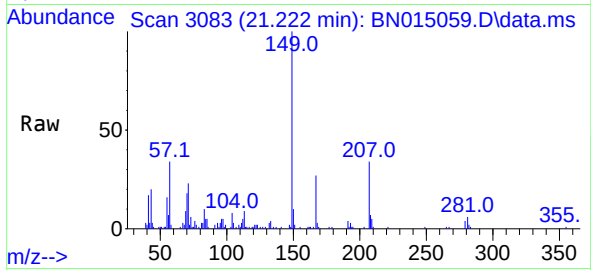

Tgt Ion:149 Resp: 48276
Ion Ratio Lower Upper
149 100
167 27.2 23.4 35.0
279 4.4 3.4 5.2

