

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
 Data File : BN015066.D
 Acq On : 25 Jun 2021 08:09
 Operator : CG/JU
 Sample : M2720-03
 Misc : GCMS CONFIRMATION
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0CP4

Quant Time: Jun 25 09:00:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 24 14:43:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	246472	20.000	ng/ul	0.00
20) Naphthalene-d8	10.499	136	974292	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.351	164	549143	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.098	188	1017266	20.000	ng/ul	0.00
79) Chrysene-d12	21.292	240	818306	20.000	ng/ul	0.00
88) Perylene-d12	23.539	264	722818	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0	0.000	ng/ul	
7) Phenol-d5	0.000	99	0	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	0.000	67	0	0.000	ng/ul	
11) 2-Chlorophenol-d4	0.000	132	0	0.000	ng/ul	
15) 4-Methylphenol-d8	0.000	113	0	0.000	ng/ul	
21) Nitrobenzene-d5	0.000	128	0	0.000	ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0	0.000	ng/ul	
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	0.000	166	0	0.000	ng/ul	
49) Acenaphthylene-d8	0.000	160	0	0.000	ng/ul	
54) 4-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
60) Fluorene-d10	0.000	176	0	0.000	ng/ul	
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/ul	
73) Anthracene-d10	0.000	188	0d	0.000	ng/ul	
81) Pyrene-d10	0.000	212	0d	0.000	ng/ul	
92) Benzo(a)pyrene-d12	0.000	264	0d	0.000	ng/ul	
Target Compounds						
					Qvalue	
80) Fluoranthene	19.163	202	108066	2.087	ng/ul	99
82) Pyrene	19.528	202	60948	1.129	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
Data File : BN015066.D
Acq On : 25 Jun 2021 08:09
Operator : CG/JU
Sample : M2720-03
Misc : GCMS CONFIRMATION
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0CP4

Quant Time: Jun 25 09:00:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 24 14:43:13 2021
Response via : Initial Calibration




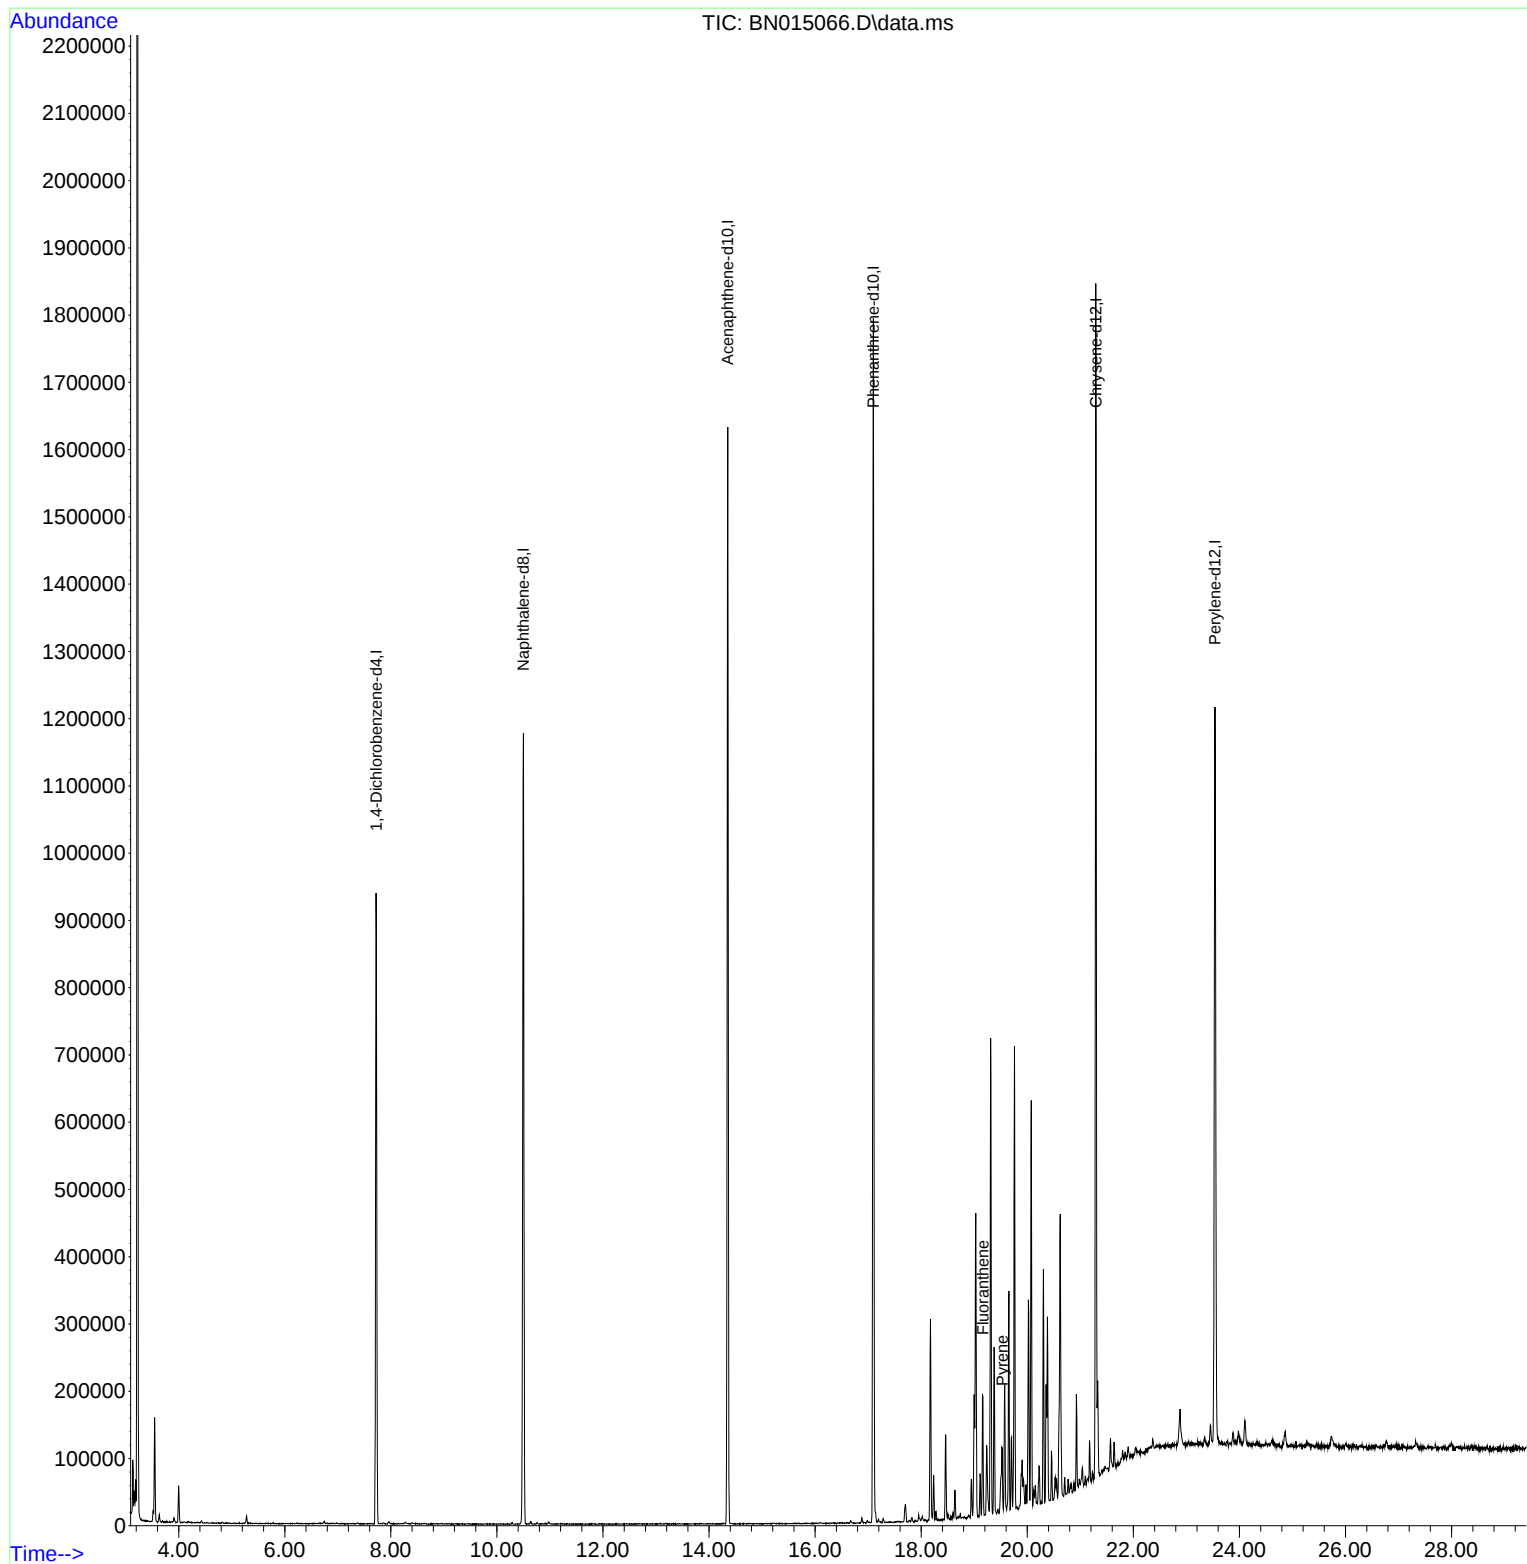


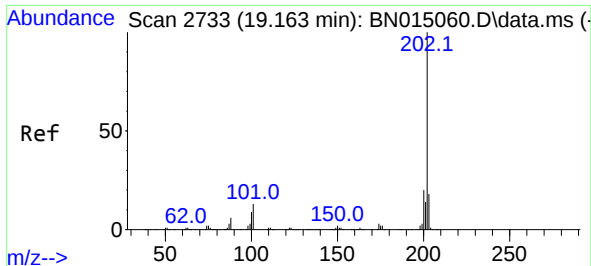

#80
Fluoranthene
Concen: 2.087 ng/u1
RT: 19.163 min Scan# 2733
Delta R.T. 0.000 min
Lab File: BN015066.D
Acq: 25 Jun 2021 08:09

Instrument :
BNA_N
ClientSampled :
C0CP4

Tgt Ion:202 Resp: 108066
Ion Ratio Lower Upper
202 100
101 11.6 9.5 14.3
100 9.1 7.4 11.2

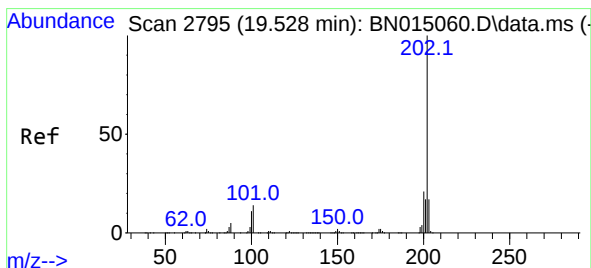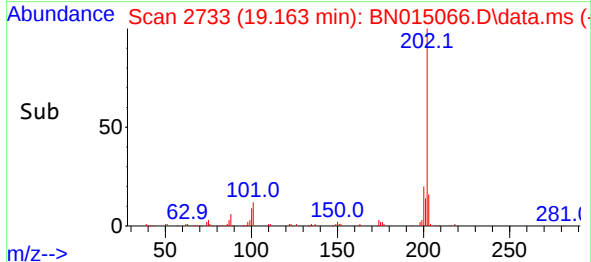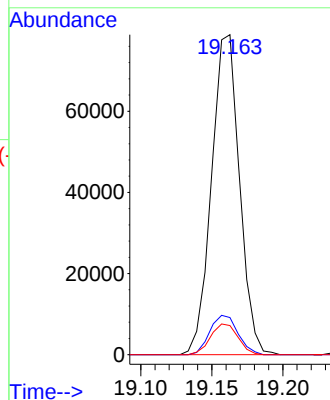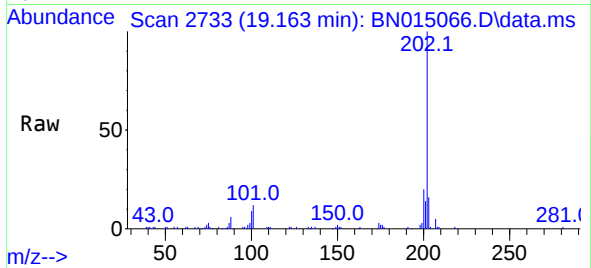

#82
Pyrene
Concen: 1.129 ng/u1
RT: 19.528 min Scan# 2795
Delta R.T. 0.000 min
Lab File: BN015066.D
Acq: 25 Jun 2021 08:09

Tgt Ion:202 Resp: 60948
Ion Ratio Lower Upper
202 100
101 13.9 11.6 17.4
100 11.0 9.2 13.8

