

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
 Data File : BN015039.D
 Acq On : 24 Jun 2021 14:06
 Operator : CG/JU
 Sample : PB137214BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK214

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	45	rVB	90616	127350	2.40%	0.214%
2	3.675	96	100	117	rBV	995411	1441357	27.15%	2.419%
3	4.005	152	156	160	rVB	13358	16826	0.32%	0.028%
4	6.899	640	648	658	rBV	1123722	1794587	33.81%	3.012%
5	7.069	670	677	695	rBV	906313	1445351	27.23%	2.426%
6	7.264	703	710	720	rVB	1214671	1870250	35.23%	3.139%
7	7.728	782	789	797	rBV	860073	1355246	25.53%	2.275%
8	8.422	900	907	918	rBV	1356341	2147052	40.45%	3.604%
9	8.869	976	983	993	rBV	998247	1638533	30.87%	2.750%
10	9.587	1097	1105	1114	rBV	761249	1216102	22.91%	2.041%
11	10.116	1188	1195	1211	rVB	1263521	2115976	39.86%	3.552%
12	10.499	1253	1260	1268	rBV	1131076	1894040	35.68%	3.179%
13	10.634	1274	1283	1290	rBV	1313846	2203411	41.51%	3.698%
14	12.087	1525	1530	1537	rVB	22769	34620	0.65%	0.058%
15	13.763	1807	1815	1826	rBV	2233700	2962198	55.81%	4.972%
16	14.046	1856	1863	1872	rBV	2508182	3693029	69.58%	6.199%
17	14.351	1909	1915	1923	rVB	1629949	2377754	44.80%	3.991%
18	14.540	1941	1947	1961	rBV	998234	1388601	26.16%	2.331%
19	15.351	2078	2085	2093	rVB	3002335	4415157	83.18%	7.411%
20	15.457	2097	2103	2114	rVV	741786	1004096	18.92%	1.685%
21	15.587	2120	2125	2131	rVB	35807	48442	0.91%	0.081%
22	16.134	2214	2218	2223	rBV4	10232	14066	0.26%	0.024%
23	16.775	2322	2327	2332	rBV5	3188	6143	0.12%	0.010%
24	16.887	2341	2346	2351	rBV2	6200	9628	0.18%	0.016%
25	17.098	2376	2382	2389	rBV	1910599	2696988	50.81%	4.527%
26	17.198	2392	2399	2414	rBV2	3341732	4734149	89.19%	7.946%
27	18.004	2532	2536	2540	rBV3	8213	12622	0.24%	0.021%
28	19.128	2720	2727	2733	rVB	39619	52846	1.00%	0.089%
29	19.386	2766	2771	2775	rVB	25814	36901	0.70%	0.062%
30	19.498	2784	2790	2804	rBV2	3814921	5307972	100.00%	8.910%
31	20.522	2961	2964	2966	rBV2	6712	5995	0.11%	0.010%
32	21.033	3047	3051	3056	rBV7	7685	12547	0.24%	0.021%
33	21.292	3090	3095	3102	rBV	2089865	2719956	51.24%	4.565%
34	21.904	3197	3199	3204	rVB5	17333	19442	0.37%	0.033%
35	22.374	3275	3279	3285	rVB2	50636	65410	1.23%	0.110%
36	22.886	3362	3366	3372	rVB2	95132	135196	2.55%	0.227%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
 Data File : BN015039.D
 Acq On : 24 Jun 2021 14:06
 Operator : CG/JU
 Sample : PB137214BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK214

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Title : SVOA CALIBRATION

37	23.404	3446	3454	3460	rBV2	2612932	4853810	91.44%	8.147%
38	23.457	3460	3463	3470	rVV	162554	268643	5.06%	0.451%
39	23.545	3471	3478	3492	rVB	1535173	2767689	52.14%	4.646%
40	24.110	3569	3574	3586	rVB	140579	270235	5.09%	0.454%
41	24.868	3697	3703	3710	rVB	120372	258224	4.86%	0.433%
42	25.745	3847	3852	3859	rVB3	61683	137937	2.60%	0.232%


Sum of corrected areas: 59576377

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
Data File : BN015039.D
Acq On : 24 Jun 2021 14:06
Operator : CG/JU
Sample : PB137214BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK214

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

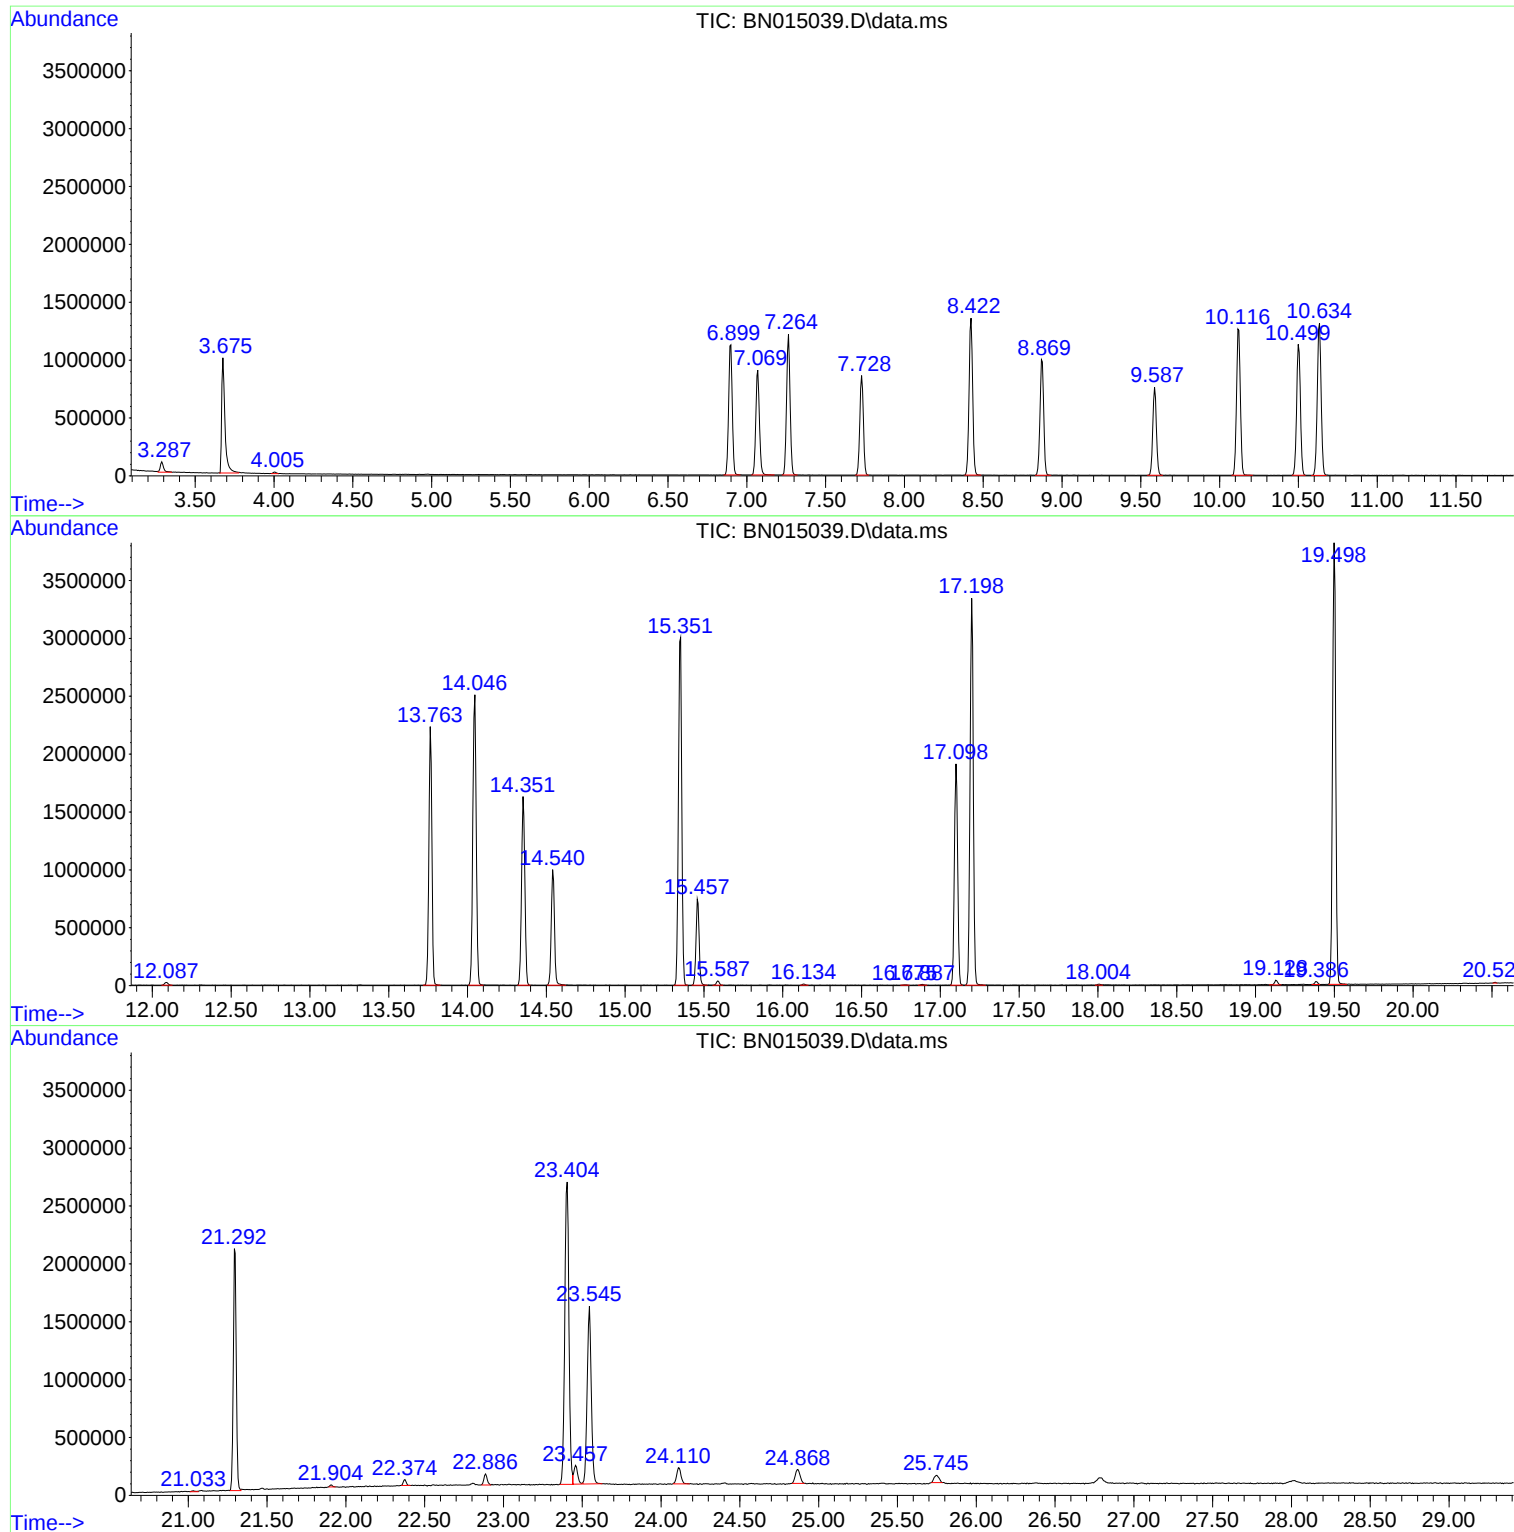

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
Data File : BN015039.D
Acq On : 24 Jun 2021 14:06
Operator : CG/JU
Sample : PB137214BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK214

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
Data File : BN015039.D
Acq On : 24 Jun 2021 14:06
Operator : CG/JU
Sample : PB137214BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK214

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
