

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
 Data File : BN015061.D
 Acq On : 25 Jun 2021 05:10
 Operator : CG/JU
 Sample : PB137214BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK214

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015061.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.287	30	34	41	rVB	81033	106258	1.81%	0.175%
2	3.675	96	100	116	rBV	933116	1395905	23.80%	2.302%
3	4.005	152	156	161	rVB	12755	17419	0.30%	0.029%
4	6.893	640	647	656	rBV	1163135	1789907	30.51%	2.951%
5	7.063	670	676	685	rBV	901131	1398992	23.85%	2.307%
6	7.263	701	710	723	rVB	1166689	1862454	31.75%	3.071%
7	7.728	782	789	796	rBV	802126	1261606	21.51%	2.080%
8	8.416	899	906	916	rBV	1339283	2163572	36.88%	3.568%
9	8.869	975	983	991	rBV	1033565	1651254	28.15%	2.723%
10	9.587	1097	1105	1114	rBV	782723	1248286	21.28%	2.058%
11	10.116	1188	1195	1203	rBV	1299707	2130653	36.32%	3.513%
12	10.498	1252	1260	1271	rBV	1090709	1792117	30.55%	2.955%
13	10.628	1275	1282	1295	rBV	1315668	2209529	37.67%	3.643%
14	12.087	1524	1530	1537	rVB2	22385	33001	0.56%	0.054%
15	13.763	1808	1815	1823	rBV	2116251	2900162	49.44%	4.782%
16	14.039	1855	1862	1870	rBV	2422471	3679859	62.73%	6.068%
17	14.351	1908	1915	1922	rBV	1524883	2253512	38.42%	3.716%
18	14.539	1940	1947	1964	rBV	1044276	1483676	25.29%	2.446%
19	15.345	2077	2084	2091	rBV	3048449	4379351	74.66%	7.221%
20	15.457	2097	2103	2111	rBV	685091	927061	15.80%	1.529%
21	15.586	2120	2125	2129	rBB	35101	42970	0.73%	0.071%
22	16.133	2214	2218	2223	rBV3	39850	51178	0.87%	0.084%
23	16.880	2340	2345	2350	rBV	5749	9133	0.16%	0.015%
24	17.098	2375	2382	2391	rBV	1884940	2595740	44.25%	4.280%
25	17.198	2392	2399	2407	rVV	3205929	4635248	79.02%	7.643%
26	19.127	2722	2727	2734	rBV	40518	54889	0.94%	0.091%
27	19.380	2766	2770	2777	rVB	28910	36857	0.63%	0.061%
28	19.498	2783	2790	2800	rBV	4018841	5560765	94.80%	9.169%
29	20.510	2958	2962	2968	rBV6	10042	17268	0.29%	0.028%
30	21.221	3079	3083	3087	rBV	33049	41984	0.72%	0.069%
31	21.292	3089	3095	3104	rVV	2458884	3008964	51.29%	4.962%
32	22.363	3274	3277	3283	rVB	35583	45518	0.78%	0.075%
33	22.874	3360	3364	3370	rVB2	64809	98156	1.67%	0.162%
34	23.398	3445	3453	3459	rBV2	3079807	5866014	100.00%	9.673%
35	23.445	3459	3461	3468	rVV	126423	182496	3.11%	0.301%
36	23.539	3469	3477	3489	rVB2	1627623	3173197	54.09%	5.232%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
Data File : BN015061.D
Acq On : 25 Jun 2021 05:10
Operator : CG/JU
Sample : PB137214BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK214

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Title : SVOA CALIBRATION

37	24.098	3567	3572	3579	rVB2	111423	197494	3.37%	0.326%
38	24.851	3695	3700	3711	rVB	102540	219925	3.75%	0.363%
39	25.733	3846	3850	3858	rVB3	59720	122768	2.09%	0.202%




Sum of corrected areas: 60645138

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
Data File : BN015061.D
Acq On : 25 Jun 2021 05:10
Operator : CG/JU
Sample : PB137214BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK214

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

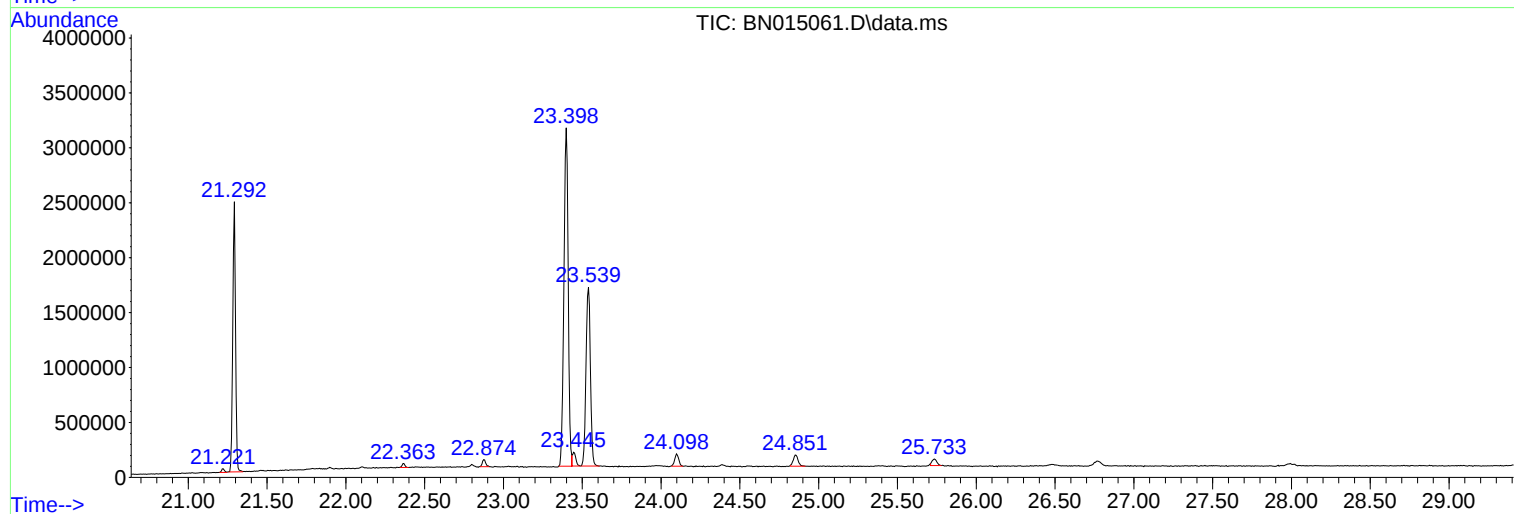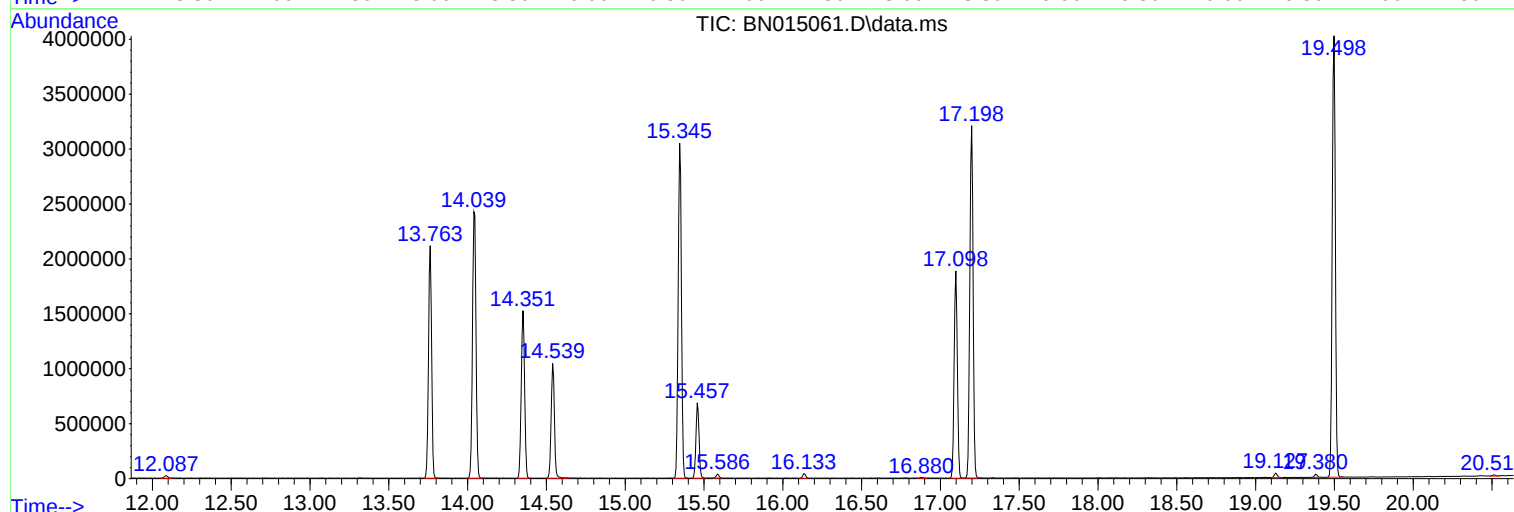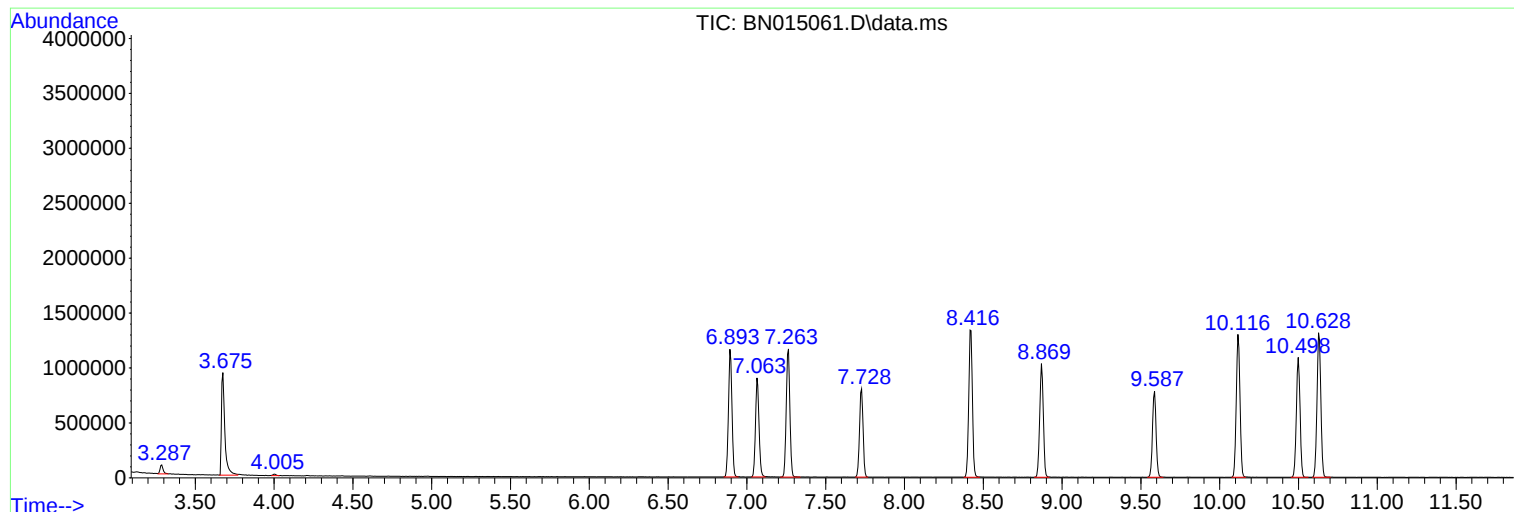

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
Data File : BN015061.D
Acq On : 25 Jun 2021 05:10
Operator : CG/JU
Sample : PB137214BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK214

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062521\
Data File : BN015061.D
Acq On : 25 Jun 2021 05:10
Operator : CG/JU
Sample : PB137214BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK214

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
