


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062525\
Data File : BN037376.D
Acq On : 25 Jun 2025 08:57
Operator : RC/JU
Sample : DFTPP379
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP379

Integration File: LSCINT.P

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN062025.MA.M
Title : SVOA CALIBRATION
Last Update : Thu Jun 19 14:59:41 2025

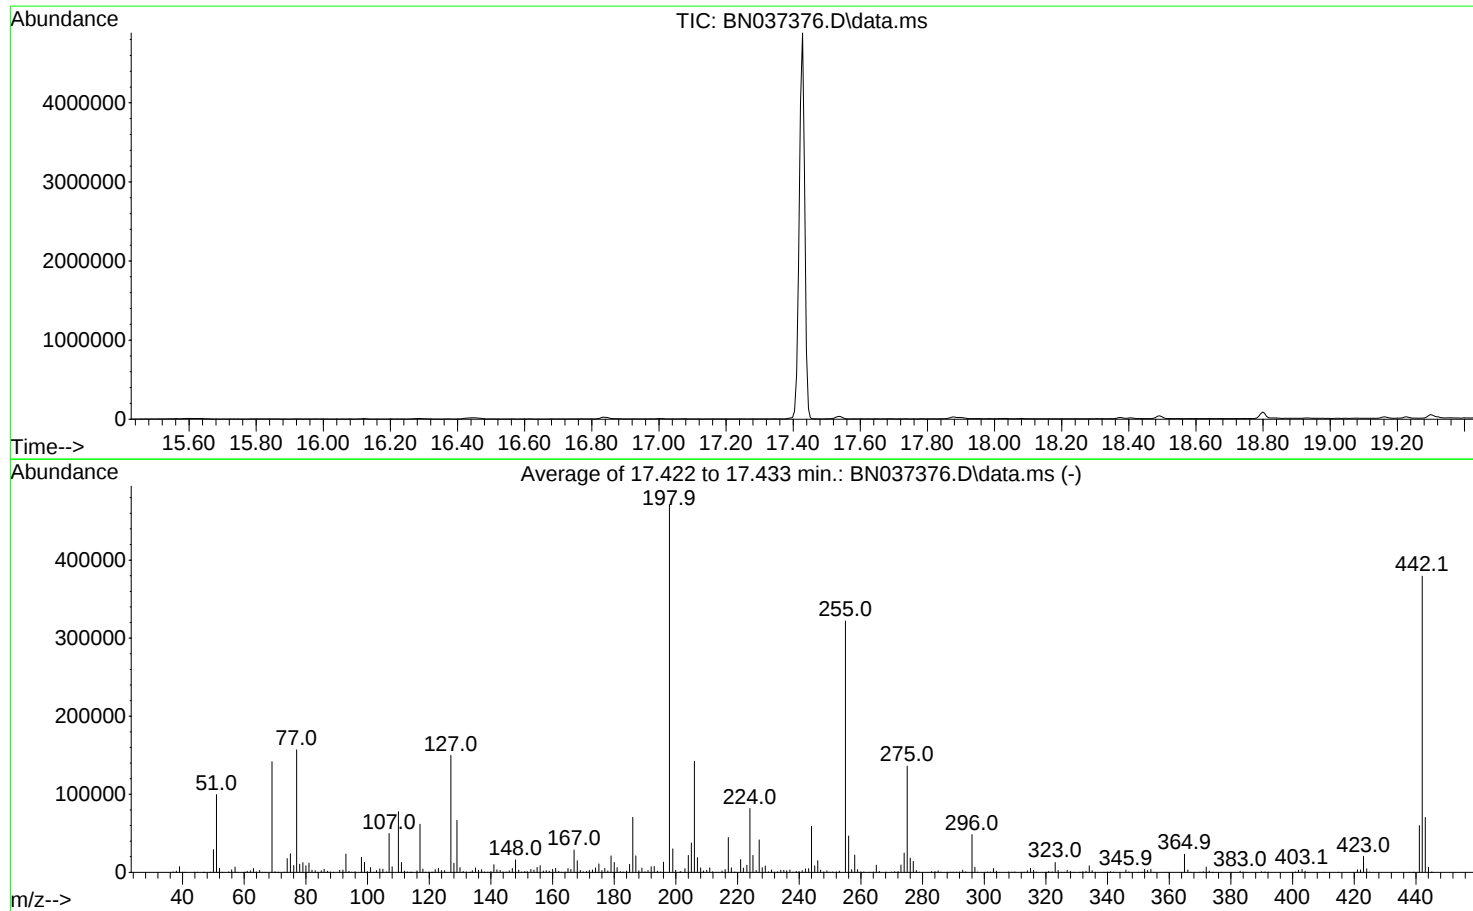

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.2	99675	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.1	141848	PASS
70	69	0.00	2	0.6	820	PASS
127	198	10	80	31.8	149749	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	471253	PASS
199	198	5	9	6.4	30229	PASS
275	198	10	60	28.9	136181	PASS
365	198	1	100	4.9	23251	PASS
441	198	0.01	100	12.7	59875	PASS
442	198	50	100	80.5	379328	PASS
443	442	15	24	18.6	70376	PASS