


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062620\
 Data File : BN011055.D
 Acq On : 26 Jun 2020 10:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 26 11:59:47 2020

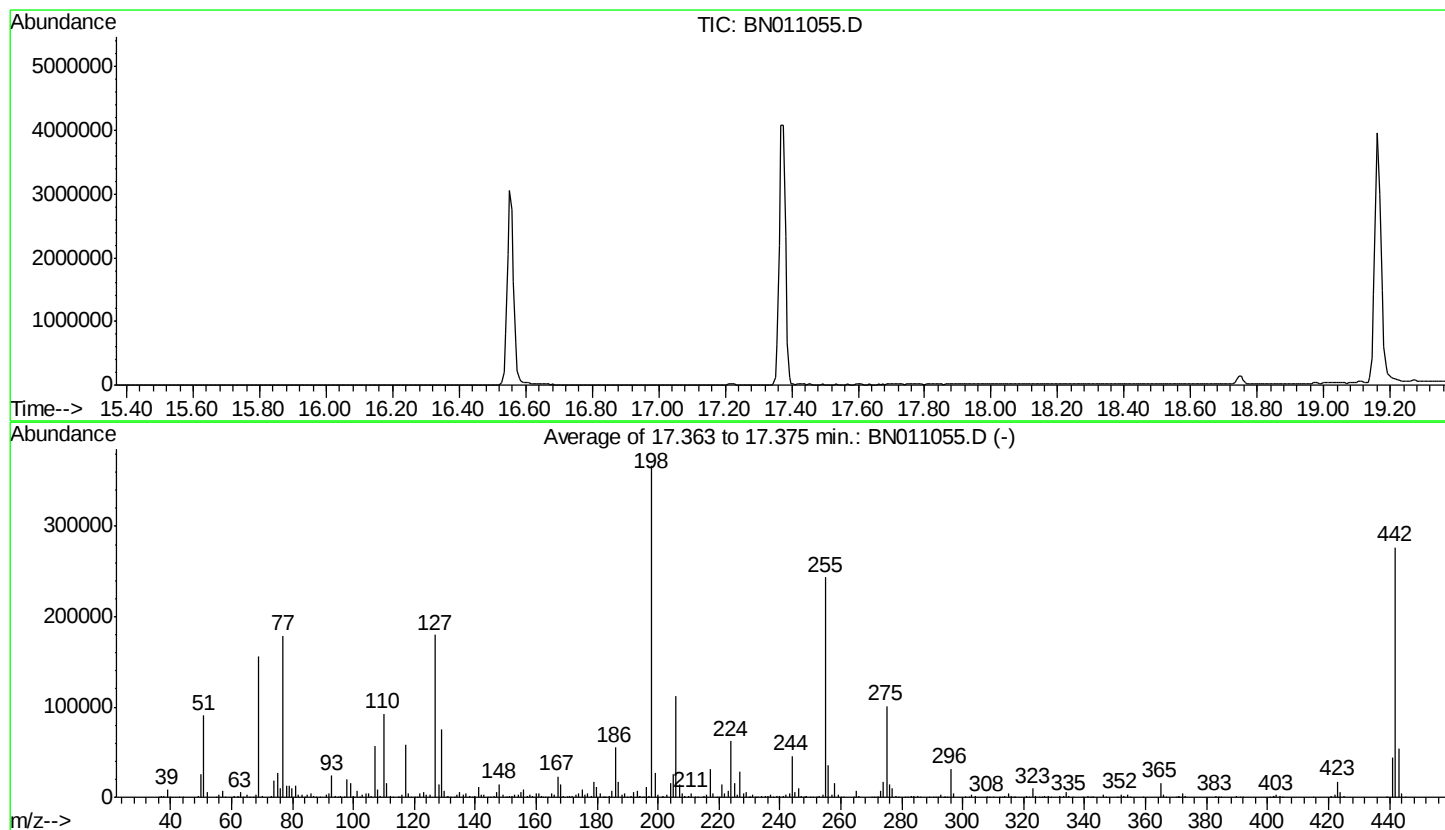

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.6	90378	PASS
68	69	0.00	2	2.0	3128	PASS
69	198	0.00	100	42.3	155434	PASS
70	69	0.00	2	0.6	872	PASS
127	198	10	80	49.0	179888	PASS
197	198	0.00	2	0.3	1099	PASS
198	198	100	100	100.0	367338	PASS
199	198	5	9	7.3	26968	PASS
275	198	10	60	27.6	101250	PASS
365	198	1	100	4.4	16251	PASS
441	198	0.01	100	12.0	44106	PASS
442	198	50	100	75.5	277173	PASS
443	442	15	24	19.5	54154	PASS