

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062625\
 Data File : BN037402.D
 Acq On : 26 Jun 2025 20:58
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 27 03:00:26 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN062625.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 26 16:06:33 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ng	-7.57
7) Naphthalene-d8	0.000	136	0	0.000	ng	-10.34
13) Acenaphthene-d10	0.000	164	0	0.000	ng	-14.21
19) Phenanthrene-d10	0.000	188	0	0.000	ng	-16.96
29) Chrysene-d12	0.000	240	0	0.000	ng	-21.16
35) Perylene-d12	0.000	264	0	0.000	ng	-23.35
System Monitoring Compounds						
4) 2-Fluorophenol	0.000	112	0	0.000	ng	
5) Phenol-d6	0.000	99	0	0.000	ng	
8) Nitrobenzene-d5	0.000	82	0	0.000	ng	
11) 2-Methylnaphthalene-d10	0.000	152	0	0.000	ng	
14) 2,4,6-Tribromophenol	0.000	330	0	0.000	ng	
15) 2-Fluorobiphenyl	0.000	172	0	0.000	ng	
27) Fluoranthene-d10	0.000	212	0	0.000	ng	
31) Terphenyl-d14	0.000	244	0	0.000	ng	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062625\
Data File : BN037402.D
Acq On : 26 Jun 2025 20:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 27 03:00:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN062625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 26 16:06:33 2025
Response via : Initial Calibration

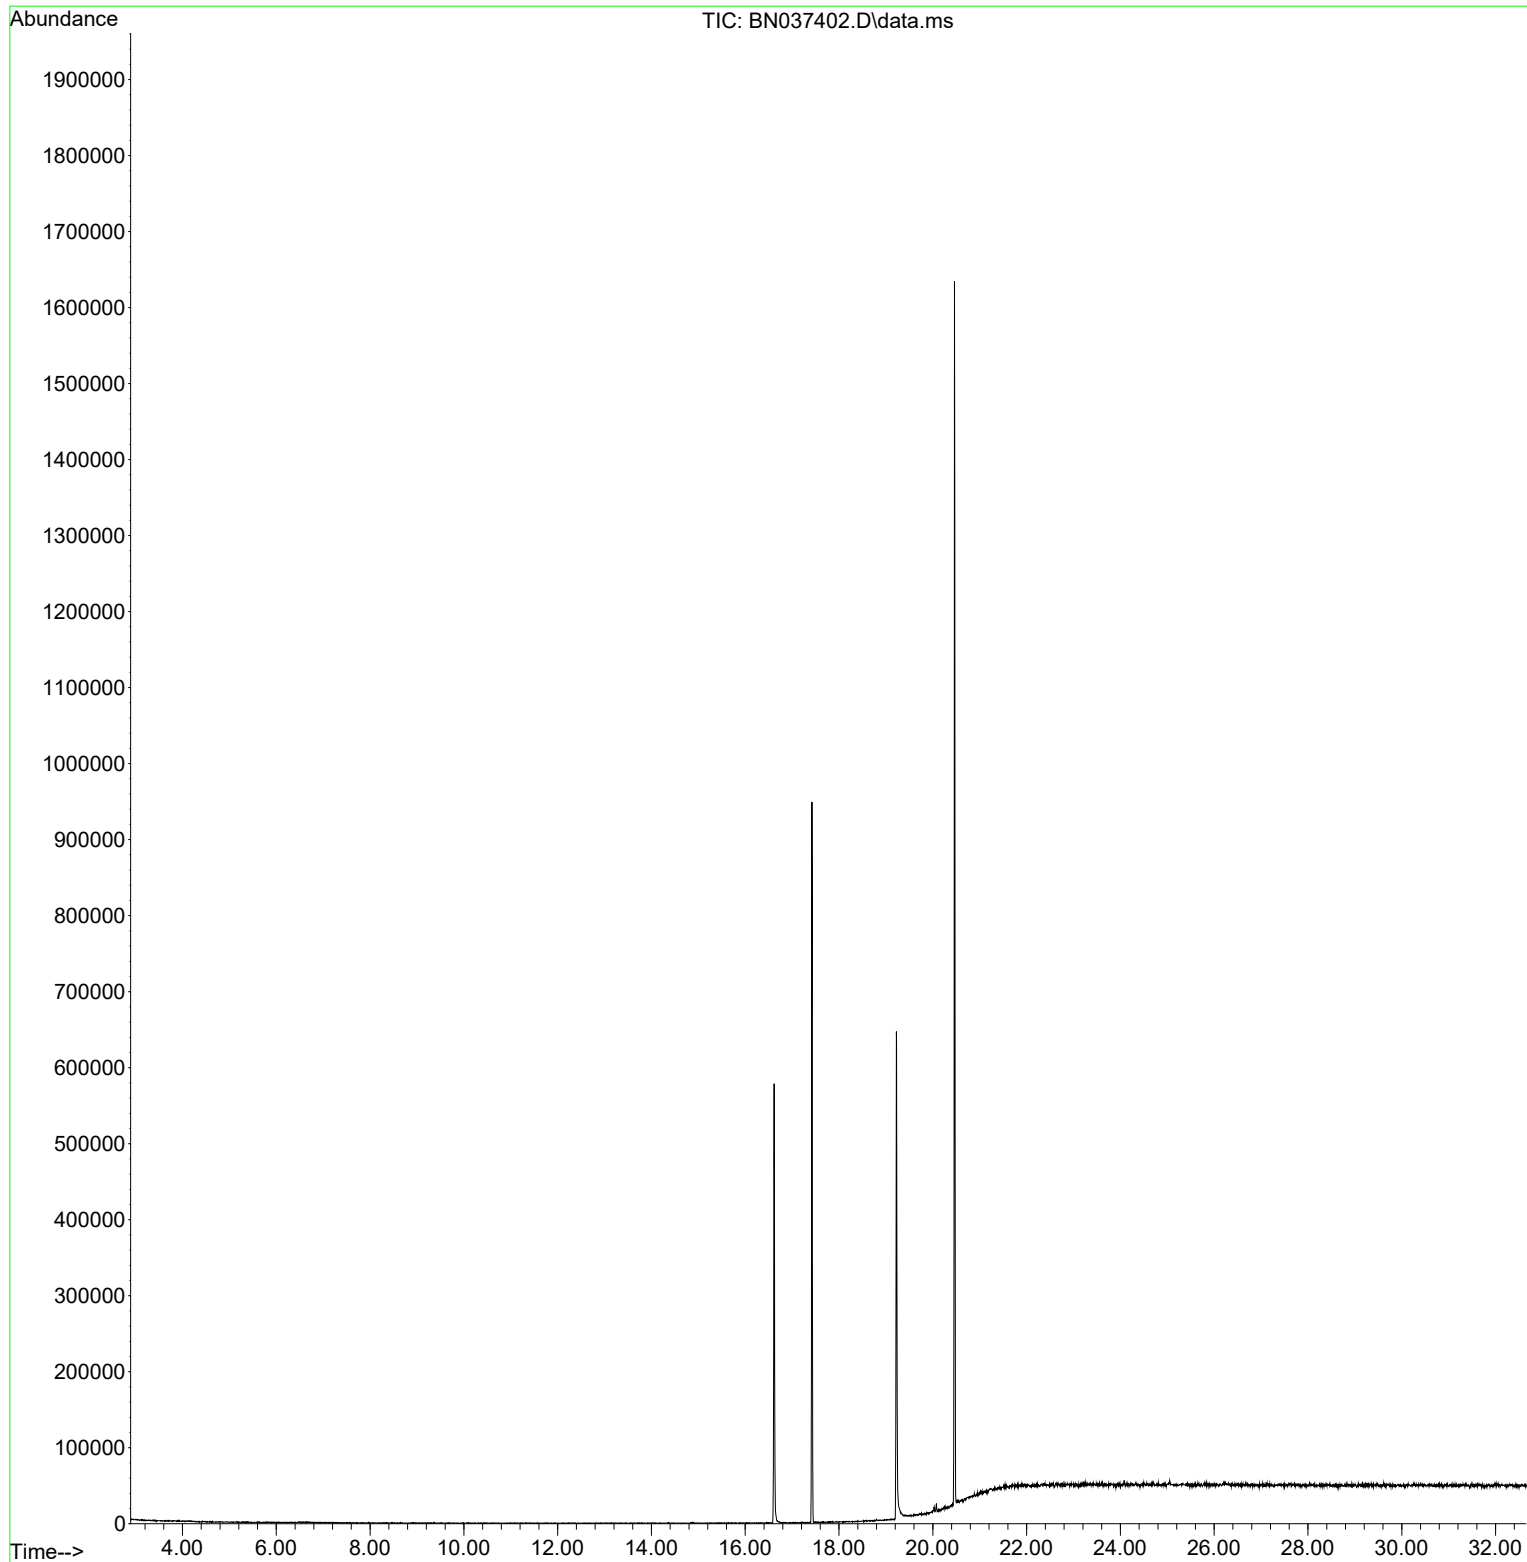


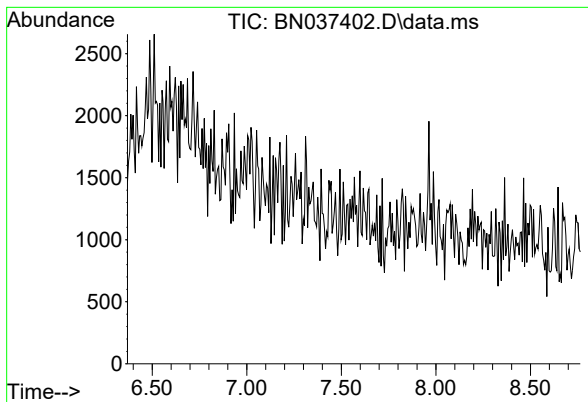


#1
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ng
 Expected RT: 7.57 min
 Lab File: BN037402.D
 Acq: 26 Jun 2025 20:58

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 152


Sig	Exp Ratio
152	100
150	145.2
115	53.6

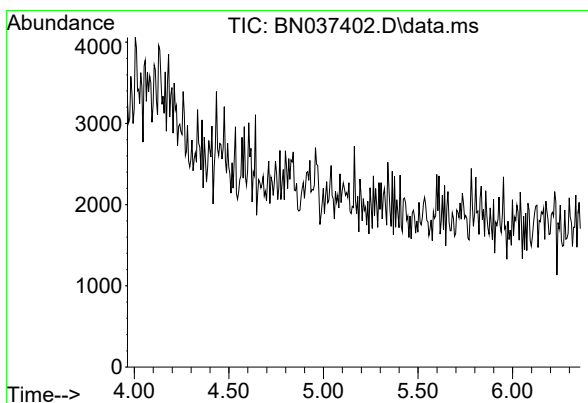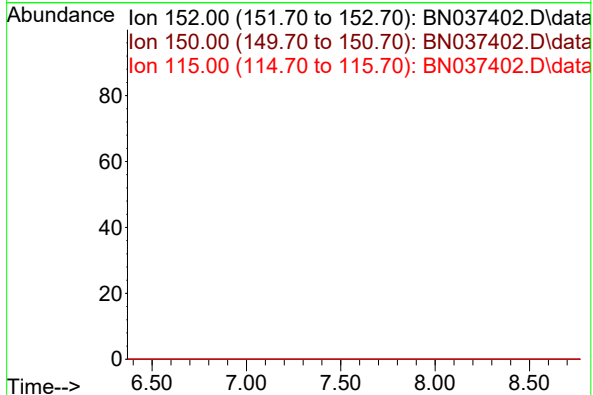


#4
 2-Fluorophenol
 Concen: 0.000 ng
 Expected RT: 5.16 min
 Lab File: BN037402.D
 Acq: 26 Jun 2025 20:58

Tgt Ion: 112

Sig	Exp Ratio
112	100
64	50.4
63	32.6

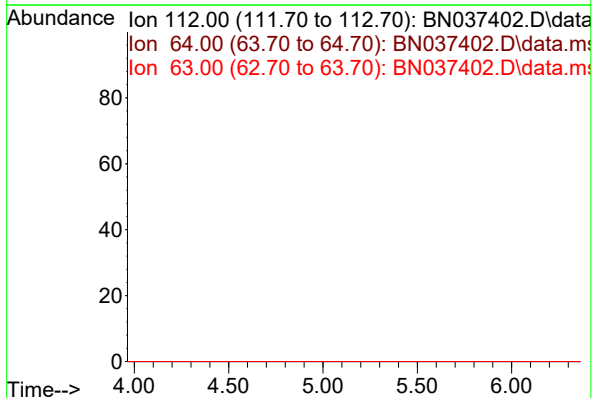


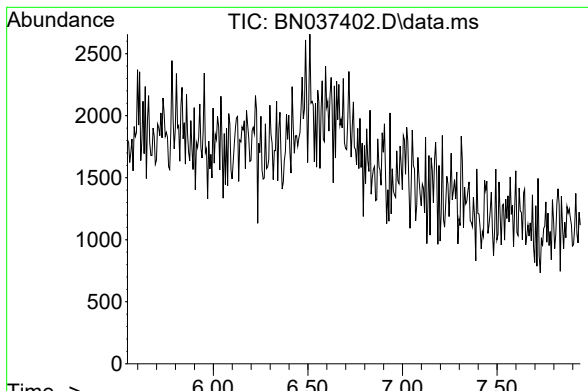


#5
 Phenol-d6
 Concen: 0.000 ng
 Expected RT: 6.74 min
 Lab File: BN037402.D
 Acq: 26 Jun 2025 20:58

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 99


Sig	Exp Ratio
99	100
42	19.5
71	44.8

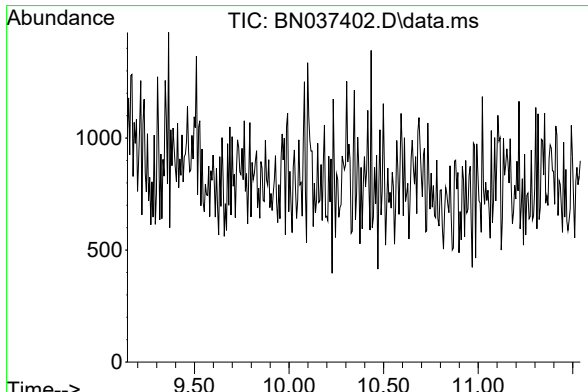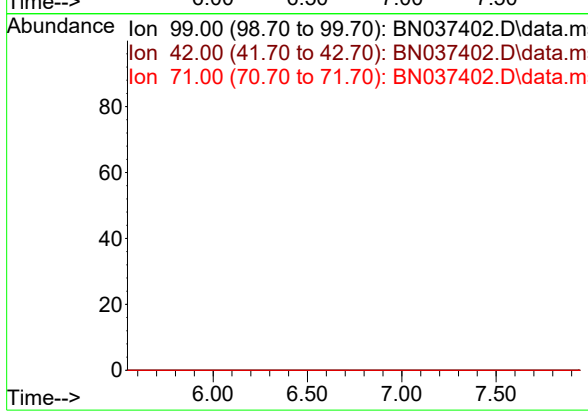


#7
 Naphthalene-d8
 Concen: 0.000 ng
 Expected RT: 10.34 min
 Lab File: BN037402.D
 Acq: 26 Jun 2025 20:58

Tgt Ion: 136

Sig	Exp Ratio
136	100
137	13.0
54	7.0
68	5.7

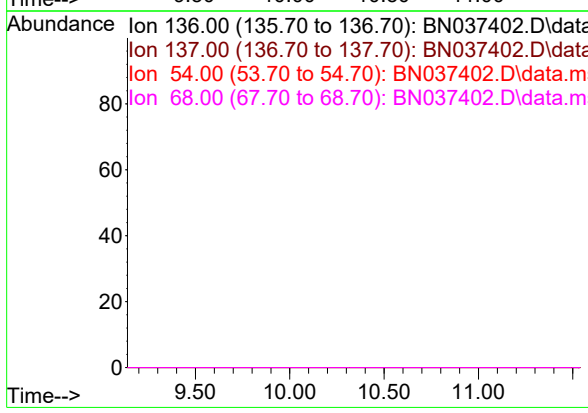


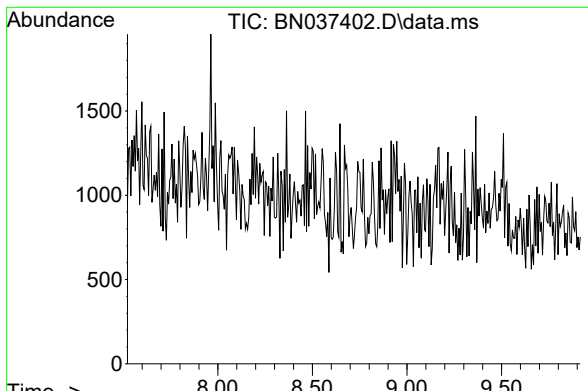


#8
 Nitrobenzene-d5
 Concen: 0.000 ng
 Expected RT: 8.72 min
 Lab File: BN037402.D
 Acq: 26 Jun 2025 20:58

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Tgt Ion: 82


Sig	Exp Ratio
82	100
128	42.5
54	47.1

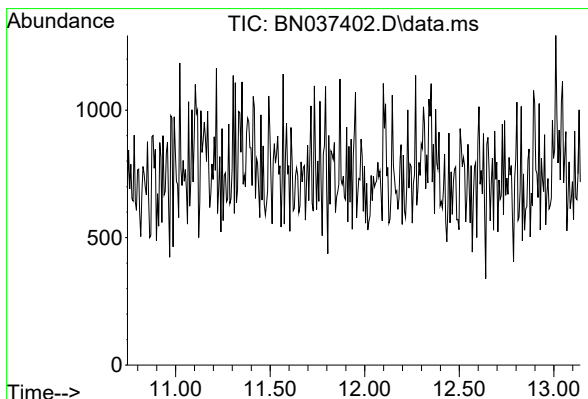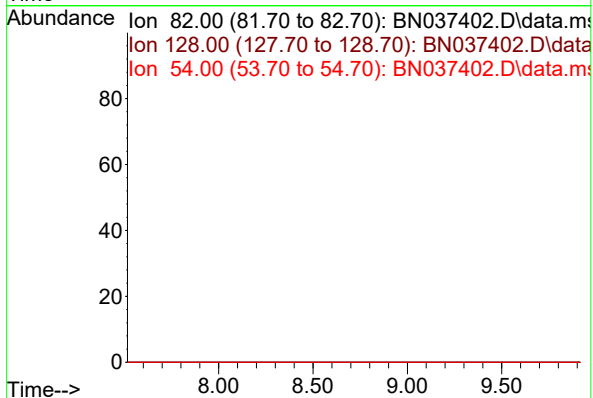


#11
 2-Methylnaphthalene-d10
 Concen: 0.000 ng
 Expected RT: 11.94 min
 Lab File: BN037402.D
 Acq: 26 Jun 2025 20:58

Tgt Ion: 152

Sig	Exp Ratio
152	100
151	23.0


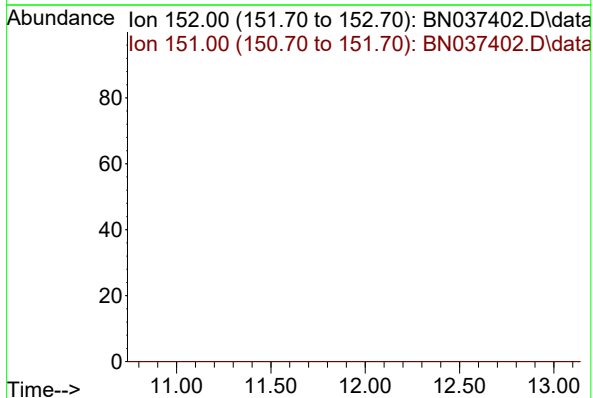


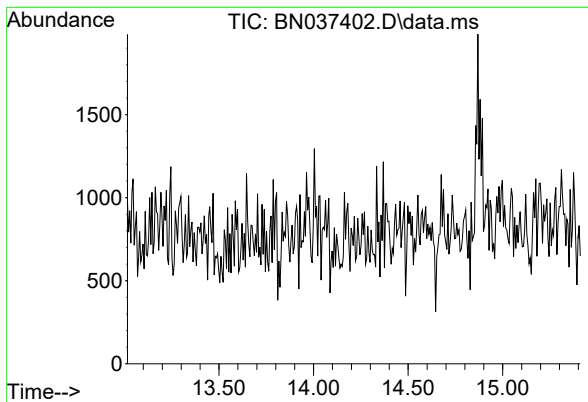

#13
 Acenaphthene-d10
 Concen: 0.000 ng
 Expected RT: 14.21 min
 Lab File: BN037402.D
 Acq: 26 Jun 2025 20:58


Instrument :
 BNA_N
 ClientSampleId :
 DFTPP


Tgt Ion: 164
 Sig Exp Ratio
 164 100
 162 103.2
 160 52.7

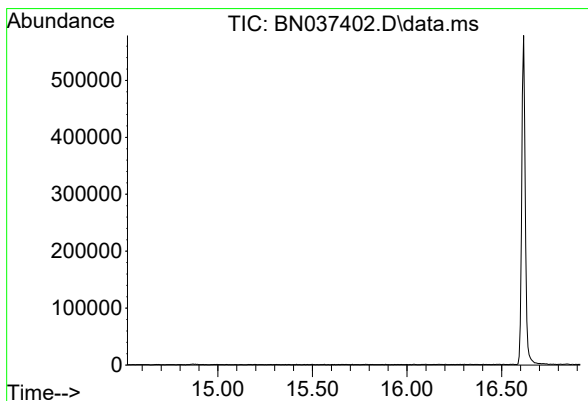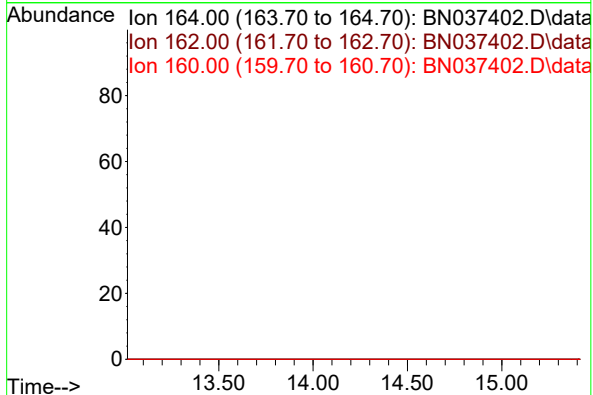

#14
 2,4,6-Tribromophenol
 Concen: 0.000 ng
 Expected RT: 15.72 min
 Lab File: BN037402.D
 Acq: 26 Jun 2025 20:58

Tgt Ion: 330
 Sig Exp Ratio
 330 100
 332 97.3
 141 30.0

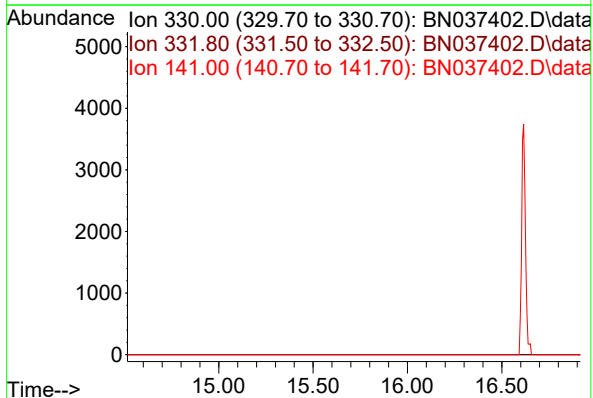


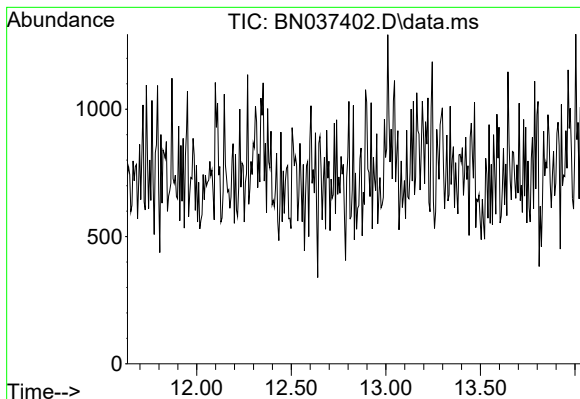


#15
2-Fluorobiphenyl
Concen: 0.000 ng
Expected RT: 12.83 min

Lab File: BN037402.D
Acq: 26 Jun 2025 20:58

Instrument :
BNA_N
ClientSampleId :
DFTPP


Tgt Ion: 172
Sig Exp Ratio
172 100
171 36.0
170 25.4

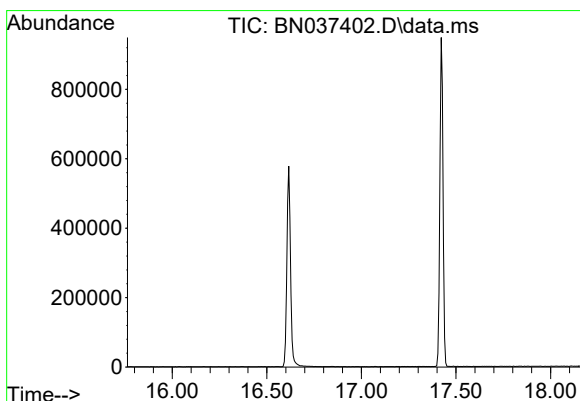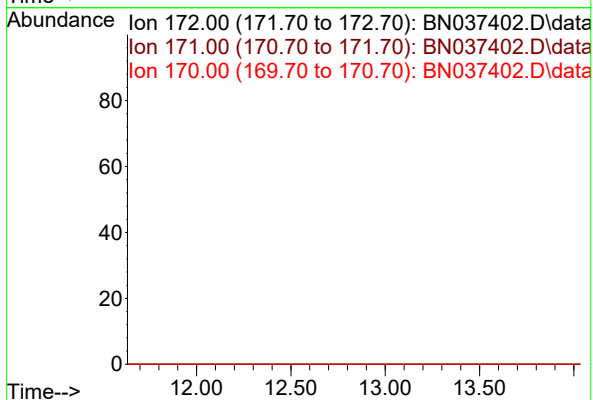


#19
Phenanthrene-d10
Concen: 0.000 ng
Expected RT: 16.96 min

Lab File: BN037402.D
Acq: 26 Jun 2025 20:58

Tgt Ion: 188
Sig Exp Ratio
188 100
94 0.0
80 7.8


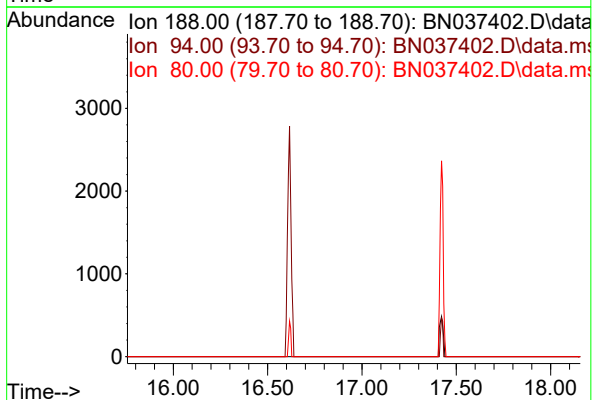


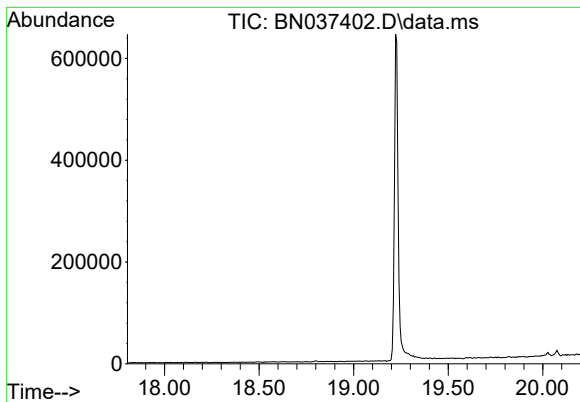

#27
 Fluoranthene-d10
 Concen: 0.000 ng
 Expected RT: 19.00 min
 Lab File: BN037402.D
 Acq: 26 Jun 2025 20:58


Instrument :
 BNA_N
 ClientSampleId :
 DFTPP


Tgt Ion: 212
 Sig Exp Ratio
 212 100
 106 5.6
 104 3.4

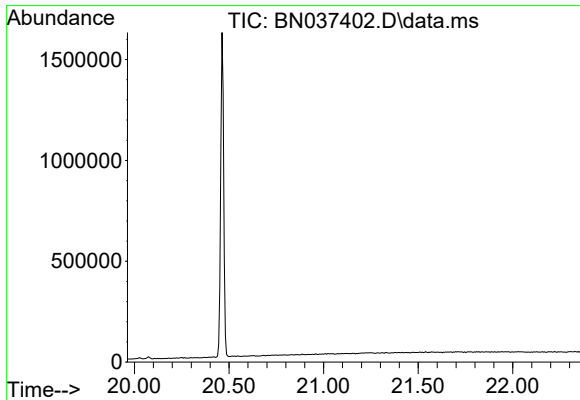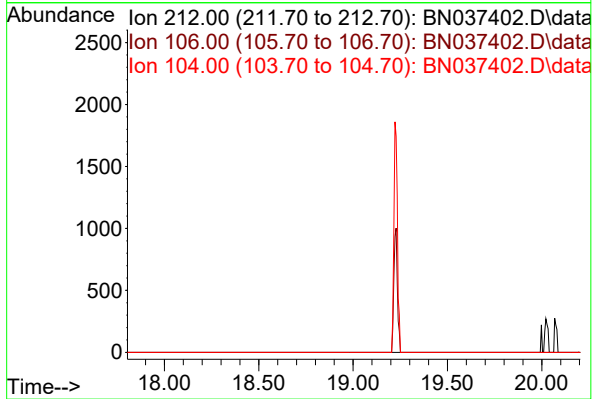

#29
 Chrysene-d12
 Concen: 0.000 ng
 Expected RT: 21.16 min
 Lab File: BN037402.D
 Acq: 26 Jun 2025 20:58

Tgt Ion: 240
 Sig Exp Ratio
 240 100
 120 6.6
 236 28.4

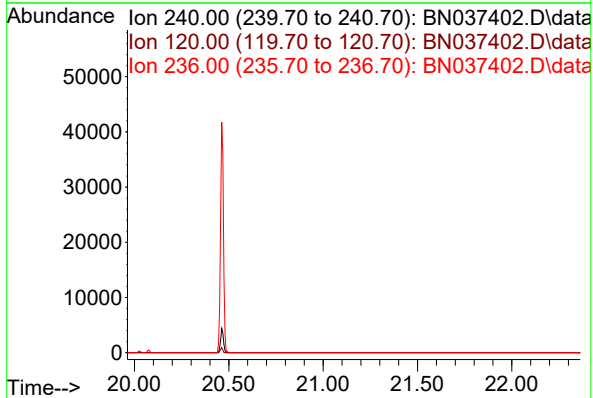


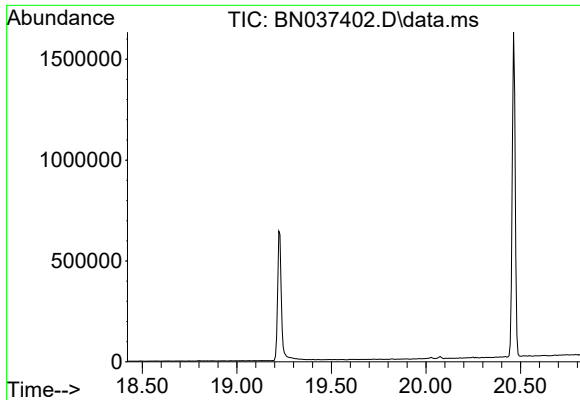


#31
Terphenyl-d14
Concen: 0.000 ng
Expected RT: 19.62 min

Lab File: BN037402.D
Acq: 26 Jun 2025 20:58

Instrument :
BNA_N
ClientSampleId :
DFTPP

Tgt Ion: 244
Sig Exp Ratio
244 100
212 11.4
122 7.9

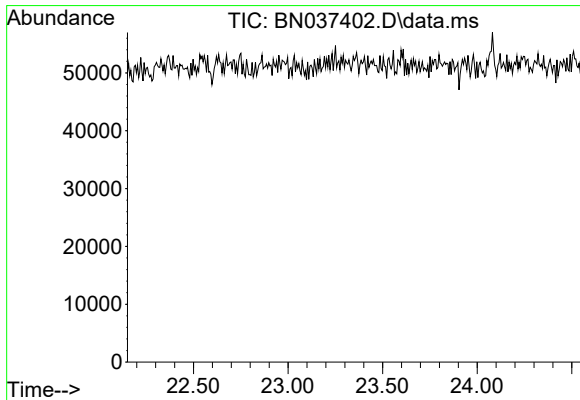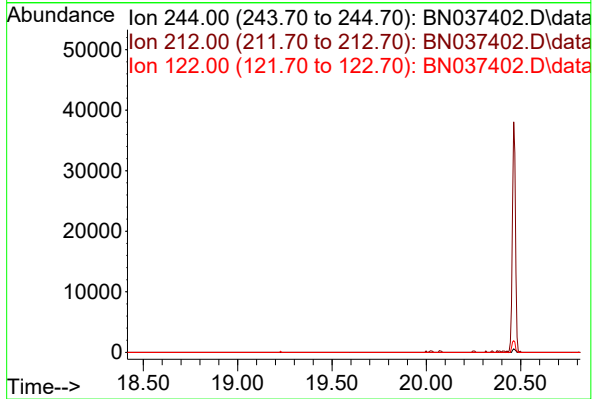

#35
Perylene-d12
Concen: 0.000 ng
Expected RT: 23.35 min

Lab File: BN037402.D
Acq: 26 Jun 2025 20:58

Tgt Ion: 264
Sig Exp Ratio
264 100
260 26.7
265 70.3

