
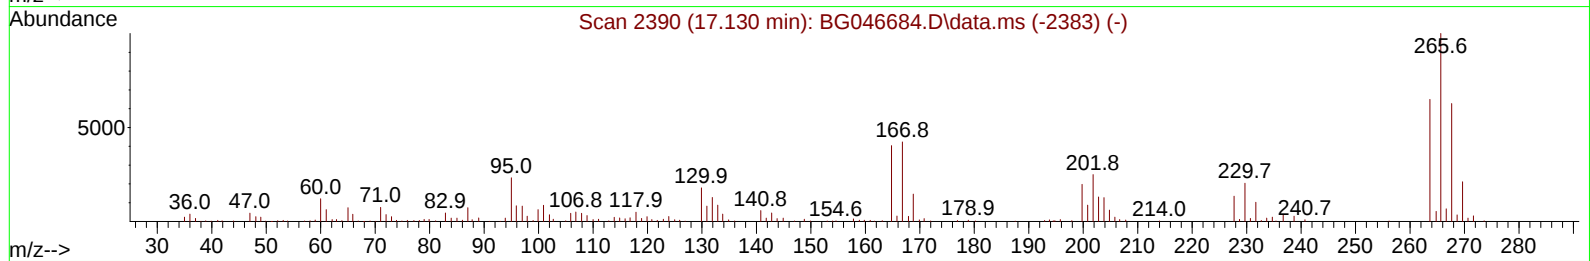
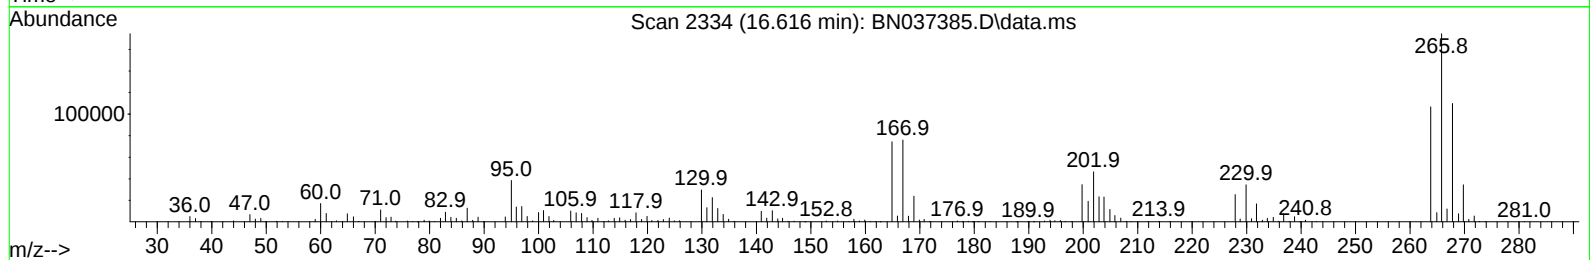


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062625\
Data File : BN037385.D
Acq On : 26 Jun 2025 10:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 17:27:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 21 02:21:08 2025
Response via : Initial Calibration

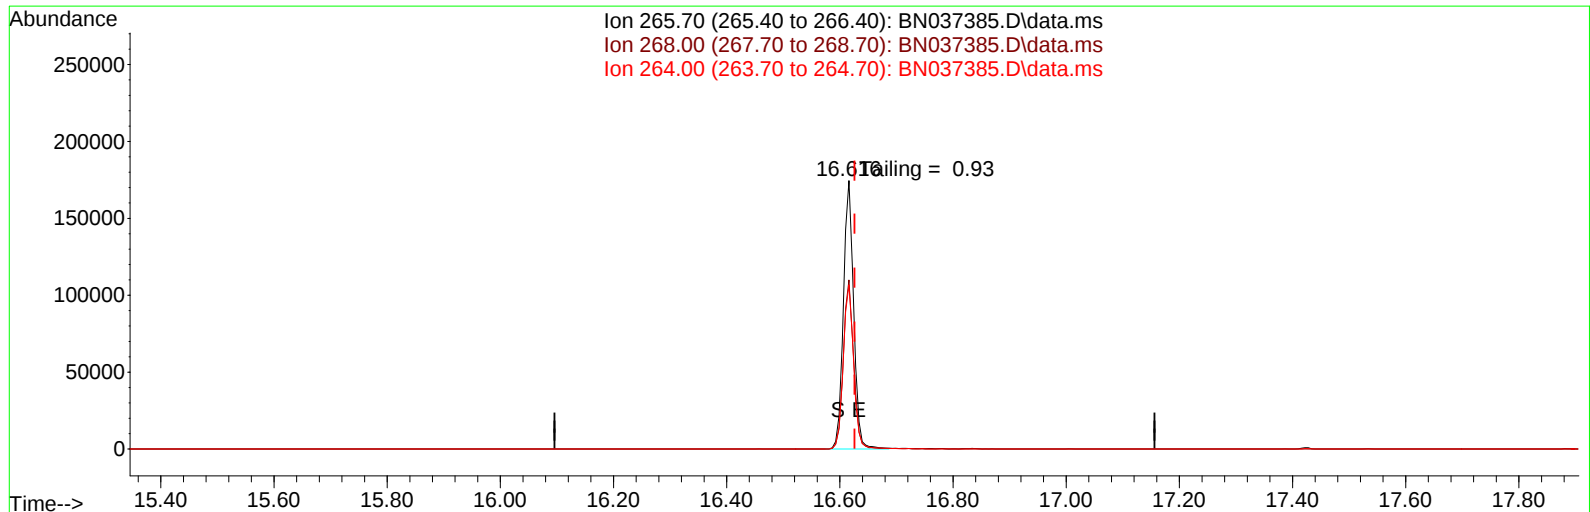

TIC: BN037385.D\data.ms

(70) Pentachlorophenol (C)




16.616min (-0.010) 22827.65 ng

response 218916

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.95
264.00	61.60	61.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062625\
Data File : BN037385.D
Acq On : 26 Jun 2025 10:01
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 26 17:27:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 21 02:21:08 2025
Response via : Initial Calibration

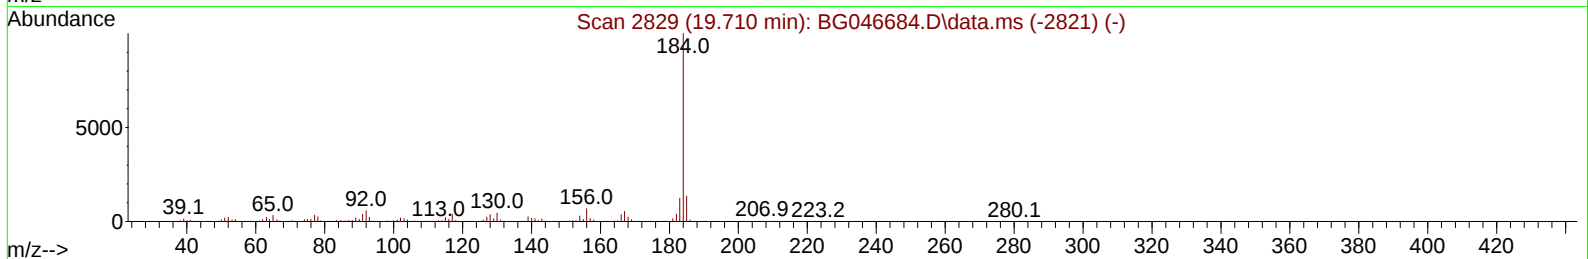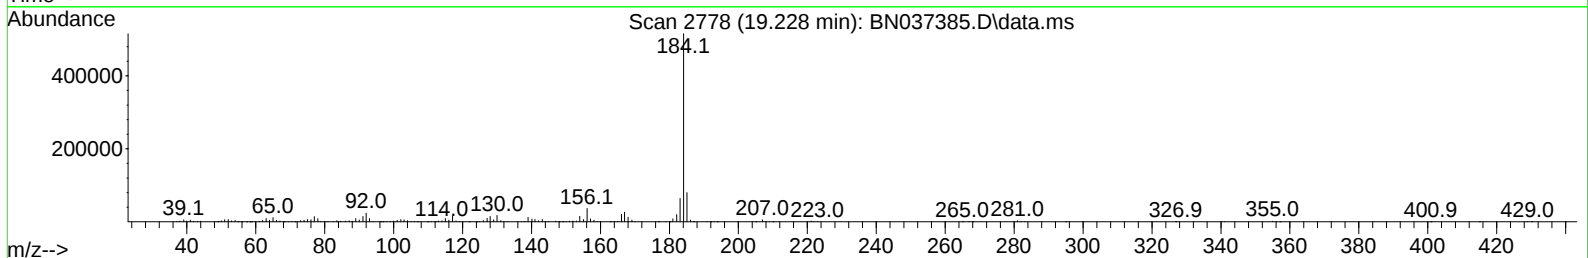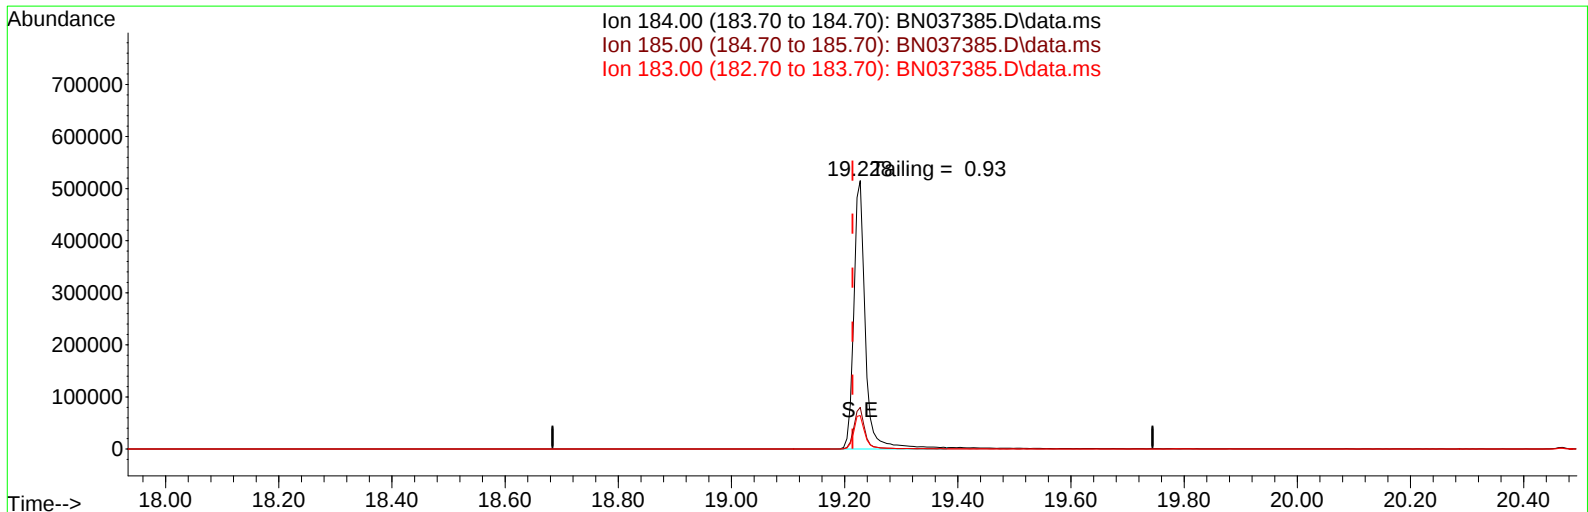

TIC: BN037385.D\data.ms

(77) Benzidine

19.228min (+ 0.014) 0.00 ng

response 733495

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.54
183.00	13.20	12.50
0.00	0.00	0.00