
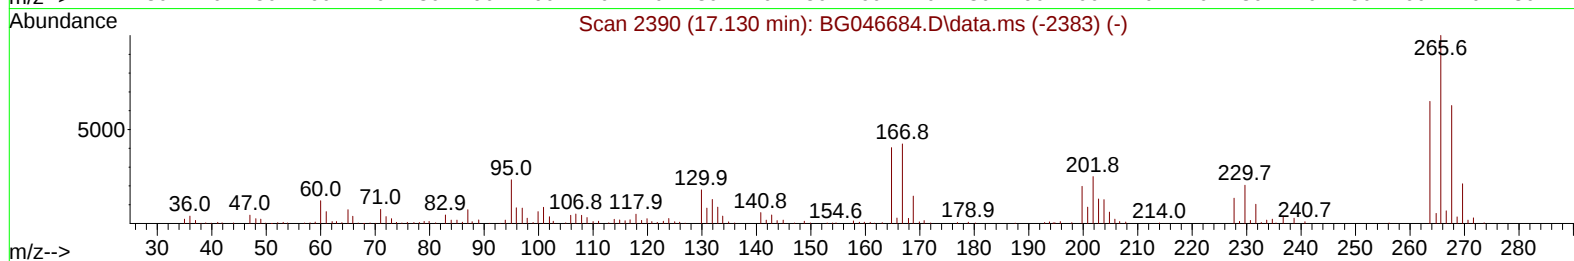
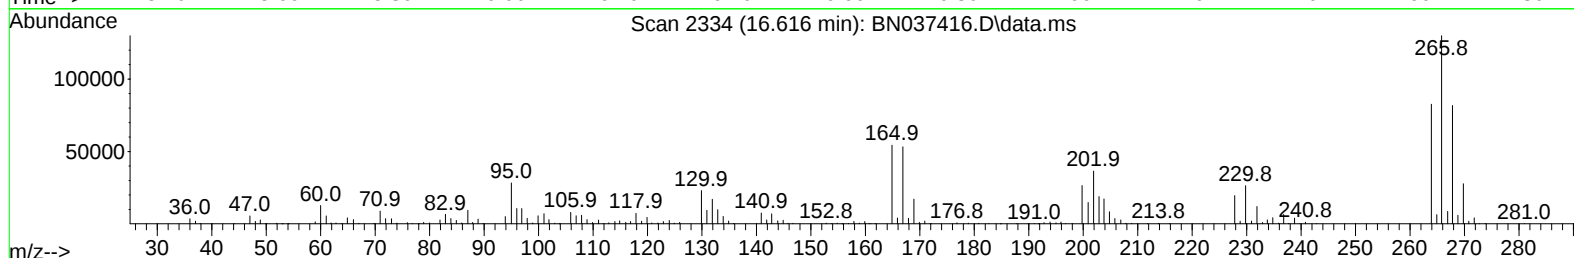


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062725\
Data File : BN037416.D
Acq On : 27 Jun 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 15:30:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 27 04:09:23 2025
Response via : Initial Calibration

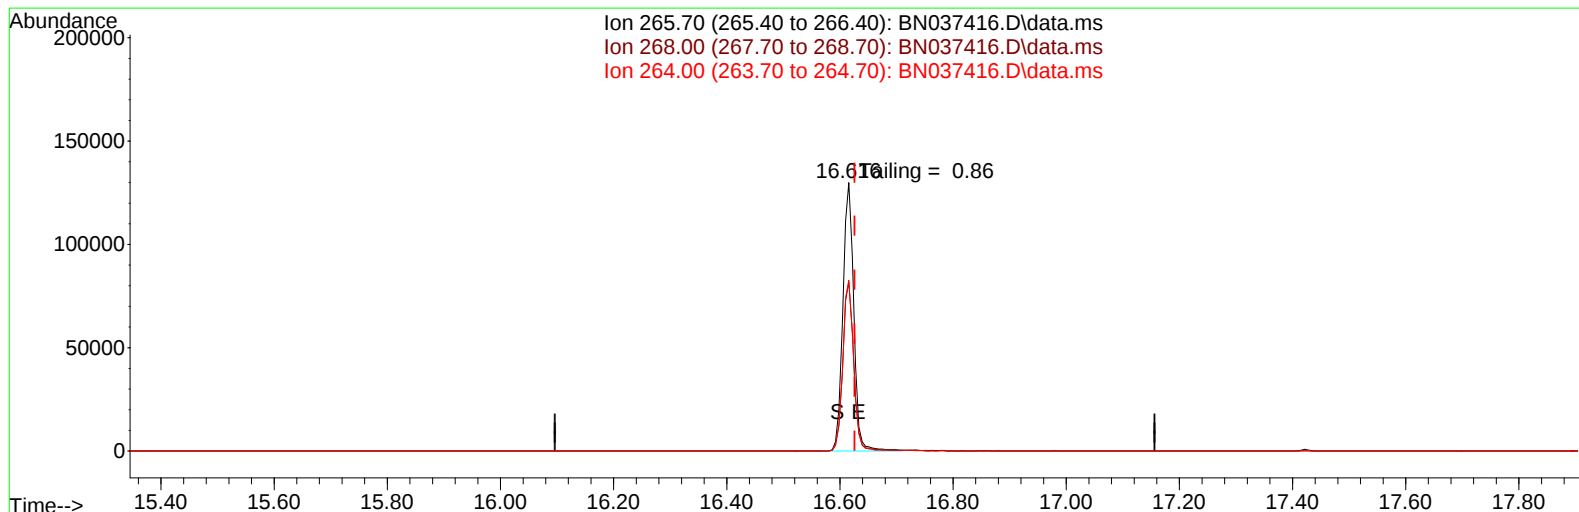

TIC: BN037416.D\data.ms

(70) Pentachlorophenol (C)




16.616min (-0.010) 18836.45 ng

response 173545

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.94
264.00	61.60	63.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062725\
Data File : BN037416.D
Acq On : 27 Jun 2025 09:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 15:30:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 27 04:09:23 2025
Response via : Initial Calibration

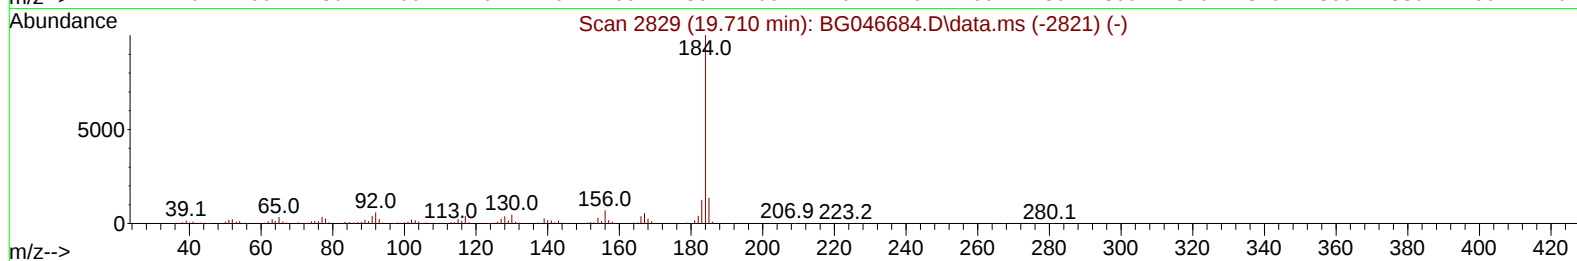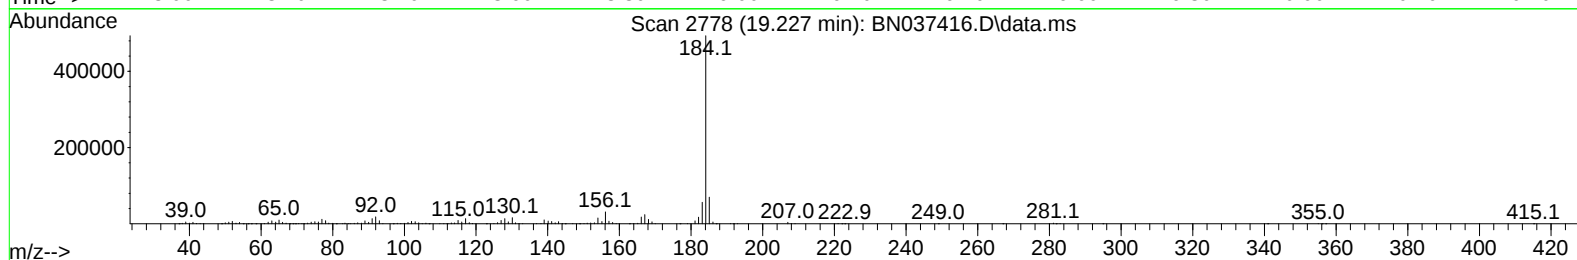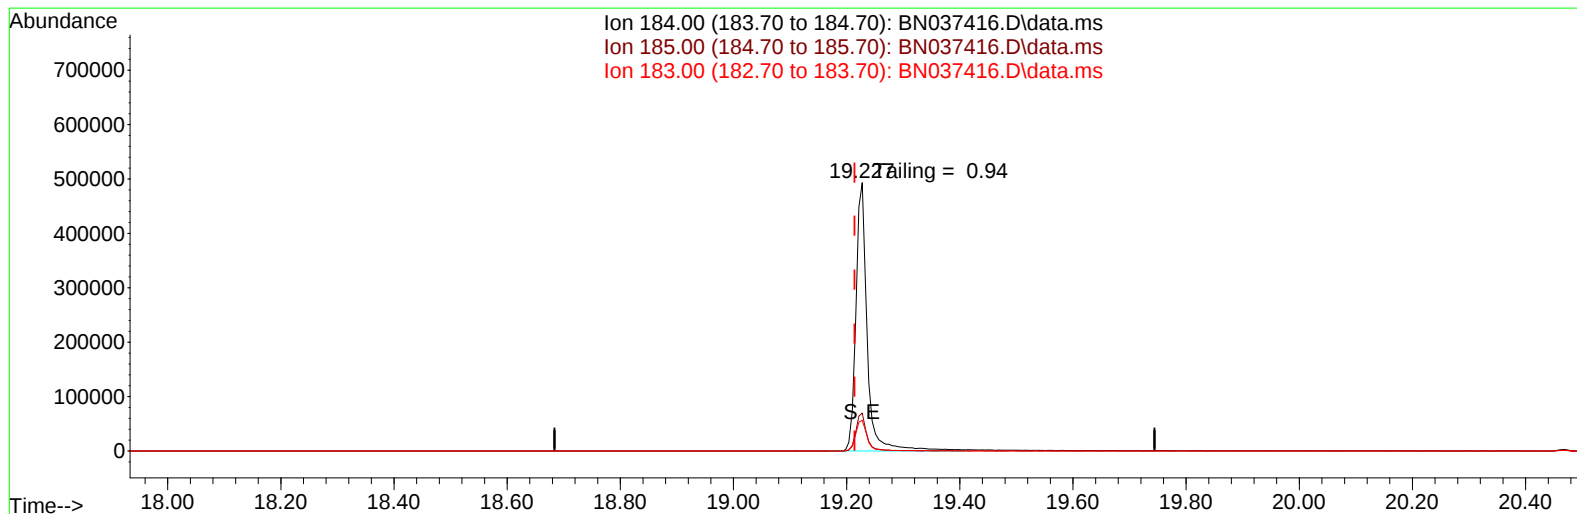

TIC: BN037416.D\data.ms

(77) Benzidine**19.227min (+ 0.013) 0.00 ng****response 690171**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.12
183.00	13.20	11.44
0.00	0.00	0.00