
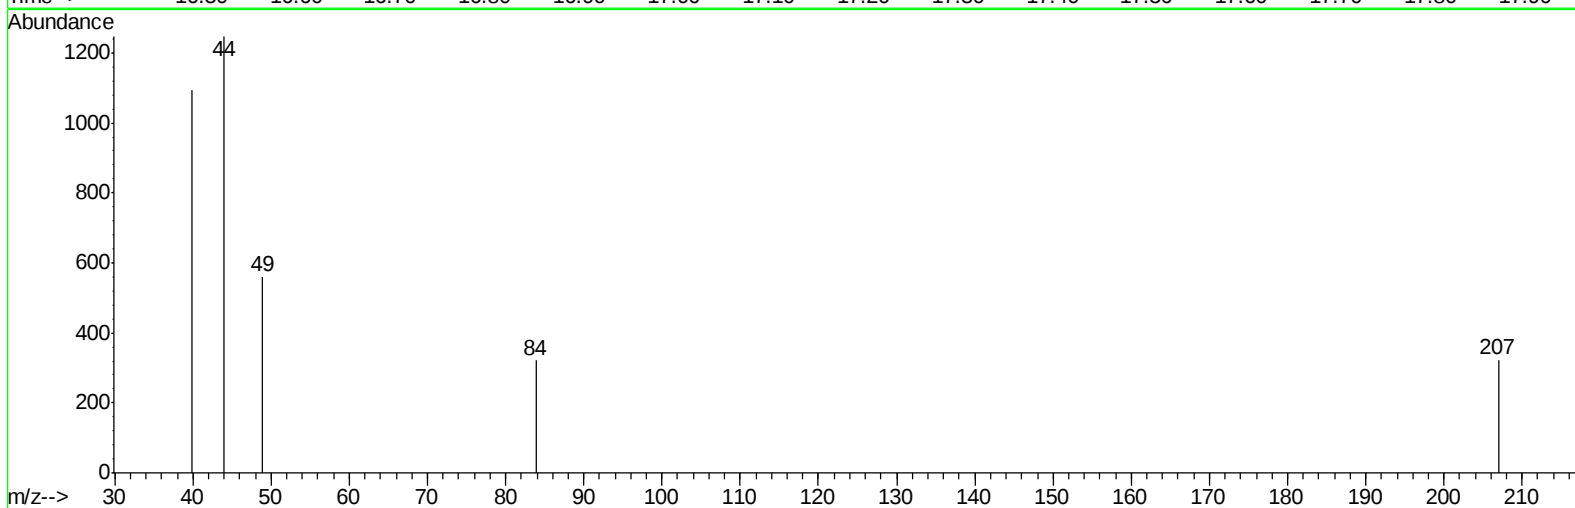


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062819\
Data File : BN006619.D
Acq On : 28 Jun 2019 18:43
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 07:22:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 05:26:43 2019
Response via : Initial Calibration

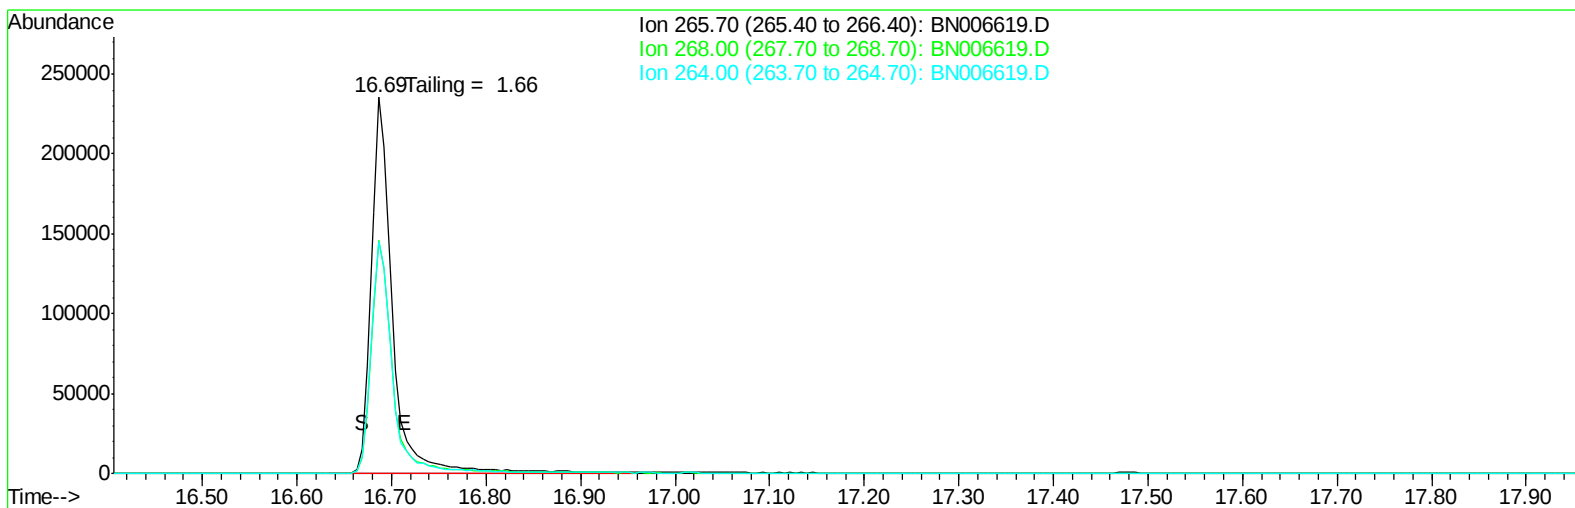

TIC: BN006619.D

(70) Pentachlorophenol (C)



10.907min (-10.907) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	61.90	0.00#
264.00	61.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN062819\
Data File : BN006619.D
Acq On : 28 Jun 2019 18:43
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 07:22:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 28 05:26:43 2019
Response via : Initial Calibration

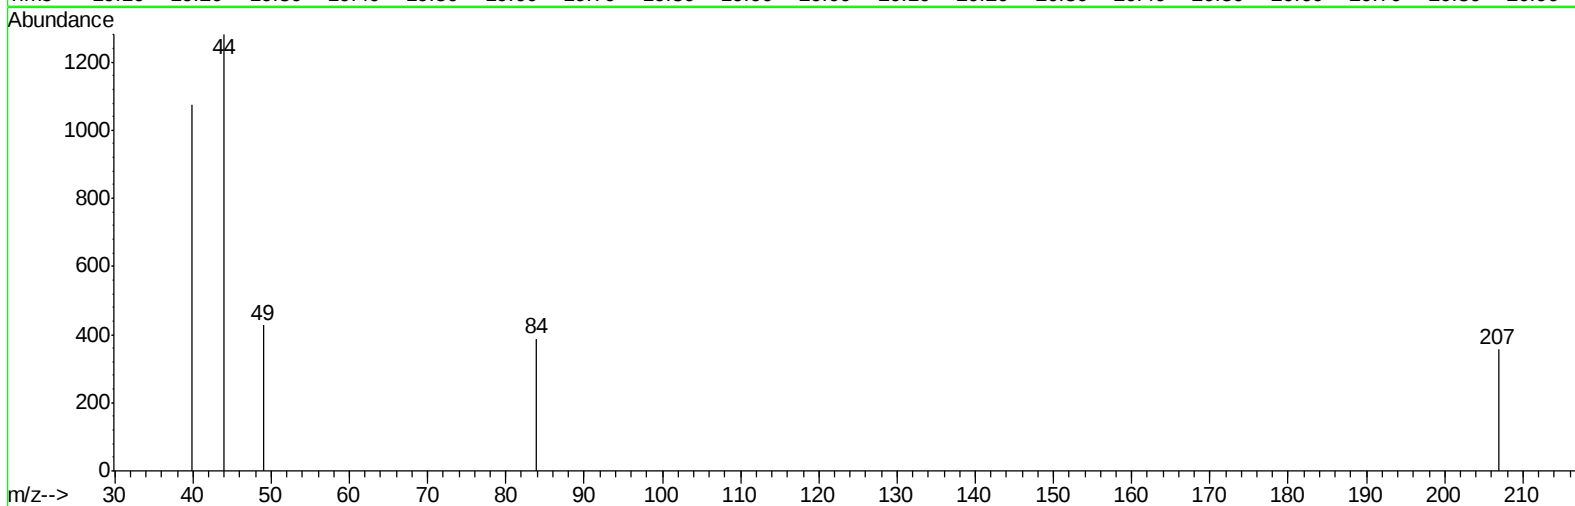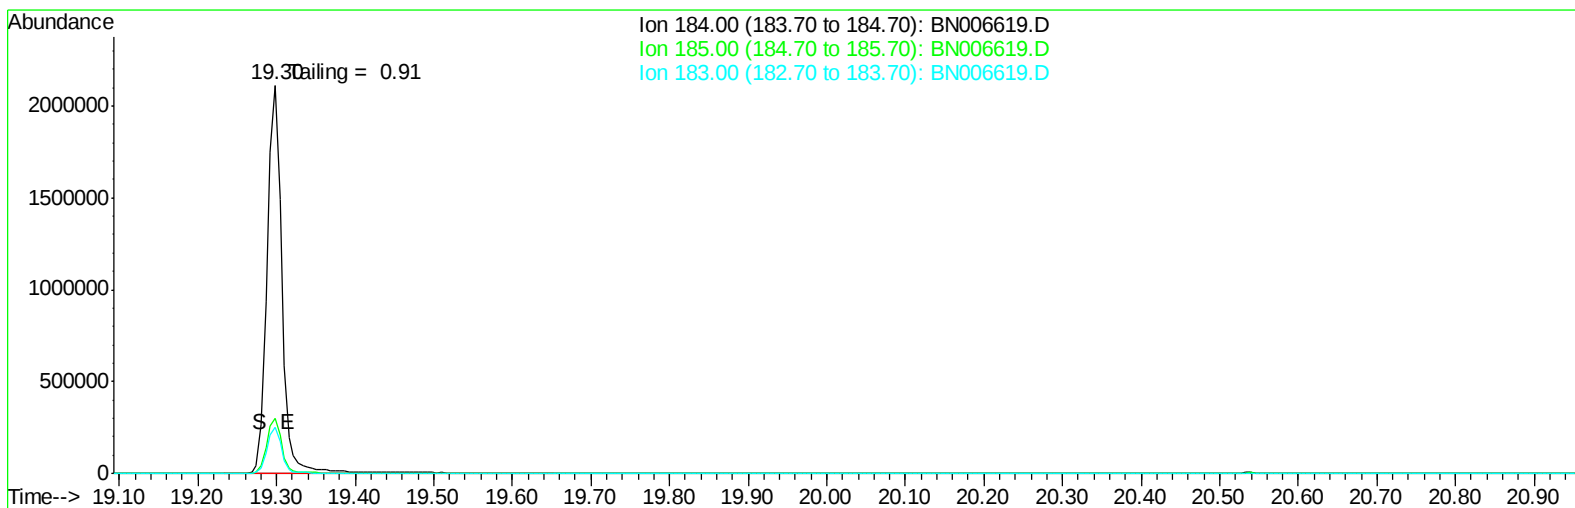

TIC: BN006619.D

(77) Benzidine

12.424min (-12.424) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.20	0.00#
183.00	12.00	0.00#
0.00	0.00	0.00