


Data Path : \\74.0.250.170\TERASTORAGE\SVOASRV\HPCHEM1\BNA_N\DATA\BN062819\
 Data File : BN006603.D
 Acq On : 28 Jun 2019 08:32
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 13:47:56 2019

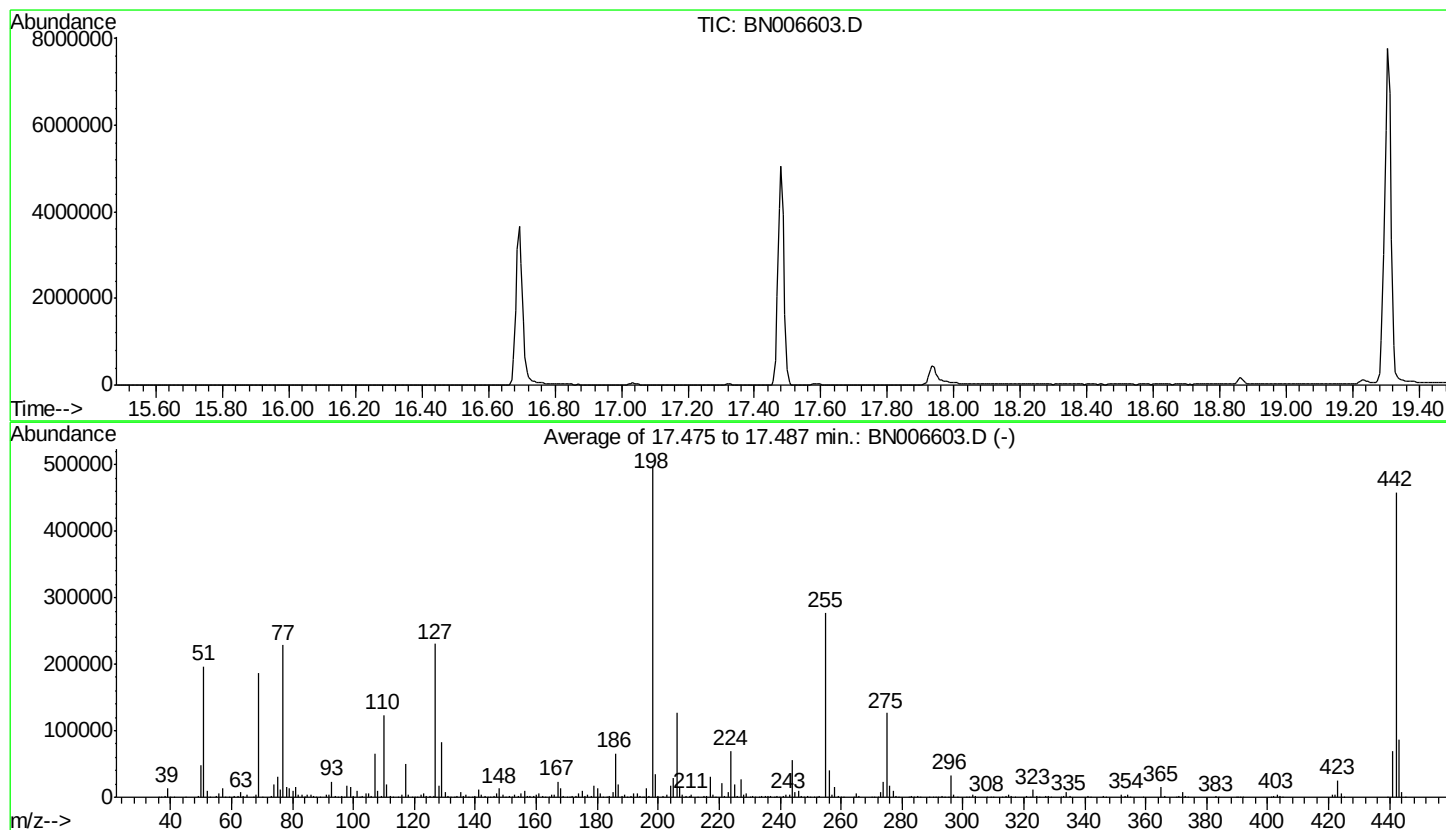

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	197120	PASS
68	69	0.00	2	1.7	3193	PASS
69	198	0.00	100	37.4	186624	PASS
70	69	0.00	2	0.5	938	PASS
127	198	10	80	46.3	230634	PASS
197	198	0.00	2	0.5	2650	PASS
198	198	100	100	100.0	498453	PASS
199	198	5	9	6.8	33866	PASS
275	198	10	60	25.5	126898	PASS
365	198	1	100	3.2	16010	PASS
441	198	0.01	100	13.9	69341	PASS
442	198	50	100	91.9	458197	PASS
443	442	15	24	19.1	87584	PASS