


Data Path : \\74.0.250.170\TERASTORAGE\SVOASRV\HPCHEM1\BNA_N\DATA\BN062819\
 Data File : BN006619.D
 Acq On : 28 Jun 2019 18:43
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 13:47:56 2019

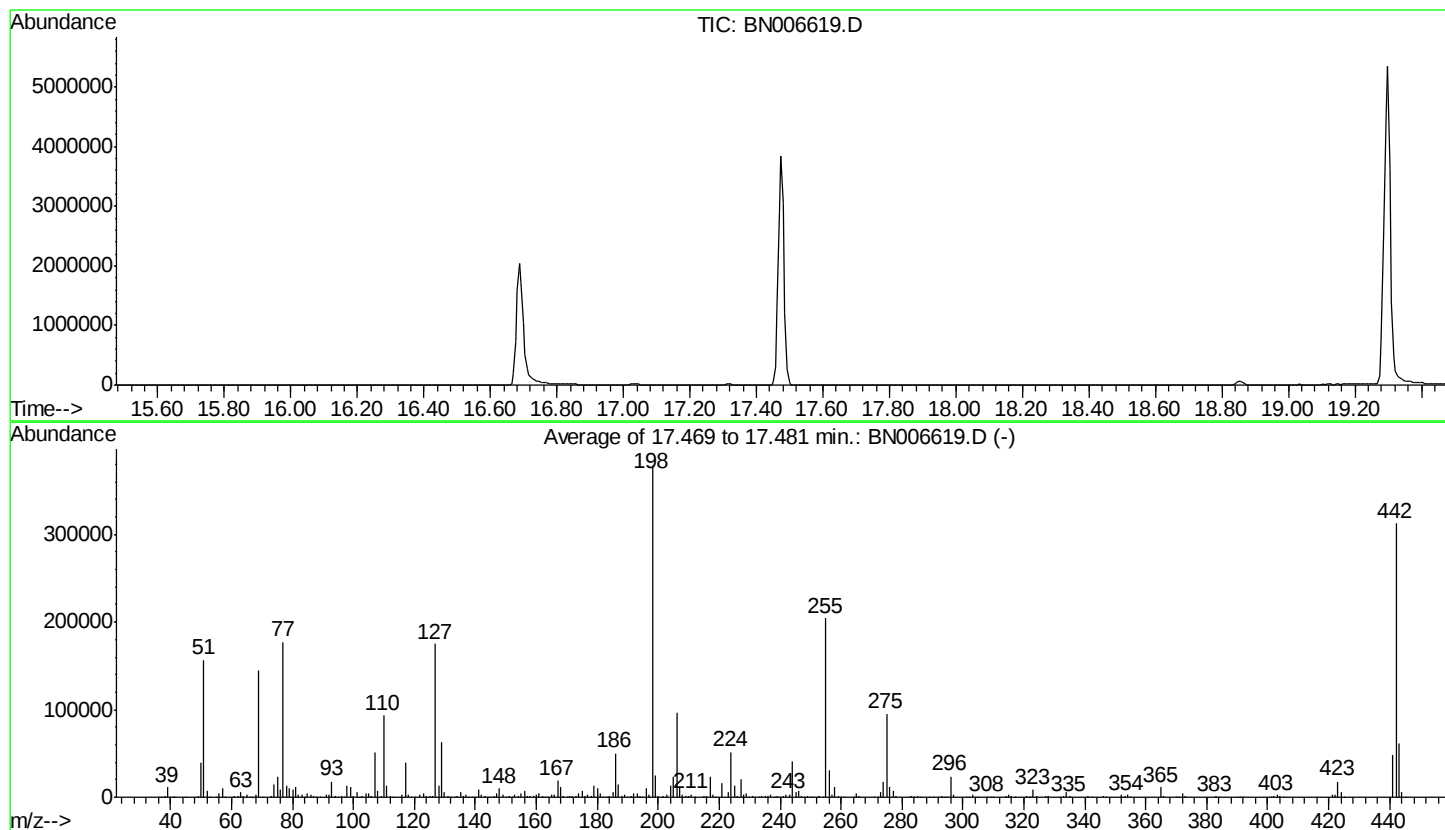

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	157072	PASS
68	69	0.00	2	1.7	2520	PASS
69	198	0.00	100	38.4	145298	PASS
70	69	0.00	2	0.5	752	PASS
127	198	10	80	46.3	175104	PASS
197	198	0.00	2	0.7	2695	PASS
198	198	100	100	100.0	378581	PASS
199	198	5	9	6.7	25253	PASS
275	198	10	60	25.1	95128	PASS
365	198	1	100	3.1	11563	PASS
441	198	0.01	100	12.9	48864	PASS
442	198	50	100	82.5	312170	PASS
443	442	15	24	19.5	60789	PASS