


Data Path : \\74.0.250.170\TERASTORAGE\SVOASRV\HPCHEM1\BNA_N\DATA\BN062819\
Data File : BN006638.D
Acq On : 29 Jun 2019 06:14
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062819.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 28 13:47:56 2019

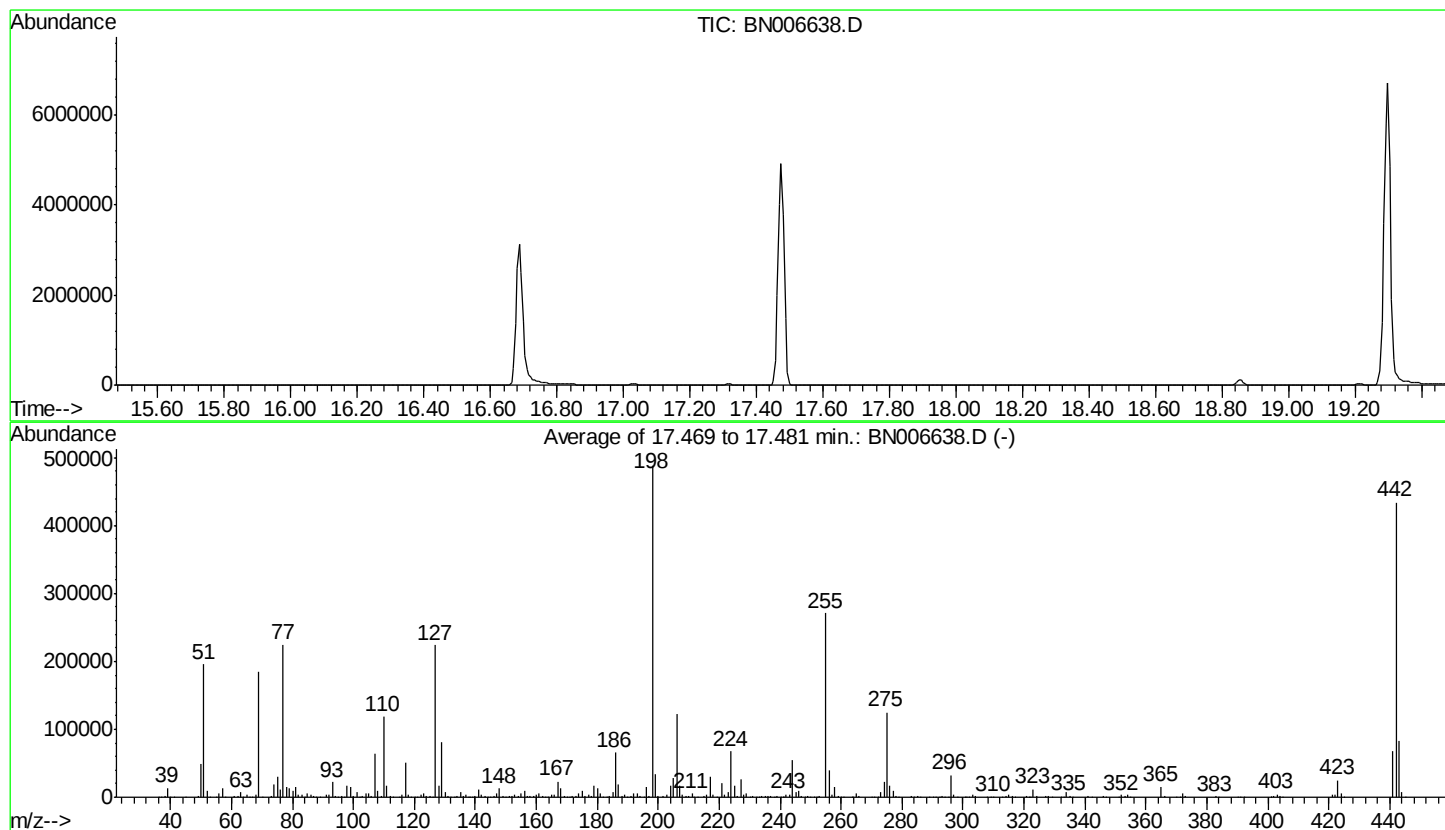

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	195520	PASS
68	69	0.00	2	1.7	3168	PASS
69	198	0.00	100	37.9	184810	PASS
70	69	0.00	2	0.5	892	PASS
127	198	10	80	45.9	224213	PASS
197	198	0.00	2	0.5	2441	PASS
198	198	100	100	100.0	488256	PASS
199	198	5	9	6.9	33485	PASS
275	198	10	60	25.5	124613	PASS
365	198	1	100	3.1	15376	PASS
441	198	0.01	100	14.0	68136	PASS
442	198	50	100	89.0	434453	PASS
443	442	15	24	19.1	83098	PASS