

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062821\
 Data File : BN015172.D
 Acq On : 28 Jun 2021 12:57
 Operator : CG/JU
 Sample : M2761-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLX83

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN015172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.681	99	101	108	rBV	59876	90975	4.51%	0.634%
2	3.999	152	155	162	rVB2	23035	31838	1.58%	0.222%
3	5.411	391	395	404	rVB2	29799	61307	3.04%	0.428%
4	5.769	453	456	460	rVB	14725	19846	0.98%	0.138%
5	6.893	641	647	655	rVB	101946	158569	7.86%	1.106%
6	7.063	671	676	685	rVB	83913	135715	6.73%	0.946%
7	7.257	704	709	716	rVB	103969	164623	8.16%	1.148%
8	7.722	782	788	795	rVB	581902	906372	44.94%	6.321%
9	7.963	825	829	834	rBV3	6682	9848	0.49%	0.069%
10	8.269	877	881	885	rBV3	5204	9620	0.48%	0.067%
11	8.416	900	906	913	rVB	111468	177131	8.78%	1.235%
12	8.534	923	926	930	rVB3	2536	3961	0.20%	0.028%
13	8.604	935	938	942	rVB4	3111	4159	0.21%	0.029%
14	8.810	971	973	976	rVV4	2829	2750	0.14%	0.019%
15	8.869	976	983	989	rVB	88188	149774	7.43%	1.045%
16	8.981	1000	1002	1006	rVB5	1890	2412	0.12%	0.017%
17	9.304	1055	1057	1061	rBV4	1661	2191	0.11%	0.015%
18	9.581	1099	1104	1110	rVB	48398	78794	3.91%	0.550%
19	10.116	1188	1195	1205	rBV	91216	147685	7.32%	1.030%
20	10.275	1218	1222	1231	rVB5	6428	12054	0.60%	0.084%
21	10.493	1252	1259	1266	rBV	745949	1246096	61.78%	8.690%
22	10.628	1275	1282	1293	rVB	104678	174124	8.63%	1.214%
23	11.963	1507	1509	1518	rVB5	1165	2888	0.14%	0.020%
24	12.087	1523	1530	1533	rBV5	2096	3770	0.19%	0.026%
25	13.181	1714	1716	1720	rVB4	2966	3625	0.18%	0.025%
26	13.275	1729	1732	1737	rVB5	1238	2098	0.10%	0.015%
27	13.669	1796	1799	1804	rBV4	1669	2158	0.11%	0.015%
28	13.757	1808	1814	1823	rVV	168329	230935	11.45%	1.611%
29	14.039	1856	1862	1872	rBV	204051	296780	14.71%	2.070%
30	14.263	1896	1900	1903	rVB3	4412	4746	0.24%	0.033%
31	14.351	1908	1915	1927	rBV	1046813	1520469	75.39%	10.604%
32	14.545	1942	1948	1952	rBV3	15609	26068	1.29%	0.182%
33	14.769	1982	1986	1992	rVB3	6373	7498	0.37%	0.052%
34	14.945	2010	2016	2019	rVB5	1810	2740	0.14%	0.019%
35	15.175	2049	2055	2057	rBV4	1430	2600	0.13%	0.018%
36	15.222	2060	2063	2068	rVB3	3329	3931	0.19%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062821\
 Data File : BN015172.D
 Acq On : 28 Jun 2021 12:57
 Operator : CG/JU
 Sample : M2761-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLX83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Title : SVOA CALIBRATION

37	15.345	2078	2084	2090	rBV	269290	383983	19.04%	2.678%
38	15.457	2099	2103	2108	rBV4	11199	15646	0.78%	0.109%
39	15.504	2108	2111	2115	rVV2	3704	3869	0.19%	0.027%
40	15.586	2120	2125	2130	rBV3	1438	3693	0.18%	0.026%
41	15.769	2152	2156	2161	rBV2	28154	36829	1.83%	0.257%
42	16.081	2206	2209	2212	rBV5	1866	2112	0.10%	0.015%
43	16.869	2335	2343	2350	rVB3	5666	11935	0.59%	0.083%
44	16.922	2350	2352	2353	rBV2	2203	2108	0.10%	0.015%
45	17.098	2375	2382	2392	rBV	1187519	1785113	88.51%	12.449%
46	17.192	2392	2398	2407	rVV2	292571	421387	20.89%	2.939%
47	17.298	2411	2416	2420	rVB5	3197	4525	0.22%	0.032%
48	17.469	2442	2445	2447	rBV3	3202	2463	0.12%	0.017%
49	17.528	2452	2455	2456	rBV2	2569	2745	0.14%	0.019%
50	17.610	2465	2469	2473	rBV4	5789	7755	0.38%	0.054%
51	17.780	2494	2498	2500	rBV4	4837	5891	0.29%	0.041%
52	17.833	2504	2507	2509	rBV4	2459	3269	0.16%	0.023%
53	17.969	2525	2530	2531	rBV4	3590	3583	0.18%	0.025%
54	17.998	2531	2535	2543	rBV7	9814	19512	0.97%	0.136%
55	18.157	2561	2562	2567	rVB4	4354	2723	0.14%	0.019%
56	18.198	2568	2569	2574	rBV5	2631	3340	0.17%	0.023%
57	18.304	2584	2587	2590	rBV3	6548	7112	0.35%	0.050%
58	18.380	2596	2600	2603	rVB5	2695	4181	0.21%	0.029%
59	18.633	2641	2643	2646	rBV3	2331	2594	0.13%	0.018%
60	18.775	2666	2667	2670	rBV3	4138	2576	0.13%	0.018%
61	18.875	2683	2684	2687	rBV3	2642	3087	0.15%	0.022%
62	18.939	2691	2695	2702	rBV7	8669	17164	0.85%	0.120%
63	19.163	2729	2733	2737	rVB	16849	22567	1.12%	0.157%
64	19.286	2751	2754	2757	rBV5	4918	5097	0.25%	0.036%
65	19.498	2784	2790	2794	rBV	370834	532502	26.40%	3.714%
66	19.904	2857	2859	2862	rBV4	3562	5090	0.25%	0.035%
67	20.063	2883	2886	2889	rBV2	8187	9803	0.49%	0.068%
68	20.516	2960	2963	2968	rVB2	21601	22484	1.11%	0.157%
69	20.563	2969	2971	2973	rVV2	5832	3941	0.20%	0.027%
70	21.027	3048	3050	3059	rVB6	20328	31395	1.56%	0.219%
71	21.227	3080	3084	3088	rVB	53392	58311	2.89%	0.407%
72	21.298	3090	3096	3108	rBV	1544586	1988463	98.59%	13.867%
73	21.904	3196	3199	3203	rBV	45540	49780	2.47%	0.347%
74	22.163	3240	3243	3249	rBV4	29743	39745	1.97%	0.277%
75	22.374	3276	3279	3282	rVB	29305	34265	1.70%	0.239%
76	22.886	3362	3366	3375	rVB2	80101	128370	6.36%	0.895%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062821\
 Data File : BN015172.D
 Acq On : 28 Jun 2021 12:57
 Operator : CG/JU
 Sample : M2761-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 J LX83

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
 Title : SVOA CALIBRATION

77	23.404	3448	3454	3459	rBV2	243233	459457	22.78%	3.204%
78	23.457	3459	3463	3470	rVB2	91367	158168	7.84%	1.103%
79	23.545	3471	3478	3493	rVB2	997393	2016937	100.00%	14.066%
80	24.110	3569	3574	3581	rVB2	77963	153247	7.60%	1.069%
81	24.857	3696	3701	3713	rVB3	70745	160062	7.94%	1.116%




Sum of corrected areas: 14339029

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062821\
Data File : BN015172.D
Acq On : 28 Jun 2021 12:57
Operator : CG/JU
Sample : M2761-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLX83

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

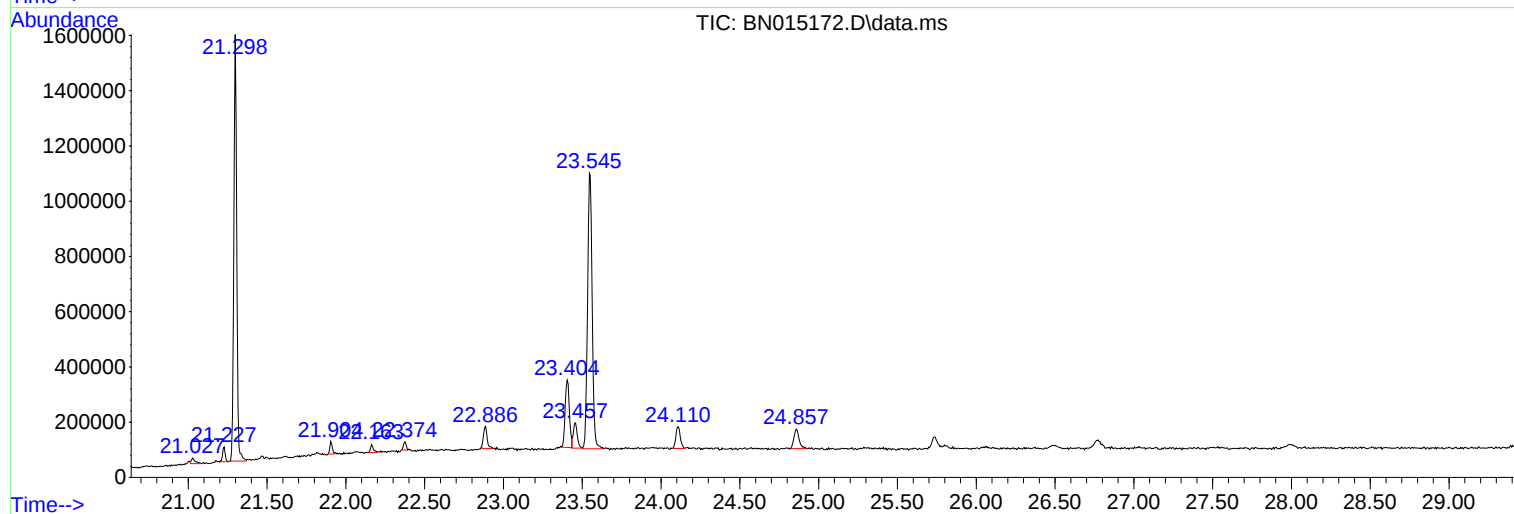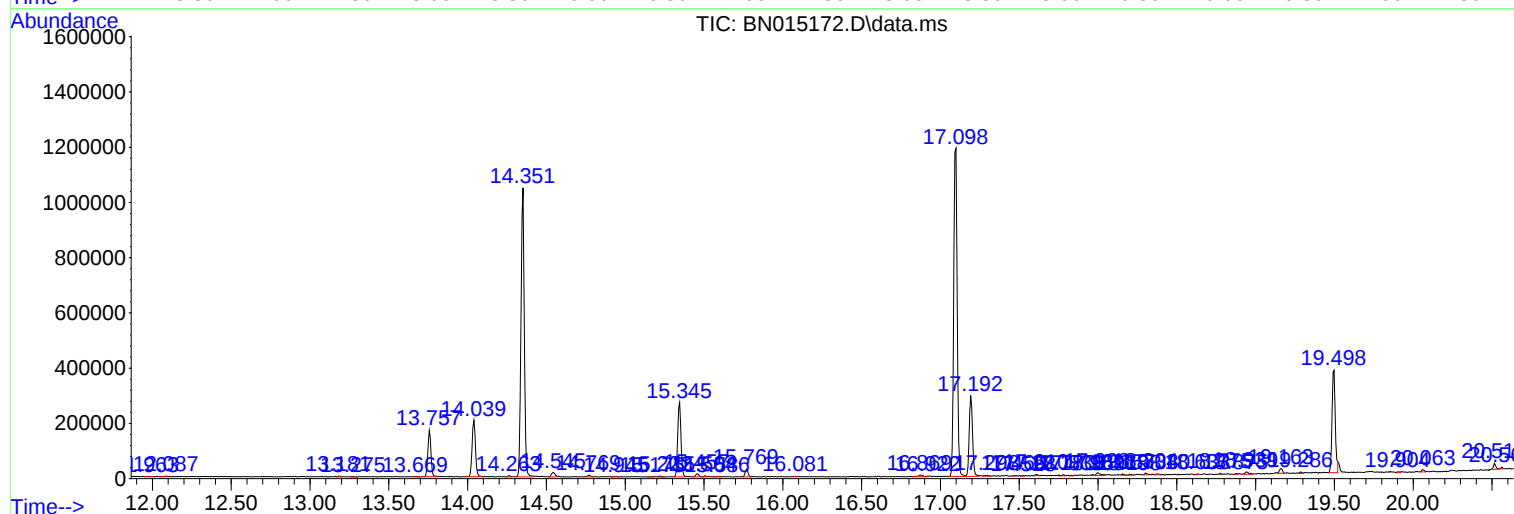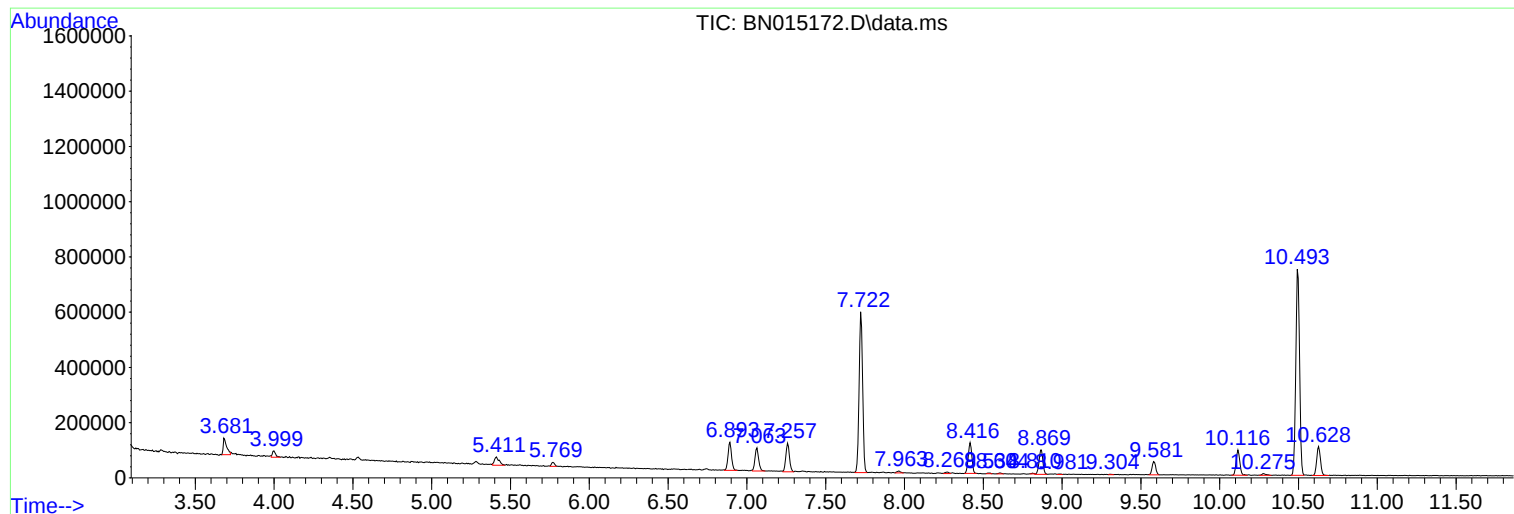

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062821\
Data File : BN015172.D
Acq On : 28 Jun 2021 12:57
Operator : CG/JU
Sample : M2761-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLX83

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062821\
Data File : BN015172.D
Acq On : 28 Jun 2021 12:57
Operator : CG/JU
Sample : M2761-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLX83

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-BN061821MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
