

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062822\
 Data File : BN020563.D
 Acq On : 29 Jun 2022 10:35
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Jun 29 13:57:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 02:03:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.739	152	3803	0.400	ng	0.00
7) Naphthalene-d8	10.520	136	11470	0.400	ng	# 0.00
13) Acenaphthene-d10	14.367	164	6578	0.400	ng	0.00
19) Phenanthrene-d10	17.103	188	13748	0.400	ng	#-0.01
29) Chrysene-d12	21.306	240	11106	0.400	ng	# 0.00
35) Perylene-d12	23.583	264	8580	0.400	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.341	112	3566	0.338	ng	0.00
5) Phenol-d6	6.937	99	4385	0.348	ng	0.00
8) Nitrobenzene-d5	8.886	82	3188	0.343	ng	-0.01
11) 2-Methylnaphthalene-d10	12.114	152	7277	0.370	ng	0.00
14) 2,4,6-Tribromophenol	15.862	330	799	0.322	ng	0.00
15) 2-Fluorobiphenyl	12.988	172	10568	0.389	ng	-0.01
27) Fluoranthene-d10	19.143	212	14962	0.366	ng	0.00
31) Terphenyl-d14	19.746	244	10578	0.399	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.225	88	1806	0.362	ng	96
3) n-Nitrosodimethylamine	3.564	42	1478	0.325	ng	98
6) bis(2-Chloroethyl)ether	7.168	93	3859	0.356	ng	100
9) Naphthalene	10.562	128	13164	0.384	ng	99
10) Hexachlorobutadiene	10.861	225	2341	0.375	ng	# 100
12) 2-Methylnaphthalene	12.189	142	8590	0.377	ng	99
16) Acenaphthylene	14.078	152	11644	0.368	ng	99
17) Acenaphthene	14.420	154	8284	0.385	ng	96
18) Fluorene	15.415	166	10567	0.376	ng	100
20) 4,6-Dinitro-2-methylph...	15.522	198	437	0.387	ng	# 64
21) 4-Bromophenyl-phenylether	16.303	248	2966	0.371	ng	100
22) Hexachlorobenzene	16.426	284	3415	0.386	ng	100
23) Atrazine	16.579	200	1977	0.314	ng	98
24) Pentachlorophenol	16.774	266	727	0.440	ng	95
25) Phenanthrene	17.144	178	17296	0.373	ng	100
26) Anthracene	17.246	178	14159	0.354	ng	100
28) Fluoranthene	19.173	202	18887	0.373	ng	100
30) Pyrene	19.535	202	19084	0.406	ng	100
32) Benzo(a)anthracene	21.288	228	14196	0.358	ng	99
33) Chrysene	21.342	228	17241	0.392	ng	99
34) Bis(2-ethylhexyl)phtha...	21.225	149	6964	0.312	ng	99
36) Indeno(1,2,3-cd)pyrene	25.919	276	13070	0.342	ng	98
37) Benzo(b)fluoranthene	22.896	252	13433	0.406	ng	98
38) Benzo(k)fluoranthene	22.940	252	13736	0.390	ng	97
39) Benzo(a)pyrene	23.486	252	10940	0.382	ng	95
40) Dibenzo(a,h)anthracene	25.928	278	10379	0.339	ng	98
41) Benzo(g,h,i)perylene	26.624	276	11524	0.344	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062822\
 Data File : BN020563.D
 Acq On : 29 Jun 2022 10:35
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Quant Time: Jun 29 13:57:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 27 02:03:21 2022
 Response via : Initial Calibration







#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.739 min Scan# 64
Delta R.T. -0.000 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC





Tgt Ion:152 Resp: 3803
Ion Ratio Lower Upper
152 100
150 154.7 127.9 191.9
115 63.6 51.4 77.2



#2
1,4-Dioxane
Concen: 0.362 ng
RT: 3.225 min Scan# 20
Delta R.T. -0.007 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35



Tgt Ion: 88 Resp: 1806
Ion Ratio Lower Upper
88 100
43 33.9 30.2 45.2
58 88.6 73.0 109.6








#3
n-Nitrosodimethylamine
Concen: 0.325 ng
RT: 3.564 min Scan# 61
Delta R.T. 0.007 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion: 42 Resp: 1478
Ion Ratio Lower Upper
42 100
74 107.0 84.0 126.0
44 12.5 9.8 14.8



#4
2-Fluorophenol
Concen: 0.338 ng
RT: 5.341 min Scan# 313
Delta R.T. -0.007 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35

Tgt Ion: 112 Resp: 3566
Ion Ratio Lower Upper
112 100
64 62.4 49.1 73.7
63 32.9 26.3 39.5








#5
Phenol-d6
Concen: 0.348 ng
RT: 6.937 min Scan# 51
Delta R.T. -0.007 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion: 99 Resp: 4385
Ion Ratio Lower Upper
99 100
42 21.2 19.3 28.9
71 35.1 27.5 41.3



#6
bis(2-Chloroethyl)ether
Concen: 0.356 ng
RT: 7.168 min Scan# 566
Delta R.T. 0.000 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35

Tgt Ion: 93 Resp: 3859
Ion Ratio Lower Upper
93 100
63 84.3 67.4 101.0
95 33.9 26.5 39.7








#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.520 min Scan# 91
Delta R.T. 0.000 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	136	Resp:	11470
Ion Ratio	Lower	Upper	
136	100		
137	11.8	9.0	13.6
54	9.5	6.2	9.2#
68	6.4	4.4	6.6



#8
Nitrobenzene-d5
Concen: 0.343 ng
RT: 8.886 min Scan# 778
Delta R.T. -0.011 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35

Tgt Ion:	82	Resp:	3188
Ion Ratio	Lower	Upper	
82	100		
128	38.3	35.0	52.6
54	63.4	46.2	69.4









#9
Naphthalene
Concen: 0.384 ng
RT: 10.562 min Scan# 91
Delta R.T. -0.011 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:128 Resp: 13164
Ion Ratio Lower Upper
128 100
129 11.7 8.9 13.3
127 13.5 10.8 16.2



#10
Hexachlorobutadiene
Concen: 0.375 ng
RT: 10.861 min Scan# 963
Delta R.T. -0.011 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35

Tgt Ion:225 Resp: 2341
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.5 50.9 76.3








#11
2-Methylnaphthalene-d10
Concen: 0.370 ng
RT: 12.114 min Scan# 1183
Delta R.T. -0.007 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:152 Resp: 7277
Ion Ratio Lower Upper
152 100
151 20.6 16.2 24.4



#12
2-Methylnaphthalene
Concen: 0.377 ng
RT: 12.189 min Scan# 1203
Delta R.T. -0.004 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35

Tgt Ion:142 Resp: 8590
Ion Ratio Lower Upper
142 100
141 88.9 71.6 107.4
115 38.6 29.8 44.8





#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.367 min Scan# 1461

Delta R.T. 0.000 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:164 Resp: 6578

Ion Ratio Lower Upper

164 100

162 103.8 82.1 123.1

160 46.4 38.6 58.0

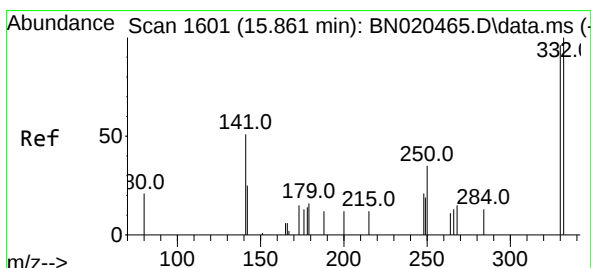

#14

2,4,6-Tribromophenol

Concen: 0.322 ng

RT: 15.862 min Scan# 1601

Delta R.T. 0.000 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35




Tgt Ion:330 Resp: 799

Ion Ratio Lower Upper

330 100

332 153.1 77.6 116.4#

141 54.2 41.0 61.4








#15
2-Fluorobiphenyl
Concen: 0.389 ng
RT: 12.988 min Scan# 11
Delta R.T. -0.011 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:	172	Resp:	10568
Ion Ratio	Lower	Upper	
172	100		
171	35.9	27.2	40.8
170	24.6	18.2	27.4



#16
Acenaphthylene
Concen: 0.368 ng
RT: 14.078 min Scan# 1434
Delta R.T. -0.011 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35

Tgt Ion:	152	Resp:	11644
Ion Ratio	Lower	Upper	
152	100		
151	19.5	16.2	24.4
153	13.0	10.7	16.1








#17
Acenaphthene
Concen: 0.385 ng
RT: 14.420 min Scan# 1466
Delta R.T. -0.011 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:154 Resp: 8284
Ion Ratio Lower Upper
154 100
153 113.9 87.5 131.3
152 56.5 43.8 65.6



#18
Fluorene
Concen: 0.376 ng
RT: 15.415 min Scan# 1559
Delta R.T. 0.000 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35

Tgt Ion:166 Resp: 10567
Ion Ratio Lower Upper
166 100
165 98.6 78.6 118.0
167 13.6 10.8 16.2









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.103 min Scan# 1722
Delta R.T. -0.010 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:188 Resp: 13748
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 14.4 7.4 11.2#

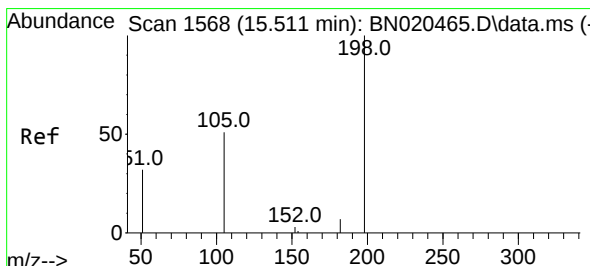

#20
4,6-Dinitro-2-methylphenol
Concen: 0.387 ng
RT: 15.522 min Scan# 1569
Delta R.T. 0.011 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35

Tgt Ion:198 Resp: 437
Ion Ratio Lower Upper
198 100
182 30.3 12.1 18.1#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.371 ng
RT: 16.303 min Scan# 1644
Delta R.T. -0.010 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:248 Resp: 2966
Ion Ratio Lower Upper
248 100
250 94.5 75.3 112.9
141 83.7 67.3 100.9

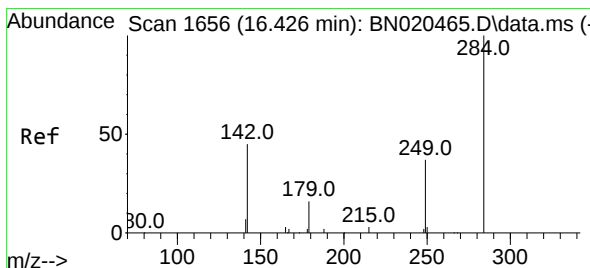

#22
Hexachlorobenzene
Concen: 0.386 ng
RT: 16.426 min Scan# 1656
Delta R.T. 0.000 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35

Tgt Ion:284 Resp: 3415
Ion Ratio Lower Upper
284 100
142 44.1 35.2 52.8
249 33.2 26.6 40.0





#23

Atrazine

Concen: 0.314 ng

RT: 16.579 min Scan# 1671

Delta R.T. 0.000 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:200 Resp: 1977

Ion Ratio Lower Upper

200 100

173 28.0 23.6 35.4

215 46.9 36.6 54.8



#24

Pentachlorophenol

Concen: 0.440 ng

RT: 16.774 min Scan# 1690

Delta R.T. -0.010 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35




Tgt Ion:266 Resp: 727


Ion Ratio Lower Upper

266 100

264 62.2 51.3 76.9

268 60.2 52.6 79.0



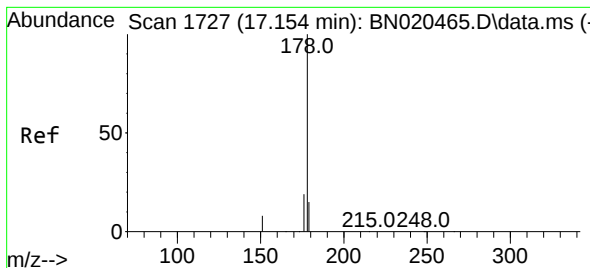

#25

Phenanthrene

Concen: 0.373 ng

RT: 17.144 min Scan# 1726

Delta R.T. -0.010 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:178 Resp: 17296

Ion Ratio Lower Upper

178 100

176 19.4 15.3 22.9

179 15.3 12.2 18.4

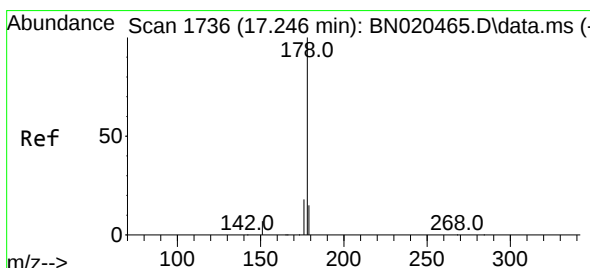

#26

Anthracene

Concen: 0.354 ng

RT: 17.246 min Scan# 1736

Delta R.T. 0.000 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35




Tgt Ion:178 Resp: 14159

Ion Ratio Lower Upper

178 100

176 18.5 14.9 22.3

179 15.0 12.2 18.4








#27
Fluoranthene-d10
Concen: 0.366 ng
RT: 19.143 min Scan# 2080
Delta R.T. -0.004 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 14962
Ion Ratio Lower Upper
212 100
106 15.3 12.6 19.0
104 8.7 7.2 10.8



#28
Fluoranthene
Concen: 0.373 ng
RT: 19.173 min Scan# 2087
Delta R.T. -0.008 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35

Tgt Ion:202 Resp: 18887
Ion Ratio Lower Upper
202 100
101 12.3 9.6 14.4
203 16.9 13.5 20.3



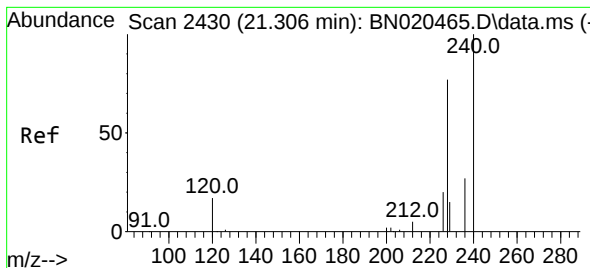

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.306 min Scan# 2430

Delta R.T. 0.000 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:240 Resp: 11106

Ion Ratio Lower Upper

240 100

120 10.0 14.6 21.8#

236 26.7 22.6 33.8

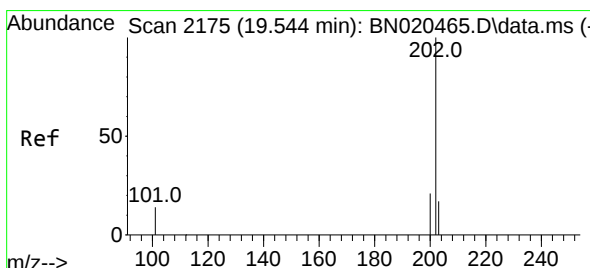

#30

Pyrene

Concen: 0.406 ng

RT: 19.535 min Scan# 2173

Delta R.T. -0.008 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35




Tgt Ion:202 Resp: 19084

Ion Ratio Lower Upper

202 100

200 20.9 16.6 25.0

203 17.7 14.2 21.2








#31
 Terphenyl-d14
 Concen: 0.399 ng
 RT: 19.746 min Scan# 21
 Delta R.T. -0.008 min
 Lab File: BN020563.D
 Acq: 29 Jun 2022 10:35




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:244 Resp: 10578
 Ion Ratio Lower Upper
 244 100
 212 9.1 7.1 10.7
 122 0.0 0.0 0.0



#32
 Benzo(a)anthracene
 Concen: 0.358 ng
 RT: 21.288 min Scan# 2428
 Delta R.T. -0.009 min
 Lab File: BN020563.D
 Acq: 29 Jun 2022 10:35

Tgt Ion:228 Resp: 14196
 Ion Ratio Lower Upper
 228 100
 226 26.9 21.2 31.8
 229 19.8 15.6 23.4





#33

Chrysene

Concen: 0.392 ng

RT: 21.342 min Scan# 2434

Delta R.T. 0.000 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC




Tgt Ion:228 Resp: 17241

Ion Ratio Lower Upper

228 100

226 29.5 23.4 35.0

229 20.6 15.7 23.5



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.312 ng

RT: 21.225 min Scan# 2421

Delta R.T. -0.009 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35




Tgt Ion:149 Resp: 6964

Ion Ratio Lower Upper

149 100

167 26.3 21.7 32.5

279 3.1 2.2 3.2








#35
Perylene-d12
Concen: 0.400 ng
RT: 23.583 min Scan# 2961
Delta R.T. -0.017 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:264 Resp: 8580
Ion Ratio Lower Upper
264 100
260 27.0 20.9 31.3
265 36.2 28.0 42.0



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.342 ng
RT: 25.919 min Scan# 3754
Delta R.T. -0.017 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35

Tgt Ion:276 Resp: 13070
Ion Ratio Lower Upper
276 100
138 30.7 25.9 38.9
277 24.3 19.8 29.8





#37

Benzo(b)fluoranthene

Concen: 0.406 ng

RT: 22.896 min Scan# 21

Delta R.T. -0.012 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC





Tgt Ion:252 Resp: 13433

Ion Ratio Lower Upper

252 100

253 23.9 18.5 27.7

125 15.3 11.4 17.0

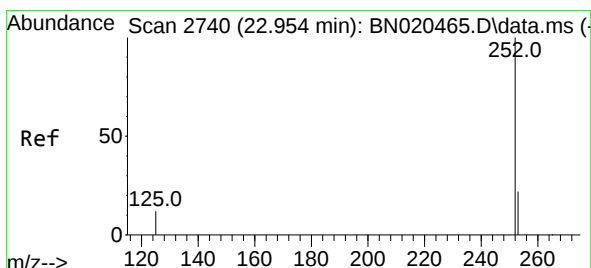

#38

Benzo(k)fluoranthene

Concen: 0.390 ng

RT: 22.940 min Scan# 2735

Delta R.T. -0.015 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35




Tgt Ion:252 Resp: 13736

Ion Ratio Lower Upper

252 100

253 24.4 18.0 27.0

125 14.1 11.0 16.4





#39

Benzo(a)pyrene

Concen: 0.382 ng

RT: 23.486 min Scan# 2922

Delta R.T. -0.012 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC




Tgt Ion:252 Resp: 10940

Ion Ratio Lower Upper

252 100

253 25.7 19.0 28.4

125 20.2 13.8 20.8



#40

Dibenzo(a,h)anthracene

Concen: 0.339 ng

RT: 25.928 min Scan# 3757

Delta R.T. -0.020 min

Lab File: BN020563.D

Acq: 29 Jun 2022 10:35




Tgt Ion:278 Resp: 10379

Ion Ratio Lower Upper

278 100

139 23.3 18.6 28.0


279 26.8 19.7 29.5





#41
Benzo(g,h,i)perylene
Concen: 0.344 ng
RT: 26.624 min Scan# 3995
Delta R.T. -0.029 min
Lab File: BN020563.D
Acq: 29 Jun 2022 10:35

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC



Tgt Ion:276 Resp: 11524
Ion Ratio Lower Upper
276 100
277 24.7 19.5 29.3
138 28.7 22.6 34.0

