
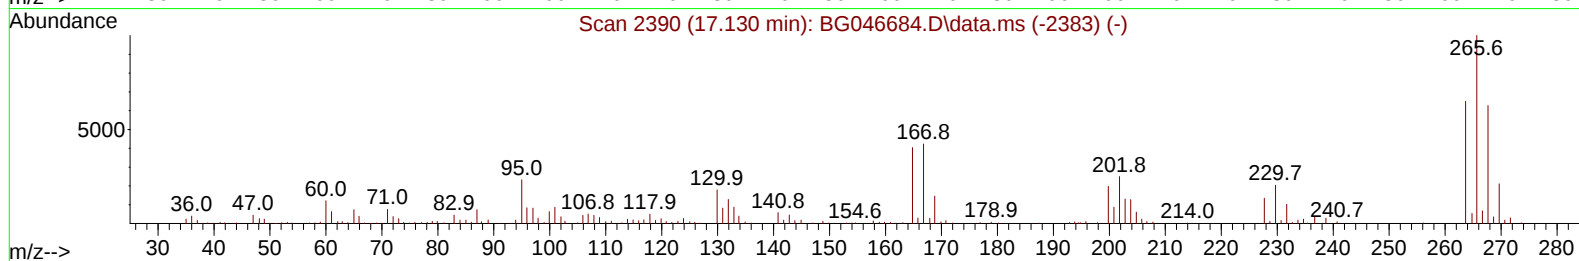
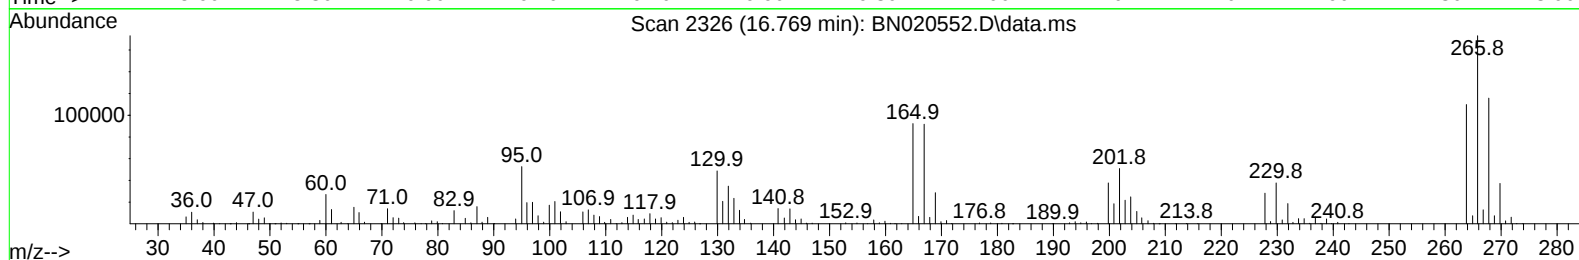


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062822\
Data File : BN020552.D
Acq On : 29 Jun 2022 04:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 07:26:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 07:25:57 2022
Response via : Initial Calibration

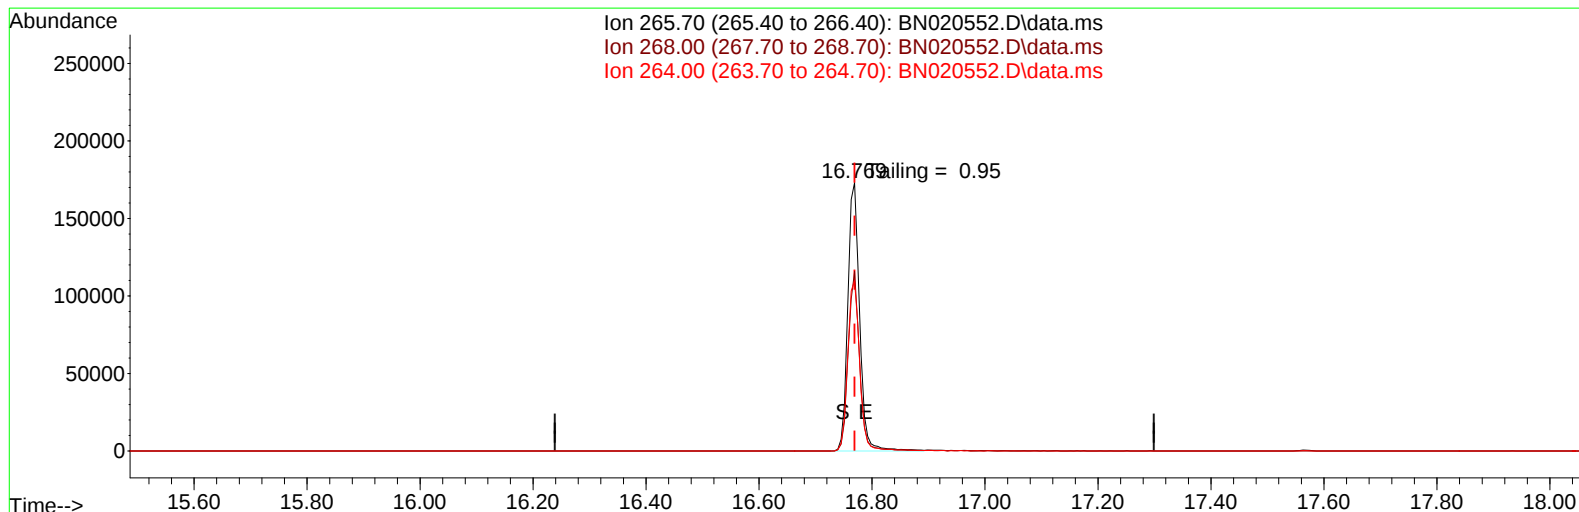

TIC: BN020552.D\data.ms

(70) Pentachlorophenol (C)




16.769min (0.000) 18092.85 ng

response 251603

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.83
264.00	61.60	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062822\
Data File : BN020552.D
Acq On : 29 Jun 2022 04:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 07:26:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 07:25:57 2022
Response via : Initial Calibration

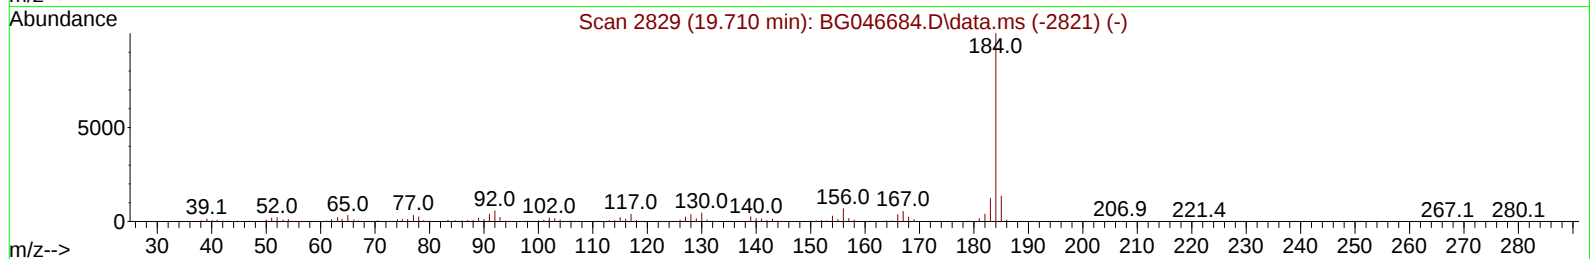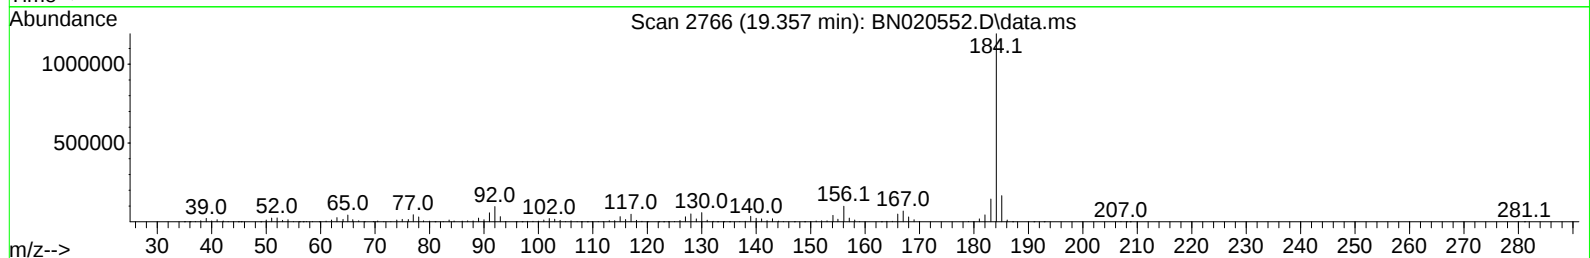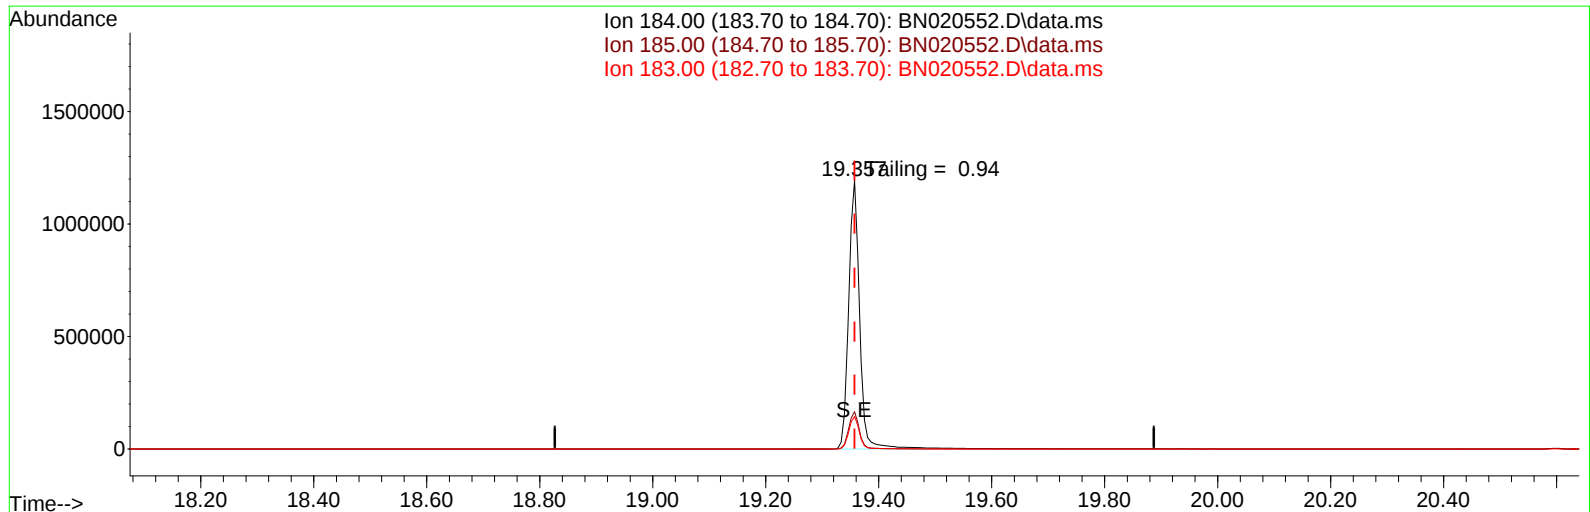

TIC: BN020552.D\data.ms

(77) Benzidine

19.357min (0.000) 0.00 ng

response 1621569

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.91
183.00	13.20	12.12
0.00	0.00	0.00