


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062822\
 Data File : BN020533.D
 Acq On : 28 Jun 2022 14:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 02:03:21 2022

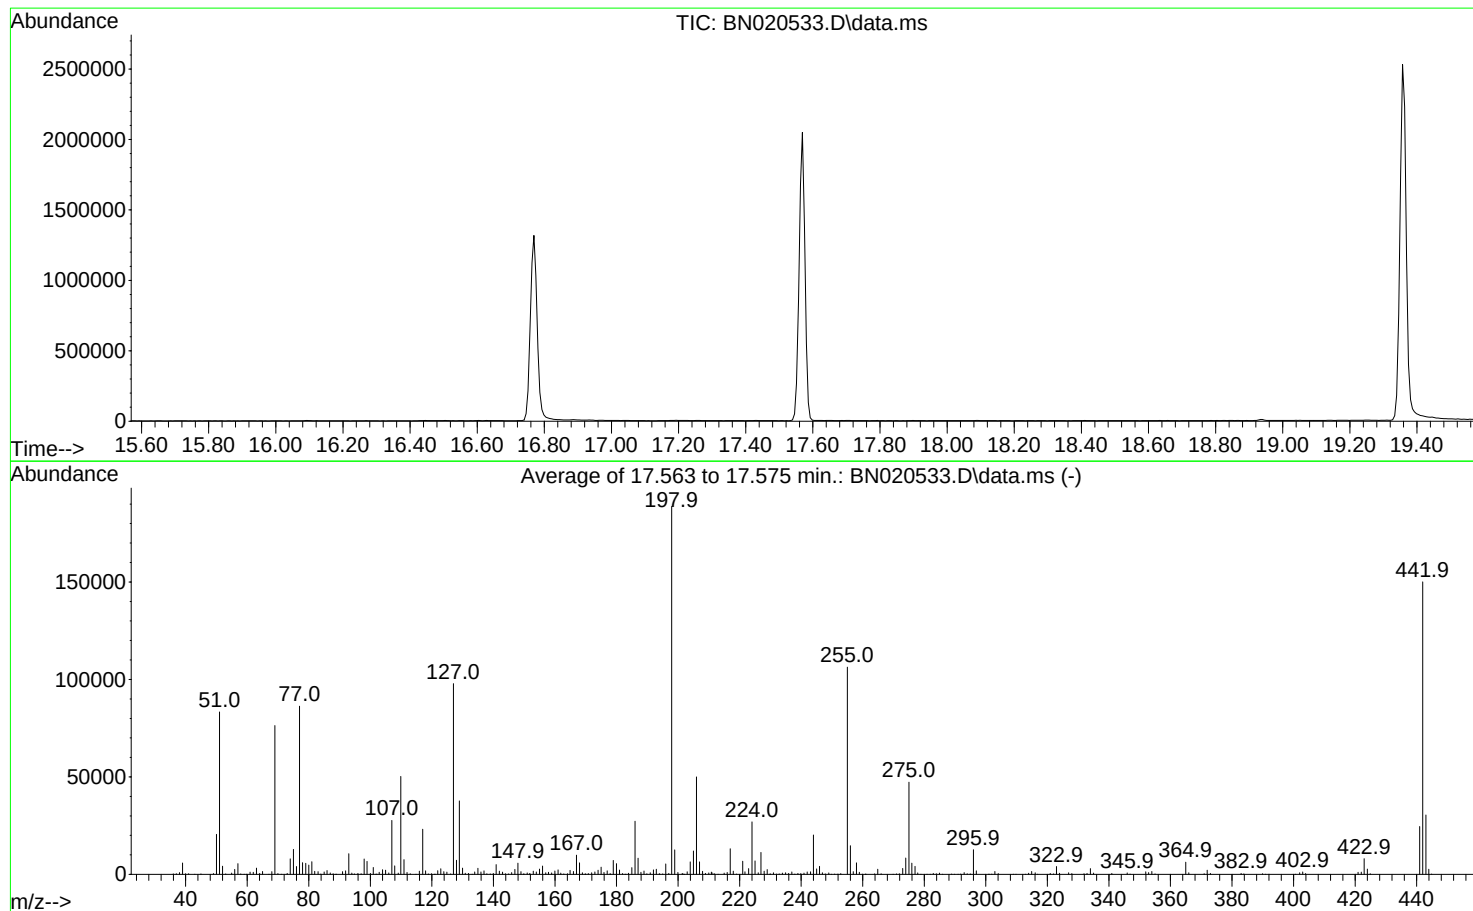




AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.1	83307	PASS
68	69	0.00	2	1.8	1387	PASS
69	198	0.00	100	40.5	76376	PASS
70	69	0.00	2	0.6	454	PASS
127	198	10	80	51.9	97893	PASS
197	198	0.00	2	0.2	460	PASS
198	198	100	100	100.0	188736	PASS
199	198	5	9	6.6	12531	PASS
275	198	10	60	25.1	47320	PASS
365	198	1	100	3.3	6278	PASS
441	198	0.01	100	13.0	24533	PASS
442	442	50	100	100.0	150035	PASS
443	442	15	24	20.3	30485	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062822\
Data File : BN020533.D
Acq On : 28 Jun 2022 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 29 03:30:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 03:29:56 2022
Response via : Initial Calibration

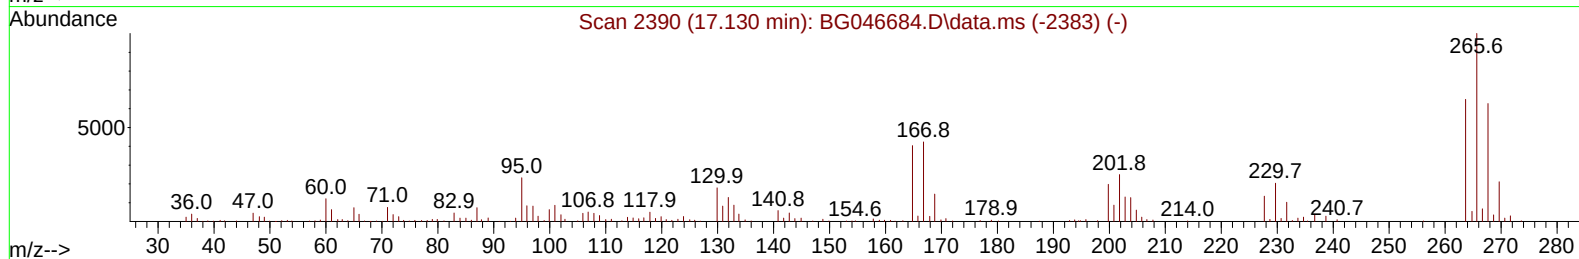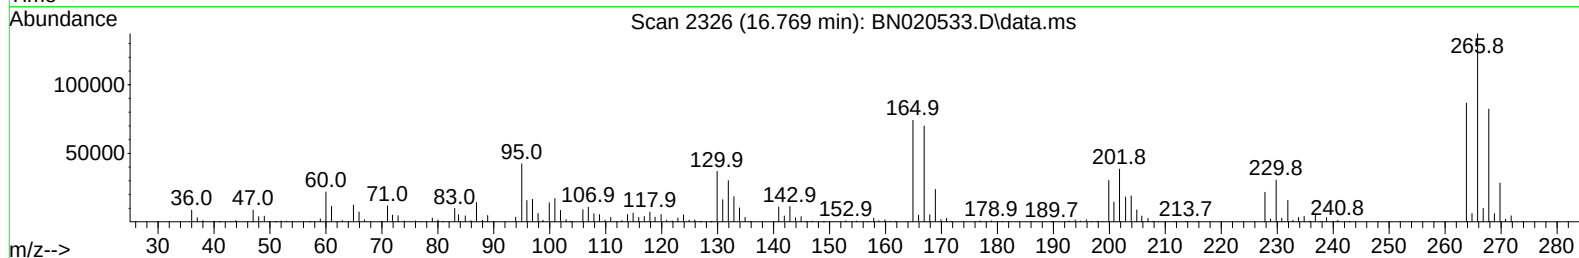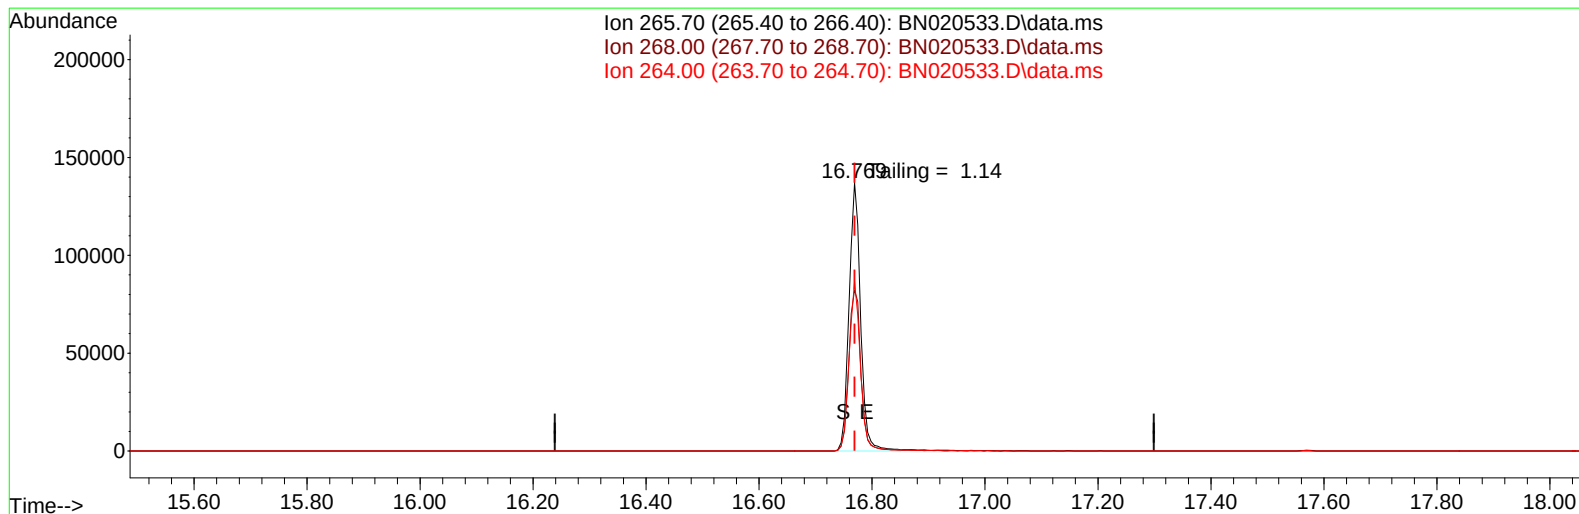

TIC: BN020533.D\data.ms

(70) Pentachlorophenol (C)

16.769min (0.000) 16537.12 ng




response 194539

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.97
264.00	61.60	63.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062822\
Data File : BN020533.D
Acq On : 28 Jun 2022 14:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 29 03:30:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 03:29:56 2022
Response via : Initial Calibration

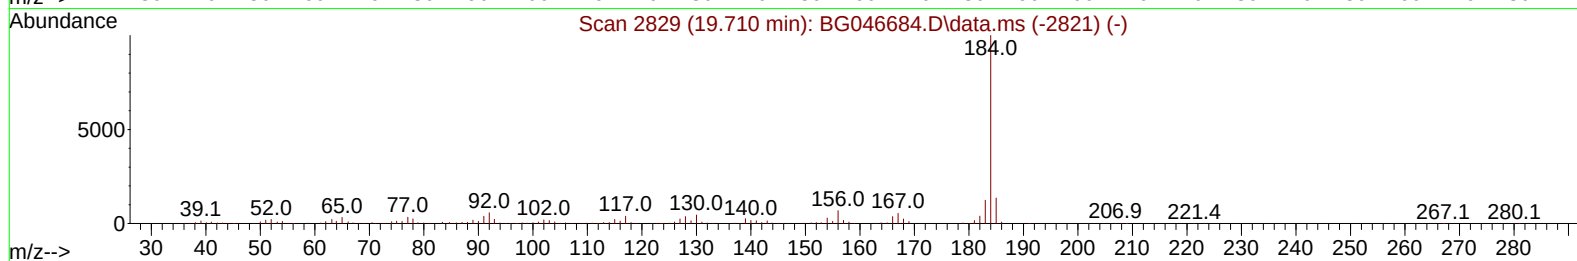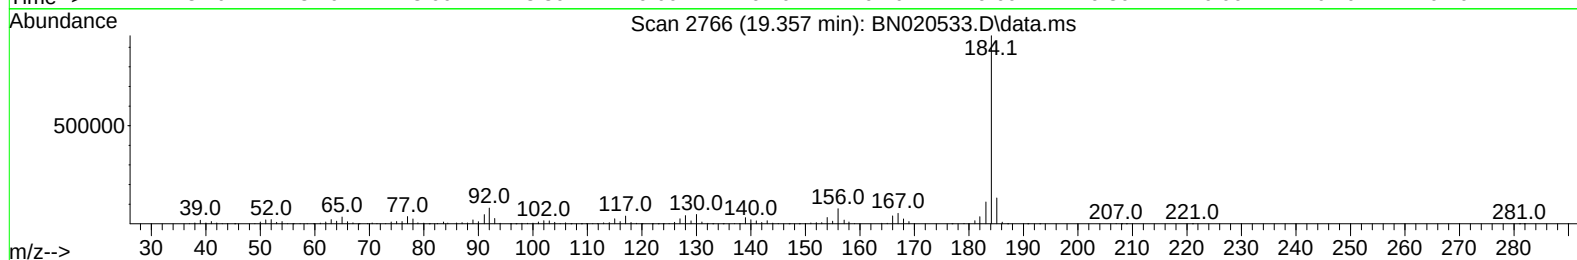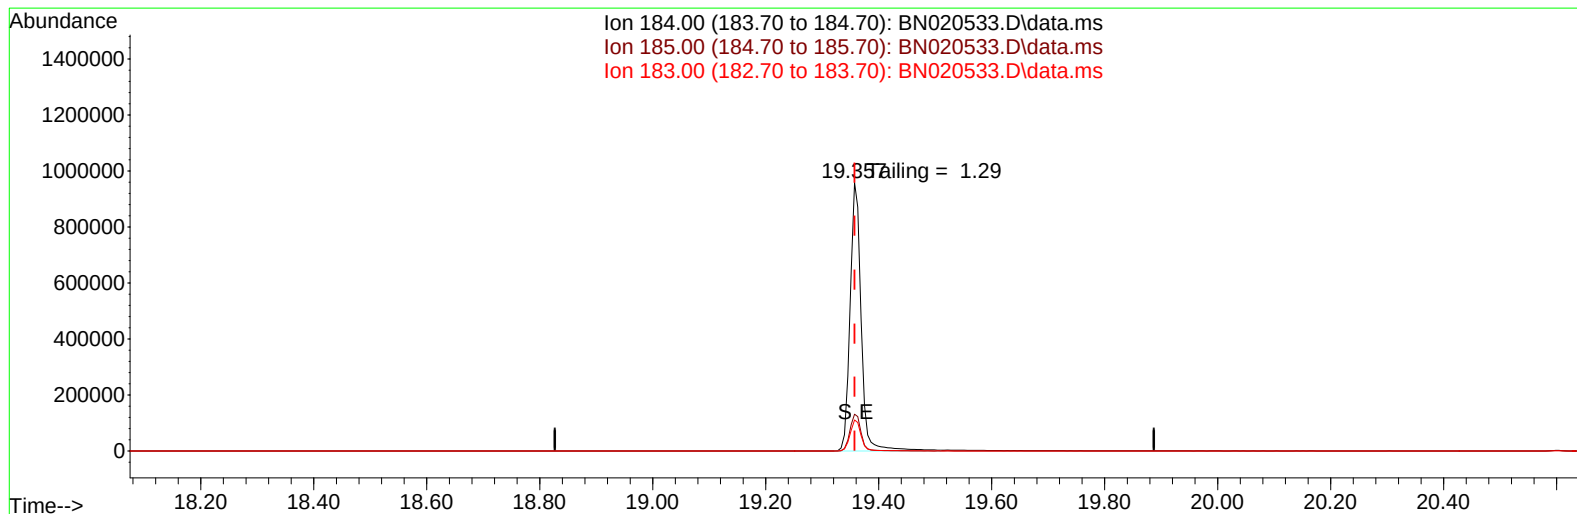

TIC: BN020533.D\data.ms

(77) Benzidine

19.357min (0.000) 0.00 ng

response 1309488

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.74
183.00	13.20	11.59
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/28/2022	BNA_N	<u>BN020533.D</u>
Compound Name	Response	Retention Time
DDT	609321	20.604
DDD	27743	20.163
DDE	1608	19.651
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29351	638672	4.60

Instrument :
BNA_N
ClientSampleId :
DFTPP