
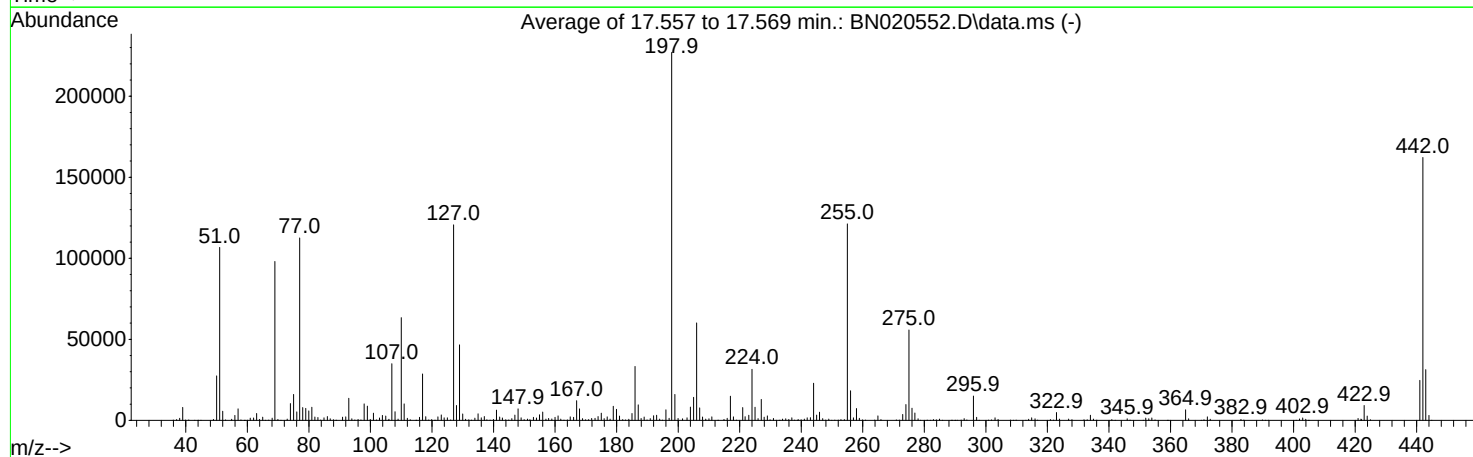


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062822\
 Data File : BN020552.D
 Acq On : 29 Jun 2022 04:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 02:03:21 2022

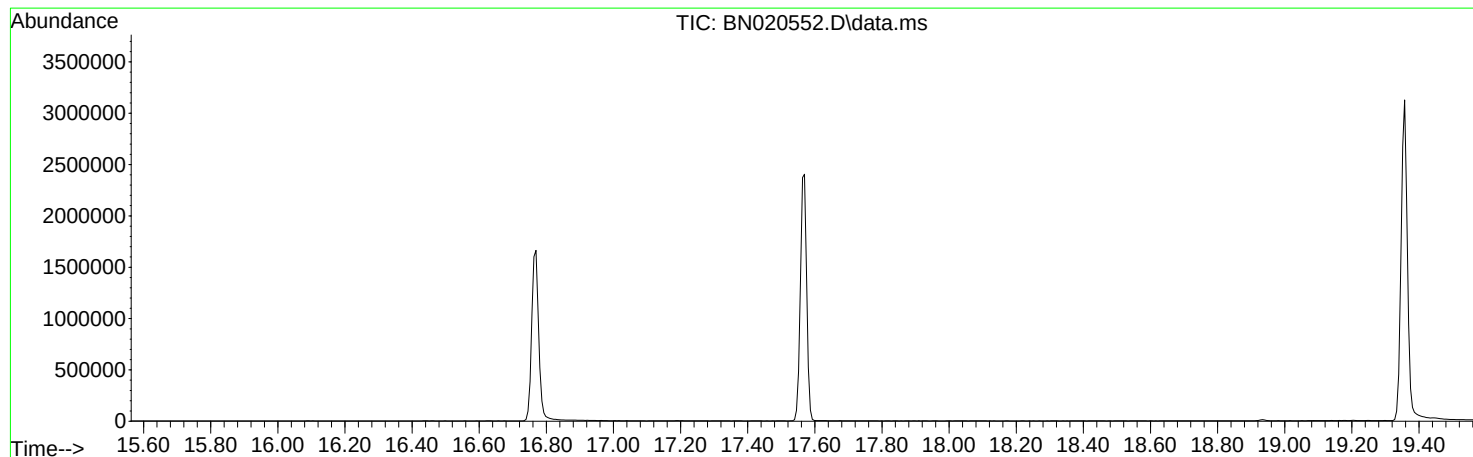




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	106693	PASS
68	69	0.00	2	1.4	1339	PASS
69	198	0.00	100	43.2	98085	PASS
70	69	0.00	2	0.6	559	PASS
127	198	10	80	53.1	120608	PASS
197	198	0.00	2	0.6	1312	PASS
198	198	100	100	100.0	226987	PASS
199	198	5	9	7.0	15973	PASS
275	198	10	60	24.6	55808	PASS
365	198	1	100	2.9	6507	PASS
441	198	0.01	100	10.9	24688	PASS
442	442	50	100	100.0	162261	PASS
443	442	15	24	19.3	31350	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062822\
 Data File : BN020552.D
 Acq On : 29 Jun 2022 04:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jun 29 07:26:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 07:25:57 2022
 Response via : Initial Calibration

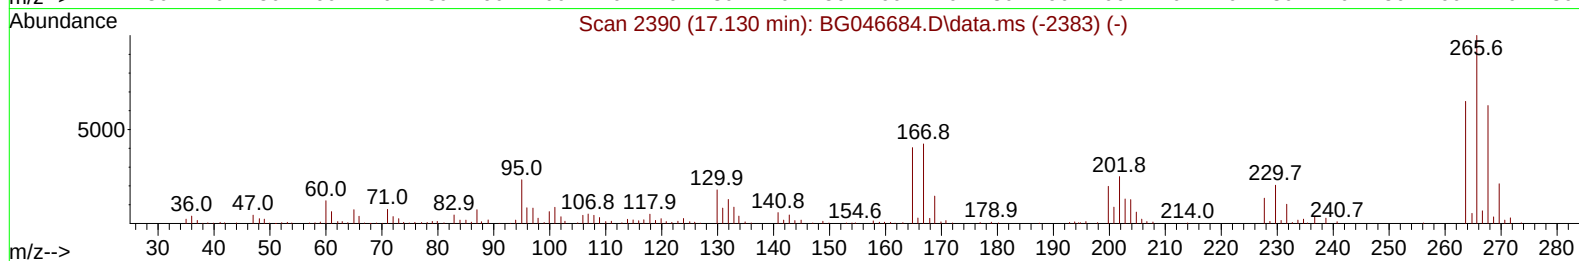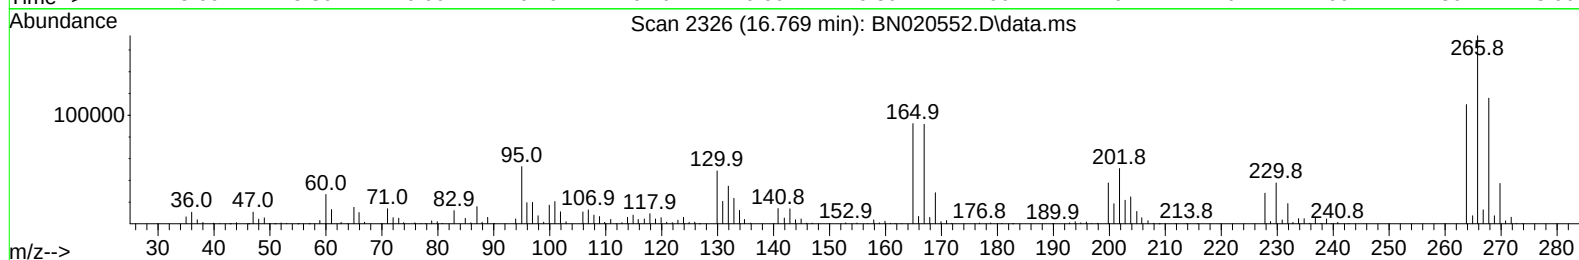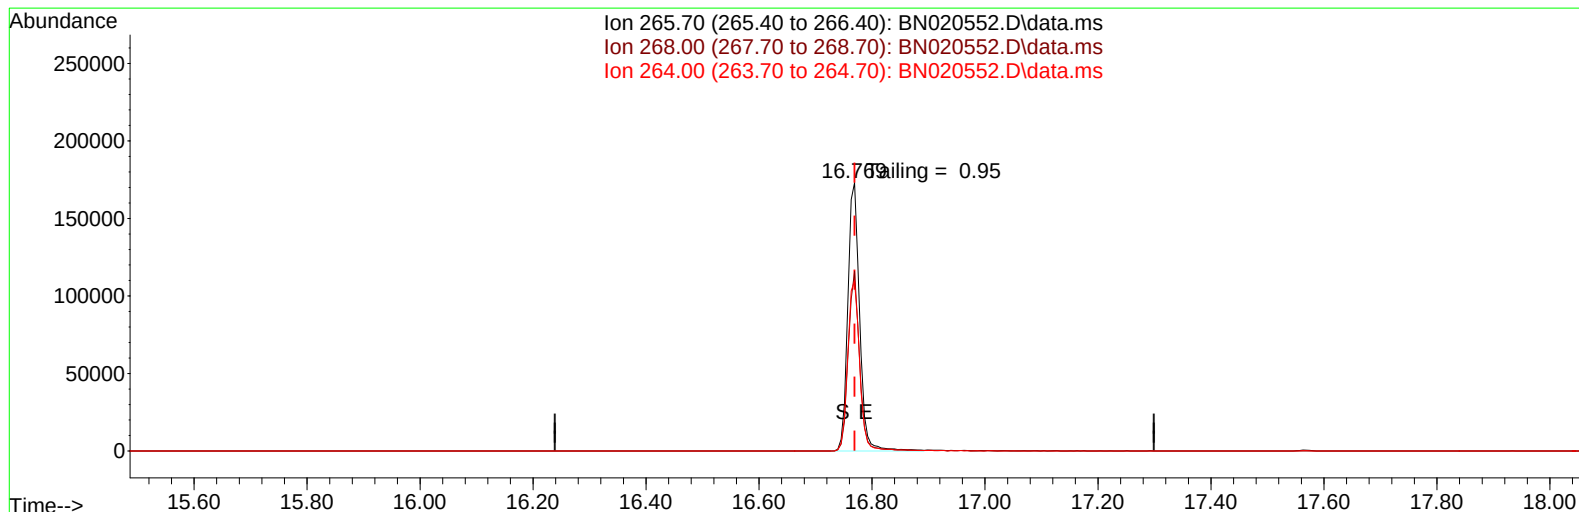

TIC: BN020552.D\data.ms

(70) Pentachlorophenol (C)

16.769min (0.000) 18092.85 ng




response 251603

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.83
264.00	61.60	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062822\
Data File : BN020552.D
Acq On : 29 Jun 2022 04:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 29 07:26:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 07:25:57 2022
Response via : Initial Calibration

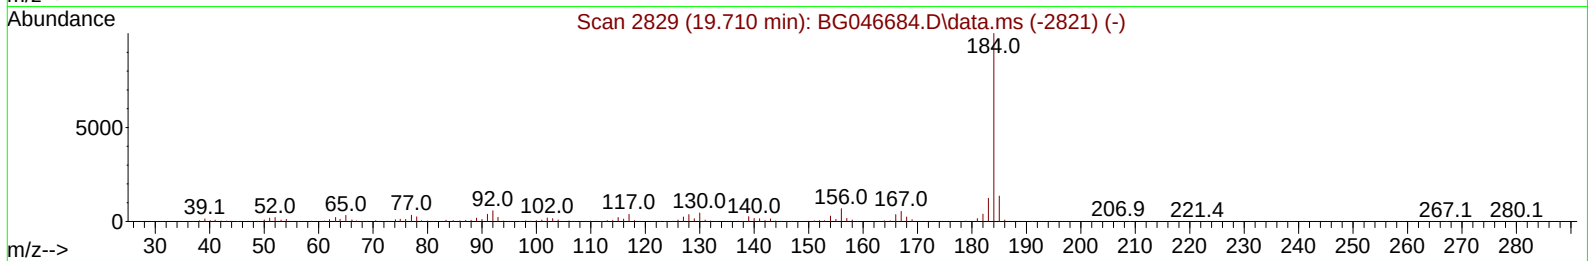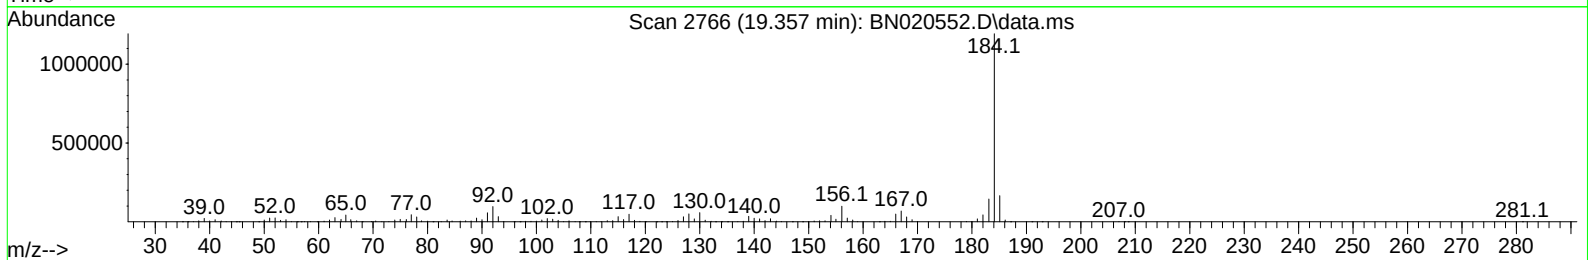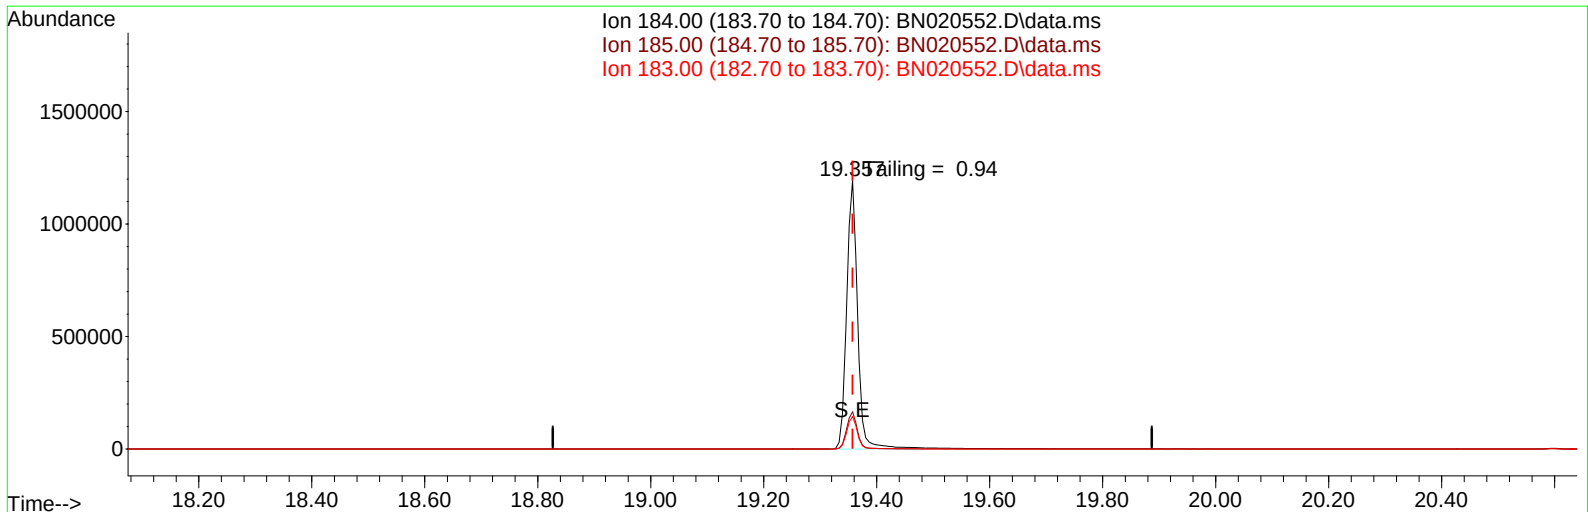

TIC: BN020552.D\data.ms

(77) Benzidine

19.357min (0.000) 0.00 ng

response 1621569

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.91
183.00	13.20	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/28/2022	BNA_N	<u>BN020552.D</u>
Compound Name	Response	Retention Time
DDT	794217	20.598
DDD	27047	20.157
DDE	1228	19.651
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28275	822492	3.44

Instrument :
BNA_N
ClientSampleId :
DFTPP