

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062921\
 Data File : BN015200.D
 Acq On : 29 Jun 2021 23:57
 Operator : CG/JU
 Sample : M2783-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE134D1-20210617

Quant Time: Jun 30 02:27:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 29 19:13:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.741	152	17012	0.40	ng	# 0.00
7) Naphthalene-d8	10.505	136	75167	0.40	ng	# 0.00
13) Acenaphthene-d10	14.346	164	34349	0.40	ng	# 0.00
19) Phenanthrene-d10	17.091	188	69783	0.40	ng	0.00
29) Chrysene-d12	21.292	240	69119	0.40	ng	#-0.01
35) Perylene-d12	23.540	264	57081	0.40	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.371	112	4485	0.12	ng	0.03
5) Phenol-d6	6.911	99	4001	0.07	ng	0.00
8) Nitrobenzene-d5	8.870	82	26244	0.38	ng	0.00
11) 2-Methylnaphthalene-d10	12.088	152	40538	0.33	ng	0.00
14) 2,4,6-Tribromophenol	15.843	330	2833	0.37	ng	0.00
15) 2-Fluorobiphenyl	12.963	172	62607	0.43	ng	-0.01
27) Fluoranthene-d10	19.133	212	82882	0.39	ng	0.00
31) Terphenyl-d14	19.734	244	83084	0.54	ng	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.361	88	6088	1.23	ng	# 77
20) 4,6-Dinitro-2-methylph...	15.487	198	4	0.19	ng	# 8
23) Atrazine	16.580	200	37	0.17	ng	# 1
24) Pentachlorophenol	16.750	266	174	0.27	ng	91
34) Bis(2-ethylhexyl)phtha...	21.217	149	7131	0.31	ng	# 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062921\
Data File : BN015200.D
Acq On : 29 Jun 2021 23:57
Operator : CG/JU
Sample : M2783-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE134D1-20210617

Quant Time: Jun 30 02:27:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 29 19:13:09 2021
Response via : Initial Calibration




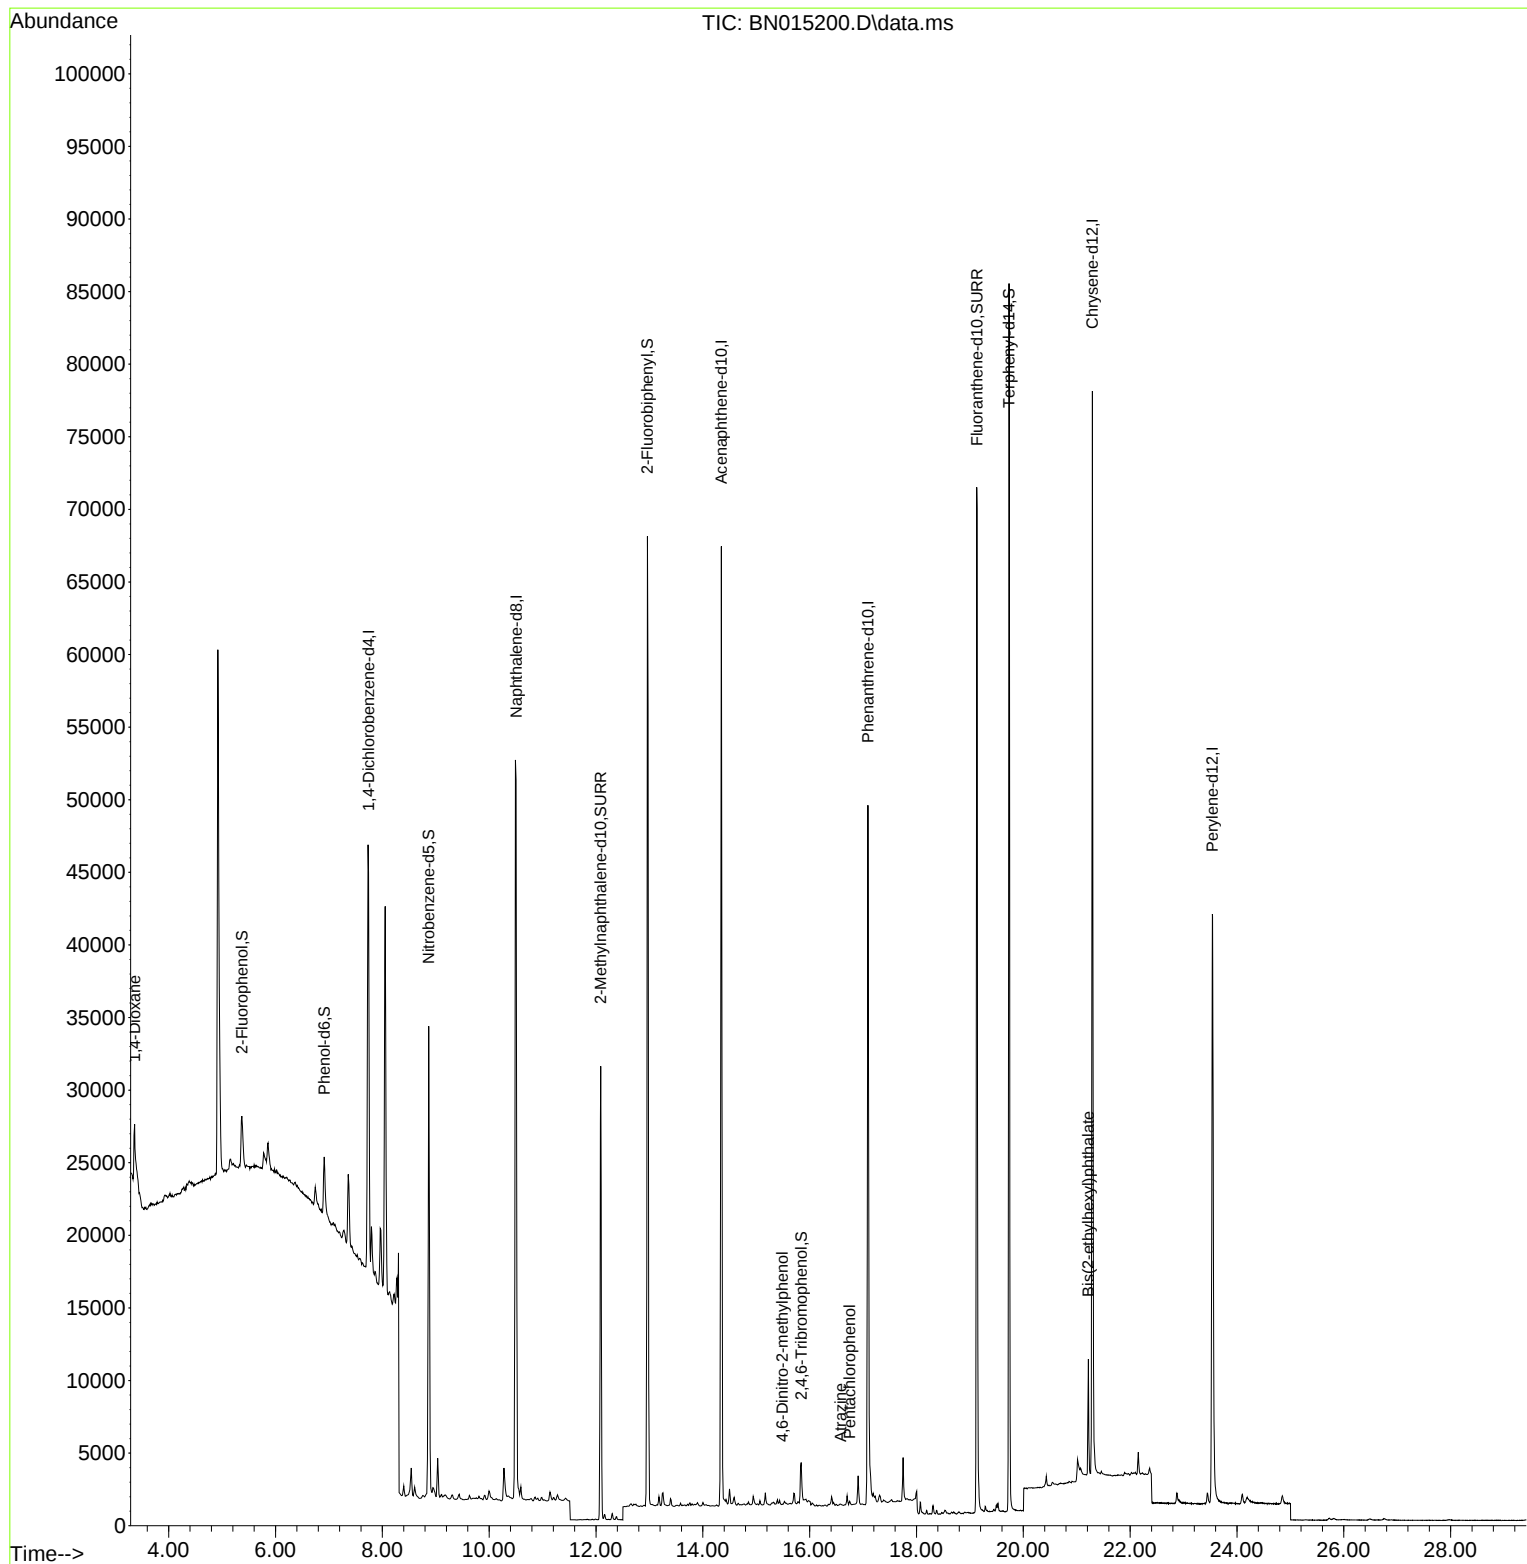


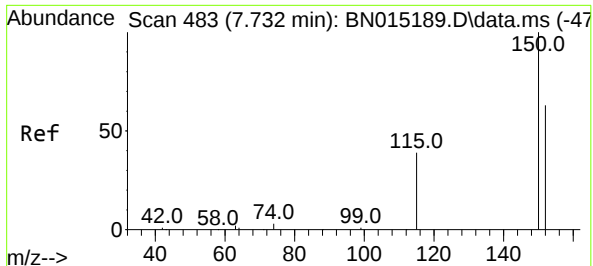

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.741 min Scan# 484
 Delta R.T. 0.009 min
 Lab File: BN015200.D
 Acq: 29 Jun 2021 23:57




Instrument :
 BNA_N
 ClientSampleId :
 RE134D1-20210617


Tgt Ion: 152 Resp: 17012
 Ion Ratio Lower Upper
 152 100
 150 152.1 119.0 178.6
 115 57.7 62.2 93.4#

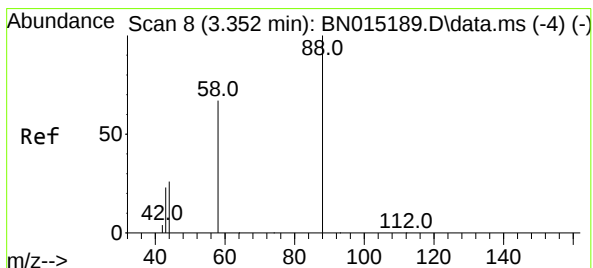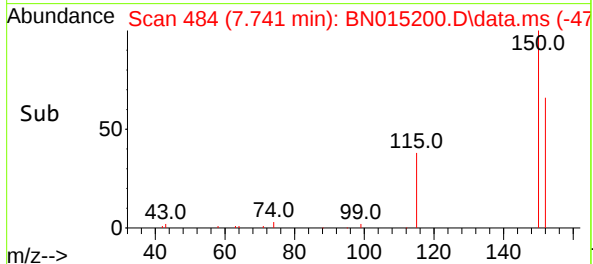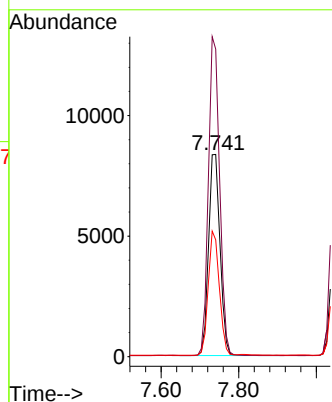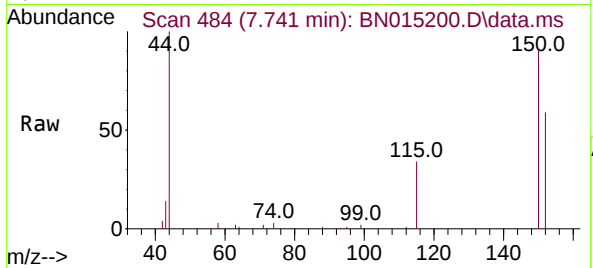

#2
 1,4-Dioxane
 Concen: 1.23 ng
 RT: 3.361 min Scan# 9
 Delta R.T. 0.009 min
 Lab File: BN015200.D
 Acq: 29 Jun 2021 23:57

Tgt Ion: 88 Resp: 6088
 Ion Ratio Lower Upper
 88 100
 43 19.5 12.9 19.3#
 58 66.7 38.1 57.1#


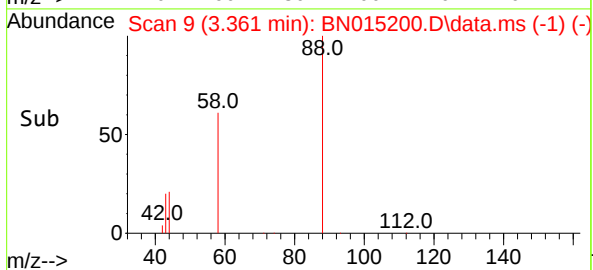

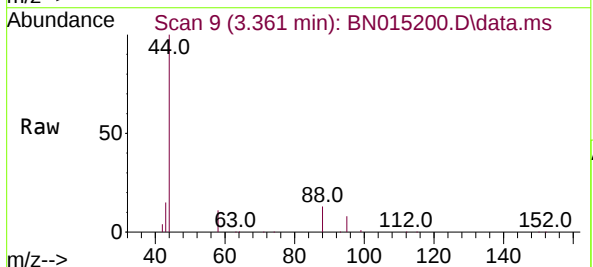


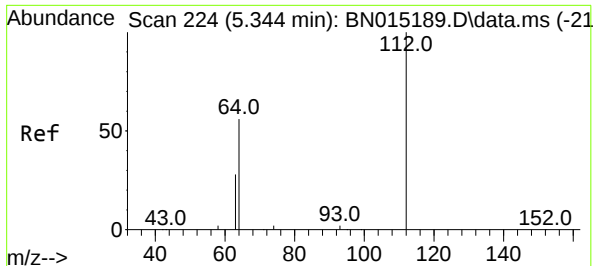

#4
2-Fluorophenol
Concen: 0.12 ng
RT: 5.371 min Scan# 227
Delta R.T. 0.027 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57




Instrument :
BNA_N
ClientSampleId :
RE134D1-20210617


Tgt Ion:112 Resp: 4485
Ion Ratio Lower Upper
112 100
64 57.8 39.0 58.6
63 31.1 20.6 30.8#

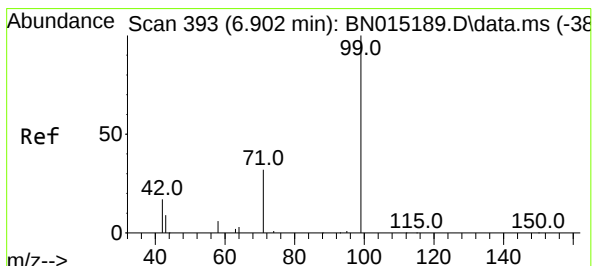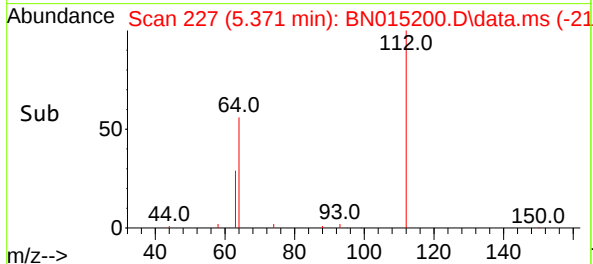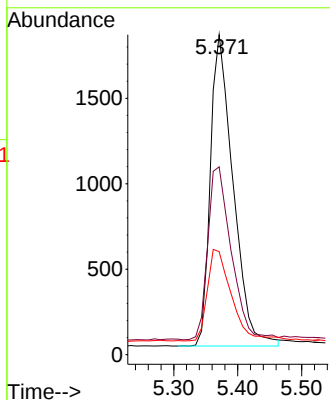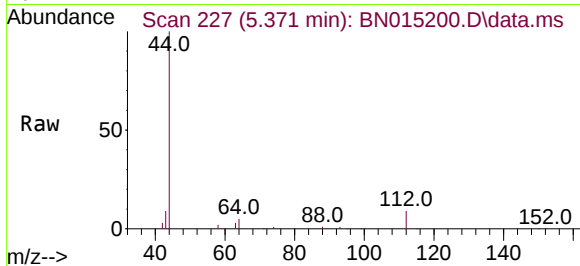

#5
Phenol-d6
Concen: 0.07 ng
RT: 6.911 min Scan# 394
Delta R.T. 0.009 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57


Tgt Ion: 99 Resp: 4001
Ion Ratio Lower Upper
99 100
42 19.3 8.9 13.3#
71 36.2 35.6 53.4

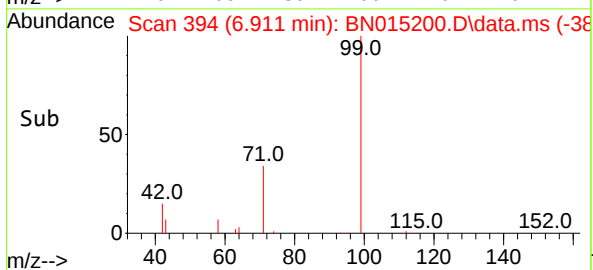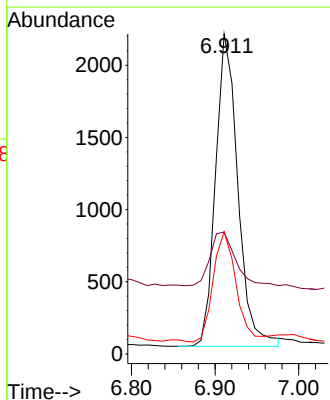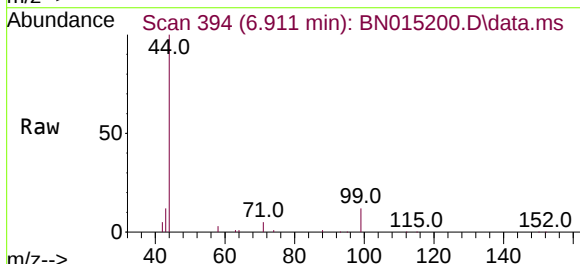






#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.505 min Scan# 719
Delta R.T. -0.000 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57

Instrument :
BNA_N
ClientSampleId :
RE134D1-20210617



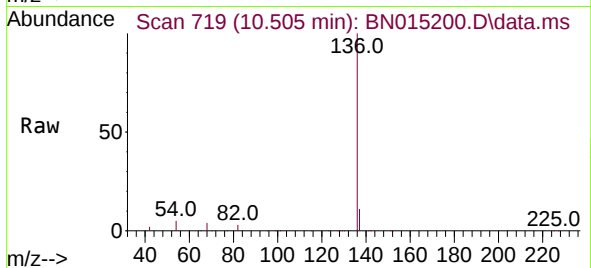



Tgt Ion:	136	Resp:	75167
Ion Ratio	Lower	Upper	
136	100		
137	11.0	9.8	14.8
54	5.3	5.4	8.2#
68	4.3	4.9	7.3#



#8
Nitrobenzene-d5
Concen: 0.38 ng
RT: 8.870 min Scan# 590
Delta R.T. -0.000 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57

Tgt Ion:	82	Resp:	26244
Ion Ratio	Lower	Upper	
82	100		
128	34.7	31.6	47.4
54	52.6	29.0	43.4#


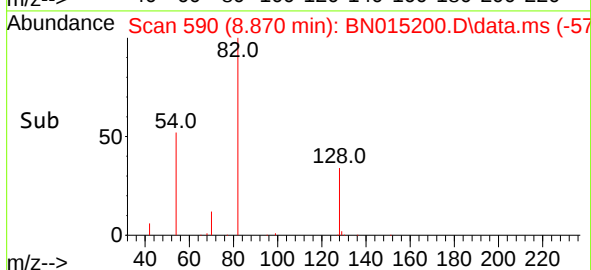




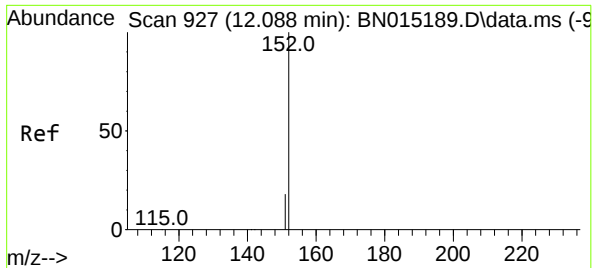

#11
2-Methylnaphthalene-d10
Concen: 0.33 ng
RT: 12.088 min Scan# 927
Delta R.T. -0.000 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57




Instrument :
BNA_N
ClientSampleId :
RE134D1-20210617


Tgt Ion:152 Resp: 40538
Ion Ratio Lower Upper
152 100
151 20.5 16.7 25.1

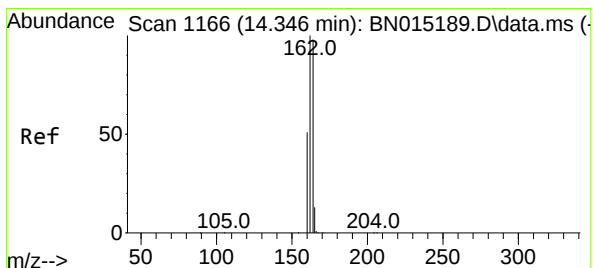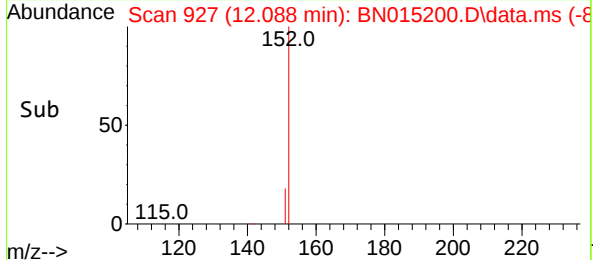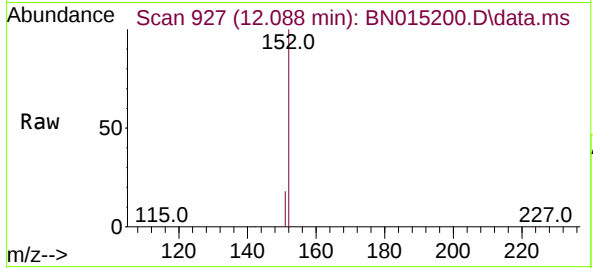

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.346 min Scan# 1166
Delta R.T. -0.000 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57

Tgt Ion:164 Resp: 34349
Ion Ratio Lower Upper
164 100
162 102.4 83.8 125.6
160 56.4 37.4 56.0#


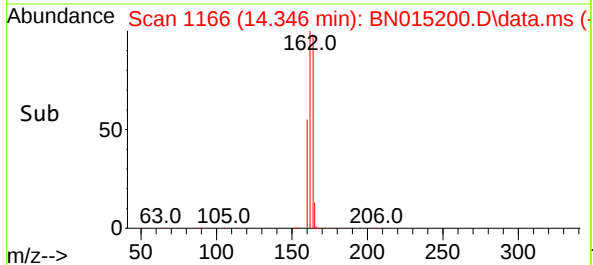

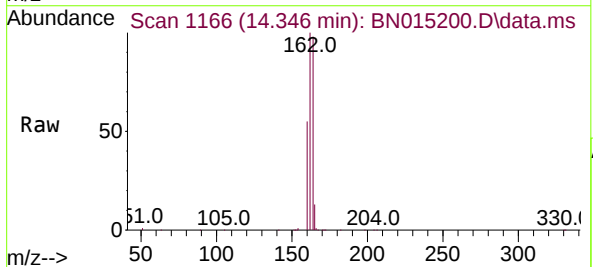




#14
2,4,6-Tribromophenol
Concen: 0.37 ng
RT: 15.843 min Scan# 1284
Delta R.T. -0.000 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57




Instrument :
BNA_N
ClientSampleId :
RE134D1-20210617


Tgt Ion: 330 Resp: 2833
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 39.9 22.4 33.6#

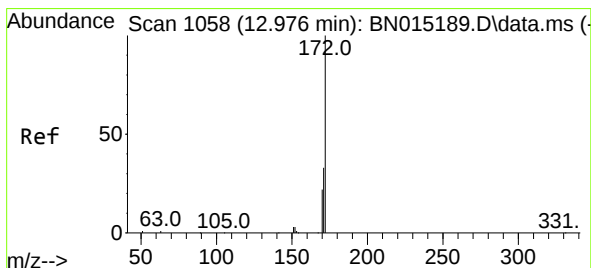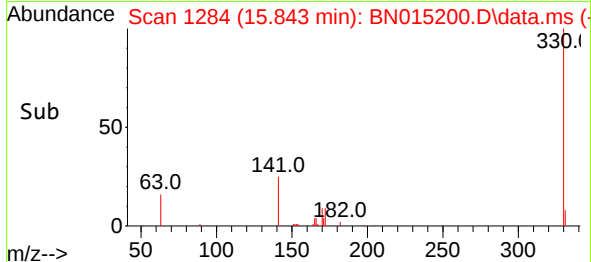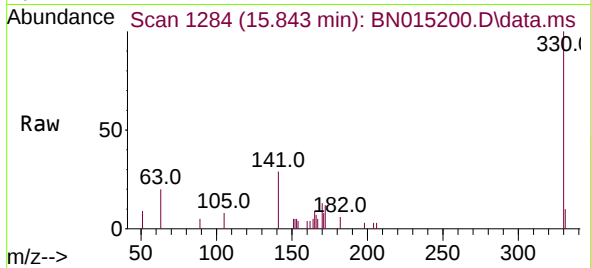

#15
2-Fluorobiphenyl
Concen: 0.43 ng
RT: 12.963 min Scan# 1057
Delta R.T. -0.013 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57

Tgt Ion: 172 Resp: 62607
Ion Ratio Lower Upper
172 100
171 35.6 30.6 45.8
170 24.9 20.2 30.4


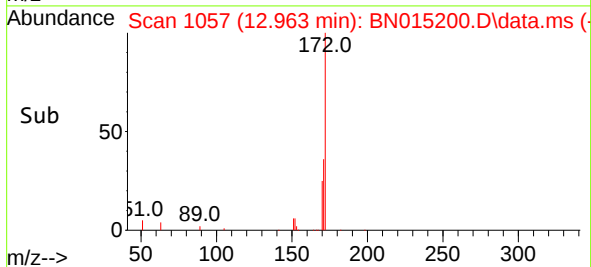

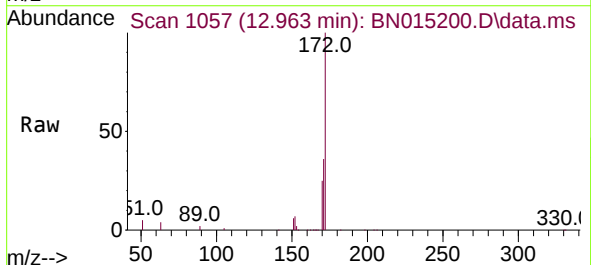




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.091 min Scan# 1386
Delta R.T. -0.001 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57




Instrument :
BNA_N
ClientSampleId :
RE134D1-20210617


Tgt Ion:188 Resp: 69783
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.4 9.0 13.4

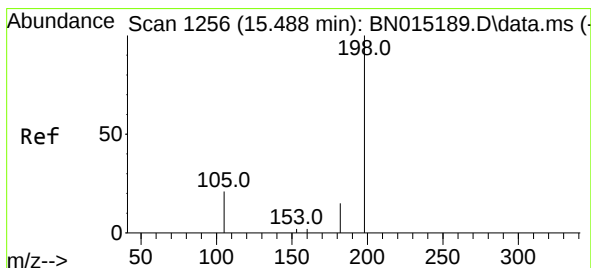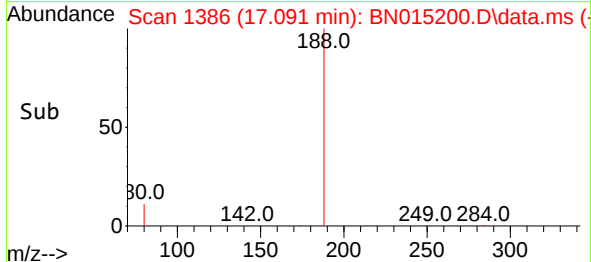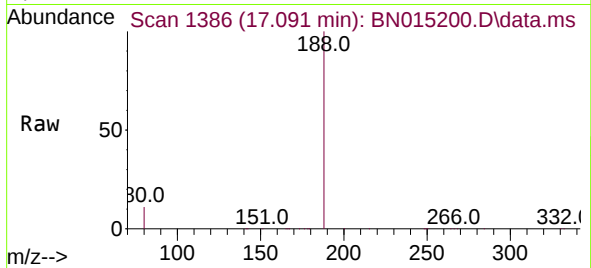

#20
4,6-Dinitro-2-methylphenol
Concen: 0.19 ng
RT: 15.487 min Scan# 1256
Delta R.T. -0.001 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57

Tgt Ion:198 Resp: 4
Ion Ratio Lower Upper
198 100
182 102.0 34.5 51.7#
77 0.0 0.0 0.0


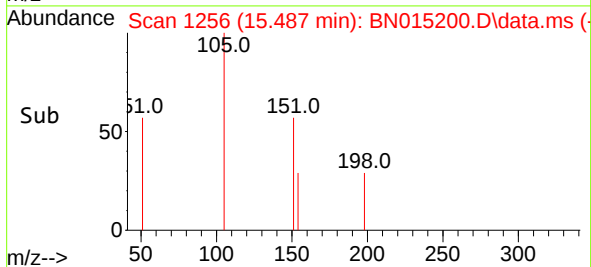

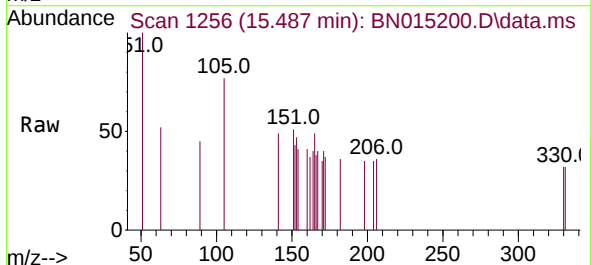




#23
Atrazine
Concen: 0.17 ng
RT: 16.580 min Scan# 1344
Delta R.T. 0.024 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57




Instrument :
BNA_N
ClientSampleId :
RE134D1-20210617


Tgt Ion:200 Resp: 37
Ion Ratio Lower Upper
200 100
173 131.1 21.7 32.5#
215 111.5 43.1 64.7#

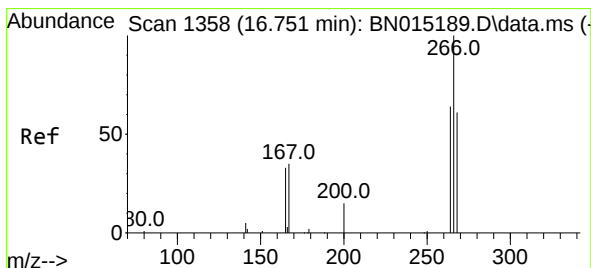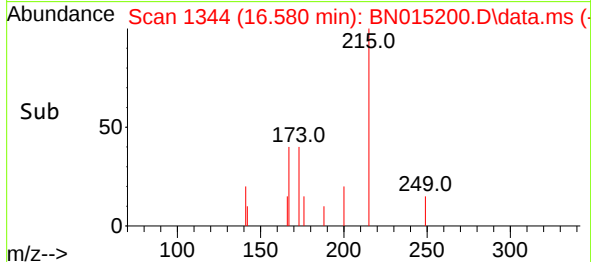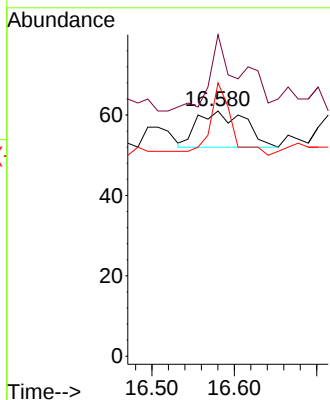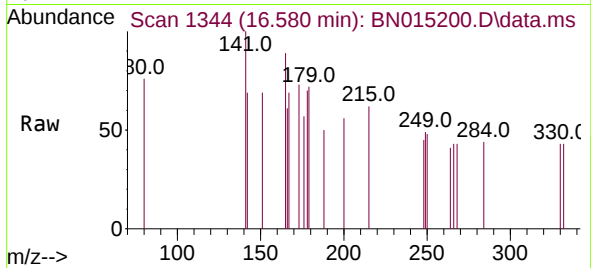

#24
Pentachlorophenol
Concen: 0.27 ng
RT: 16.750 min Scan# 1358
Delta R.T. -0.001 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57

Tgt Ion:266 Resp: 174
Ion Ratio Lower Upper
266 100
264 55.2 51.0 76.4
268 58.0 50.6 76.0


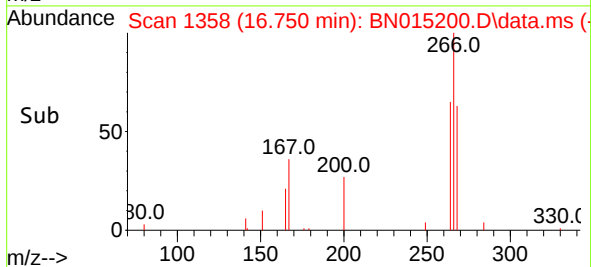
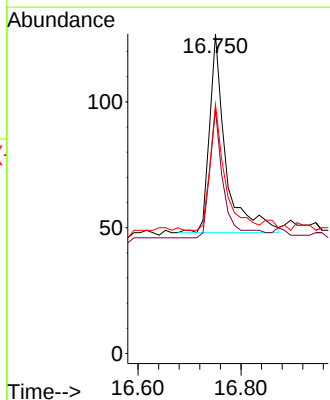
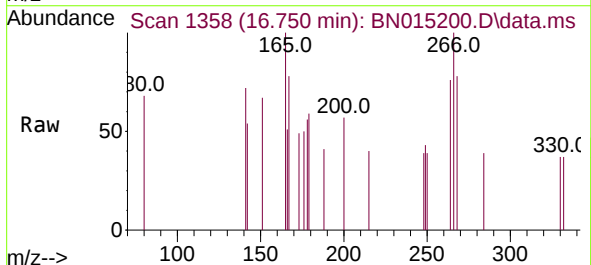


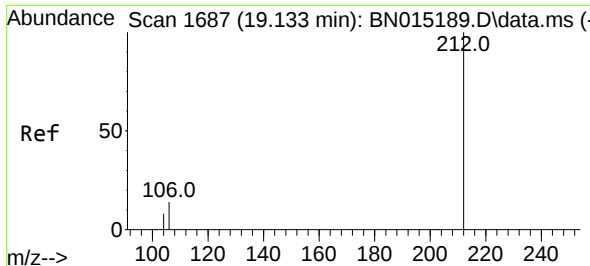

#27
Fluoranthene-d10
Concen: 0.39 ng
RT: 19.133 min Scan# 1687
Delta R.T. -0.000 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57




Instrument :
BNA_N
ClientSampleId :
RE134D1-20210617


Tgt Ion:212 Resp: 82882
Ion Ratio Lower Upper
212 100
106 14.0 7.0 10.6#
104 8.1 4.1 6.1#

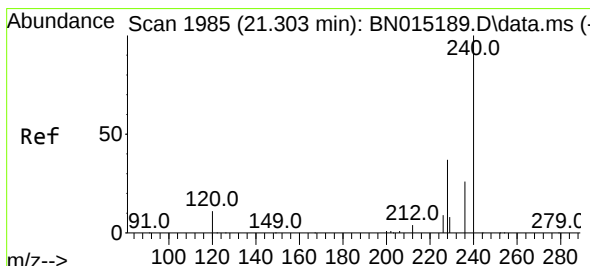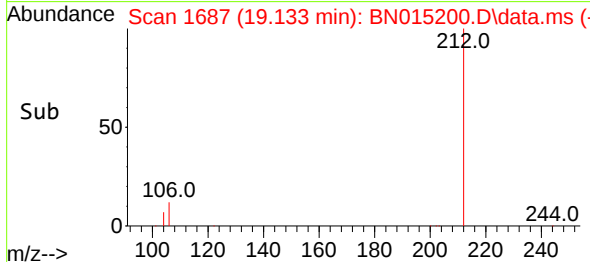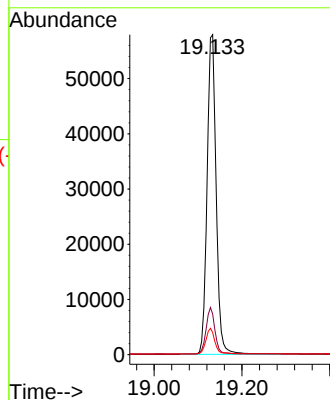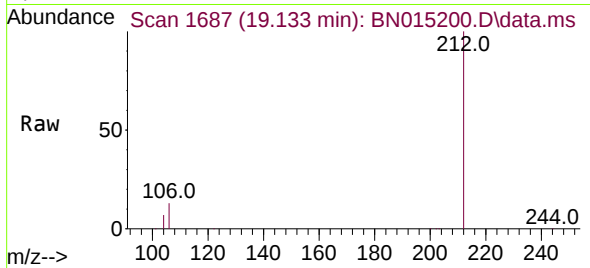

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.292 min Scan# 1984
Delta R.T. -0.011 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57


Tgt Ion:240 Resp: 69119
Ion Ratio Lower Upper
240 100
120 10.8 4.2 6.4#
236 26.4 21.4 32.2

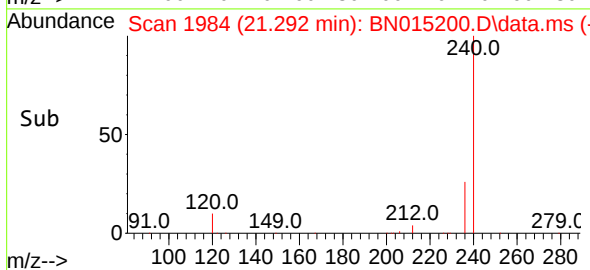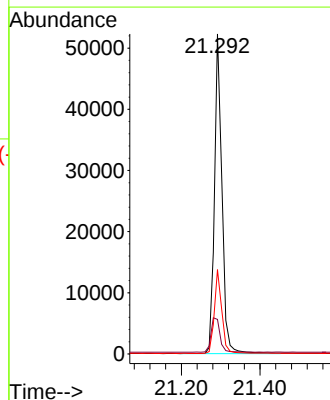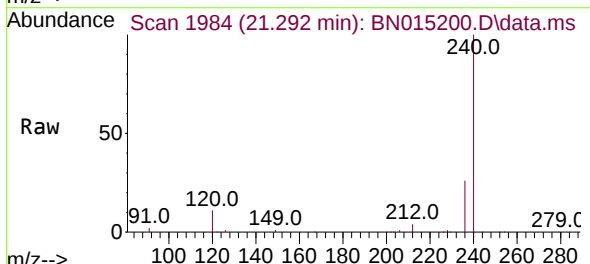






#31
Terphenyl-d14
Concen: 0.54 ng
RT: 19.734 min Scan# 1808
Delta R.T. -0.010 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57

Instrument :
BNA_N
ClientSampleId :
RE134D1-20210617



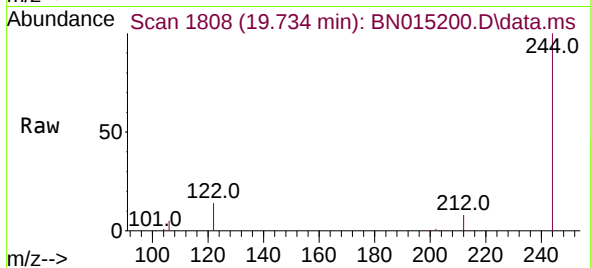



Tgt Ion:244 Resp: 83084
Ion Ratio Lower Upper
244 100
212 8.1 6.3 9.5
122 13.6 6.2 9.2#

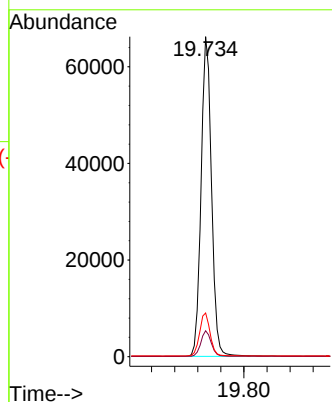

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.31 ng
RT: 21.217 min Scan# 1977
Delta R.T. -0.011 min
Lab File: BN015200.D
Acq: 29 Jun 2021 23:57


Tgt Ion:149 Resp: 7131
Ion Ratio Lower Upper
149 100
167 26.5 28.9 43.3#
279 3.4 4.9 7.3#

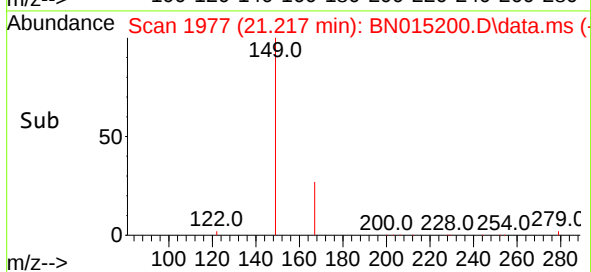

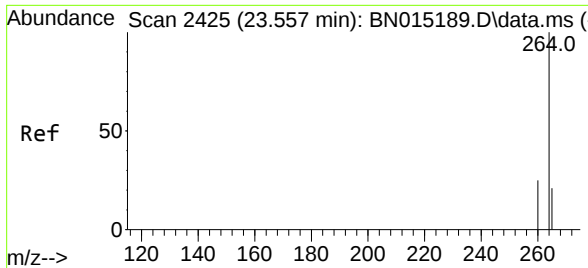

#35
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.540 min Scan# 2420
 Delta R.T. -0.017 min
 Lab File: BN015200.D
 Acq: 29 Jun 2021 23:57

Instrument :
 BNA_N
 ClientSampleId :
 RE134D1-20210617

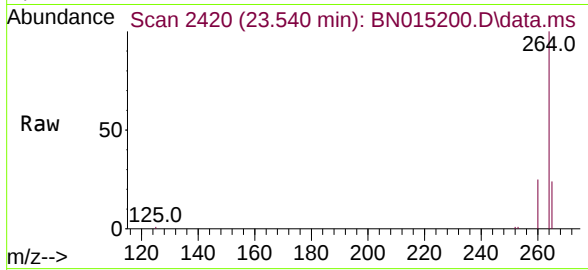

Tgt Ion:264 Resp: 57081

Ion	Ratio	Lower	Upper
264	100		
260	25.1	20.6	31.0
265	23.8	21.4	32.2

