

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062921\
 Data File : BN015207.D
 Acq On : 30 Jun 2021 04:10
 Operator : CG/JU
 Sample : M2783-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE115D2-20210617

Quant Time: Jun 30 06:20:34 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 29 19:13:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.732	152	16310	0.40	ng	# 0.00
7) Naphthalene-d8	10.493	136	73676	0.40	ng	#-0.01
13) Acenaphthene-d10	14.346	164	34000	0.40	ng	0.00
19) Phenanthrene-d10	17.091	188	67257	0.40	ng	0.00
29) Chrysene-d12	21.292	240	62607	0.40	ng	#-0.01
35) Perylene-d12	23.537	264	52228	0.40	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.371	112	4491	0.13	ng	0.03
5) Phenol-d6	6.911	99	4191	0.08	ng	0.00
8) Nitrobenzene-d5	8.870	82	26285	0.39	ng	0.00
11) 2-Methylnaphthalene-d10	12.088	152	42226	0.35	ng	0.00
14) 2,4,6-Tribromophenol	15.843	330	2657	0.36	ng	0.00
15) 2-Fluorobiphenyl	12.963	172	63934	0.45	ng	-0.01
27) Fluoranthene-d10	19.128	212	78589	0.38	ng	0.00
31) Terphenyl-d14	19.734	244	75914	0.55	ng	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.352	88	52720	11.14	ng	# 70
6) bis(2-Chloroethyl)ether	7.169	93	2598	0.05	ng	# 83
20) 4,6-Dinitro-2-methylph...	15.450	198	3	0.19	ng	# 1
23) Atrazine	16.544	200	9	0.17	ng	# 13
24) Pentachlorophenol	16.751	266	31	0.24	ng	# 74
34) Bis(2-ethylhexyl)phtha...	21.218	149	4866	0.30	ng	# 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062921\
Data File : BN015207.D
Acq On : 30 Jun 2021 04:10
Operator : CG/JU
Sample : M2783-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE115D2-20210617

Quant Time: Jun 30 06:20:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 29 19:13:09 2021
Response via : Initial Calibration




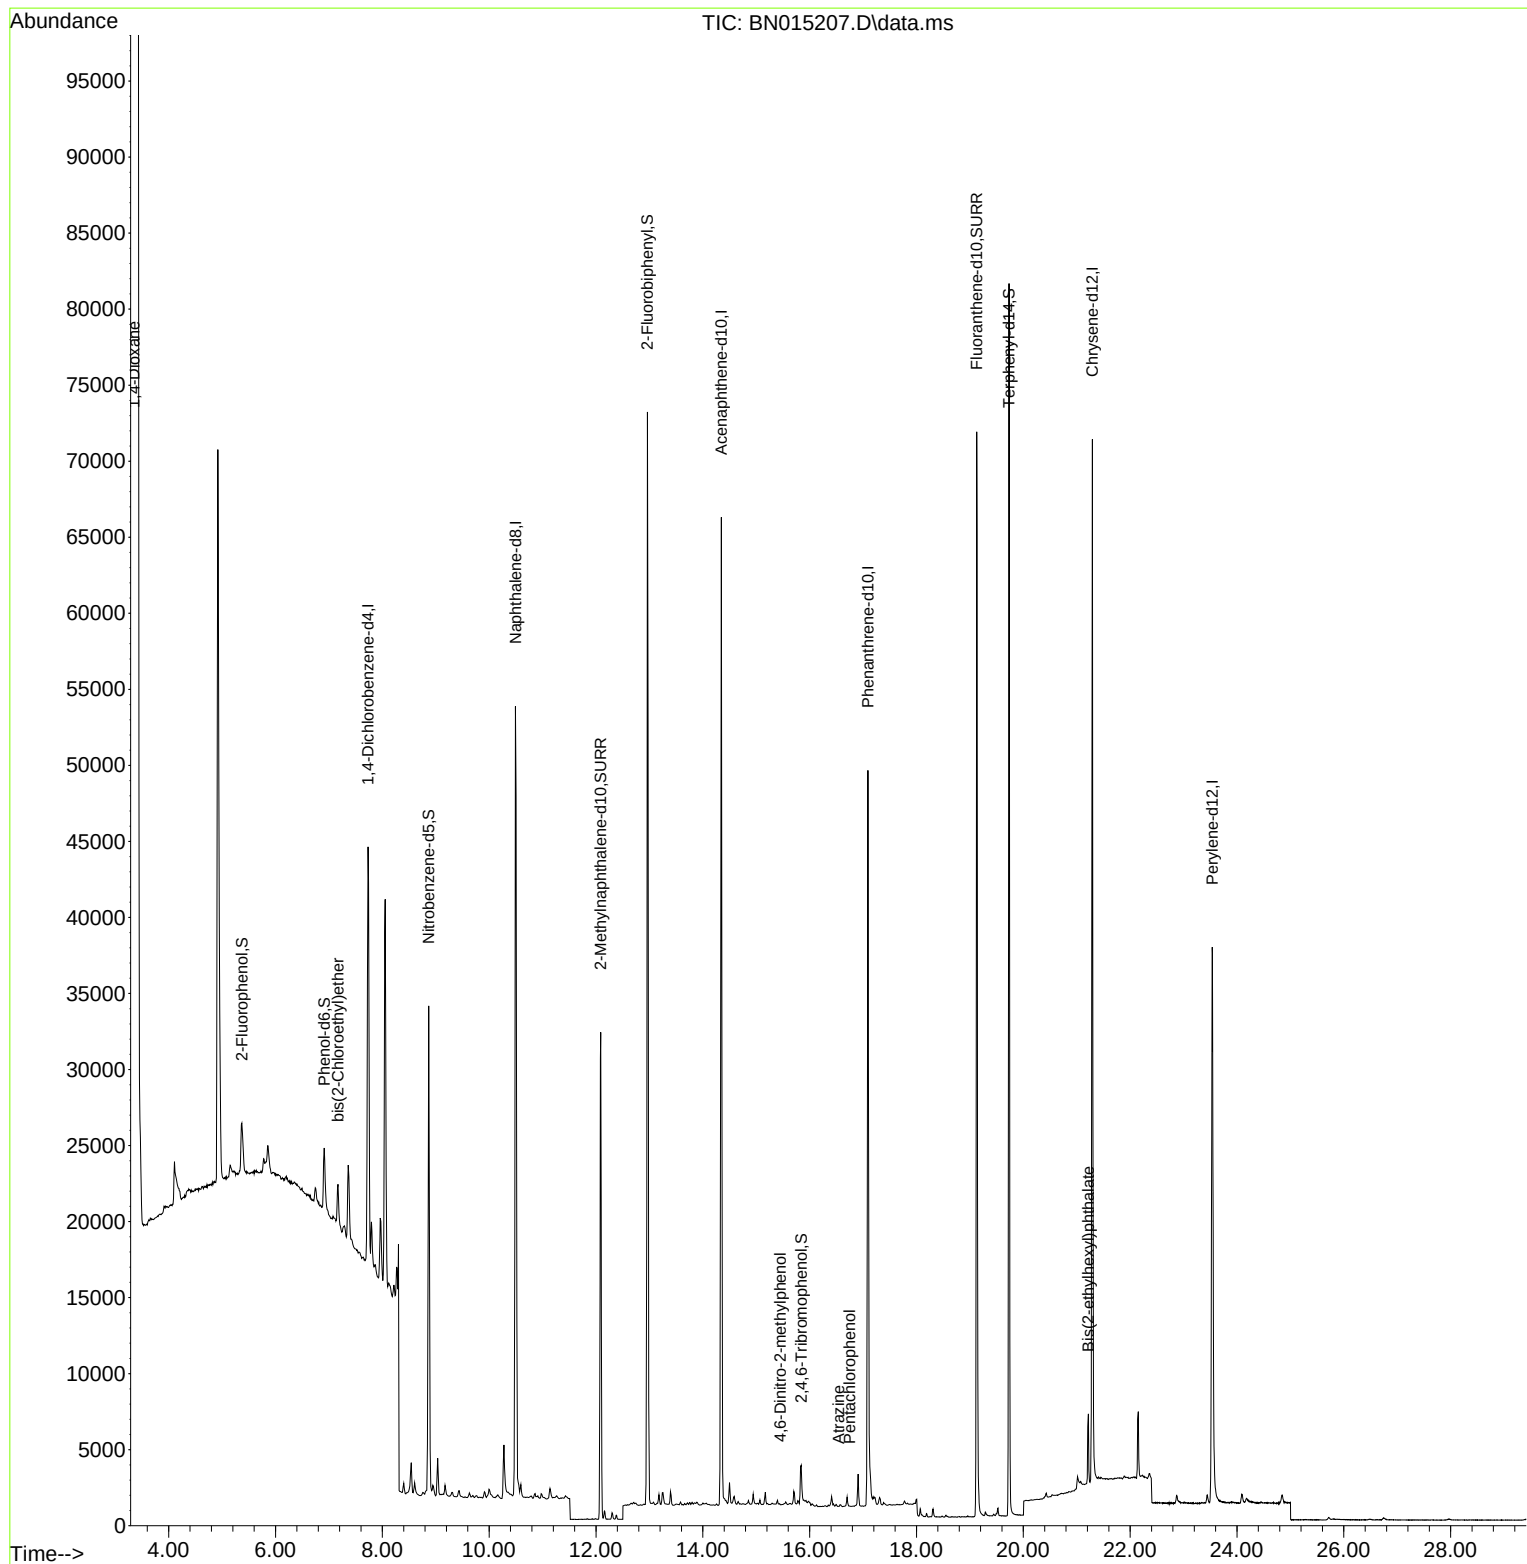


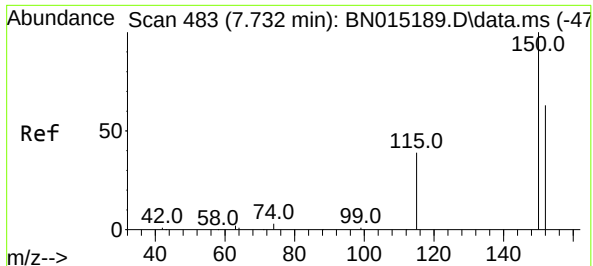

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.732 min Scan# 483
 Delta R.T. -0.000 min
 Lab File: BN015207.D
 Acq: 30 Jun 2021 04:10




Instrument :
 BNA_N
 ClientSampleId :
 RE115D2-20210617


Tgt Ion:152 Resp: 16310
 Ion Ratio Lower Upper
 152 100
 150 158.2 119.0 178.6
 115 61.5 62.2 93.4#

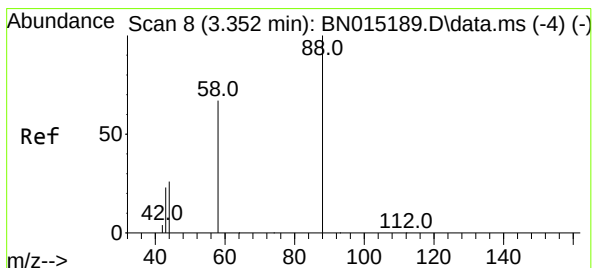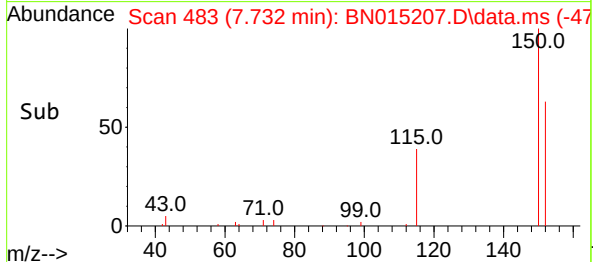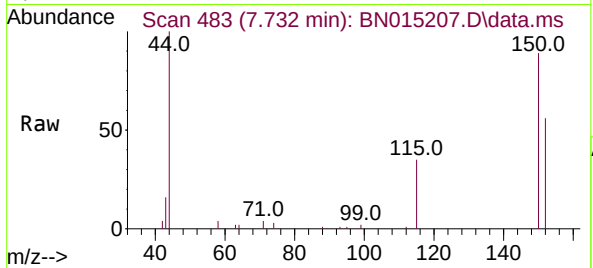

#2
 1,4-Dioxane
 Concen: 11.14 ng
 RT: 3.352 min Scan# 8
 Delta R.T. -0.000 min
 Lab File: BN015207.D
 Acq: 30 Jun 2021 04:10

Tgt Ion: 88 Resp: 52720
 Ion Ratio Lower Upper
 88 100
 43 26.4 12.9 19.3#
 58 68.7 38.1 57.1#


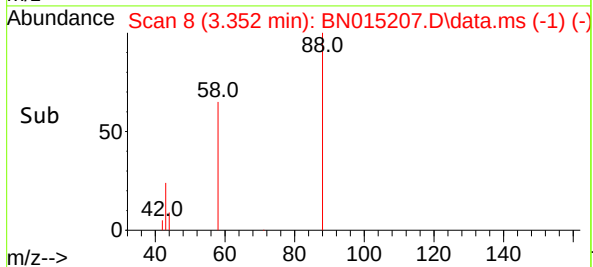

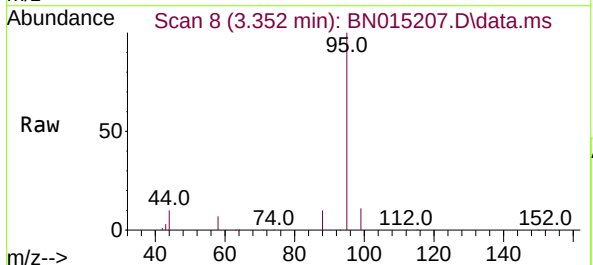


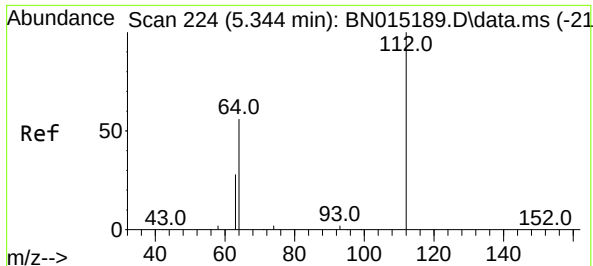

#4
2-Fluorophenol
Concen: 0.13 ng
RT: 5.371 min Scan# 227
Delta R.T. 0.028 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10




Instrument :
BNA_N
ClientSampleId :
RE115D2-20210617


Tgt Ion:112 Resp: 4491
Ion Ratio Lower Upper
112 100
64 57.9 39.0 58.6
63 31.0 20.6 30.8#

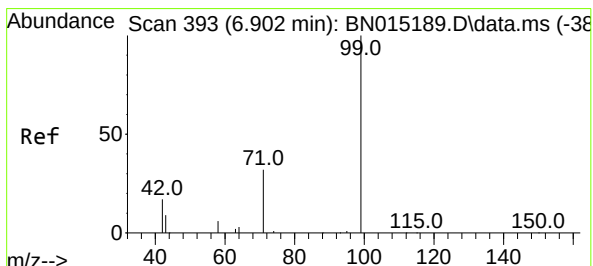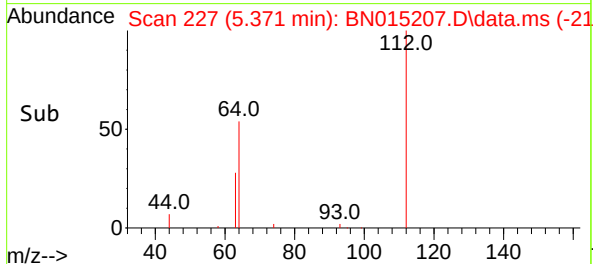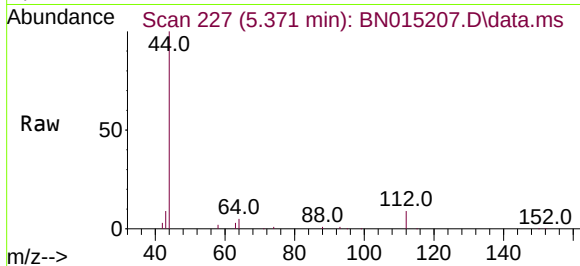

#5
Phenol-d6
Concen: 0.08 ng
RT: 6.911 min Scan# 394
Delta R.T. 0.009 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10

Tgt Ion: 99 Resp: 4191
Ion Ratio Lower Upper
99 100
42 18.5 8.9 13.3#
71 36.4 35.6 53.4


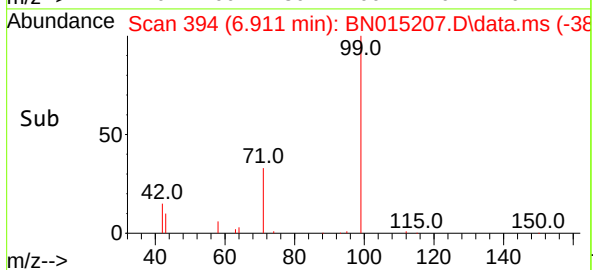

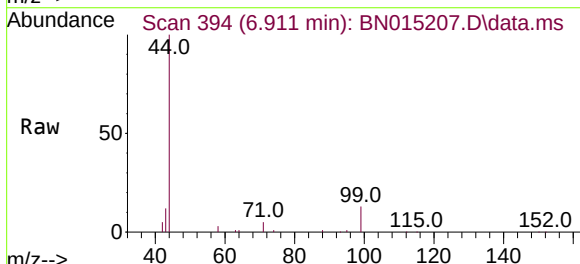


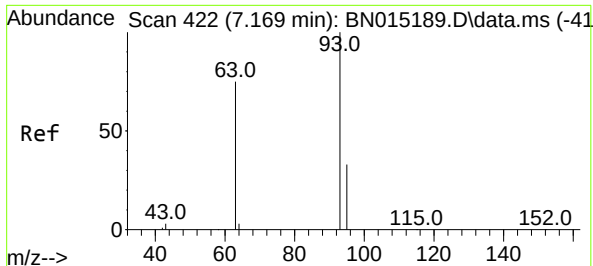

#6
bis(2-Chloroethyl)ether
Concen: 0.05 ng
RT: 7.169 min Scan# 422
Delta R.T. -0.000 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10




Instrument :
BNA_N
ClientSampleId :
RE115D2-20210617


Tgt Ion: 93 Resp: 2598
Ion Ratio Lower Upper
93 100
63 75.4 46.6 70.0#
95 30.8 28.6 42.8

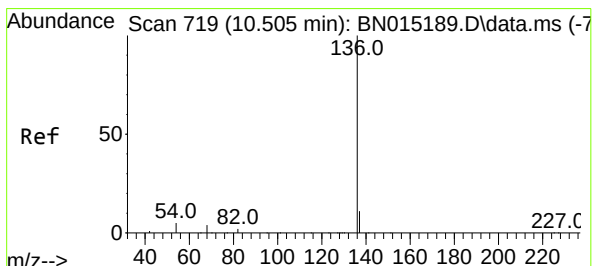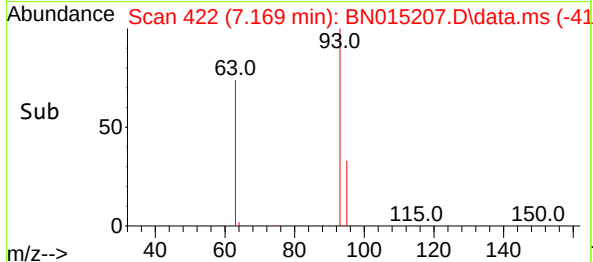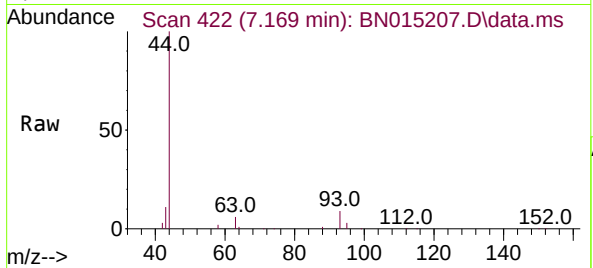

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.493 min Scan# 718
Delta R.T. -0.013 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10

Tgt Ion: 136 Resp: 73676
Ion Ratio Lower Upper
136 100
137 11.0 9.8 14.8
54 10.6 5.4 8.2#
68 8.0 4.9 7.3#


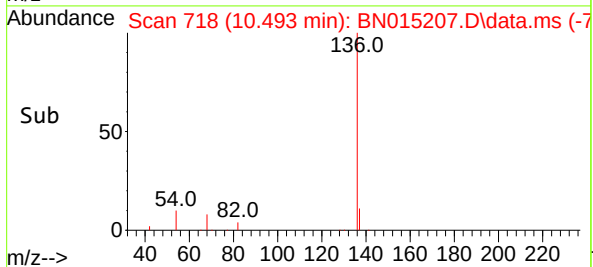

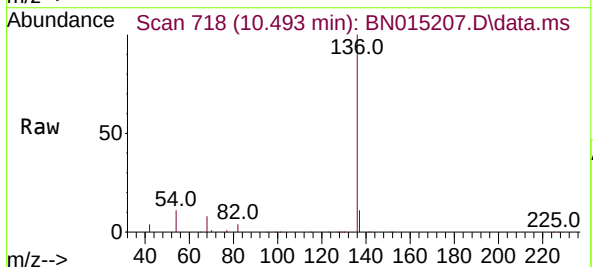


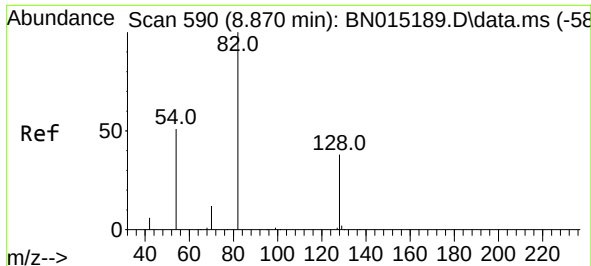

#8
Nitrobenzene-d5
Concen: 0.39 ng
RT: 8.870 min Scan# 590
Delta R.T. -0.000 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10




Instrument :
BNA_N
ClientSampleId :
RE115D2-20210617


Tgt Ion	Ratio	Lower	Upper
82	100		
128	37.0	31.6	47.4
54	50.7	29.0	43.4

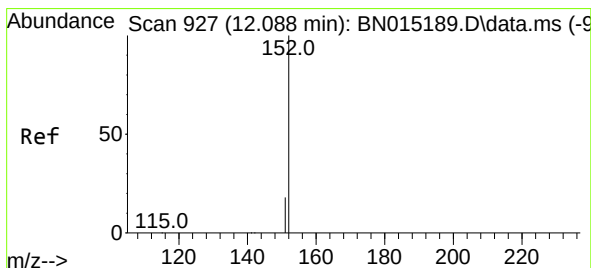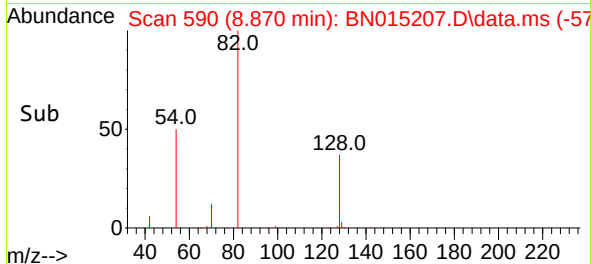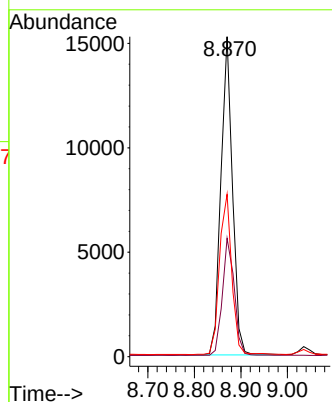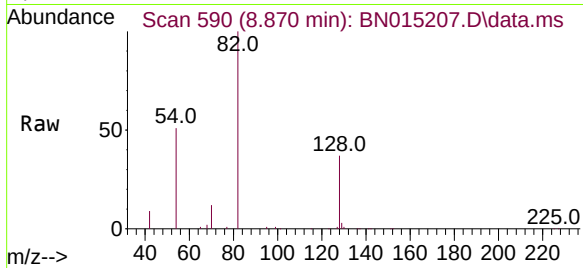

#11
2-Methylnaphthalene-d10
Concen: 0.35 ng
RT: 12.088 min Scan# 927
Delta R.T. -0.000 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.4	16.7	25.1


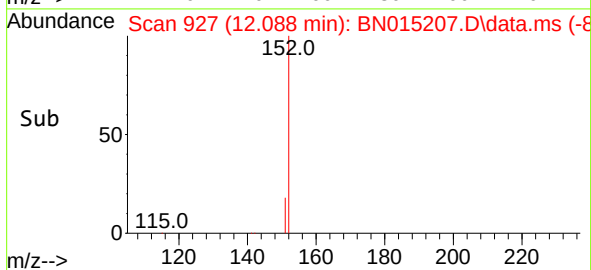
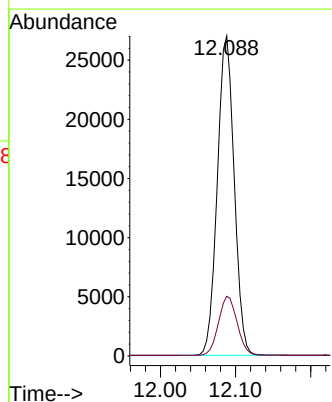
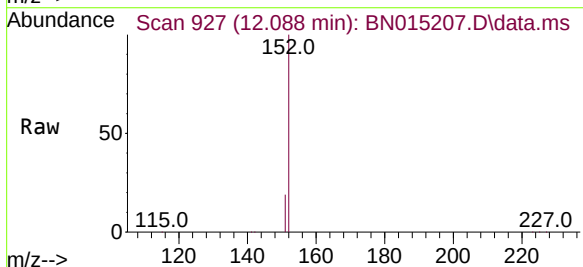


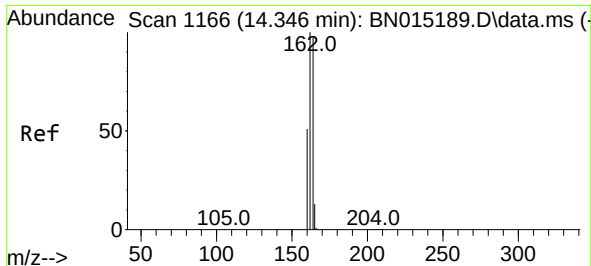

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.346 min Scan# 1166
Delta R.T. -0.000 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10




Instrument :
BNA_N
ClientSampleId :
RE115D2-20210617


Tgt Ion:164 Resp: 34000
Ion Ratio Lower Upper
164 100
162 101.3 83.8 125.6
160 54.3 37.4 56.0

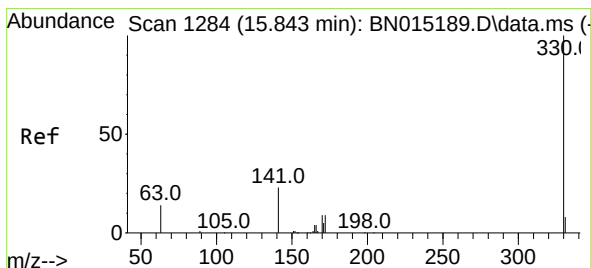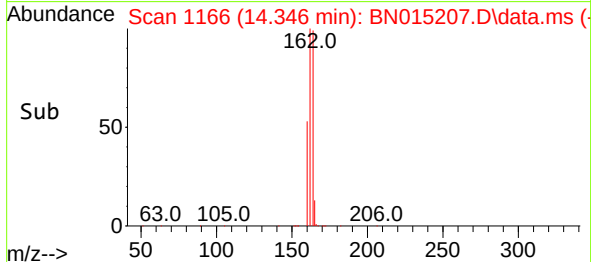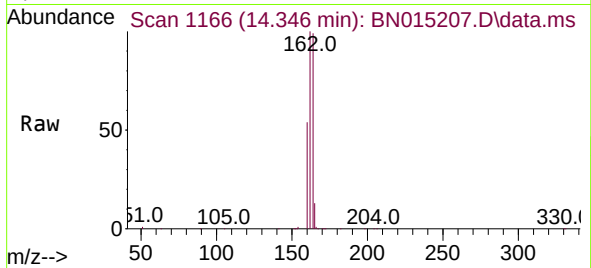

#14
2,4,6-Tribromophenol
Concen: 0.36 ng
RT: 15.843 min Scan# 1284
Delta R.T. -0.000 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10

Tgt Ion:330 Resp: 2657
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 39.6 22.4 33.6#


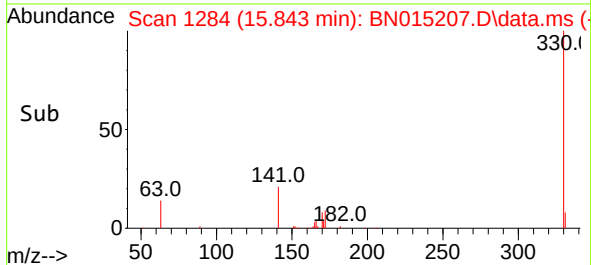

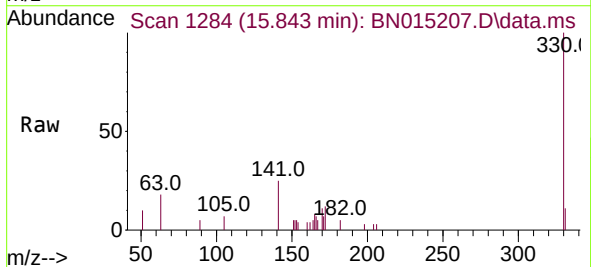


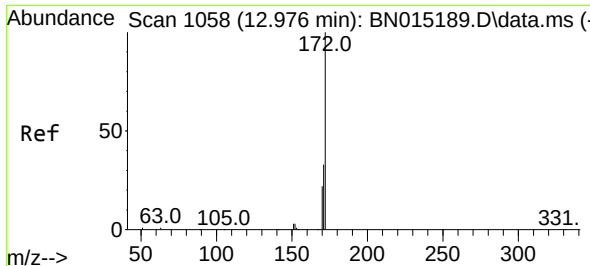

#15
2-Fluorobiphenyl
Concen: 0.45 ng
RT: 12.963 min Scan# 1057
Delta R.T. -0.013 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10




Instrument :
BNA_N
ClientSampleId :
RE115D2-20210617


Tgt Ion:172 Resp: 63934
Ion Ratio Lower Upper
172 100
171 35.7 30.6 45.8
170 24.6 20.2 30.4

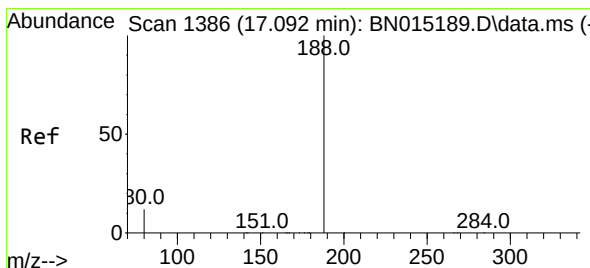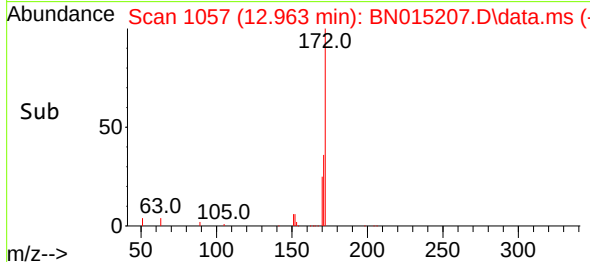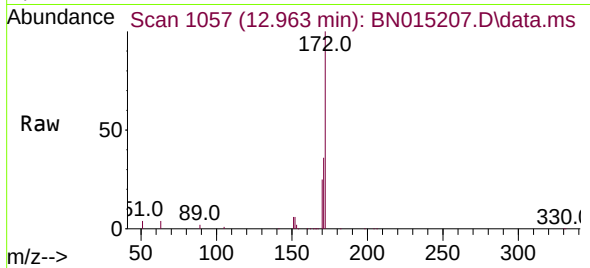

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.091 min Scan# 1386
Delta R.T. -0.001 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10

Tgt Ion:188 Resp: 67257
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.5 9.0 13.4


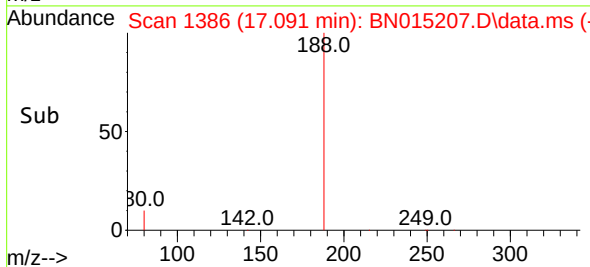

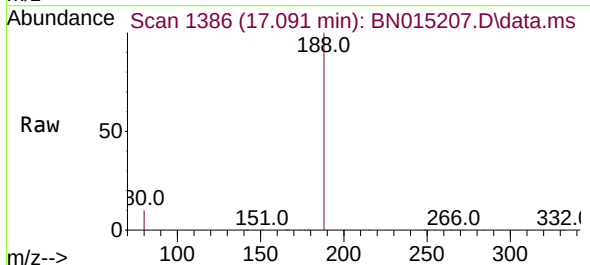


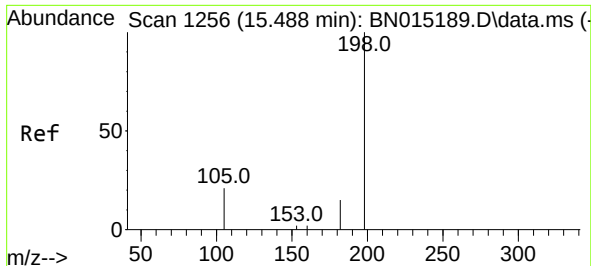

#20
4,6-Dinitro-2-methylphenol
Concen: 0.19 ng
RT: 15.450 min Scan# 1253
Delta R.T. -0.038 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10




Instrument :
BNA_N
ClientSampleId :
RE115D2-20210617


Tgt Ion:198 Resp: 3
Ion Ratio Lower Upper
198 100
182 117.0 34.5 51.7#
77 0.0 0.0 0.0

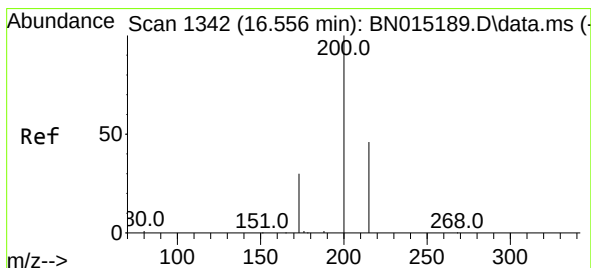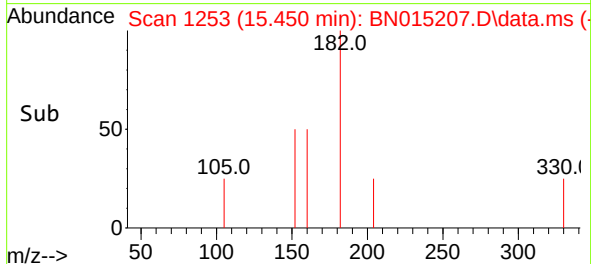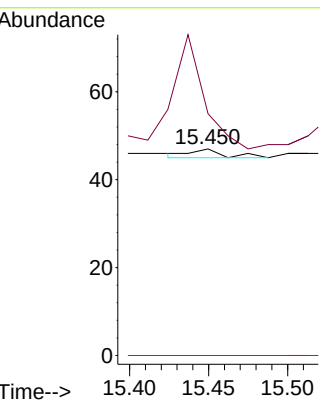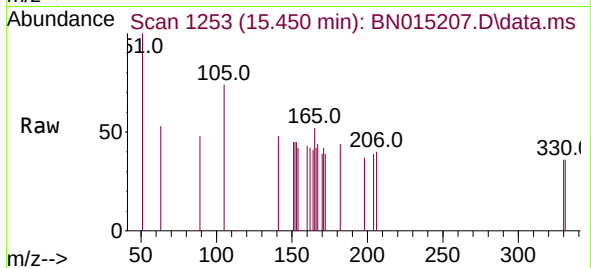

#23
Atrazine
Concen: 0.17 ng
RT: 16.544 min Scan# 1341
Delta R.T. -0.012 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10

Tgt Ion:200 Resp: 9
Ion Ratio Lower Upper
200 100
173 102.0 21.7 32.5#
215 96.0 43.1 64.7#


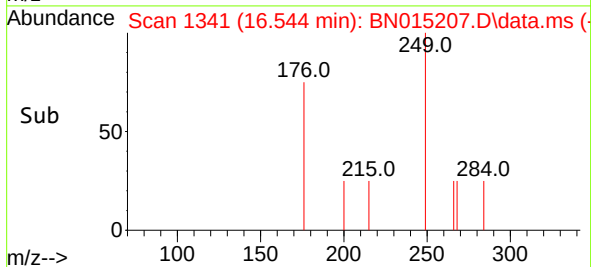
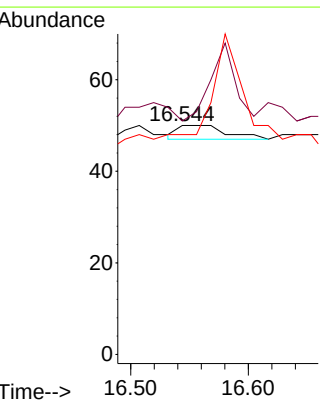
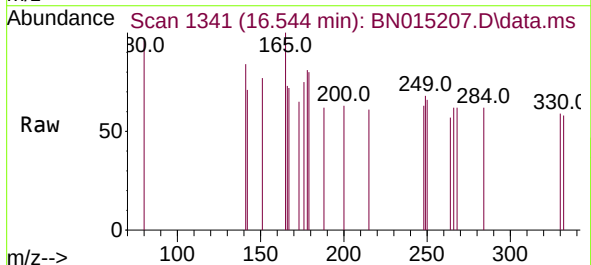


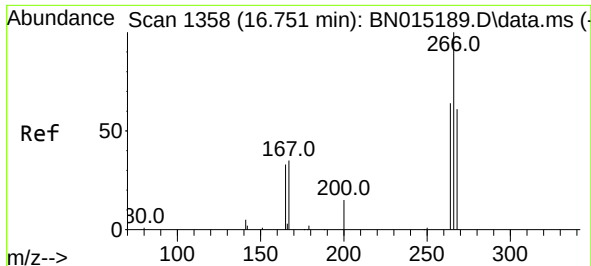

#24
Pentachlorophenol
Concen: 0.24 ng
RT: 16.751 min Scan# 1358
Delta R.T. -0.000 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10




Instrument :
BNA_N
ClientSampleId :
RE115D2-20210617


Tgt Ion:266 Resp: 31
Ion Ratio Lower Upper
266 100
264 38.7 51.0 76.4#
268 48.4 50.6 76.0#

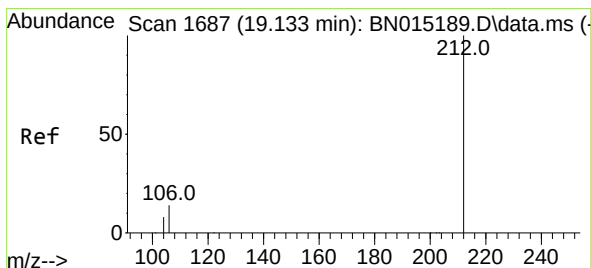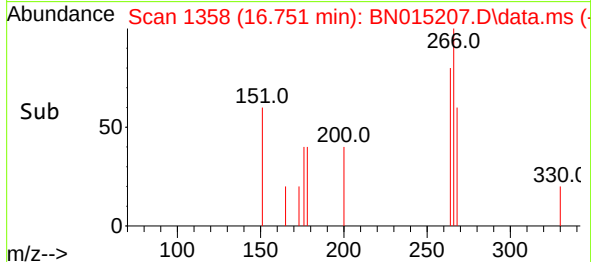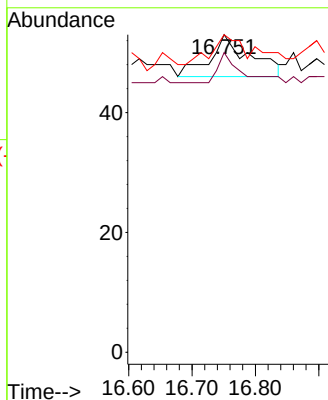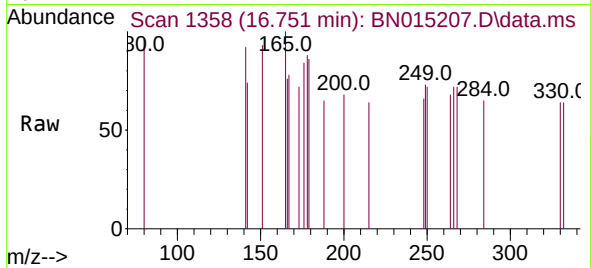

#27
Fluoranthene-d10
Concen: 0.38 ng
RT: 19.128 min Scan# 1686
Delta R.T. -0.005 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10

Tgt Ion:212 Resp: 78589
Ion Ratio Lower Upper
212 100
106 14.0 7.0 10.6#
104 8.0 4.1 6.1#


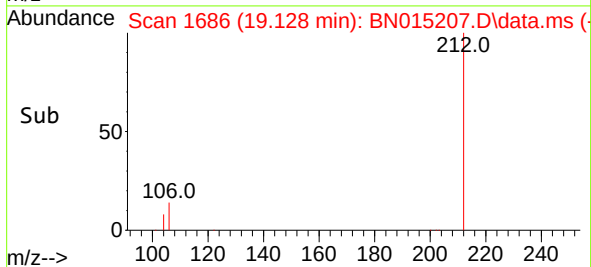
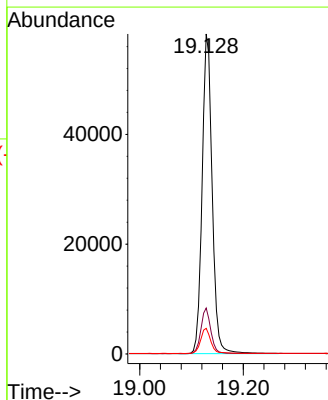
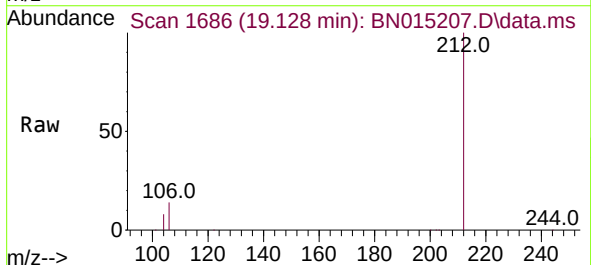


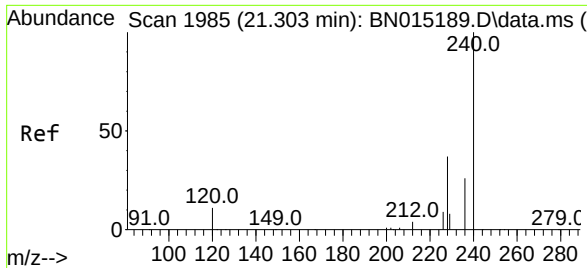

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.292 min Scan# 1984
Delta R.T. -0.011 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10




Instrument :
BNA_N
ClientSampleId :
RE115D2-20210617


Tgt Ion:240 Resp: 62607
Ion Ratio Lower Upper
240 100
120 8.9 4.2 6.4#
236 26.2 21.4 32.2

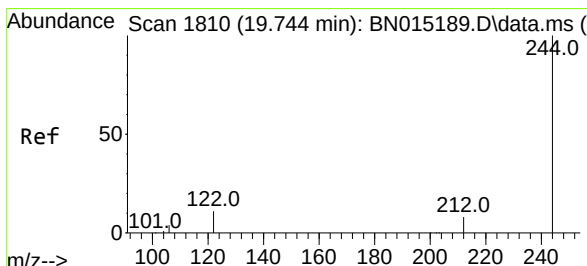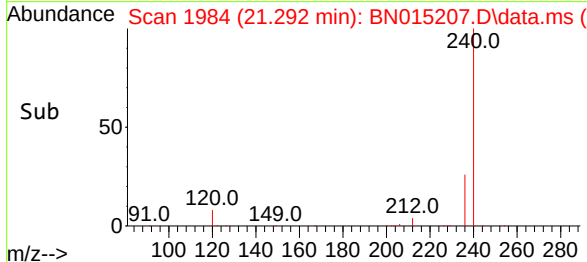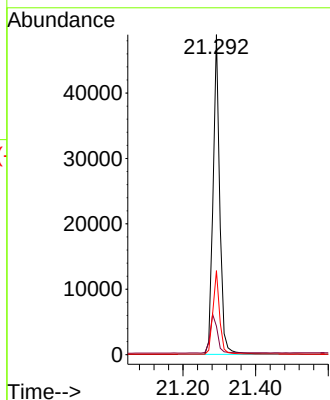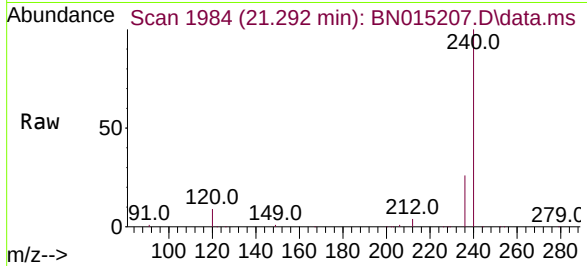

#31
Terphenyl-d14
Concen: 0.55 ng
RT: 19.734 min Scan# 1808
Delta R.T. -0.010 min
Lab File: BN015207.D
Acq: 30 Jun 2021 04:10

Tgt Ion:244 Resp: 75914
Ion Ratio Lower Upper
244 100
212 7.9 6.3 9.5
122 12.7 6.2 9.2#


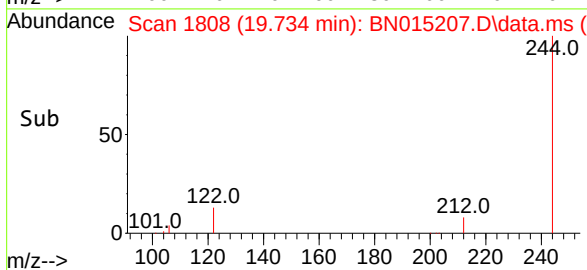
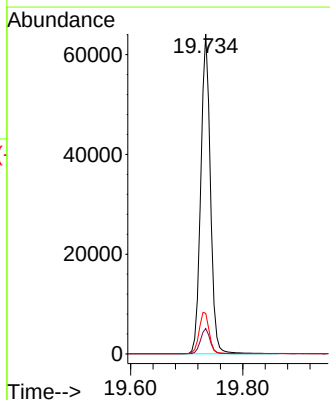
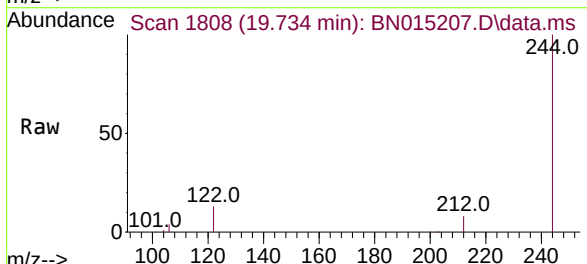


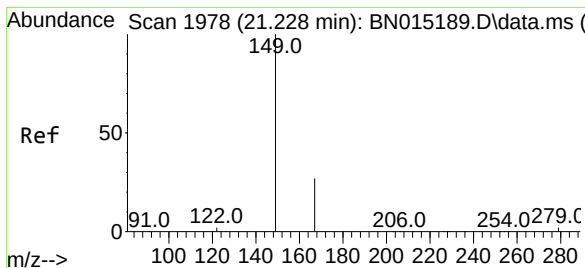

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.30 ng
 RT: 21.218 min Scan# 1977
 Delta R.T. -0.010 min
 Lab File: BN015207.D
 Acq: 30 Jun 2021 04:10

Instrument :
 BNA_N
 ClientSampleId :
 RE115D2-20210617

Tgt Ion:149 Resp: 4866
 Ion Ratio Lower Upper
 149 100
 167 25.5 28.9 43.3#
 279 3.6 4.9 7.3#

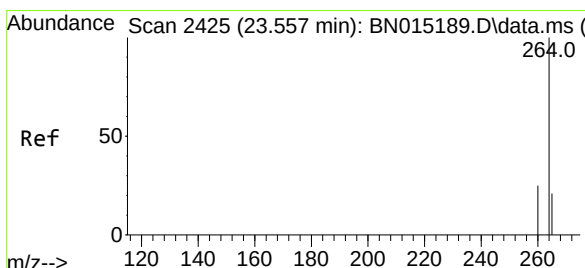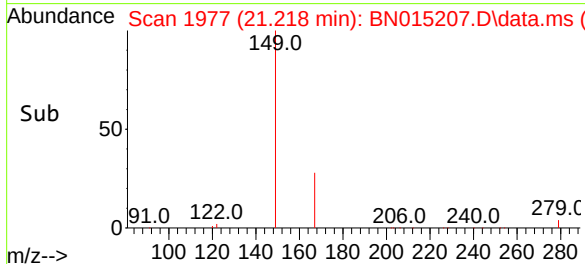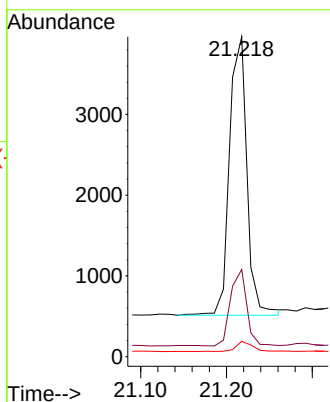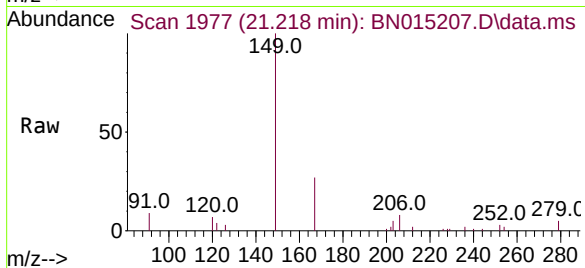

#35
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.537 min Scan# 2419
 Delta R.T. -0.021 min
 Lab File: BN015207.D
 Acq: 30 Jun 2021 04:10

Tgt Ion:264 Resp: 52228
 Ion Ratio Lower Upper
 264 100
 260 25.7 20.6 31.0
 265 24.2 21.4 32.2

