
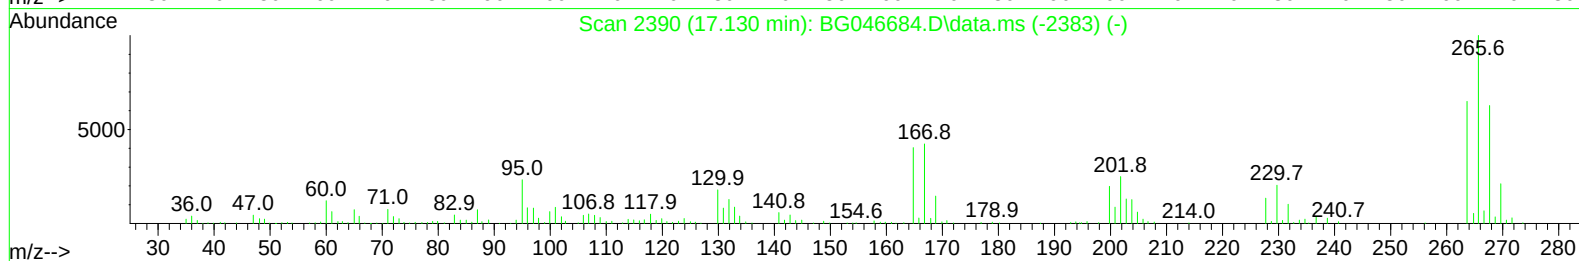
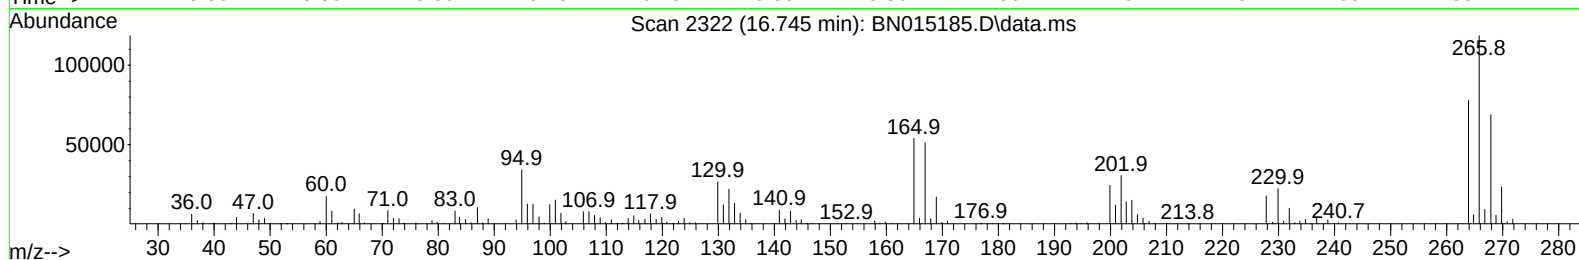


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062921\
 Data File : BN015185.D
 Acq On : 29 Jun 2021 13:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 14:54:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 10:10:58 2021
 Response via : Initial Calibration

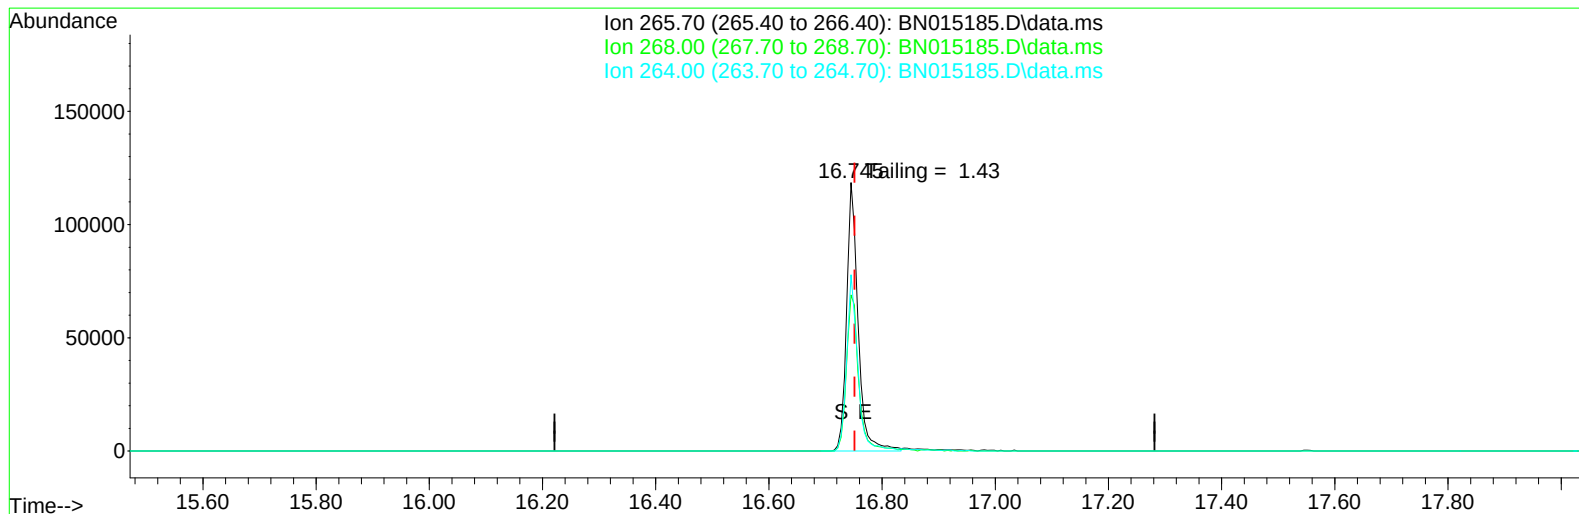

TIC: BN015185.D\data.ms

(70) Pentachlorophenol (C)




16.745min (-0.006) 32943.76 ng

response 169340

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.13
264.00	61.60	65.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062921\
 Data File : BN015185.D
 Acq On : 29 Jun 2021 13:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 14:54:22 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 10:10:58 2021
 Response via : Initial Calibration

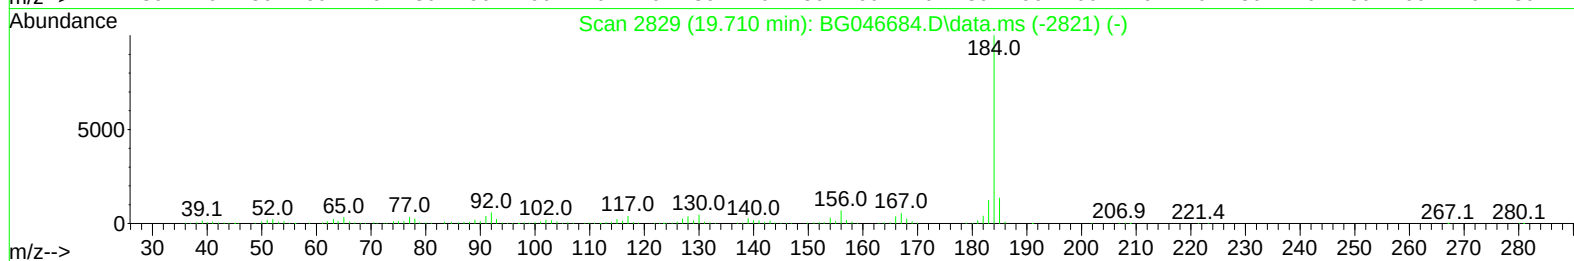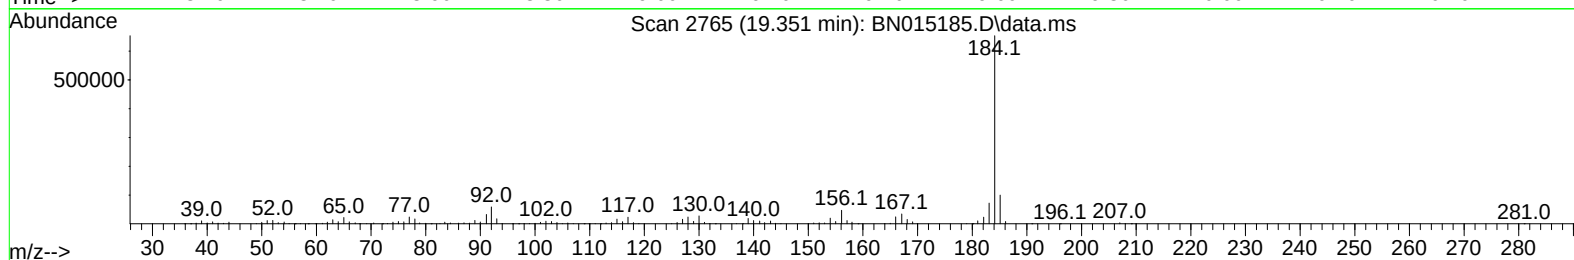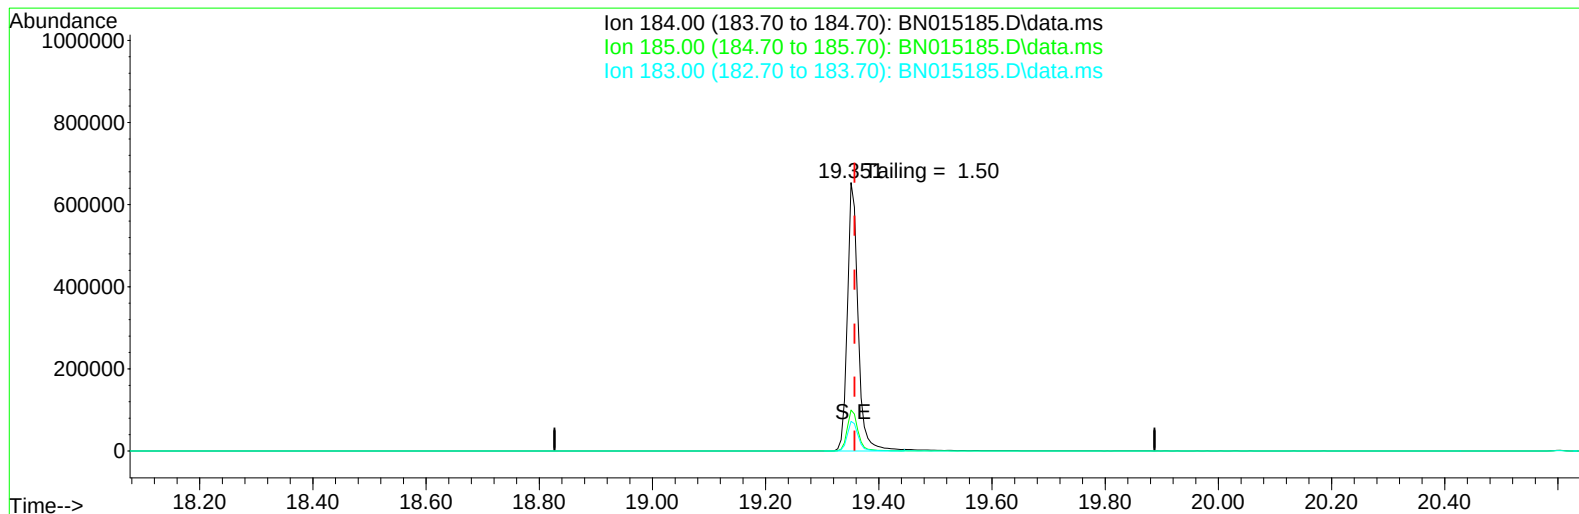

TIC: BN015185.D\data.ms

(77) Benzidine

19.351min (-0.006) 0.00 ng

response 870073

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.26
183.00	13.20	11.04
0.00	0.00	0.00