

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062921\
 Data File : BN015188.D
 Acq On : 29 Jun 2021 15:27
 Operator : CG/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Manual Integrations
 APPROVED

mohammad
 6/30/2021 2:14:30 PM

Quant Time: Jun 29 16:43:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 29 16:42:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.741	152	17622	0.400	ng	# 0.00
7) Naphthalene-d8	10.505	136	78018	0.400	ng	# 0.00
13) Acenaphthene-d10	14.345	164	36420	0.400	ng	0.00
19) Phenanthrene-d10	17.091	188	64589	0.400	ng	0.00
29) Chrysene-d12	21.302	240	60798	0.400	ng	# 0.00
35) Perylene-d12	23.557	264	62225	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.343	112	8243	0.151	ng	0.00
5) Phenol-d6	6.902	99	12410	0.180	ng	0.00
8) Nitrobenzene-d5	8.870	82	13859	0.235	ng	0.00
11) 2-Methylnaphthalene-d10	12.088	152	26784	0.200	ng	0.00
14) 2,4,6-Tribromophenol	15.843	330	1670	0.098	ng	0.00
15) 2-Fluorobiphenyl	12.975	172	31374	0.227	ng	0.00
27) Fluoranthene-d10	19.138	212	38154	0.187	ng	0.00
31) Terphenyl-d14	19.744	244	25892	0.172	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.352	88	999m	0.135	ng	
3) n-Nitrosodimethylamine	3.684	42	2164	0.132	ng	# 59
6) bis(2-Chloroethyl)ether	7.169	93	11670	0.215	ng	# 82
9) Naphthalene	10.543	128	45525	0.208	ng	98
10) Hexachlorobutadiene	10.847	225	9324	0.215	ng	# 99
12) 2-Methylnaphthalene	12.163	142	28643	0.195	ng	# 90
16) Acenaphthylene	14.066	152	35612	0.194	ng	98
17) Acenaphthene	14.409	154	23246	0.206	ng	97
18) Fluorene	15.399	166	26764	0.193	ng	99
21) 4-Bromophenyl-phenylether	16.288	248	8252	0.198	ng	# 77
22) Hexachlorobenzene	16.410	284	11008	0.250	ng	# 91
23) Atrazine	16.556	200	3397	0.091	ng	92
24) Pentachlorophenol	16.750	266	428	0.026	ng	98
25) Phenanthrene	17.140	178	43082	0.219	ng	99
26) Anthracene	17.225	178	33962	0.176	ng	99
28) Fluoranthene	19.168	202	44736	0.200	ng	# 97
30) Pyrene	19.530	202	42253	0.175	ng	99
32) Benzo(a)anthracene	21.292	228	37952	0.166	ng	97
33) Chrysene	21.345	228	46357	0.211	ng	98
34) Bis(2-ethylhexyl)phtha...	21.228	149	9670	0.060	ng	# 84
36) Indeno(1,2,3-cd)pyrene	25.819	276	48884	0.235	ng	# 88
37) Benzo(b)fluoranthene	22.886	252	46356	0.199	ng	# 93
38) Benzo(k)fluoranthene	22.927	252	51837	0.230	ng	# 94
39) Benzo(a)pyrene	23.461	252	43763	0.213	ng	# 84
40) Dibenzo(a,h)anthracene	25.833	278	38966	0.232	ng	# 91
41) Benzo(g,h,i)perylene	26.507	276	39610	0.220	ng	# 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062921\
Data File : BN015188.D
Acq On : 29 Jun 2021 15:27
Operator : CG/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Manual Integrations
APPROVED

mohammad
6/30/2021 2:14:30 PM

Quant Time: Jun 29 16:43:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 29 16:42:28 2021
Response via : Initial Calibration

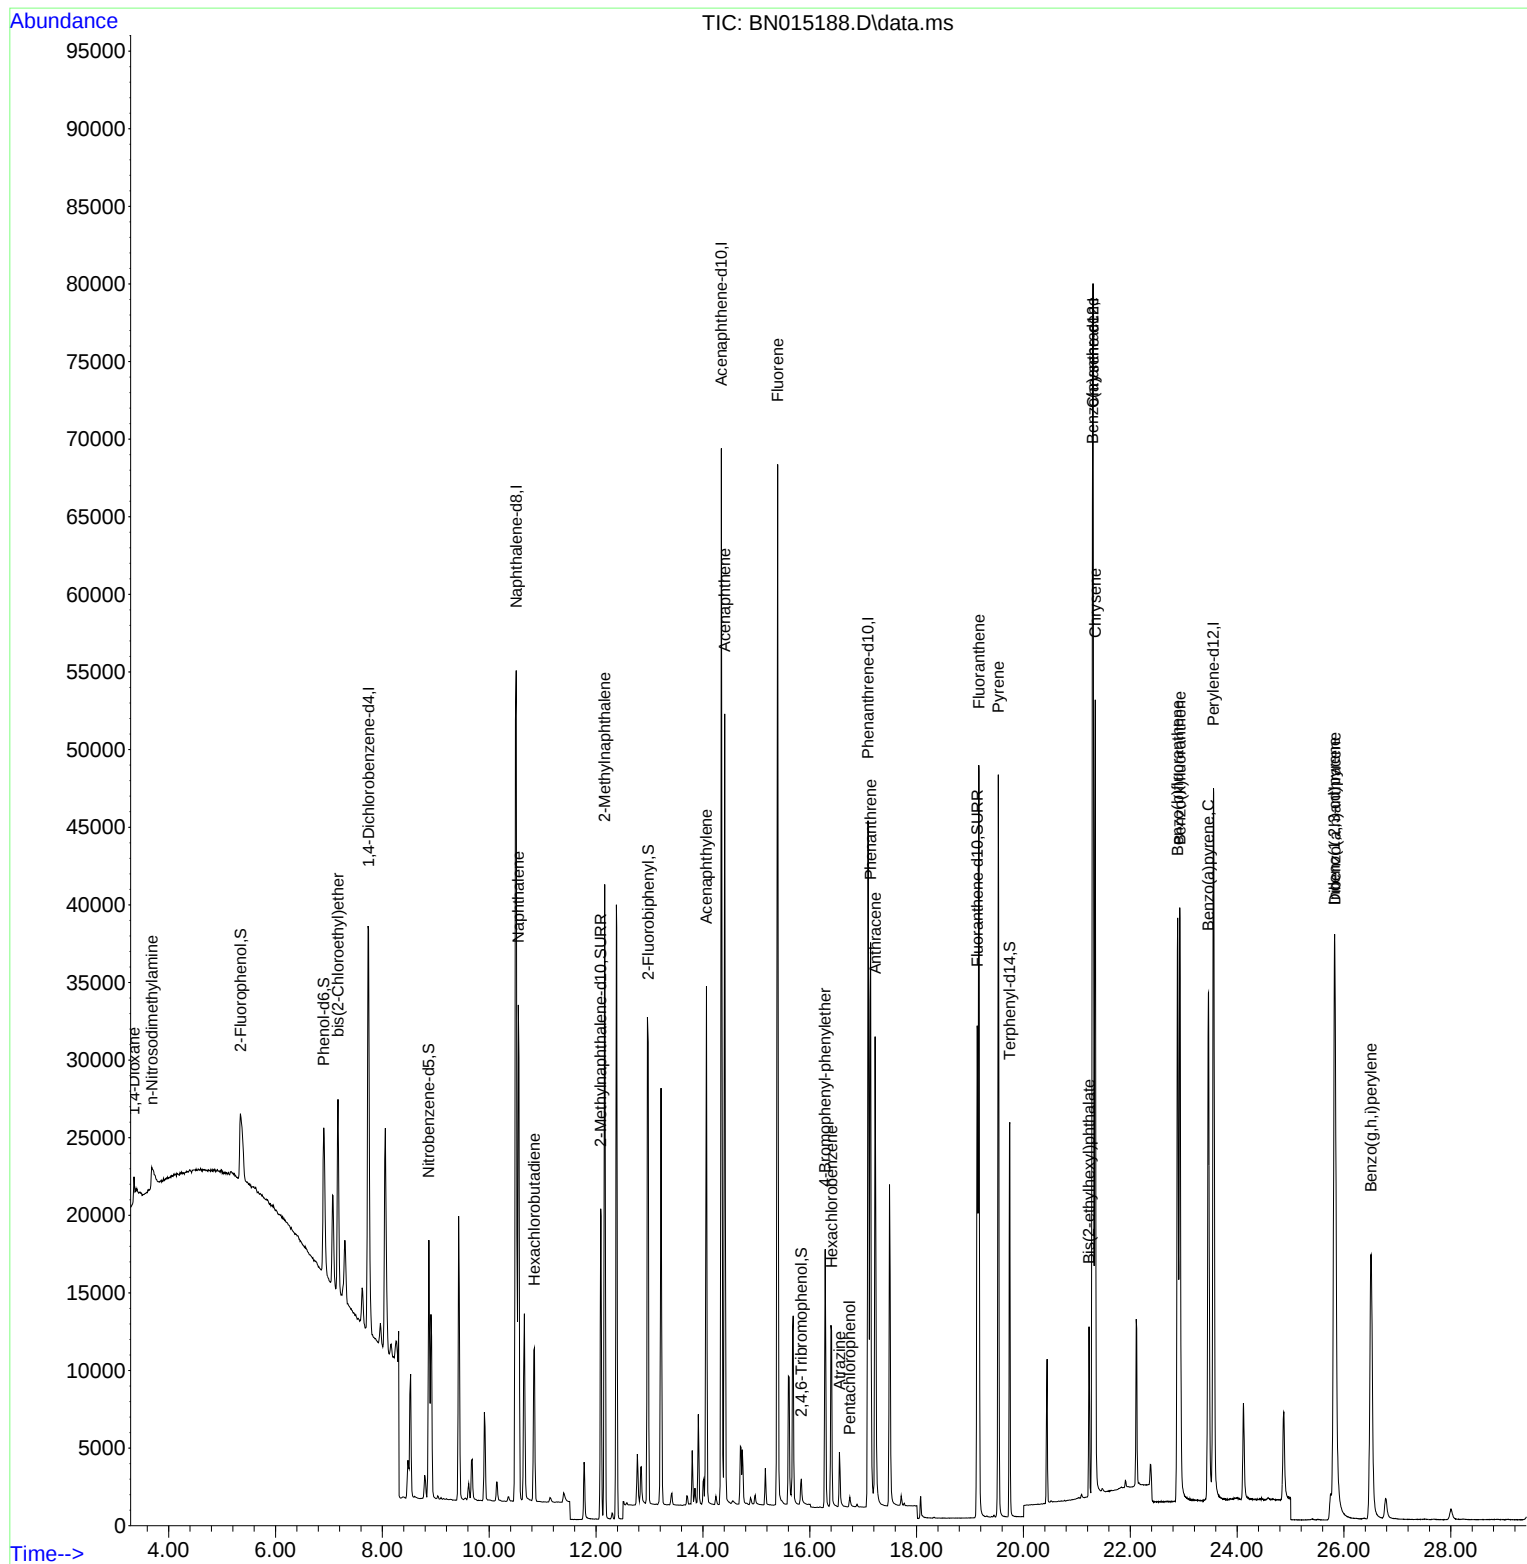

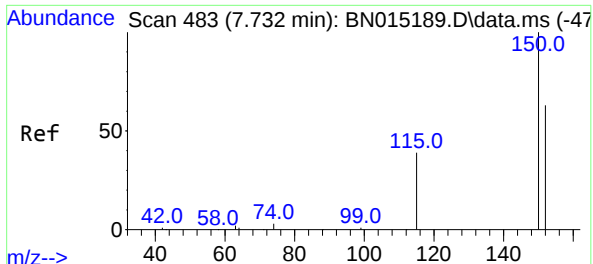





#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.741 min Scan# 484
Delta R.T. 0.009 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

Tgt Ion:152 Resp: 17622
Ion Ratio Lower Upper
152 100
150 154.0 119.0 178.6
115 59.3 62.2 93.4#

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
6/30/2021 2:14:30 PM

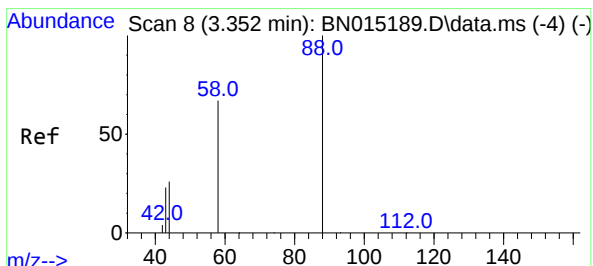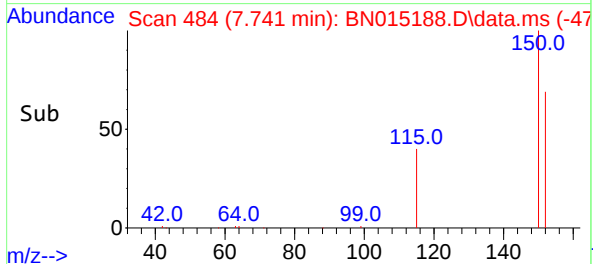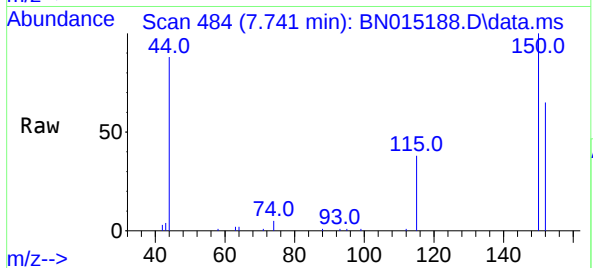

#2
1,4-Dioxane
Concen: 0.135 ng m
RT: 3.352 min Scan# 8
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

Tgt Ion: 88 Resp: 999
Ion Ratio Lower Upper
88 100
43 32.6 12.9 19.3#
58 79.0 38.1 57.1#

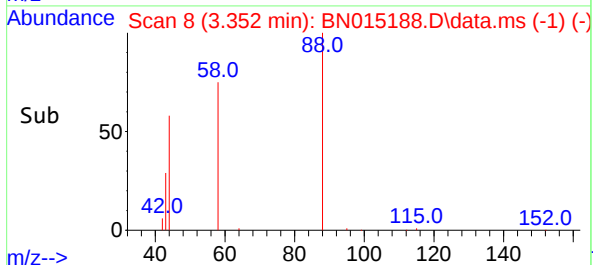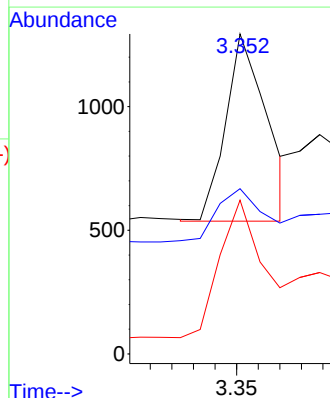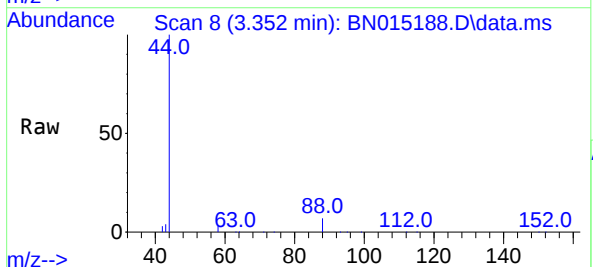

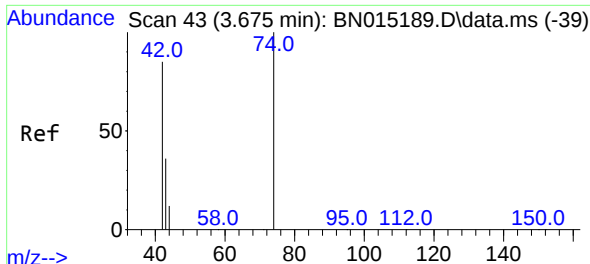





#3
n-Nitrosodimethylamine
Concen: 0.132 ng
RT: 3.684 min Scan# 44
Delta R.T. 0.009 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

Tgt Ion: 42 Resp: 2164
Ion Ratio Lower Upper
42 100
74 126.8 149.5 224.3#
44 0.0 4.2 6.2#

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
6/30/2021 2:14:30 PM



#4
2-Fluorophenol
Concen: 0.151 ng
RT: 5.343 min Scan# 224
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

Tgt Ion: 112 Resp: 8243
Ion Ratio Lower Upper
112 100
64 57.2 39.0 58.6
63 30.0 20.6 30.8

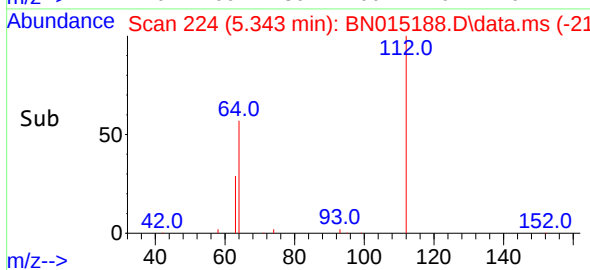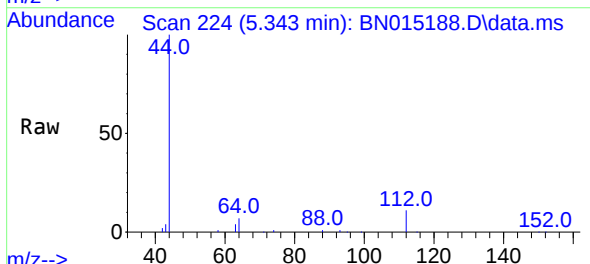







#5
Phenol-d6
Concen: 0.180 ng
RT: 6.902 min Scan# 393
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

Tgt Ion: 99 Resp: 12410
Ion Ratio Lower Upper
99 100
42 18.7 8.9 13.3#
71 32.0 35.6 53.4#

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2




Manual Integrations
APPROVED


mohammad
6/30/2021 2:14:30 PM

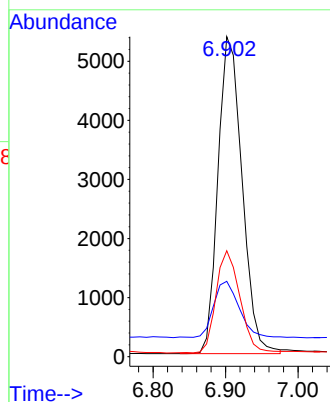

#6
bis(2-Chloroethyl)ether
Concen: 0.215 ng
RT: 7.169 min Scan# 422
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27


Tgt Ion: 93 Resp: 11670
Ion Ratio Lower Upper
93 100
63 77.5 46.6 70.0#
95 32.7 28.6 42.8





#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.505 min Scan# 719
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Tgt Ion: 136 Resp: 78018
Ion Ratio Lower Upper
136 100
137 11.0 9.8 14.8
54 5.4 5.4 8.2#
68 4.4 4.9 7.3#

Manual Integrations
APPROVED



mohammad
6/30/2021 2:14:30 PM




#8
Nitrobenzene-d5
Concen: 0.235 ng
RT: 8.870 min Scan# 590
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27




Tgt Ion: 82 Resp: 13859
Ion Ratio Lower Upper
82 100
128 36.1 31.6 47.4
54 53.0 29.0 43.4#






#9
Naphthalene
Concen: 0.208 ng
RT: 10.543 min Scan# 722
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27




Tgt Ion:	128	Resp:	45525
Ion Ratio	Lower	Upper	
128	100		
129	11.1	9.1	13.7
127	13.3	11.8	17.6




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED



mohammad
6/30/2021 2:14:30 PM




#10
Hexachlorobutadiene
Concen: 0.215 ng
RT: 10.847 min Scan# 746
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27







Tgt Ion:	225	Resp:	9324
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.7	50.2	75.2

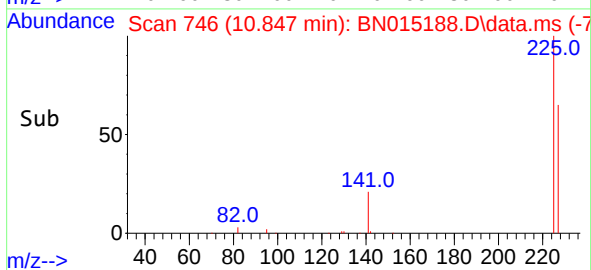

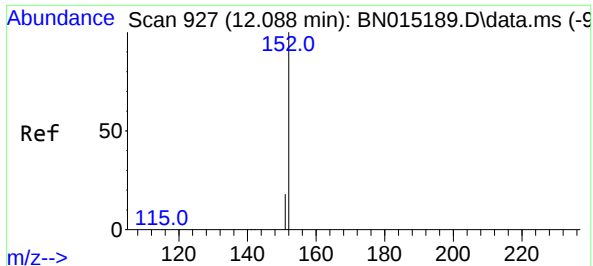




#11
2-Methylnaphthalene-d10
Concen: 0.200 ng
RT: 12.088 min Scan# 927
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

Tgt Ion:152 Resp: 26784
Ion Ratio Lower Upper
152 100
151 20.3 16.7 25.1

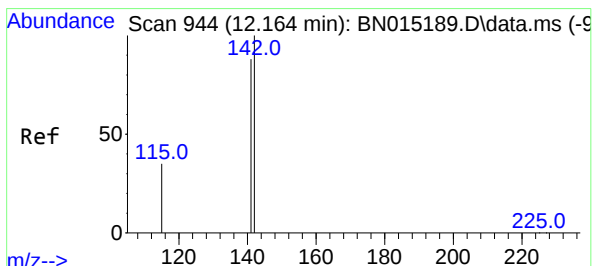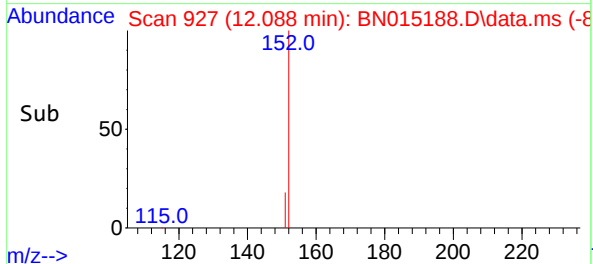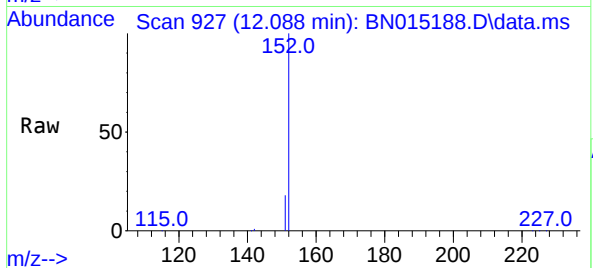

#12
2-Methylnaphthalene
Concen: 0.195 ng
RT: 12.163 min Scan# 944
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27


Tgt Ion:142 Resp: 28643
Ion Ratio Lower Upper
142 100
141 87.9 72.3 108.5
115 35.2 40.7 61.1#

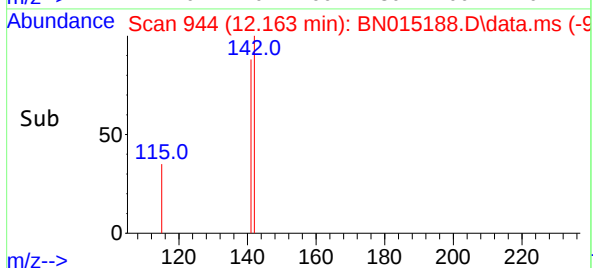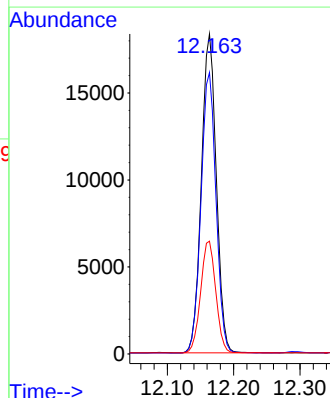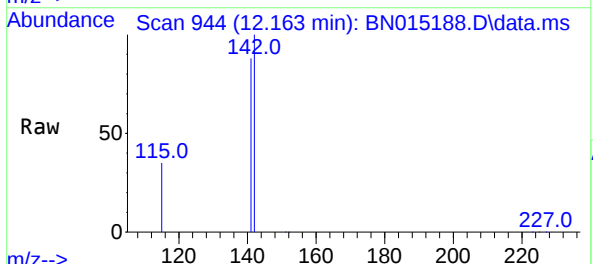

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Manual Integrations
APPROVED

mohammad
6/30/2021 2:14:30 PM



#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.345 min Scan# 1166
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2



Tgt Ion:164 Resp: 36420
Ion Ratio Lower Upper
164 100
162 102.9 83.8 125.6
160 52.9 37.4 56.0




Manual Integrations
APPROVED


mohammad
6/30/2021 2:14:30 PM

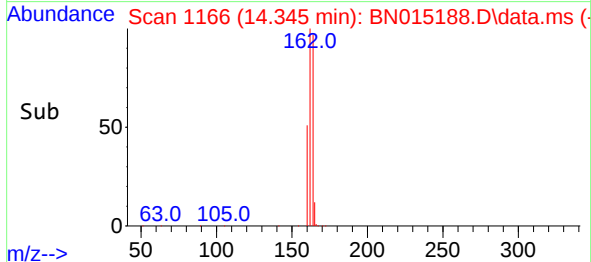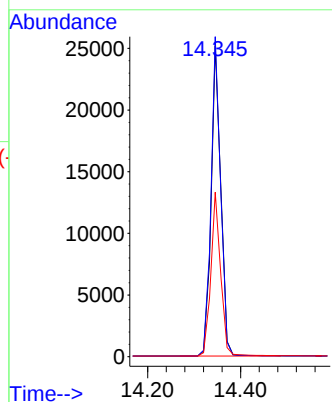


#14
2,4,6-Tribromophenol
Concen: 0.098 ng
RT: 15.843 min Scan# 1284
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

Tgt Ion:330 Resp: 1670
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 39.6 22.4 33.6#

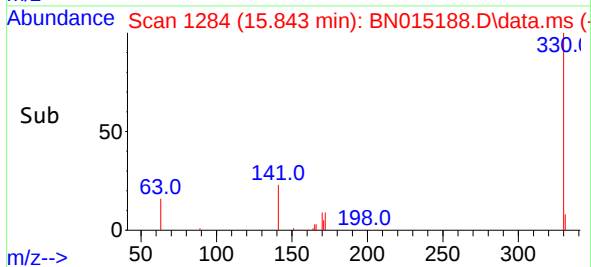

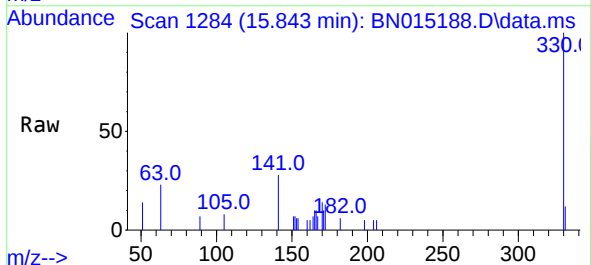





#15
2-Fluorobiphenyl
Concen: 0.227 ng
RT: 12.975 min Scan# 1058
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27





Tgt Ion:172 Resp: 31374
Ion Ratio Lower Upper
172 100
171 33.3 30.6 45.8
170 21.5 20.2 30.4

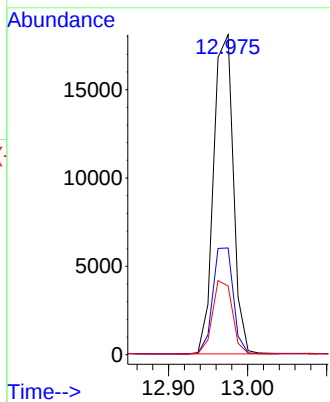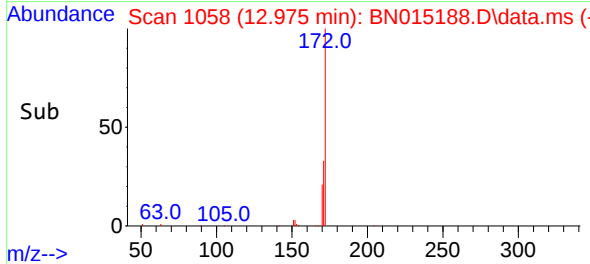

#16
Acenaphthylene
Concen: 0.194 ng
RT: 14.066 min Scan# 1144
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

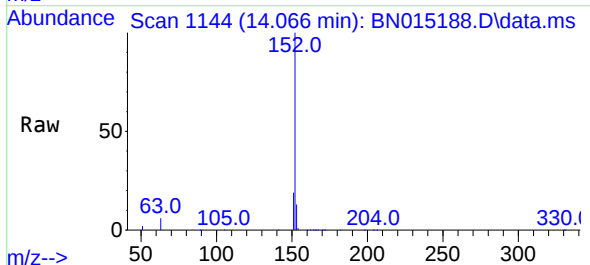


Tgt Ion:152 Resp: 35612
Ion Ratio Lower Upper
152 100
151 19.4 16.7 25.1
153 13.0 10.5 15.7

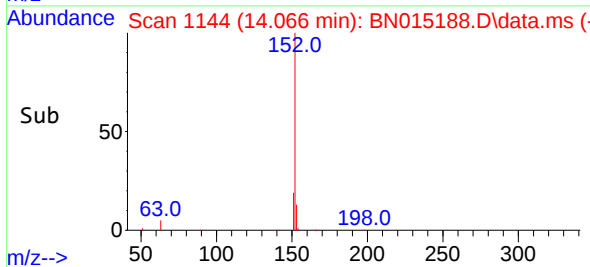

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Manual Integrations
APPROVED

mohammad
6/30/2021 2:14:30 PM



#17
Acenaphthene
Concen: 0.206 ng
RT: 14.409 min Scan# 1171
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2



Tgt Ion:154 Resp: 23246
Ion Ratio Lower Upper
154 100
153 114.1 90.9 136.3
152 63.8 45.8 68.8




Manual Integrations
APPROVED


mohammad
6/30/2021 2:14:30 PM

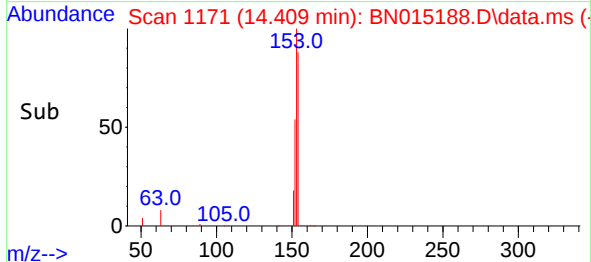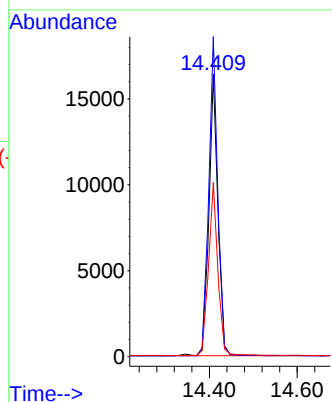


#18
Fluorene
Concen: 0.193 ng
RT: 15.399 min Scan# 1249
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

Tgt Ion:166 Resp: 26764
Ion Ratio Lower Upper
166 100
165 98.3 79.2 118.8
167 13.5 10.7 16.1

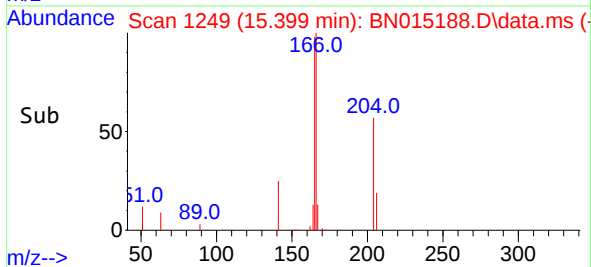
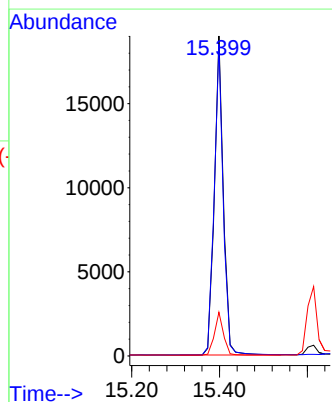
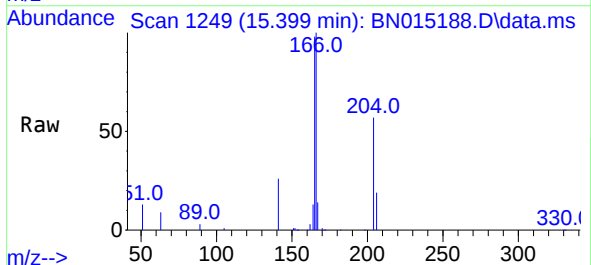





#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.091 min Scan# 1386
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27





Tgt Ion:188 Resp: 64589
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 11.9 9.0 13.4



#21
4-Bromophenyl-phenylether
Concen: 0.198 ng
RT: 16.288 min Scan# 1320
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27




Tgt Ion:248 Resp: 8252
Ion Ratio Lower Upper
248 100
250 92.8 86.2 129.4
141 73.0 36.2 54.2#

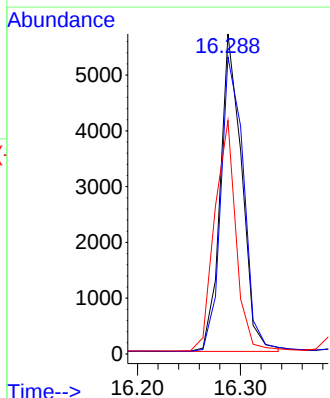

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Manual Integrations
APPROVED

mohammad
6/30/2021 2:14:30 PM



#22
Hexachlorobenzene
Concen: 0.250 ng
RT: 16.410 min Scan# 1330
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Tgt Ion:284 Resp: 11008
Ion Ratio Lower Upper
284 100
142 35.4 22.2 33.2#
249 30.7 26.6 39.8

Manual Integrations
APPROVED



mohammad
6/30/2021 2:14:30 PM

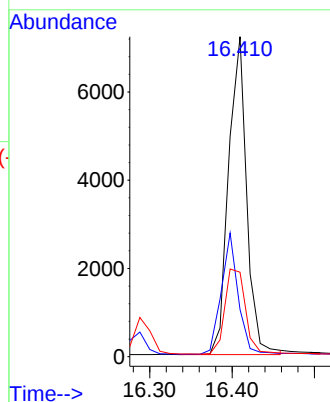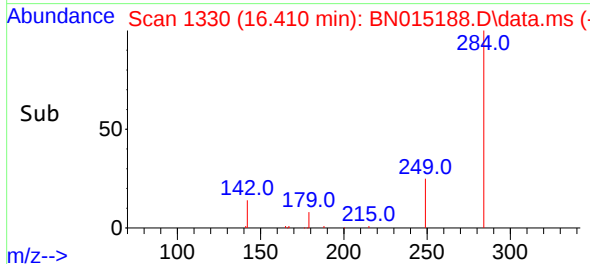


#23
Atrazine
Concen: 0.091 ng
RT: 16.556 min Scan# 1342
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

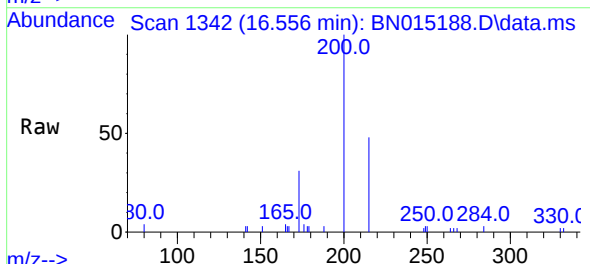


Tgt Ion:200 Resp: 3397
Ion Ratio Lower Upper
200 100
173 31.3 21.7 32.5
215 47.7 43.1 64.7









#24
Pentachlorophenol
Concen: 0.026 ng
RT: 16.750 min Scan# 1358
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27





Tgt Ion:266 Resp: 428
Ion Ratio Lower Upper
266 100
264 61.9 51.0 76.4
268 64.3 50.6 76.0

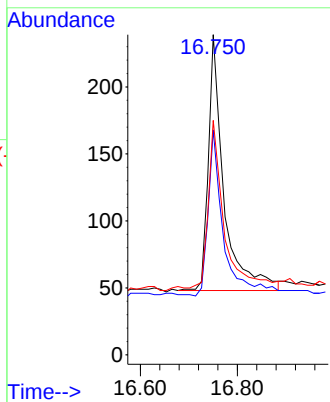

#25
Phenanthrene
Concen: 0.219 ng
RT: 17.140 min Scan# 1390
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

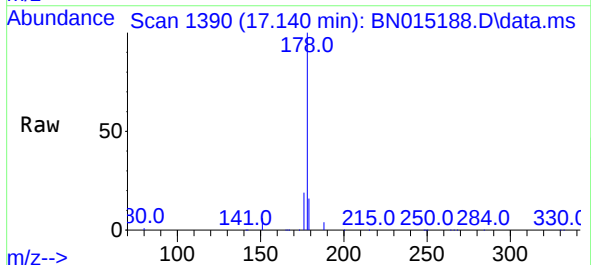


Tgt Ion:178 Resp: 43082
Ion Ratio Lower Upper
178 100
176 19.0 15.6 23.4
179 15.7 12.1 18.1

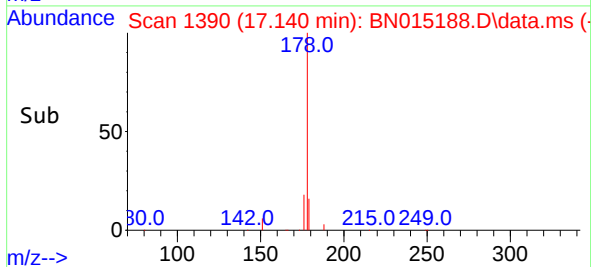

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Manual Integrations
APPROVED

mohammad
6/30/2021 2:14:30 PM



#26
 Anthracene
 Concen: 0.176 ng
 RT: 17.225 min Scan# 1397
 Delta R.T. -0.000 min
 Lab File: BN015188.D
 Acq: 29 Jun 2021 15:27




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2




Tgt Ion:178 Resp: 33962
 Ion Ratio Lower Upper
 178 100
 176 18.4 15.1 22.7
 179 15.3 12.2 18.2

Manual Integrations
 APPROVED



mohammad
 6/30/2021 2:14:30 PM

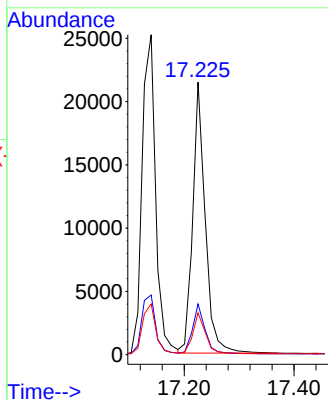


#27
 Fluoranthene-d10
 Concen: 0.187 ng
 RT: 19.138 min Scan# 1688
 Delta R.T. 0.005 min
 Lab File: BN015188.D
 Acq: 29 Jun 2021 15:27

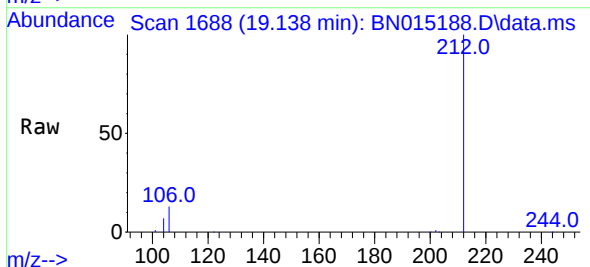


Tgt Ion:212 Resp: 38154
 Ion Ratio Lower Upper
 212 100
 106 14.1 7.0 10.6#
 104 7.8 4.1 6.1#


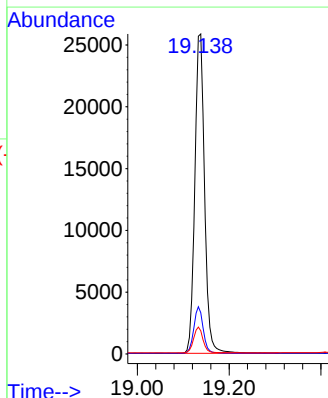






#28
Fluoranthene
Concen: 0.200 ng
RT: 19.168 min Scan# 1694
Delta R.T. 0.005 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27





Tgt Ion:202 Resp: 44736
Ion Ratio Lower Upper
202 100
101 11.6 6.6 10.0#
203 17.2 13.9 20.9

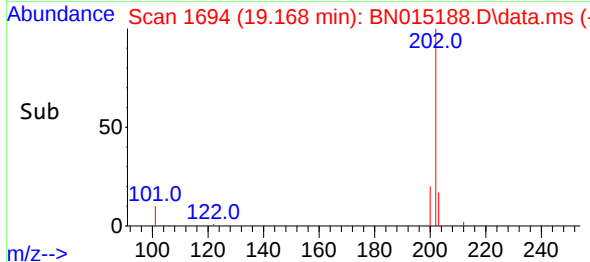

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.302 min Scan# 1985
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

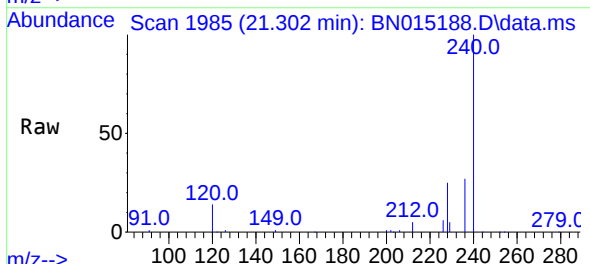


Tgt Ion:240 Resp: 60798
Ion Ratio Lower Upper
240 100
120 14.0 4.2 6.4#
236 27.2 21.4 32.2

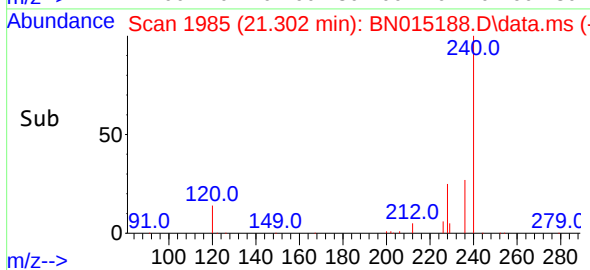

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED

mohammad
6/30/2021 2:14:30 PM







#30
Pyrene
Concen: 0.175 ng
RT: 19.530 min Scan# 1767
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

Tgt Ion:	202	Resp:	42253
Ion Ratio	Lower	Upper	
202	100		
200	20.5	16.9	25.3
203	17.4	13.9	20.9

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2




Manual Integrations
APPROVED


mohammad
6/30/2021 2:14:30 PM




#31
Terphenyl-d14
Concen: 0.172 ng
RT: 19.744 min Scan# 1810
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

Tgt Ion:	244	Resp:	25892
Ion Ratio	Lower	Upper	
244	100		
212	8.0	6.3	9.5
122	12.1	6.2	9.2#

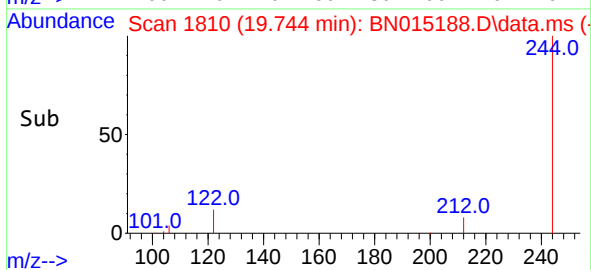




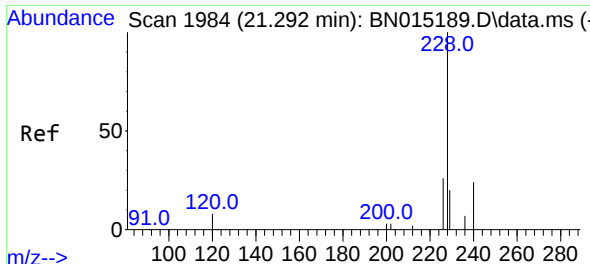


#32
Benzo(a)anthracene
Concen: 0.166 ng
RT: 21.292 min Scan# 1984
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27





Tgt Ion:228 Resp: 37952
Ion Ratio Lower Upper
228 100
226 26.5 23.0 34.6
229 19.4 15.7 23.5



#33
Chrysene
Concen: 0.211 ng
RT: 21.345 min Scan# 1989
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

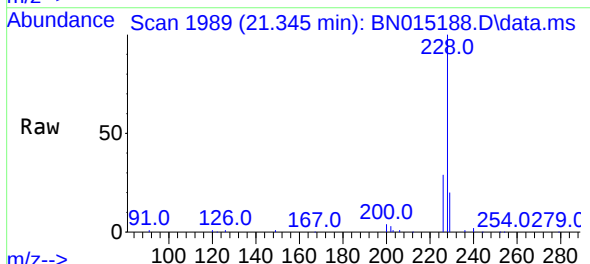


Tgt Ion:228 Resp: 46357
Ion Ratio Lower Upper
228 100
226 29.2 25.0 37.6
229 19.9 15.9 23.9

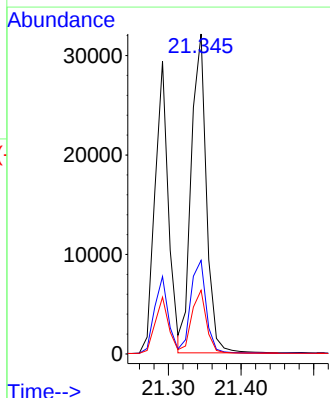

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Manual Integrations
APPROVED

mohammad
6/30/2021 2:14:30 PM

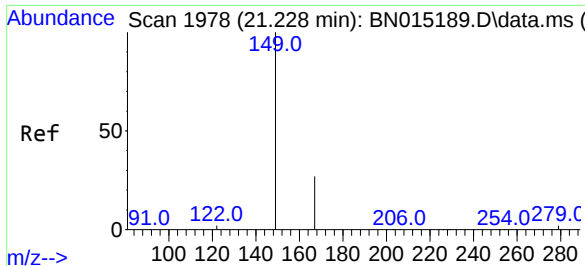

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.060 ng
RT: 21.228 min Scan# 1978
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

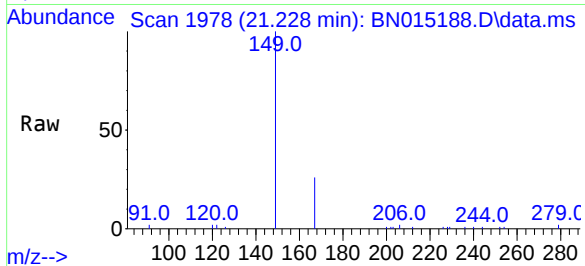

Tgt Ion:149 Resp: 9670
Ion Ratio Lower Upper
149 100
167 26.2 28.9 43.3#
279 3.2 4.9 7.3#




Manual Integrations
APPROVED


mohammad
6/30/2021 2:14:30 PM

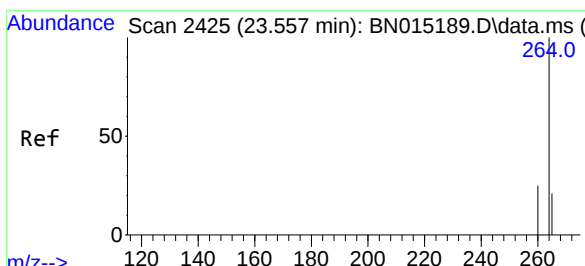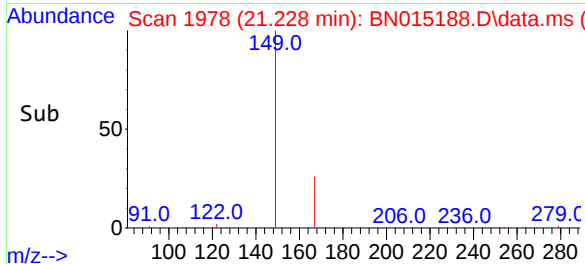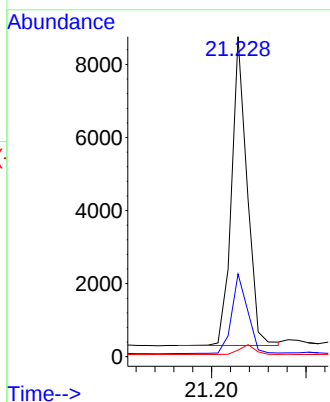

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.557 min Scan# 2425
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

Tgt Ion:264 Resp: 62225
Ion Ratio Lower Upper
264 100
260 25.2 20.6 31.0
265 23.7 21.4 32.2

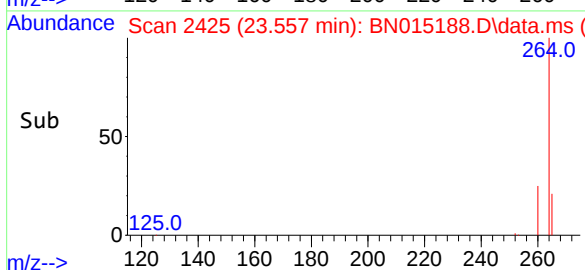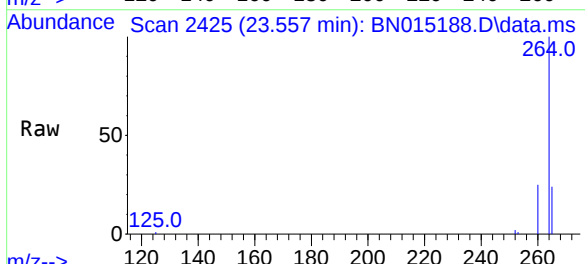







#36
 Indeno(1,2,3-cd)pyrene
 Concen: 0.235 ng
 RT: 25.819 min Scan# 3086
 Delta R.T. 0.003 min
 Lab File: BN015188.D
 Acq: 29 Jun 2021 15:27

Tgt Ion: 276 Resp: 48884
 Ion Ratio Lower Upper
 276 100
 138 25.4 10.0 15.0#
 277 24.9 20.4 30.6

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2




Manual Integrations
 APPROVED


mohammad
 6/30/2021 2:14:30 PM

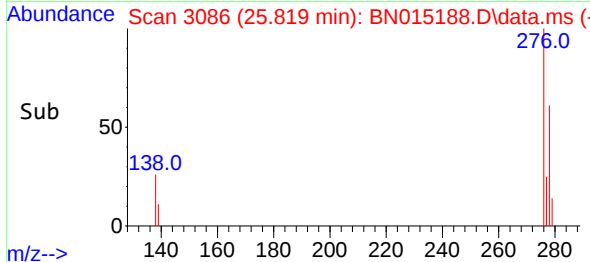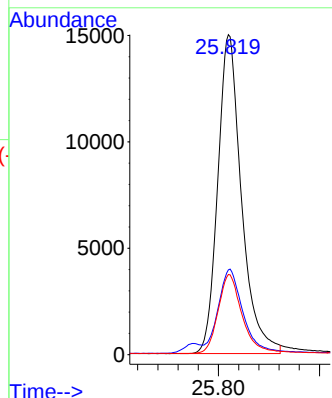


#37
 Benzo(b)fluoranthene
 Concen: 0.199 ng
 RT: 22.886 min Scan# 2229
 Delta R.T. 0.003 min
 Lab File: BN015188.D
 Acq: 29 Jun 2021 15:27

Tgt Ion: 252 Resp: 46356
 Ion Ratio Lower Upper
 252 100
 253 22.6 18.5 27.7
 125 16.6 5.8 8.6#

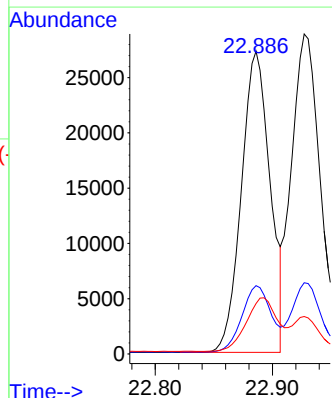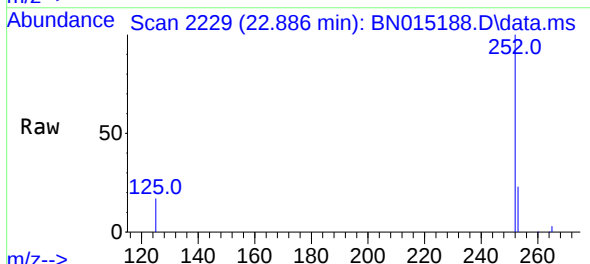




#38
Benzo(k)fluoranthene
Concen: 0.230 ng
RT: 22.927 min Scan# 2241
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27




Tgt Ion:252 Resp: 51837
Ion Ratio Lower Upper
252 100
253 22.3 19.1 28.7
125 11.7 5.4 8.0#




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED



mohammad
6/30/2021 2:14:30 PM




#39
Benzo(a)pyrene
Concen: 0.213 ng
RT: 23.461 min Scan# 2397
Delta R.T. 0.003 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

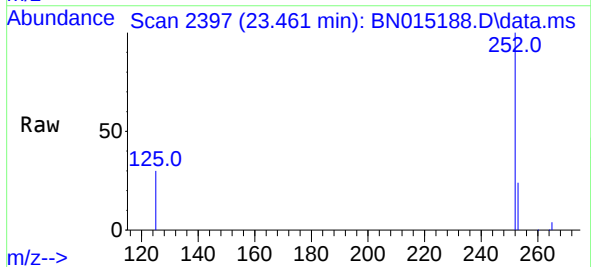

Tgt Ion:252 Resp: 43763
Ion Ratio Lower Upper
252 100
253 24.5 19.4 29.2
125 29.7 7.4 11.2#

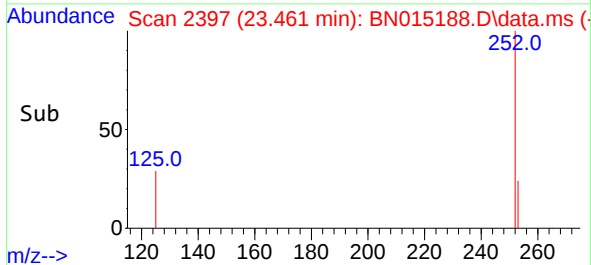







#40
Dibenzo(a,h)anthracene
Concen: 0.232 ng
RT: 25.833 min Scan# 3090
Delta R.T. -0.000 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

Tgt Ion: 278 Resp: 38966
Ion Ratio Lower Upper
278 100
139 18.5 9.0 13.4#
279 23.7 21.0 31.4

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED

mohammad
6/30/2021 2:14:30 PM

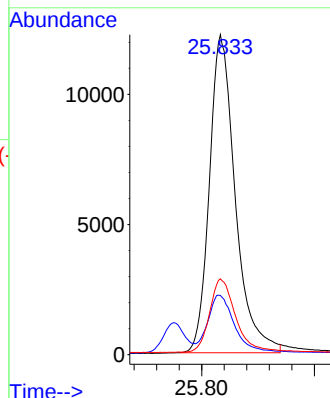

#41
Benzo(g,h,i)perylene
Concen: 0.220 ng
RT: 26.507 min Scan# 3287
Delta R.T. 0.003 min
Lab File: BN015188.D
Acq: 29 Jun 2021 15:27

Tgt Ion: 276 Resp: 39610
Ion Ratio Lower Upper
276 100
277 23.8 19.7 29.5
138 23.8 9.8 14.6#

