

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062921\  
 Data File : BN015205.D  
 Acq On : 30 Jun 2021 02:58  
 Operator : CG/JU  
 Sample : M2783-07  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 RE114D2-20210617

Manual Integrations  
 APPROVED

mohammad  
 6/30/2021 2:15:09 PM

Quant Time: Jun 30 06:20:18 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN062921.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jun 29 19:13:09 2021  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc  | Units | Dev(Min) |
|-------------------------------|--------|------|----------|-------|-------|----------|
| -----                         |        |      |          |       |       |          |
| Internal Standards            |        |      |          |       |       |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.732  | 152  | 17344    | 0.400 | ng    | # 0.00   |
| 7) Naphthalene-d8             | 10.493 | 136  | 78530    | 0.400 | ng    | #-0.01   |
| 13) Acenaphthene-d10          | 14.346 | 164  | 36964    | 0.400 | ng    | 0.00     |
| 19) Phenanthrene-d10          | 17.092 | 188  | 73985    | 0.400 | ng    | 0.00     |
| 29) Chrysene-d12              | 21.292 | 240  | 66230    | 0.400 | ng    | #-0.01   |
| 35) Perylene-d12              | 23.540 | 264  | 54980    | 0.400 | ng    | -0.02    |
|                               |        |      |          |       |       |          |
| System Monitoring Compounds   |        |      |          |       |       |          |
| 4) 2-Fluorophenol             | 5.371  | 112  | 5146     | 0.137 | ng    | 0.03     |
| 5) Phenol-d6                  | 6.911  | 99   | 4760     | 0.083 | ng    | 0.00     |
| 8) Nitrobenzene-d5            | 8.870  | 82   | 27395    | 0.382 | ng    | 0.00     |
| 11) 2-Methylnaphthalene-d10   | 12.088 | 152  | 44607    | 0.346 | ng    | 0.00     |
| 14) 2,4,6-Tribromophenol      | 15.843 | 330  | 2710     | 0.350 | ng    | 0.00     |
| 15) 2-Fluorobiphenyl          | 12.963 | 172  | 68855    | 0.444 | ng    | -0.01    |
| 27) Fluoranthene-d10          | 19.128 | 212  | 84122    | 0.374 | ng    | 0.00     |
| 31) Terphenyl-d14             | 19.734 | 244  | 78219    | 0.535 | ng    | 0.00     |
|                               |        |      |          |       |       |          |
| Target Compounds              |        |      |          |       |       | Qvalue   |
| 2) 1,4-Dioxane                | 3.352  | 88   | 14595m   | 2.899 | ng    |          |
| 34) Bis(2-ethylhexyl)phtha... | 21.218 | 149  | 5136     | 0.301 | ng    | # 85     |
| -----                         |        |      |          |       |       |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062921\  
Data File : BN015205.D  
Acq On : 30 Jun 2021 02:58  
Operator : CG/JU  
Sample : M2783-07  
Misc :  
ALS Vial : 21 Sample Multiplier: 1


Instrument :  
BNA\_N  
ClientSampleId :  
RE114D2-20210617

Manual Integrations  
APPROVED


mohammad  
6/30/2021 2:15:09 PM

Quant Time: Jun 30 06:20:18 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN062921.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 29 19:13:09 2021  
Response via : Initial Calibration



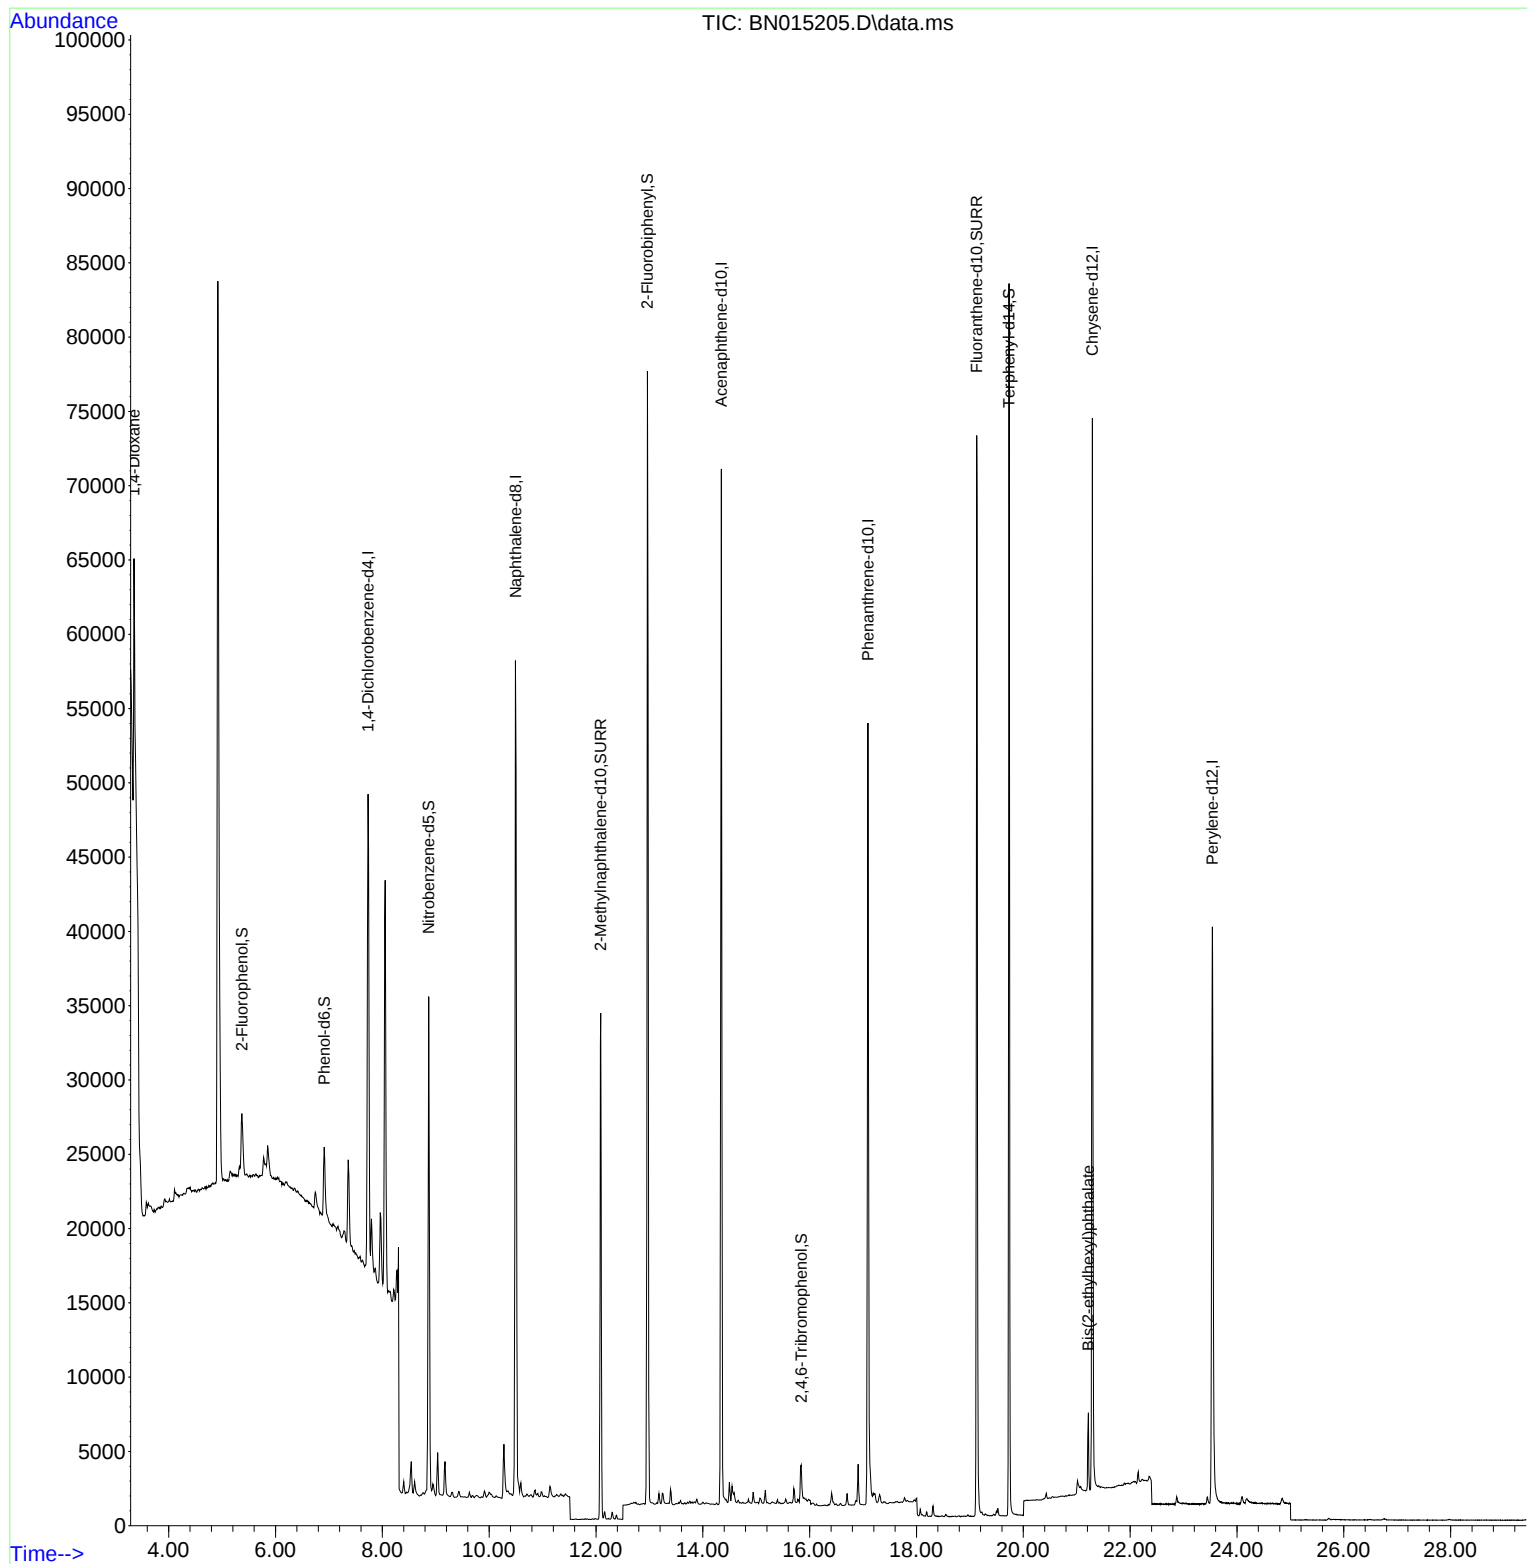


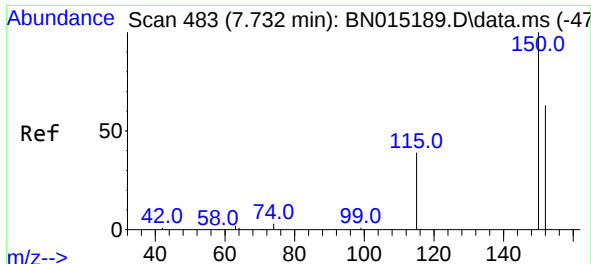


#1  
1,4-Dichlorobenzene-d4  
Concen: 0.400 ng  
RT: 7.732 min Scan# 483  
Delta R.T. -0.000 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58





Tgt Ion:152 Resp: 17344  
Ion Ratio Lower Upper  
152 100  
150 157.6 119.0 178.6  
115 62.1 62.2 93.4#

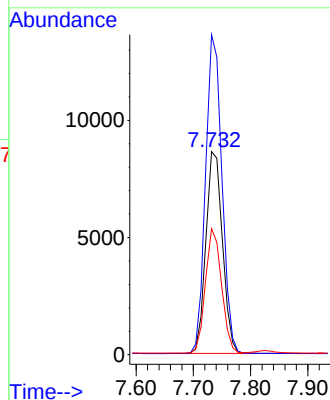

#2  
1,4-Dioxane  
Concen: 2.899 ng m  
RT: 3.352 min Scan# 8  
Delta R.T. -0.000 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58

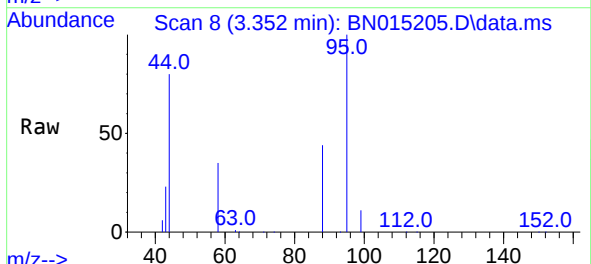


Tgt Ion: 88 Resp: 14595  
Ion Ratio Lower Upper  
88 100  
43 56.5 12.9 19.3#  
58 151.5 38.1 57.1#

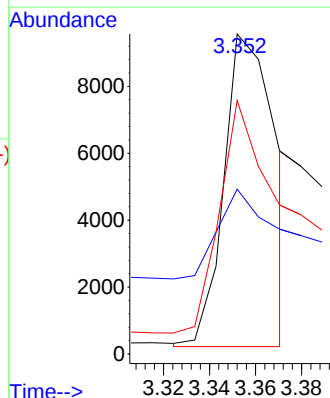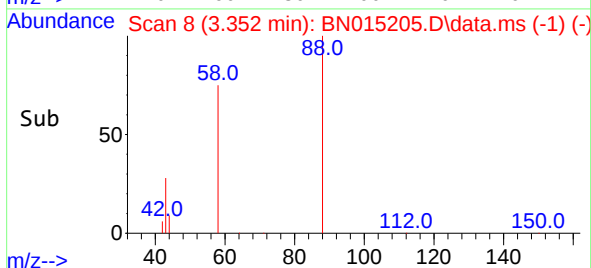

Instrument :  
BNA\_N  
ClientSampleId :  
RE114D2-20210617

Manual Integrations  
APPROVED

mohammad  
6/30/2021 2:15:09 PM

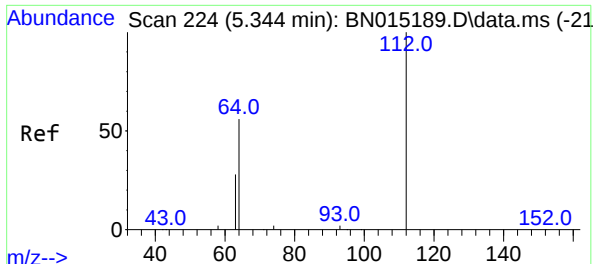





#4  
2-Fluorophenol  
Concen: 0.137 ng  
RT: 5.371 min Scan# 227  
Delta R.T. 0.028 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58

Tgt Ion: 112 Resp: 5146  
Ion Ratio Lower Upper  
112 100  
64 57.4 39.0 58.6  
63 30.9 20.6 30.8#

Instrument :  
BNA\_N  
ClientSampleId :  
RE114D2-20210617




Manual Integrations  
APPROVED


mohammad  
6/30/2021 2:15:09 PM

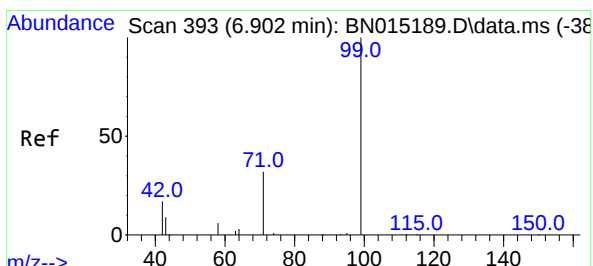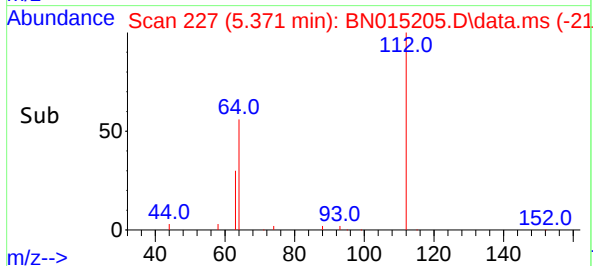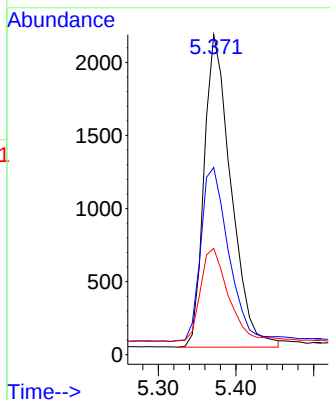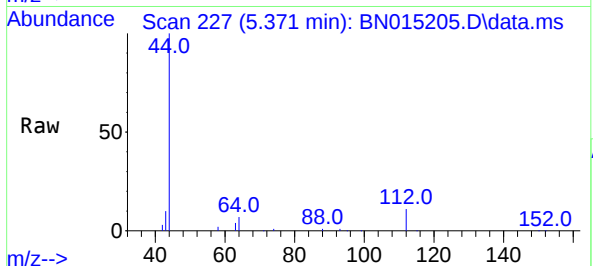

#5  
Phenol-d6  
Concen: 0.083 ng  
RT: 6.911 min Scan# 394  
Delta R.T. 0.009 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58


Tgt Ion: 99 Resp: 4760  
Ion Ratio Lower Upper  
99 100  
42 18.1 8.9 13.3#  
71 37.8 35.6 53.4

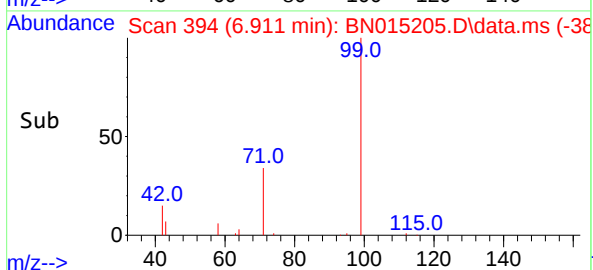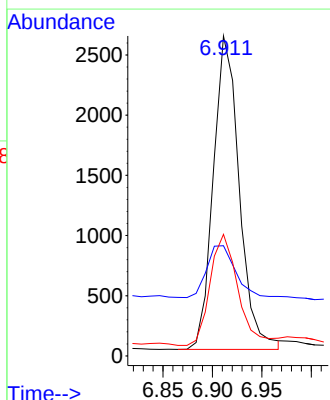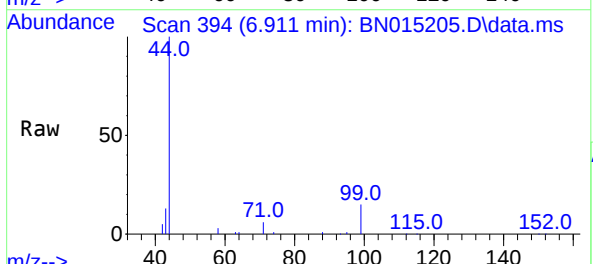



#7  
Naphthalene-d8  
Concen: 0.400 ng  
RT: 10.493 min Scan# 718  
Delta R.T. -0.013 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58




Instrument :  
BNA\_N  
ClientSampleId :  
RE114D2-20210617

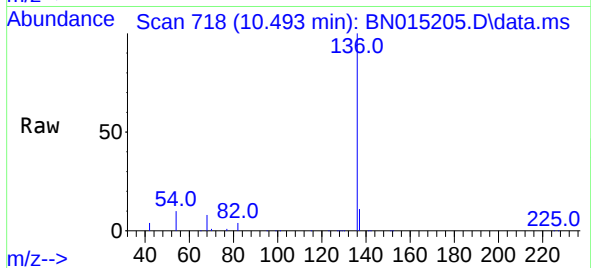

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 136   | Resp: | 78530 |
| Ion      | Ratio | Lower | Upper |
| 136      | 100   |       |       |
| 137      | 11.0  | 9.8   | 14.8  |
| 54       | 10.4  | 5.4   | 8.2#  |
| 68       | 7.8   | 4.9   | 7.3#  |




Manual Integrations  
APPROVED


mohammad  
6/30/2021 2:15:09 PM

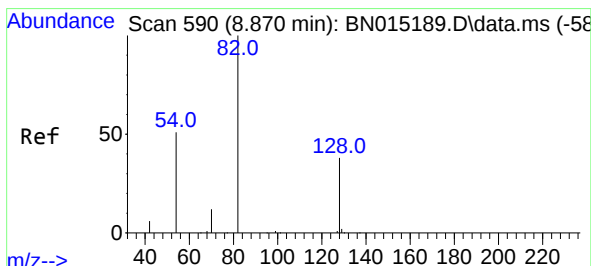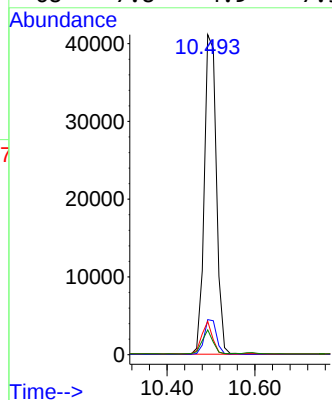

#8  
Nitrobenzene-d5  
Concen: 0.382 ng  
RT: 8.870 min Scan# 590  
Delta R.T. -0.000 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 82    | Resp: | 27395 |
| Ion      | Ratio | Lower | Upper |
| 82       | 100   |       |       |
| 128      | 37.4  | 31.6  | 47.4  |
| 54       | 51.0  | 29.0  | 43.4# |

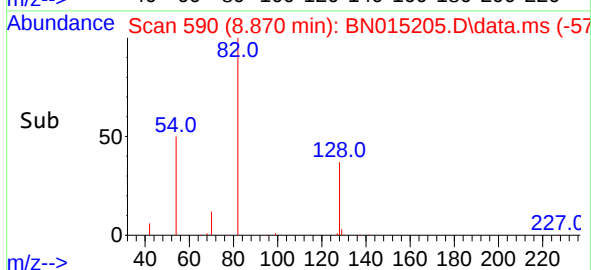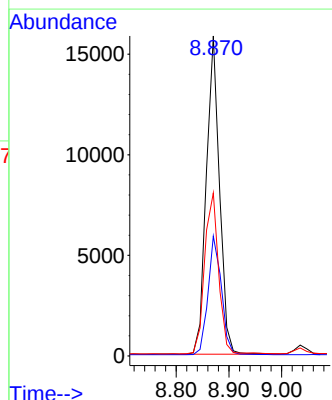


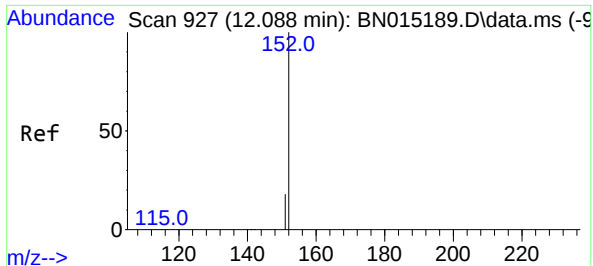


#11  
2-Methylnaphthalene-d10  
Concen: 0.346 ng  
RT: 12.088 min Scan# 927  
Delta R.T. -0.000 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58


Instrument :  
BNA\_N  
ClientSampleId :  
RE114D2-20210617

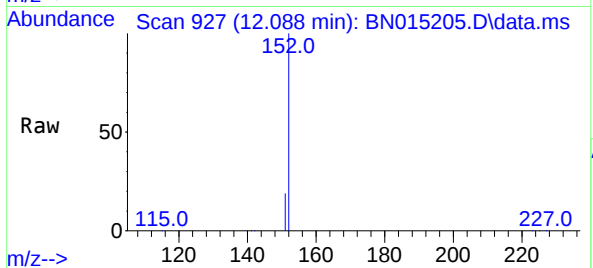



Tgt Ion:152 Resp: 44607  
Ion Ratio Lower Upper  
152 100  
151 20.3 16.7 25.1

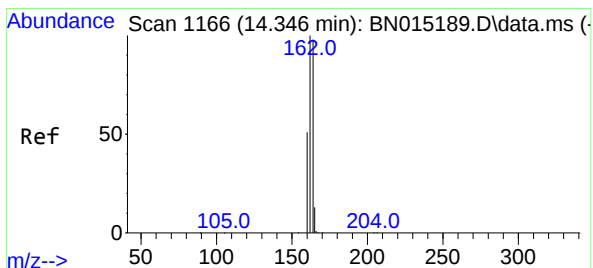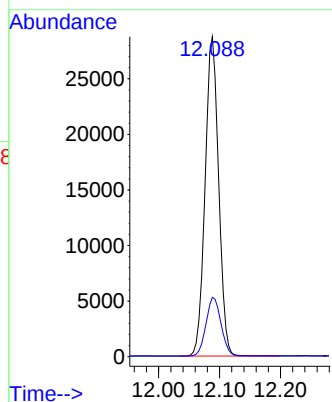


#13  
Acenaphthene-d10  
Concen: 0.400 ng  
RT: 14.346 min Scan# 1166  
Delta R.T. -0.000 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58

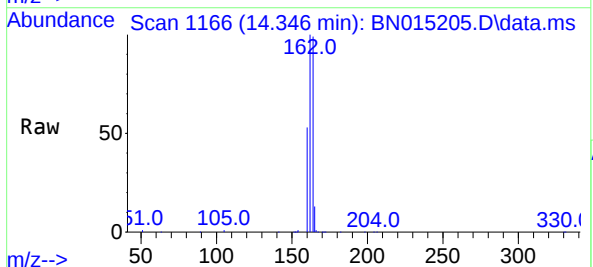


Tgt Ion:164 Resp: 36964  
Ion Ratio Lower Upper  
164 100  
162 101.0 83.8 125.6  
160 53.3 37.4 56.0

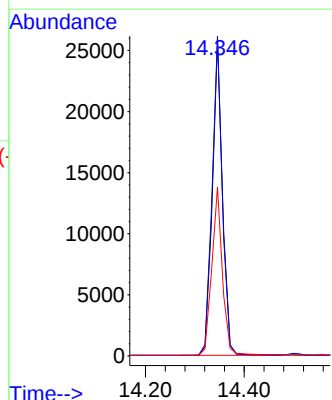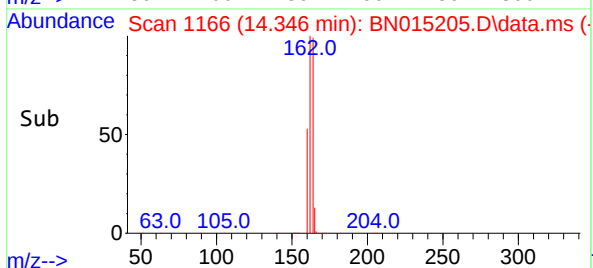

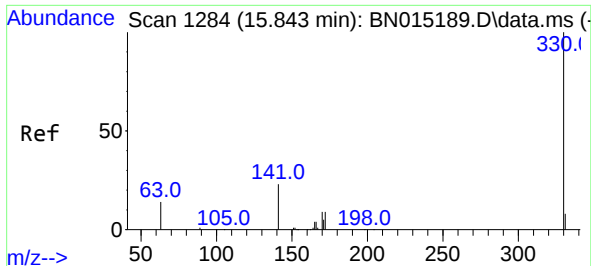

#14  
2,4,6-Tribromophenol  
Concen: 0.350 ng  
RT: 15.843 min Scan# 1284  
Delta R.T. -0.000 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58




Instrument :  
BNA\_N  
ClientSampleId :  
RE114D2-20210617

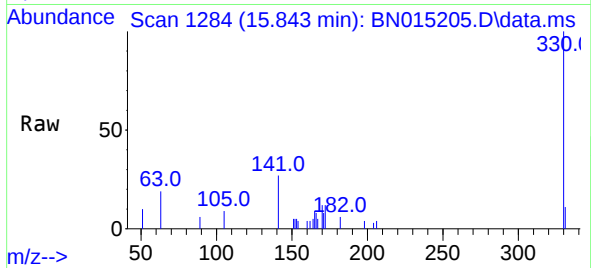


Tgt Ion:330 Resp: 2710  
Ion Ratio Lower Upper  
330 100  
332 0.0 0.0 0.0  
141 39.7 22.4 33.6#

Manual Integrations  
APPROVED



mohammad  
6/30/2021 2:15:09 PM

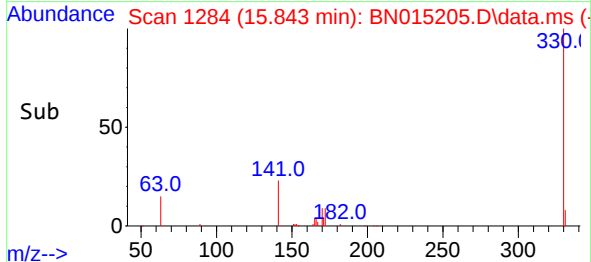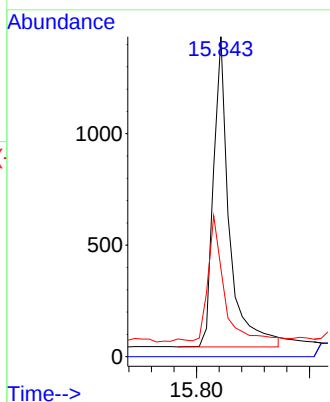


#15  
2-Fluorobiphenyl  
Concen: 0.444 ng  
RT: 12.963 min Scan# 1057  
Delta R.T. -0.013 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58

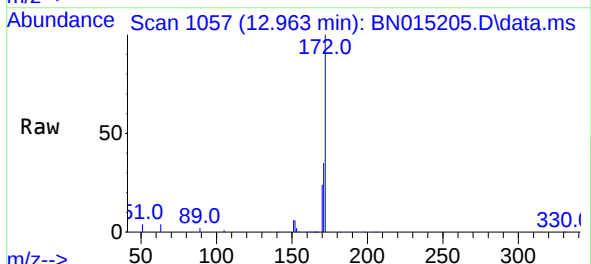

Tgt Ion:172 Resp: 68855  
Ion Ratio Lower Upper  
172 100  
171 35.1 30.6 45.8  
170 24.1 20.2 30.4

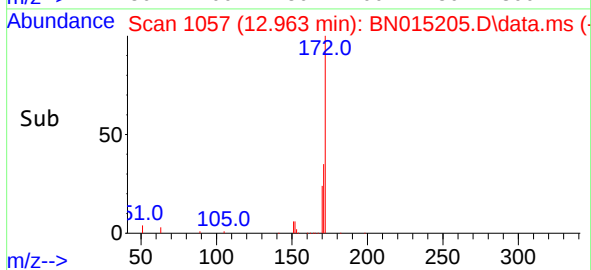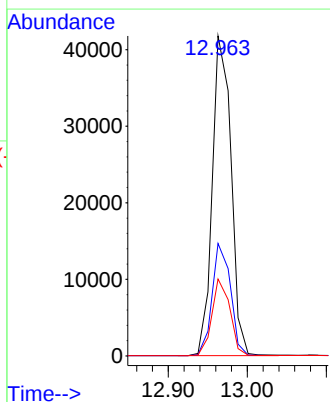







#19  
Phenanthrene-d10  
Concen: 0.400 ng  
RT: 17.092 min Scan# 1386  
Delta R.T. -0.000 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58

Tgt Ion:188 Resp: 73985  
Ion Ratio Lower Upper  
188 100  
94 0.0 0.0 0.0  
80 10.9 9.0 13.4

Instrument :  
BNA\_N  
ClientSampleId :  
RE114D2-20210617




Manual Integrations  
APPROVED


mohammad  
6/30/2021 2:15:09 PM

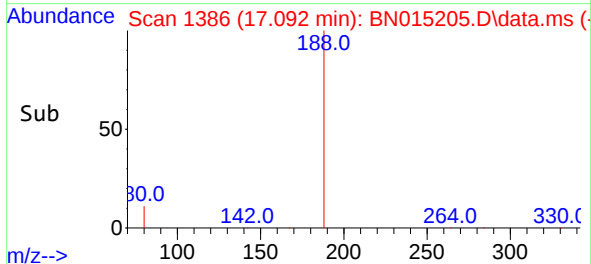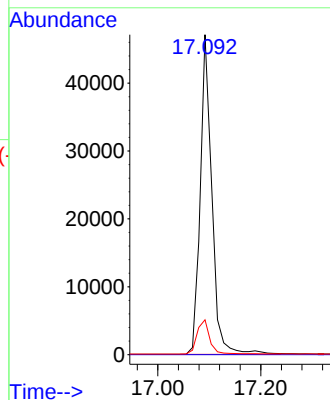

#27  
Fluoranthene-d10  
Concen: 0.374 ng  
RT: 19.128 min Scan# 1686  
Delta R.T. -0.005 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58

Tgt Ion:212 Resp: 84122  
Ion Ratio Lower Upper  
212 100  
106 13.9 7.0 10.6#  
104 7.9 4.1 6.1#

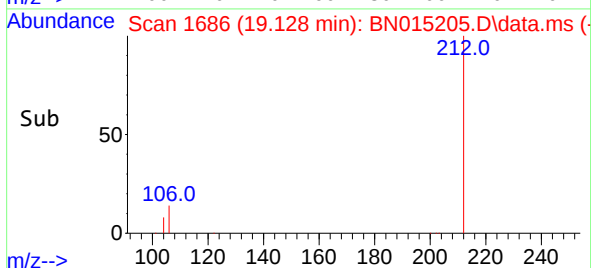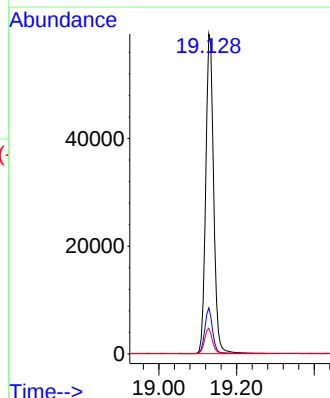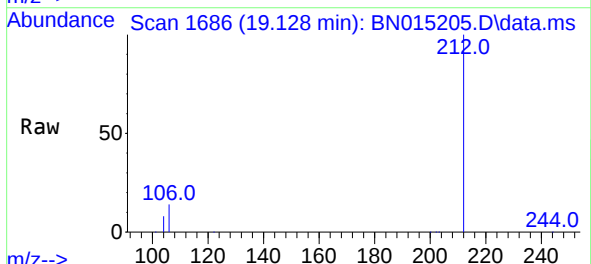

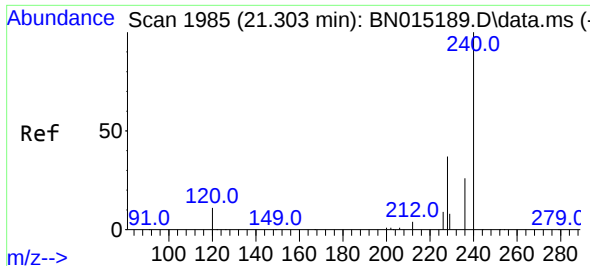





#29  
Chrysene-d12  
Concen: 0.400 ng  
RT: 21.292 min Scan# 1984  
Delta R.T. -0.011 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58

Tgt Ion:240 Resp: 66230  
Ion Ratio Lower Upper  
240 100  
120 9.2 4.2 6.4#  
236 26.4 21.4 32.2

Instrument :  
BNA\_N  
ClientSampleId :  
RE114D2-20210617




Manual Integrations  
APPROVED


mohammad  
6/30/2021 2:15:09 PM

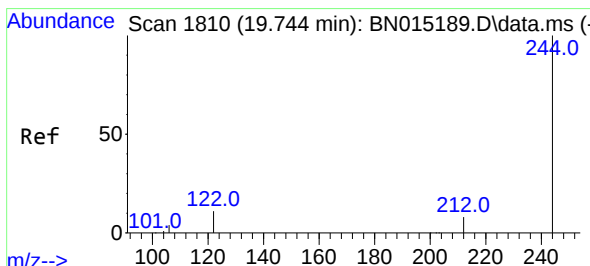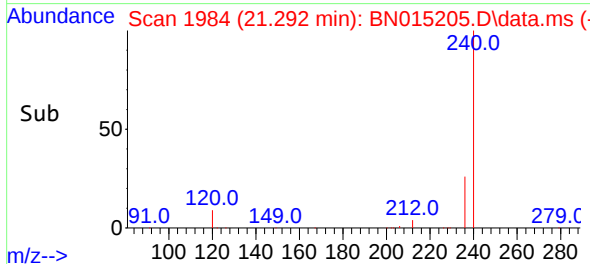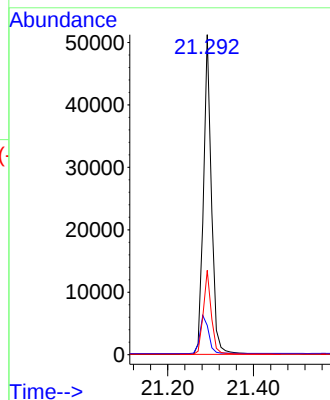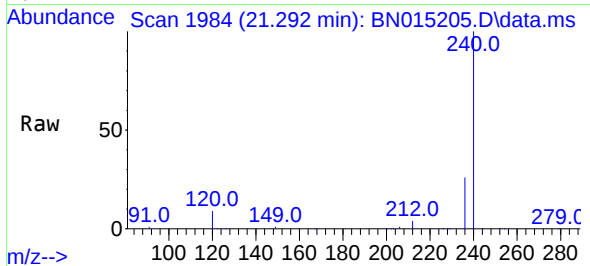

#31  
Terphenyl-d14  
Concen: 0.535 ng  
RT: 19.734 min Scan# 1808  
Delta R.T. -0.010 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58

Tgt Ion:244 Resp: 78219  
Ion Ratio Lower Upper  
244 100  
212 7.9 6.3 9.5  
122 13.0 6.2 9.2#

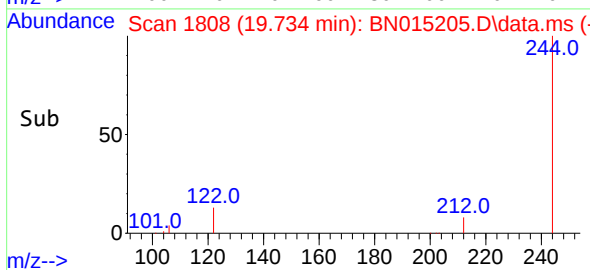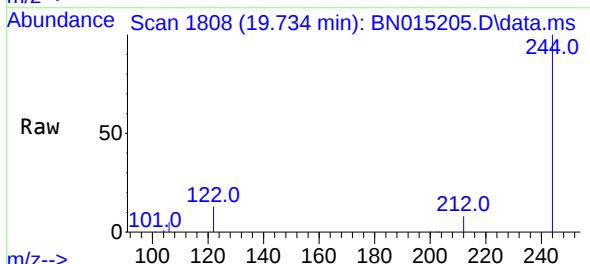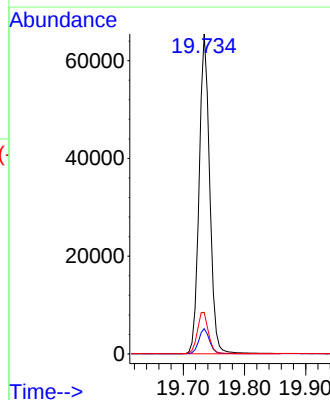

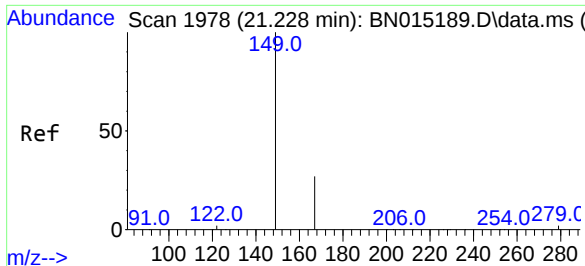





#34  
Bis(2-ethylhexyl)phthalate  
Concen: 0.301 ng  
RT: 21.218 min Scan# 1977  
Delta R.T. -0.010 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58

Tgt Ion:149 Resp: 5136  
Ion Ratio Lower Upper  
149 100  
167 26.5 28.9 43.3#  
279 3.2 4.9 7.3#

Instrument :  
BNA\_N  
ClientSampleId :  
RE114D2-20210617

Manual Integrations  
APPROVED

mohammad  
6/30/2021 2:15:09 PM

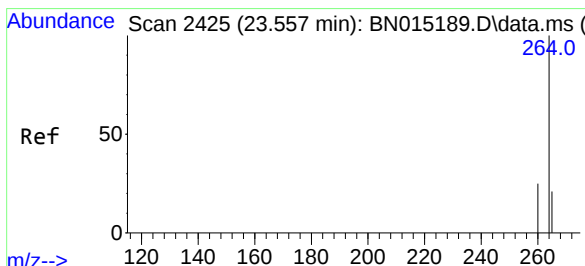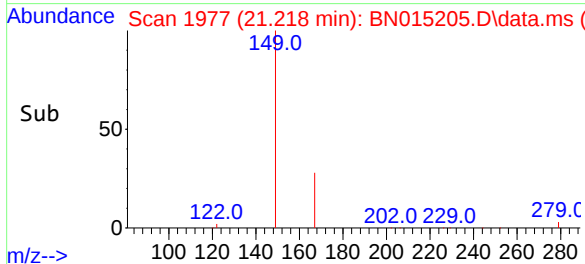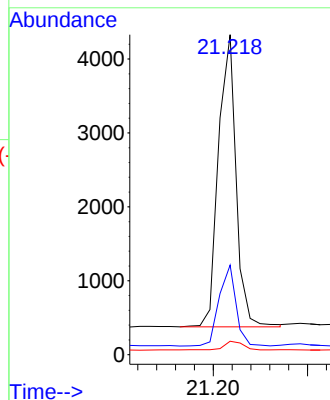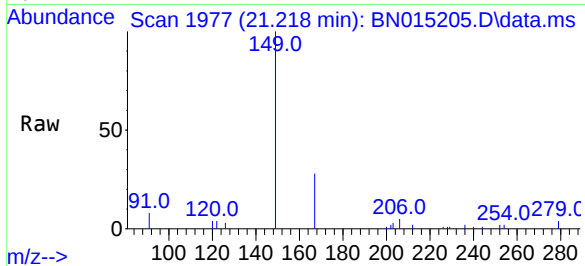

#35  
Perylene-d12  
Concen: 0.400 ng  
RT: 23.540 min Scan# 2420  
Delta R.T. -0.017 min  
Lab File: BN015205.D  
Acq: 30 Jun 2021 02:58

Tgt Ion:264 Resp: 54980  
Ion Ratio Lower Upper  
264 100  
260 24.8 20.6 31.0  
265 23.2 21.4 32.2

