

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062921\
 Data File : BN015214.D
 Acq On : 30 Jun 2021 08:57
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Jun 30 09:34:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 29 19:13:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.731	152	19594	0.400	ng	# 0.00
7) Naphthalene-d8	10.492	136	90606	0.400	ng	#-0.01
13) Acenaphthene-d10	14.346	164	43686	0.400	ng	0.00
19) Phenanthrene-d10	17.091	188	78743	0.400	ng	0.00
29) Chrysene-d12	21.292	240	79165	0.400	ng	#-0.01
35) Perylene-d12	23.547	264	74924	0.400	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.362	112	12261	0.289	ng	0.02
5) Phenol-d6	6.902	99	21580	0.333	ng	0.00
8) Nitrobenzene-d5	8.870	82	28882	0.349	ng	0.00
11) 2-Methylnaphthalene-d10	12.088	152	53533	0.360	ng	0.00
14) 2,4,6-Tribromophenol	15.843	330	3543	0.367	ng	0.00
15) 2-Fluorobiphenyl	12.963	172	68323	0.373	ng	-0.01
27) Fluoranthene-d10	19.133	212	78651	0.329	ng	0.00
31) Terphenyl-d14	19.734	244	62661	0.358	ng	-0.01
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.352	88	1980	0.348	ng	# 58
3) n-Nitrosodimethylamine	3.693	42	3548	0.308	ng	# 58
6) bis(2-Chloroethyl)ether	7.169	93	23206	0.374	ng	# 83
9) Naphthalene	10.543	128	97787	0.374	ng	97
10) Hexachlorobutadiene	10.834	225	20281	0.386	ng	# 99
12) 2-Methylnaphthalene	12.159	142	62189	0.374	ng	# 91
16) Acenaphthylene	14.066	152	78910	0.353	ng	98
17) Acenaphthene	14.409	154	51165	0.367	ng	96
18) Fluorene	15.399	166	62927	0.374	ng	99
20) 4,6-Dinitro-2-methylph...	15.475	198	327	0.403	ng	88
21) 4-Bromophenyl-phenylether	16.288	248	18992	0.349	ng	# 84
22) Hexachlorobenzene	16.410	284	25318	0.390	ng	# 91
23) Atrazine	16.556	200	6308	0.314	ng	93
24) Pentachlorophenol	16.750	266	2045	0.520	ng	99
25) Phenanthrene	17.128	178	99554	0.371	ng	99
26) Anthracene	17.225	178	79133	0.338	ng	99
28) Fluoranthene	19.163	202	107853	0.371	ng	# 97
30) Pyrene	19.525	202	101863	0.354	ng	99
32) Benzo(a)anthracene	21.281	228	94405	0.348	ng	98
33) Chrysene	21.334	228	110863	0.372	ng	98
34) Bis(2-ethylhexyl)phtha...	21.217	149	18257	0.380	ng	# 85
36) Indeno(1,2,3-cd)pyrene	25.806	276	110047	0.358	ng	# 89
37) Benzo(b)fluoranthene	22.872	252	111466	0.376	ng	# 91
38) Benzo(k)fluoranthene	22.913	252	124832	0.396	ng	# 94
39) Benzo(a)pyrene	23.447	252	106581	0.387	ng	# 78
40) Dibenzo(a,h)anthracene	25.816	278	86850	0.352	ng	# 90
41) Benzo(g,h,i)perylene	26.490	276	95598	0.378	ng	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062921\
Data File : BN015214.D
Acq On : 30 Jun 2021 08:57
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Quant Time: Jun 30 09:34:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 29 19:13:09 2021
Response via : Initial Calibration







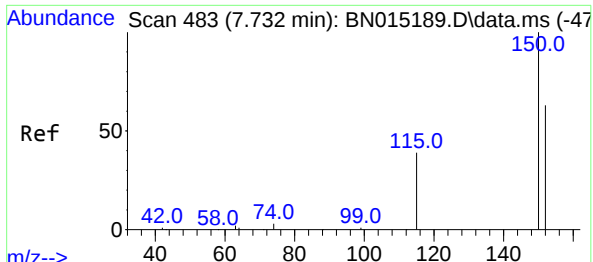

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.731 min Scan# 483
 Delta R.T. -0.001 min
 Lab File: BN015214.D
 Acq: 30 Jun 2021 08:57




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC


Tgt Ion:152 Resp: 19594
 Ion Ratio Lower Upper
 152 100
 150 157.2 119.0 178.6
 115 61.5 62.2 93.4#

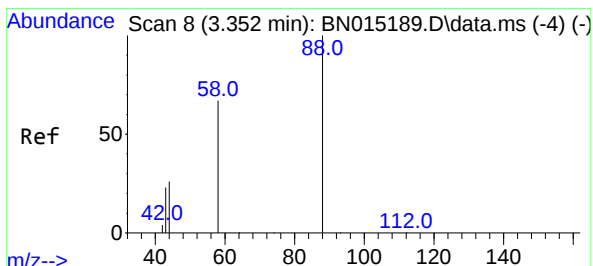

#2
 1,4-Dioxane
 Concen: 0.348 ng
 RT: 3.352 min Scan# 8
 Delta R.T. -0.000 min
 Lab File: BN015214.D
 Acq: 30 Jun 2021 08:57

Tgt Ion: 88 Resp: 1980
 Ion Ratio Lower Upper
 88 100
 43 33.7 12.9 19.3#
 58 76.4 38.1 57.1#







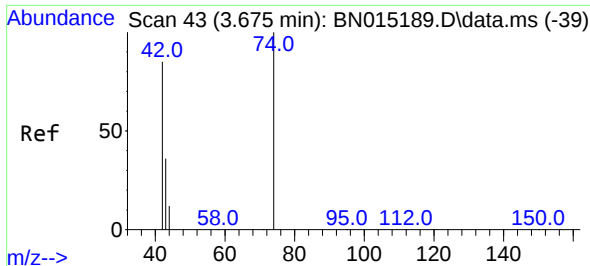

#3
n-Nitrosodimethylamine
Concen: 0.308 ng
RT: 3.693 min Scan# 45
Delta R.T. 0.018 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 42 Resp: 3548
Ion Ratio Lower Upper
42 100
74 131.2 149.5 224.3#
44 58.8 4.2 6.2#

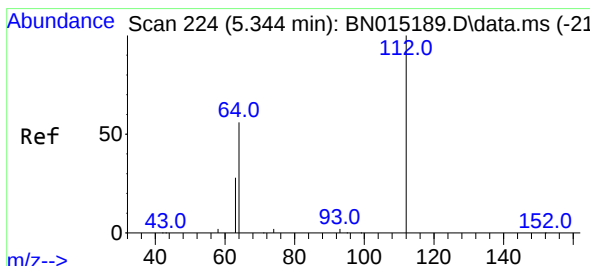

#4
2-Fluorophenol
Concen: 0.289 ng
RT: 5.362 min Scan# 226
Delta R.T. 0.018 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion: 112 Resp: 12261
Ion Ratio Lower Upper
112 100
64 57.9 39.0 58.6
63 30.7 20.6 30.8









#5
Phenol-d6
Concen: 0.333 ng
RT: 6.902 min Scan# 393
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 99 Resp: 21580
Ion Ratio Lower Upper
99 100
42 18.7 8.9 13.3#
71 31.9 35.6 53.4#



#6
bis(2-Chloroethyl)ether
Concen: 0.374 ng
RT: 7.169 min Scan# 422
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion: 93 Resp: 23206
Ion Ratio Lower Upper
93 100
63 75.9 46.6 70.0#
95 32.8 28.6 42.8









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.492 min Scan# 718
Delta R.T. -0.013 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	136	Resp:	90606
Ion Ratio	Lower	Upper	
136	100		
137	10.8	9.8	14.8
54	10.4	5.4	8.2#
68	7.8	4.9	7.3#



#8
Nitrobenzene-d5
Concen: 0.349 ng
RT: 8.870 min Scan# 590
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:	82	Resp:	28882
Ion Ratio	Lower	Upper	
82	100		
128	37.6	31.6	47.4
54	50.4	29.0	43.4#









#9
Naphthalene
Concen: 0.374 ng
RT: 10.543 min Scan# 722
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:128	Resp:	97787
Ion Ratio	Lower	Upper
128	100	
129	10.9	9.1 13.7
127	13.1	11.8 17.6



#10
Hexachlorobutadiene
Concen: 0.386 ng
RT: 10.834 min Scan# 745
Delta R.T. -0.013 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:225	Resp:	20281
Ion Ratio	Lower	Upper
225	100	
223	0.0	0.0 0.0
227	63.7	50.2 75.2







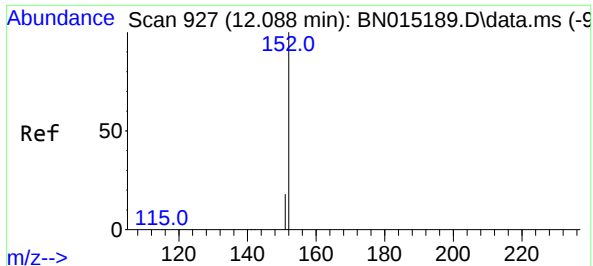

#11
2-Methylnaphthalene-d10
Concen: 0.360 ng
RT: 12.088 min Scan# 927
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 53533
Ion Ratio Lower Upper
152 100
151 20.4 16.7 25.1

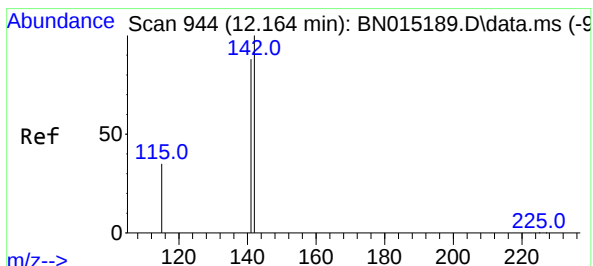

#12
2-Methylnaphthalene
Concen: 0.374 ng
RT: 12.159 min Scan# 943
Delta R.T. -0.005 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:142 Resp: 62189
Ion Ratio Lower Upper
142 100
141 88.6 72.3 108.5
115 35.7 40.7 61.1#









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.346 min Scan# 1166
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:164 Resp: 43686
Ion Ratio Lower Upper
164 100
162 100.7 83.8 125.6
160 52.3 37.4 56.0



#14
2,4,6-Tribromophenol
Concen: 0.367 ng
RT: 15.843 min Scan# 1284
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:330 Resp: 3543
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 39.1 22.4 33.6#









#15
2-Fluorobiphenyl
Concen: 0.373 ng
RT: 12.963 min Scan# 1057
Delta R.T. -0.013 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:172 Resp: 68323
Ion Ratio Lower Upper
172 100
171 35.2 30.6 45.8
170 24.5 20.2 30.4



#16
Acenaphthylene
Concen: 0.353 ng
RT: 14.066 min Scan# 1144
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:152 Resp: 78910
Ion Ratio Lower Upper
152 100
151 19.3 16.7 25.1
153 13.0 10.5 15.7









#17
Acenaphthene
Concen: 0.367 ng
RT: 14.409 min Scan# 1171
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 51165
Ion Ratio Lower Upper
154 100
153 114.5 90.9 136.3
152 64.5 45.8 68.8



#18
Fluorene
Concen: 0.374 ng
RT: 15.399 min Scan# 1249
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:166 Resp: 62927
Ion Ratio Lower Upper
166 100
165 97.8 79.2 118.8
167 13.5 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.091 min Scan# 1386
Delta R.T. -0.001 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:188 Resp: 78743
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.6 9.0 13.4



#20
4,6-Dinitro-2-methylphenol
Concen: 0.403 ng
RT: 15.475 min Scan# 1255
Delta R.T. -0.013 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:198 Resp: 327
Ion Ratio Lower Upper
198 100
182 35.1 34.5 51.7
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.349 ng
RT: 16.288 min Scan# 1320
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:248 Resp: 18992
Ion Ratio Lower Upper
248 100
250 94.7 86.2 129.4
141 61.6 36.2 54.2#



#22
Hexachlorobenzene
Concen: 0.390 ng
RT: 16.410 min Scan# 1330
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:284 Resp: 25318
Ion Ratio Lower Upper
284 100
142 35.4 22.2 33.2#
249 30.5 26.6 39.8









#23
Atrazine
Concen: 0.314 ng
RT: 16.556 min Scan# 1342
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:200 Resp: 6308
Ion Ratio Lower Upper
200 100
173 28.0 21.7 32.5
215 47.4 43.1 64.7



#24
Pentachlorophenol
Concen: 0.520 ng
RT: 16.750 min Scan# 1358
Delta R.T. -0.001 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:266 Resp: 2045
Ion Ratio Lower Upper
266 100
264 64.1 51.0 76.4
268 63.9 50.6 76.0







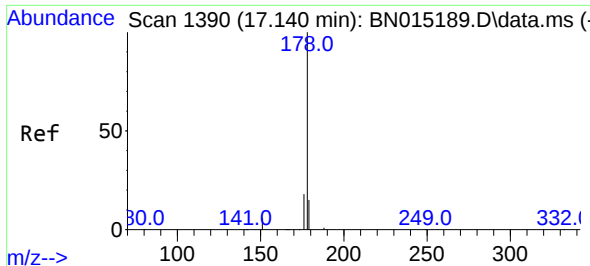

#25
Phenanthrene
Concen: 0.371 ng
RT: 17.128 min Scan# 1389
Delta R.T. -0.013 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:178	Resp:	99554
Ion Ratio	Lower	Upper
178	100	
176	19.0	15.6 23.4
179	15.4	12.1 18.1

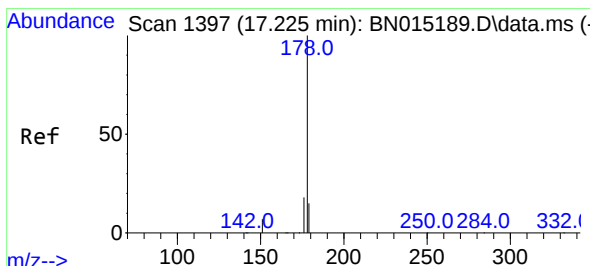

#26
Anthracene
Concen: 0.338 ng
RT: 17.225 min Scan# 1397
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:178	Resp:	79133
Ion Ratio	Lower	Upper
178	100	
176	18.3	15.1 22.7
179	15.3	12.2 18.2









#27
Fluoranthene-d10
Concen: 0.329 ng
RT: 19.133 min Scan# 1687
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 78651
Ion Ratio Lower Upper
212 100
106 13.9 7.0 10.6#
104 7.8 4.1 6.1#



#28
Fluoranthene
Concen: 0.371 ng
RT: 19.163 min Scan# 1693
Delta R.T. -0.000 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:202 Resp: 107853
Ion Ratio Lower Upper
202 100
101 11.5 6.6 10.0#
203 17.3 13.9 20.9







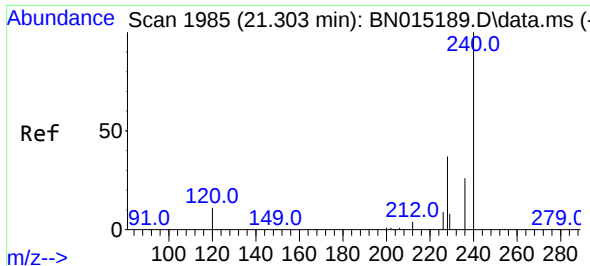

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.292 min Scan# 1984
Delta R.T. -0.011 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:240 Resp: 79165
Ion Ratio Lower Upper
240 100
120 13.6 4.2 6.4#
236 27.1 21.4 32.2

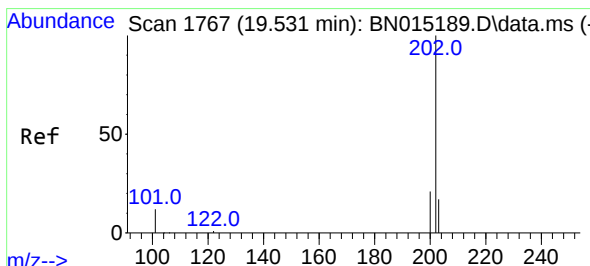

#30
Pyrene
Concen: 0.354 ng
RT: 19.525 min Scan# 1766
Delta R.T. -0.005 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:202 Resp: 101863
Ion Ratio Lower Upper
202 100
200 20.5 16.9 25.3
203 17.4 13.9 20.9









#31
Terphenyl-d14
Concen: 0.358 ng
RT: 19.734 min Scan# 1808
Delta R.T. -0.010 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:244 Resp: 62661
Ion Ratio Lower Upper
244 100
212 8.1 6.3 9.5
122 13.7 6.2 9.2#



#32
Benzo(a)anthracene
Concen: 0.348 ng
RT: 21.281 min Scan# 1983
Delta R.T. -0.011 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:228 Resp: 94405
Ion Ratio Lower Upper
228 100
226 26.7 23.0 34.6
229 19.7 15.7 23.5









#33
Chrysene
Concen: 0.372 ng
RT: 21.334 min Scan# 1988
Delta R.T. -0.011 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

Tgt Ion:228 Resp: 110863




Ion	Ratio	Lower	Upper
228	100		
226	29.2	25.0	37.6
229	19.9	15.9	23.9

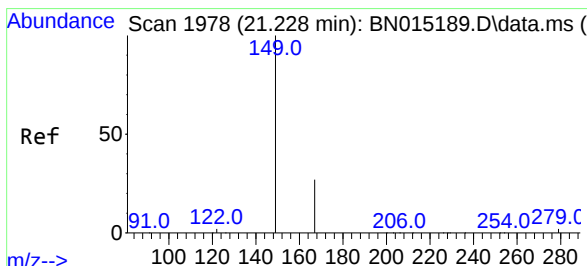


#34
Bis(2-ethylhexyl)phthalate
Concen: 0.380 ng
RT: 21.217 min Scan# 1977
Delta R.T. -0.011 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:149 Resp: 18257


Ion	Ratio	Lower	Upper
149	100		
167	26.7	28.9	43.3#
279	3.0	4.9	7.3#








#35
Perylene-d12
Concen: 0.400 ng
RT: 23.547 min Scan# 2422
Delta R.T. -0.011 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC







Tgt Ion:264 Resp: 74924
Ion Ratio Lower Upper
264 100
260 24.9 20.6 31.0
265 22.9 21.4 32.2



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.358 ng
RT: 25.806 min Scan# 3082
Delta R.T. -0.011 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57


Tgt Ion:276 Resp: 110047
Ion Ratio Lower Upper
276 100
138 24.5 10.0 15.0#
277 24.8 20.4 30.6








#37
Benzo(b)fluoranthene
Concen: 0.376 ng
RT: 22.872 min Scan# 2225
Delta R.T. -0.011 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC







Tgt Ion:252 Resp: 111466
Ion Ratio Lower Upper
252 100
253 22.6 18.5 27.7
125 19.2 5.8 8.6#



#38
Benzo(k)fluoranthene
Concen: 0.396 ng
RT: 22.913 min Scan# 2237
Delta R.T. -0.014 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:252 Resp: 124832
Ion Ratio Lower Upper
252 100
253 21.8 19.1 28.7
125 11.4 5.4 8.0#









#39
Benzo(a)pyrene
Concen: 0.387 ng
RT: 23.447 min Scan# 2393
Delta R.T. -0.011 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 106581
Ion Ratio Lower Upper
252 100
253 24.6 19.4 29.2
125 37.9 7.4 11.2#



#40
Dibenzo(a,h)anthracene
Concen: 0.352 ng
RT: 25.816 min Scan# 3085
Delta R.T. -0.017 min
Lab File: BN015214.D
Acq: 30 Jun 2021 08:57

Tgt Ion:278 Resp: 86850
Ion Ratio Lower Upper
278 100
139 18.9 9.0 13.4#
279 23.5 21.0 31.4



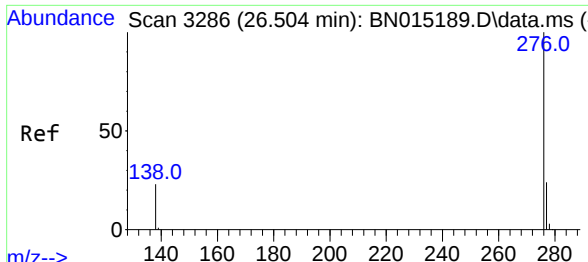

#41
 Benzo(g,h,i)perylene
 Concen: 0.378 ng
 RT: 26.490 min Scan# 3282
 Delta R.T. -0.014 min
 Lab File: BN015214.D
 Acq: 30 Jun 2021 08:57

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:	276	Resp:	95598
Ion Ratio	Lower	Upper	
276	100		
277	23.9	19.7	29.5
138	23.5	9.8	14.6#

