
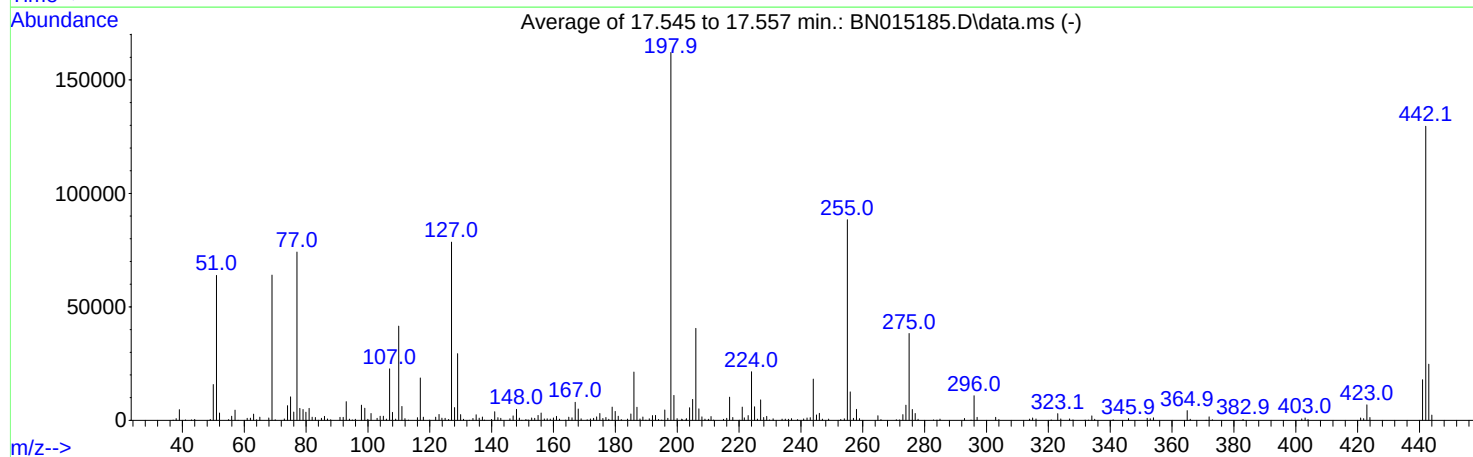


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062921\
 Data File : BN015185.D
 Acq On : 29 Jun 2021 13:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN062921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 29 19:13:09 2021

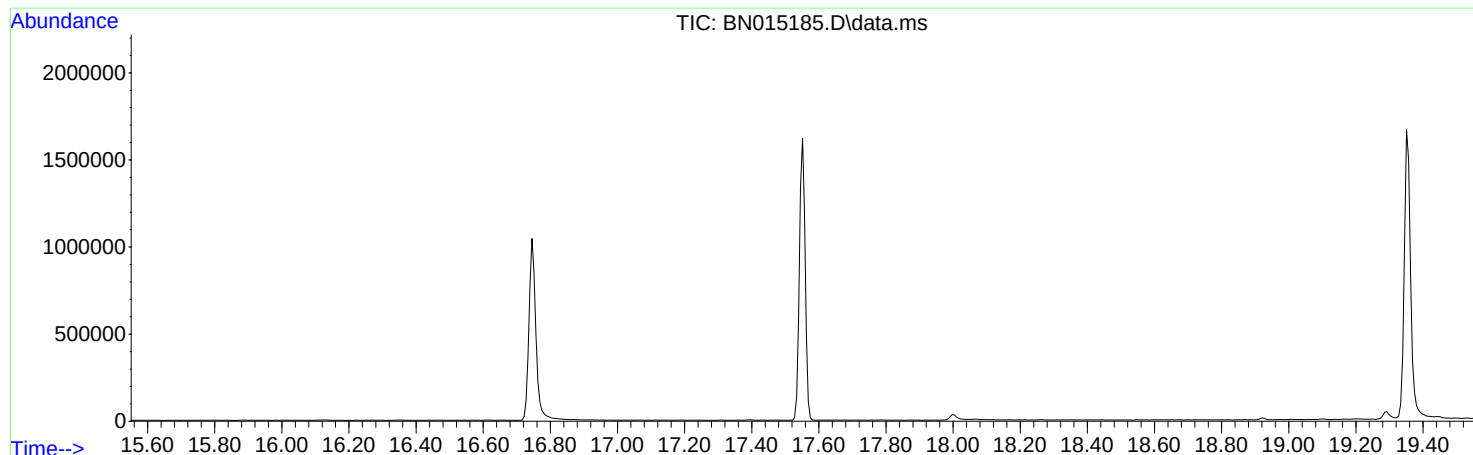




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	63909	PASS
68	69	0.00	2	1.7	1076	PASS
69	198	0.00	100	39.5	63992	PASS
70	69	0.00	2	0.4	257	PASS
127	198	10	80	48.4	78525	PASS
197	198	0.00	2	0.6	922	PASS
198	198	100	100	100.0	162091	PASS
199	198	5	9	6.8	10992	PASS
275	198	10	60	23.6	38267	PASS
365	198	1	100	2.6	4284	PASS
441	198	0.01	100	11.1	17914	PASS
442	442	50	100	100.0	129581	PASS
443	442	15	24	19.1	24744	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062921\
Data File : BN015185.D
Acq On : 29 Jun 2021 13:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 29 14:54:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

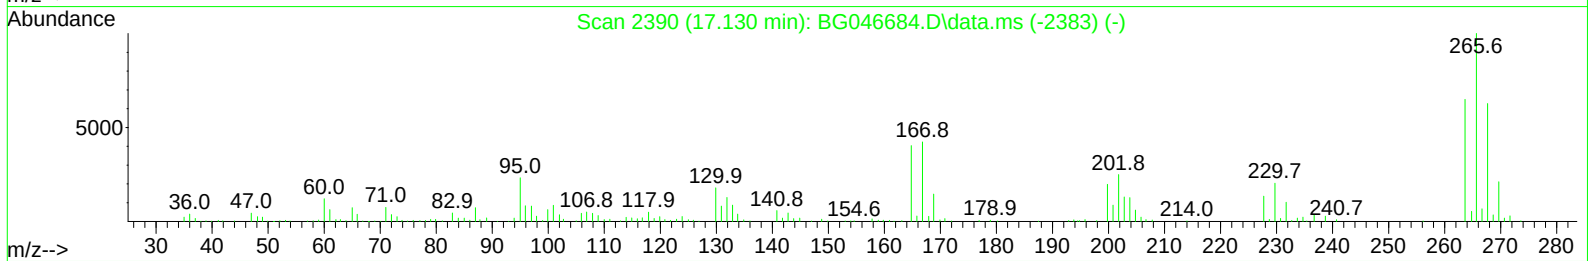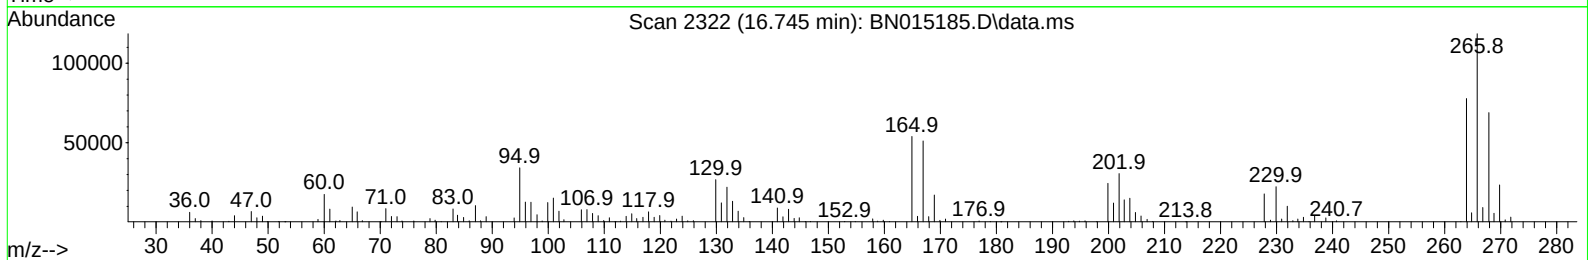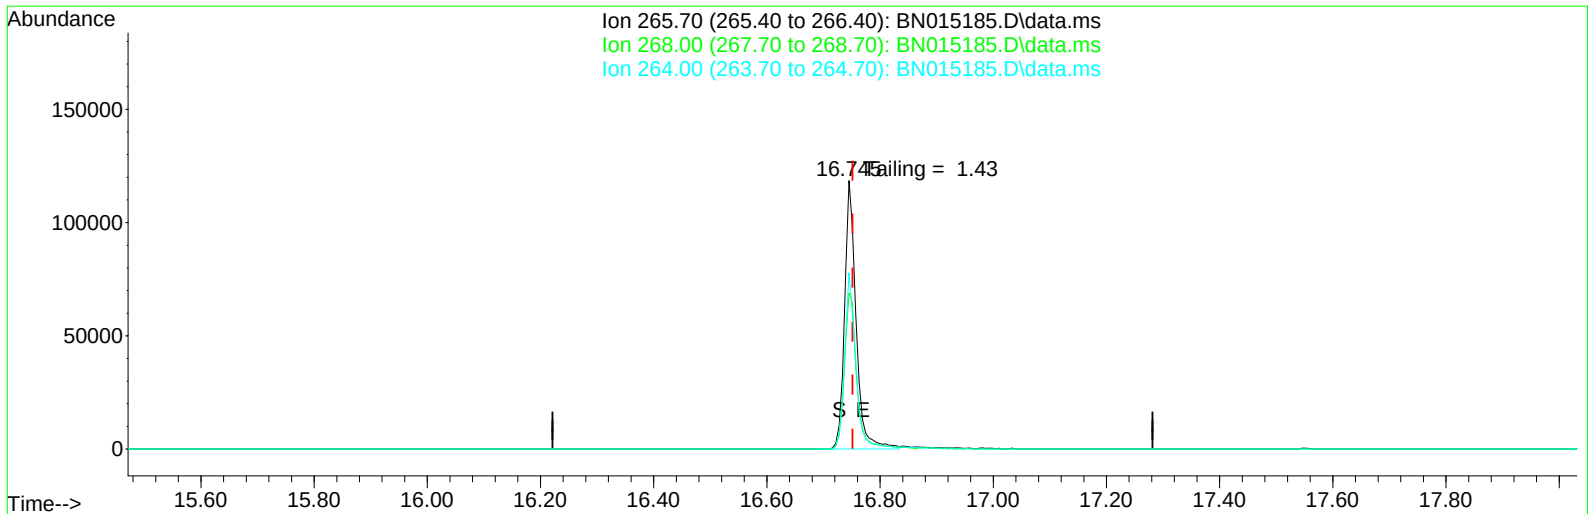

TIC: BN015185.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.006) 32943.76 ng




response 169340

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.13
264.00	61.60	65.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062921\
Data File : BN015185.D
Acq On : 29 Jun 2021 13:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jun 29 14:54:22 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

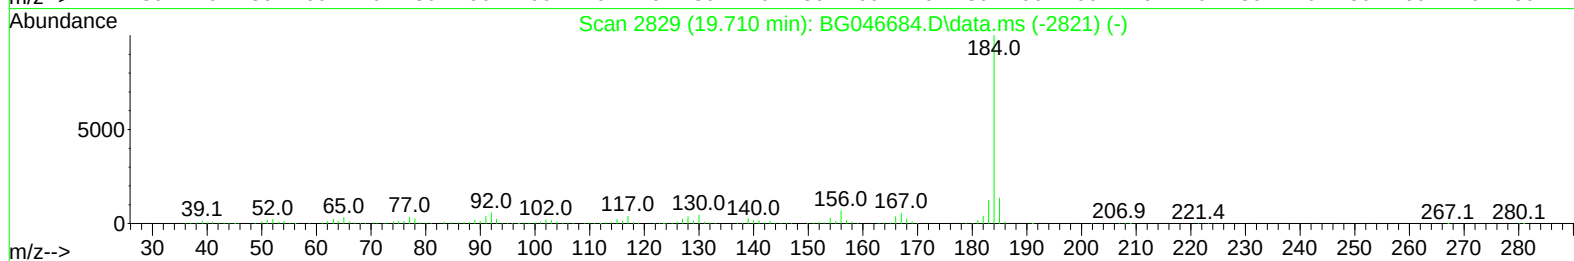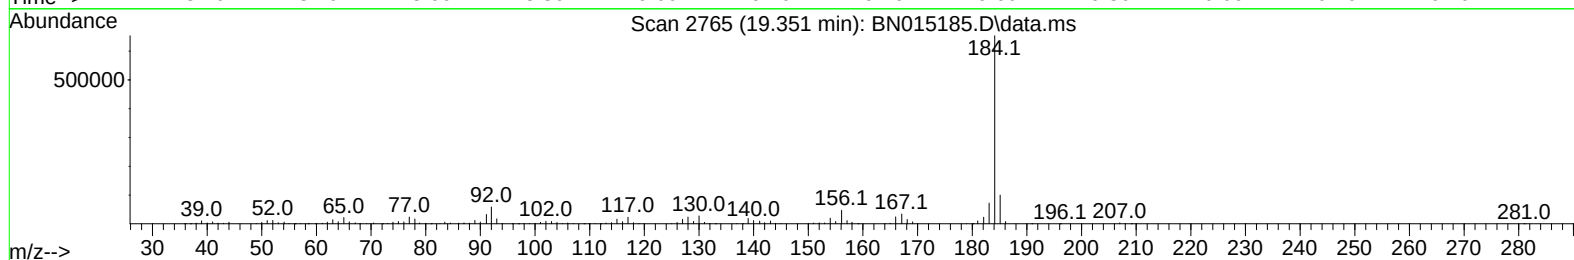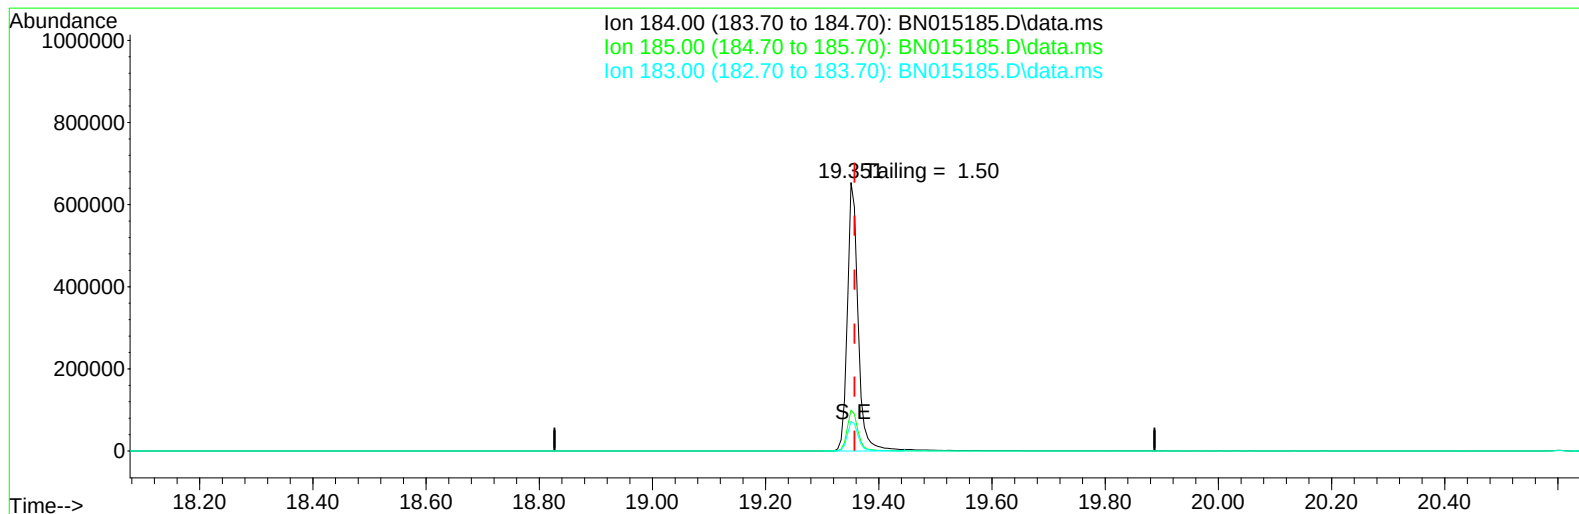

TIC: BN015185.D\data.ms

(77) Benzidine

19.351min (-0.006) 0.00 ng

response 870073

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.26
183.00	13.20	11.04
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
6/29/2021	BNA_N	<u>BN015185.D</u>
Compound Name	Response	Retention Time
DDT	452881	20.6
DDD	1762	20.15
DDE	752	19.64
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2514	455395	0.55