
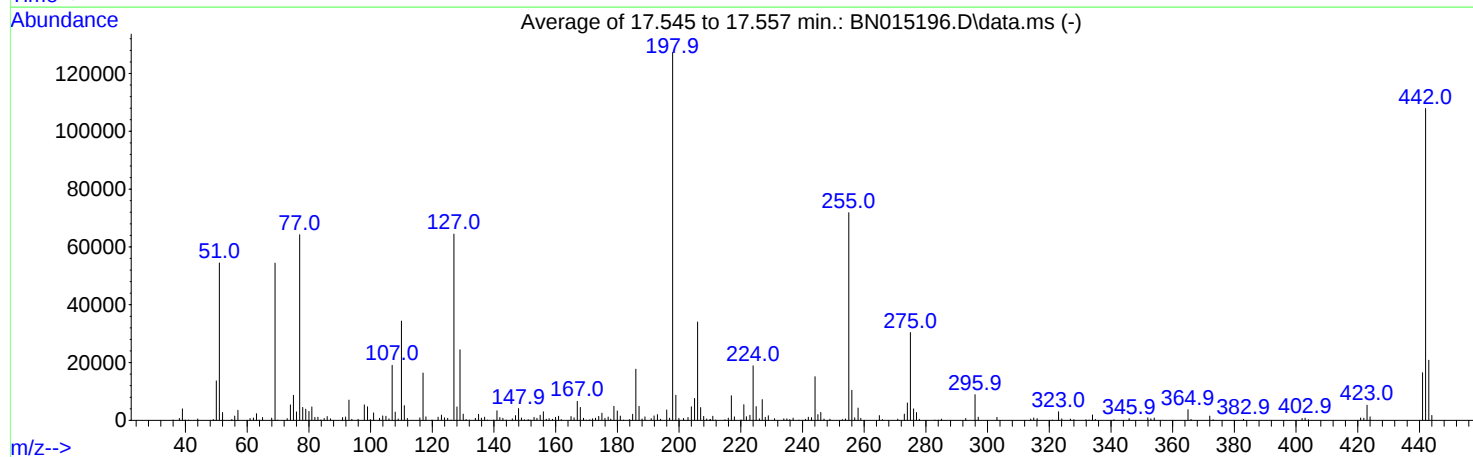


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062921\  
 Data File : BN015196.D  
 Acq On : 29 Jun 2021 21:32  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN062921.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Jun 29 19:13:09 2021

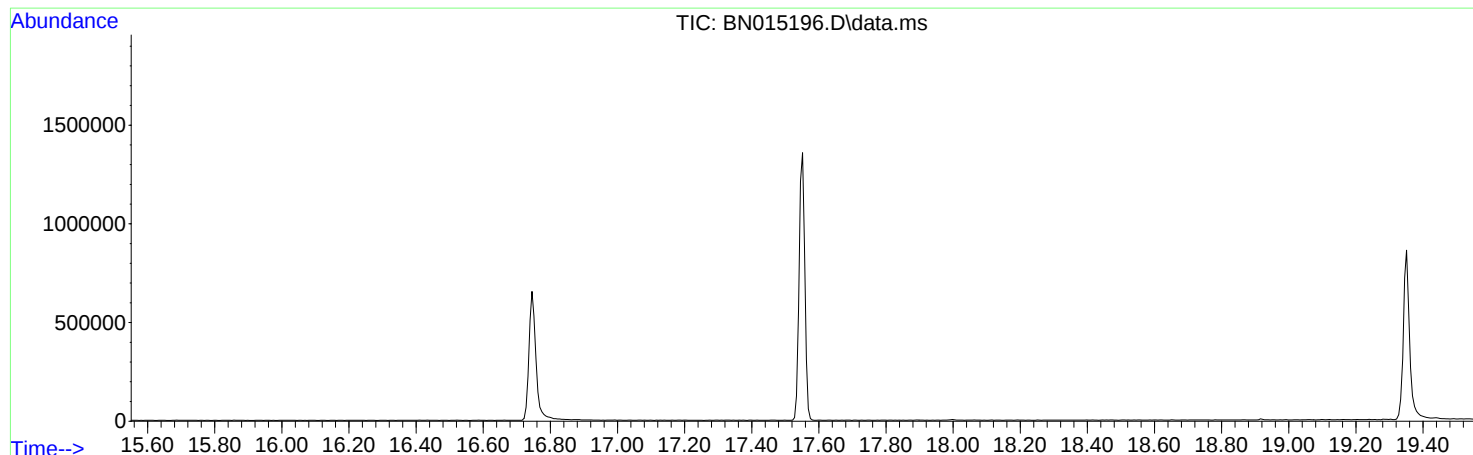




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 42.8         | 54493      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.5          | 795        | PASS                |
| 69             | 198             | 0.00            | 100             | 42.7         | 54392      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.2          | 125        | PASS                |
| 127            | 198             | 10              | 80              | 50.6         | 64427      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.6          | 777        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 127261     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 8694       | PASS                |
| 275            | 198             | 10              | 60              | 23.9         | 30405      | PASS                |
| 365            | 198             | 1               | 100             | 2.9          | 3716       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.0         | 16521      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 107880     | PASS                |
| 443            | 442             | 15              | 24              | 19.3         | 20821      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062921\  
Data File : BN015196.D  
Acq On : 29 Jun 2021 21:32  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Jun 30 02:19:51 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 23 10:10:58 2021  
Response via : Initial Calibration

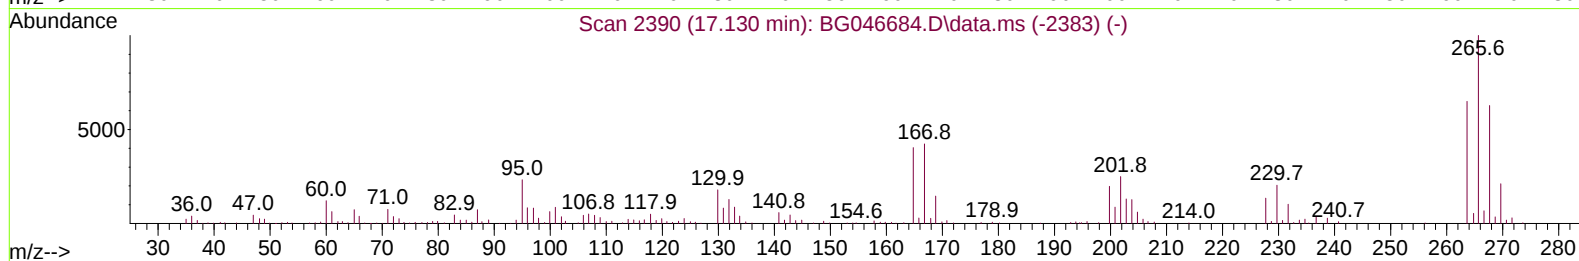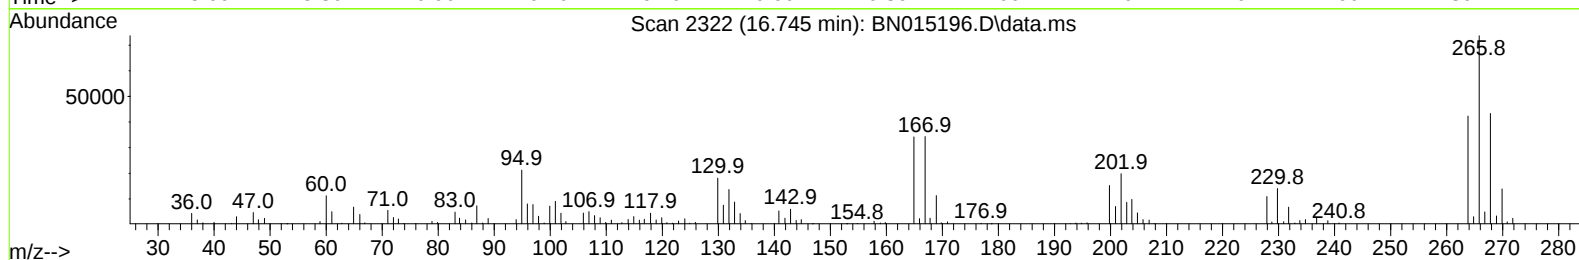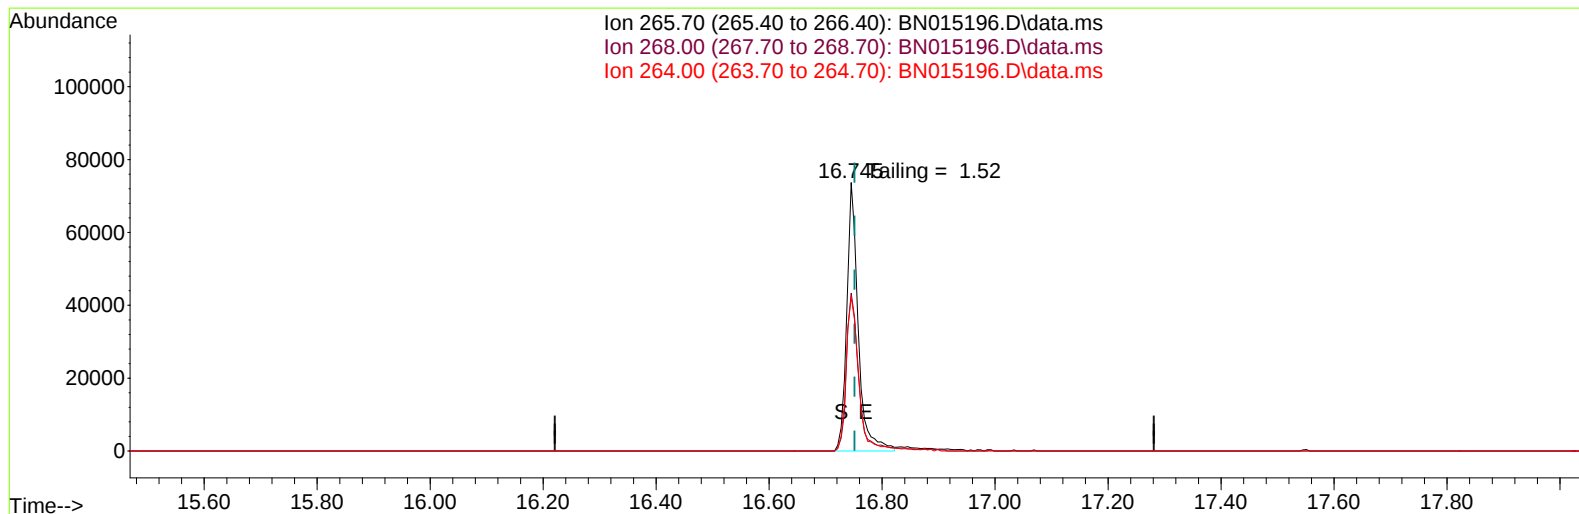

TIC: BN015196.D\data.ms

**(70) Pentachlorophenol (C)**

16.745min (-0.006) 24762.31 ng




response 104160

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 58.82  |
| 264.00 | 61.60  | 57.47  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN062921\  
Data File : BN015196.D  
Acq On : 29 Jun 2021 21:32  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Jun 30 02:19:51 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jun 23 10:10:58 2021  
Response via : Initial Calibration

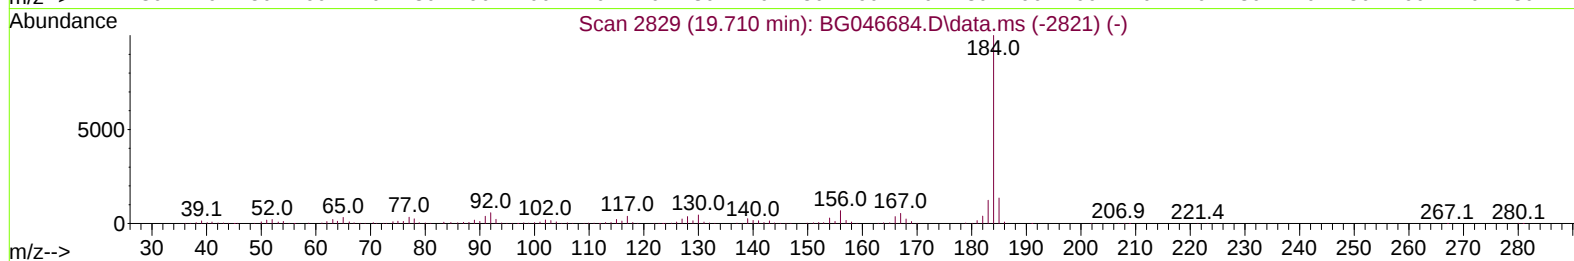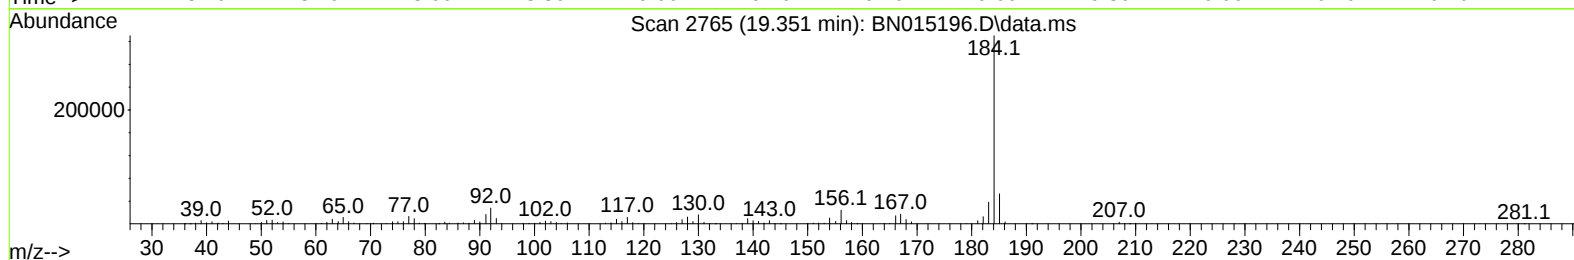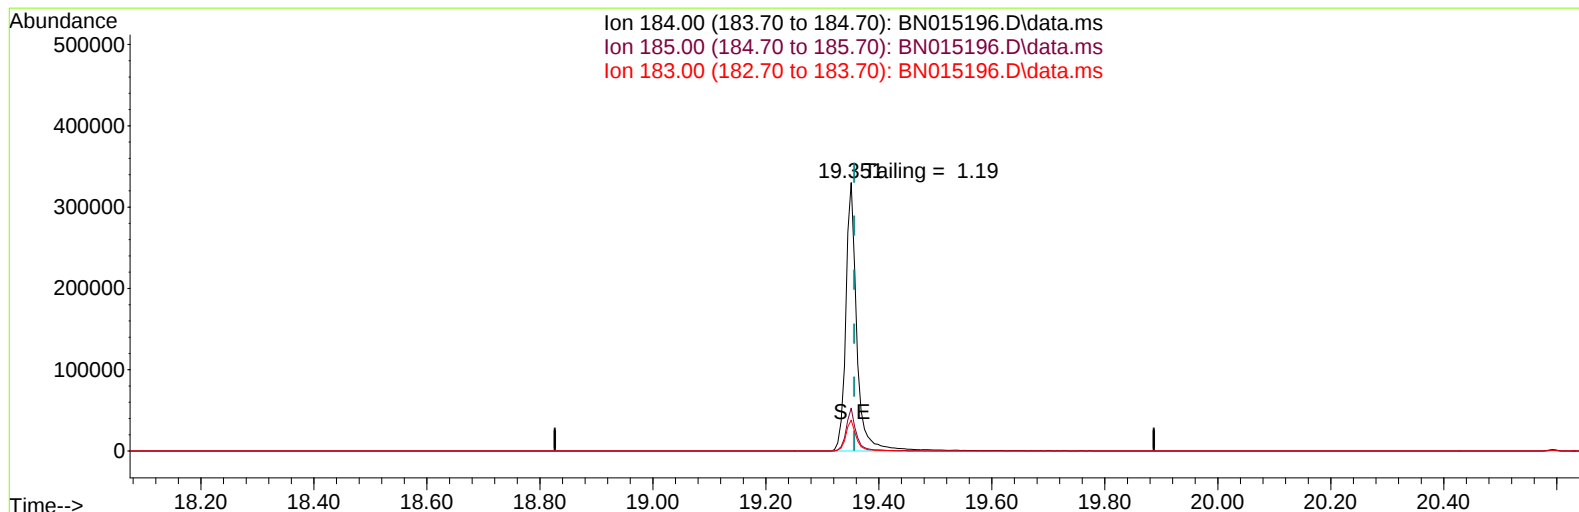

TIC: BN015196.D\data.ms

**(77) Benzidine**

**19.351min (-0.006) 0.00 ng**

**response 446263**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 15.97  |
| 183.00 | 13.20  | 11.55  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 6/29/2021     | BNA_N            | <u>BN015196.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 353520           | 20.592             |
| DDD           | 2049             | 20.151             |
| DDE           | 441              | 19.633             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 2490          | 356010           | 0.70               |
|               |                  |                    |