

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062922\
 Data File : BN020573.D
 Acq On : 29 Jun 2022 17:18
 Operator : CG/JU
 Sample : N3355-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EY0C7

Quant Time: Jun 29 19:01:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 00:17:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.737	152	3300	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.518	136	10784	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.368	164	6412	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.111	188	12707	0.400	ng/ul	0.00
17) Chrysene-d12	21.305	240	9443	0.400	ng/ul	0.00
23) Perylene-d12	23.582	264	8530	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	17696	4.629	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.119	152	5256	0.297	ng/ul	0.00
18) Fluoranthene-d10	19.141	212	12309	0.395	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.222	88	85	0.022	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN062922\
Data File : BN020573.D
Acq On : 29 Jun 2022 17:18
Operator : CG/JU
Sample : N3355-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EY0C7


Quant Time: Jun 29 19:01:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 00:17:34 2022
Response via : Initial Calibration

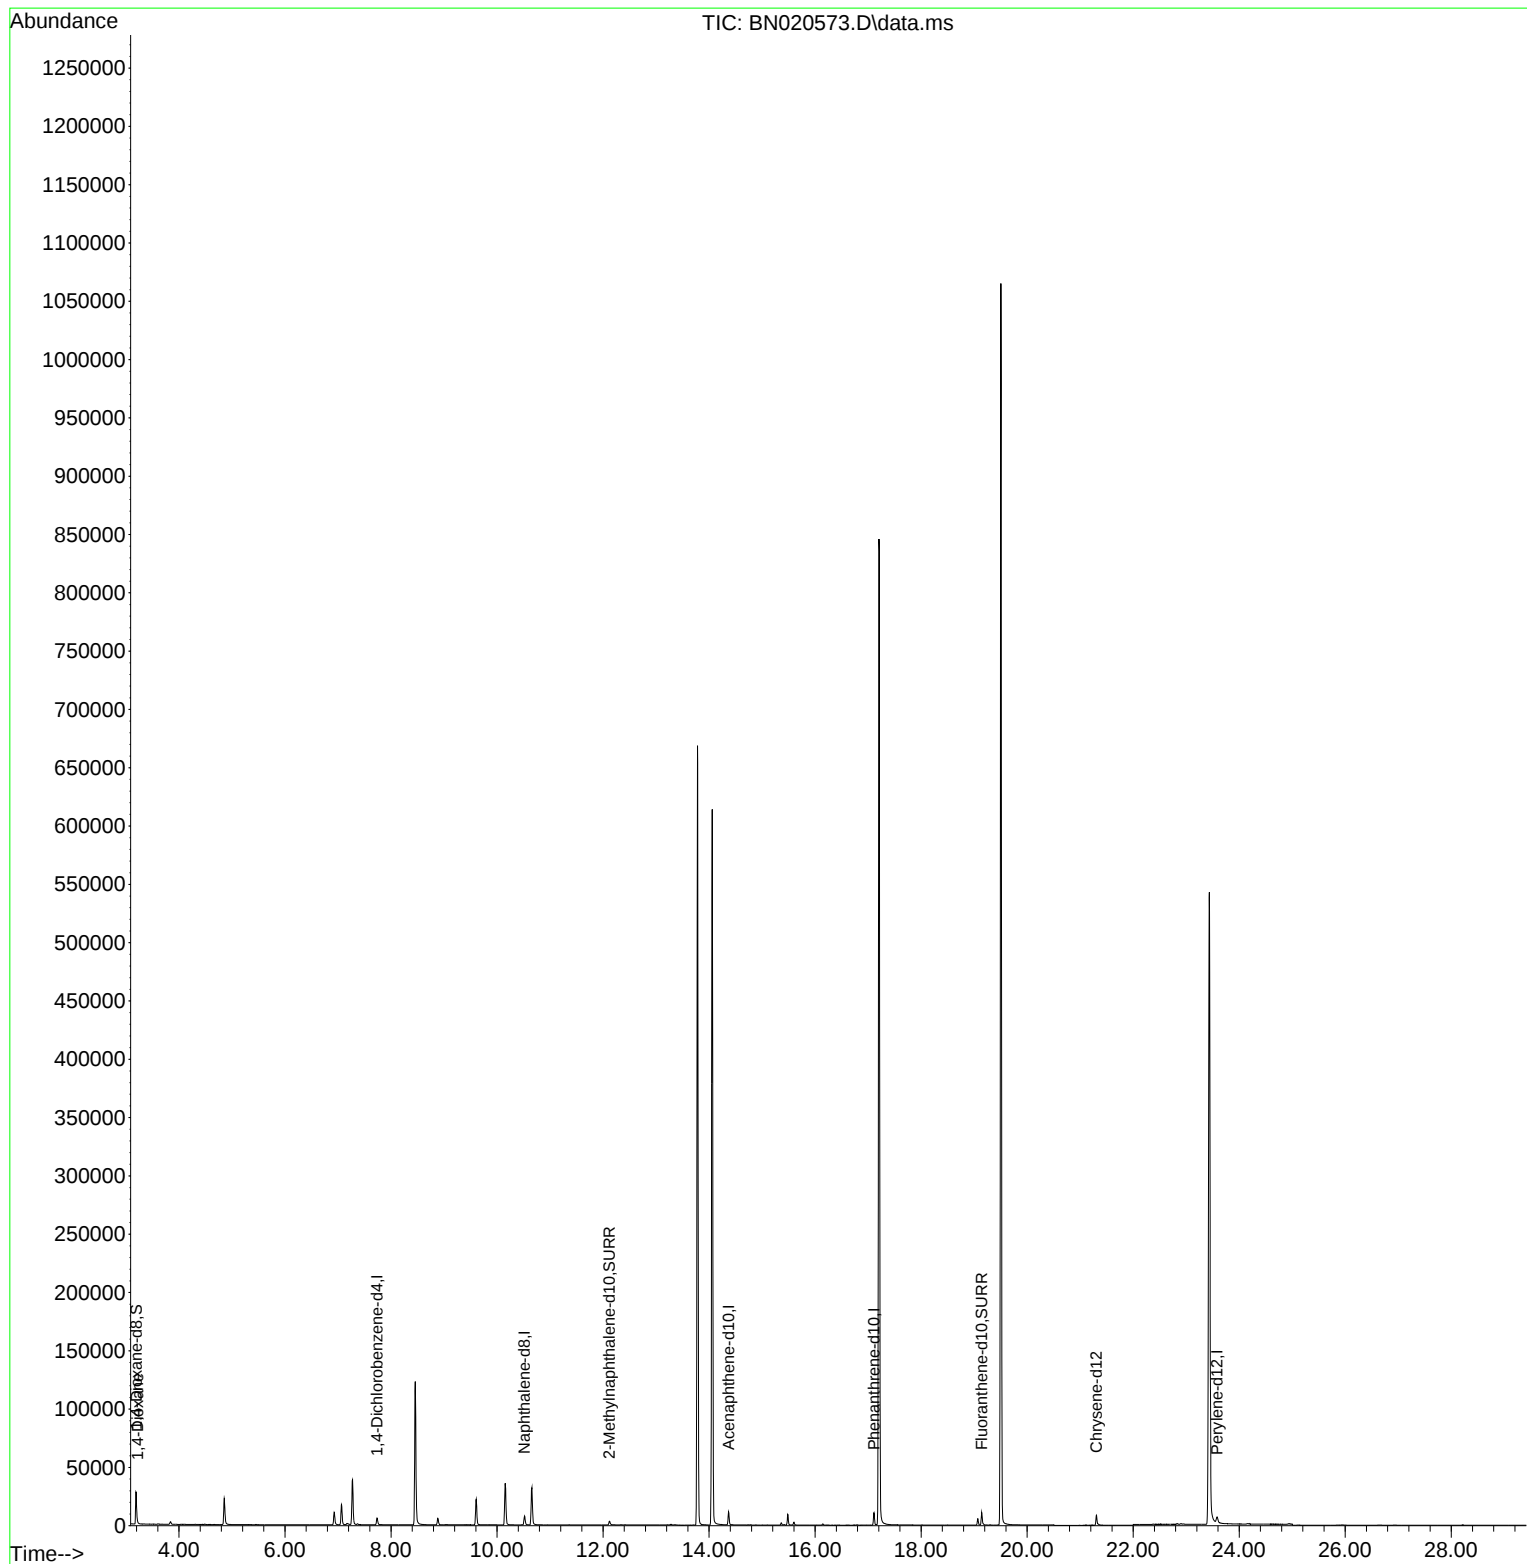

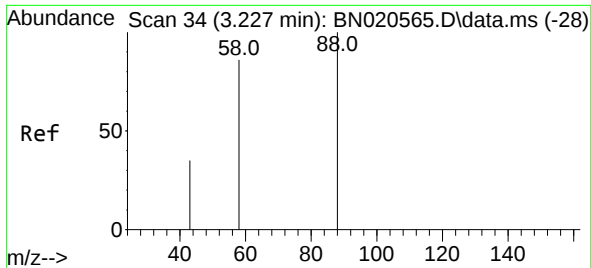

#2
 1,4-Dioxane
 Concen: 0.022 ng/ul
 RT: 3.222 min Scan# 31
 Delta R.T. -0.017 min
 Lab File: BN020573.D
 Acq: 29 Jun 2022 17:18

Instrument :
 BNA_N
 ClientSampleId :
 EY0C7

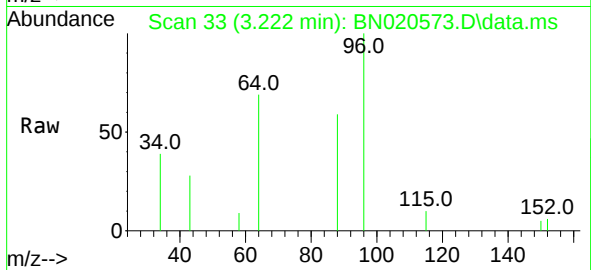

Tgt Ion: 88 Resp: 85
 Ion Ratio Lower Upper
 88 100
 43 47.7 32.5 48.7
 58 15.6 46.2 69.2#

