

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063021\
 Data File : BN015224.D
 Acq On : 30 Jun 2021 16:10
 Operator : CG/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN063021

Quant Time: Jul 01 09:32:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 01 09:06:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.722	152	17660	0.40	ng	# 0.00
7) Naphthalene-d8	10.492	136	77539	0.40	ng	0.00
13) Acenaphthene-d10	14.345	164	39472	0.40	ng	0.00
19) Phenanthrene-d10	17.091	188	73849	0.40	ng	0.00
29) Chrysene-d12	21.313	240	65526	0.40	ng	# 0.00
35) Perylene-d12	23.564	264	60693	0.40	ng	0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.343	112	18390	0.41	ng	-0.02
5) Phenol-d6	6.892	99	22845	0.40	ng	0.00
8) Nitrobenzene-d5	8.857	82	17656	0.41	ng	-0.01
11) 2-Methylnaphthalene-d10	12.083	152	49776	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.843	330	3335	0.42	ng	0.00
15) 2-Fluorobiphenyl	12.962	172	64133	0.40	ng	0.00
27) Fluoranthene-d10	19.138	212	81892	0.38	ng	0.00
31) Terphenyl-d14	19.744	244	62043	0.40	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.342	88	3391	0.41	ng	# 58
3) n-Nitrosodimethylamine	3.684	42	6124	0.39	ng	# 74
6) bis(2-Chloroethyl)ether	7.160	93	22928	0.41	ng	# 85
9) Naphthalene	10.543	128	88891	0.40	ng	97
10) Hexachlorobutadiene	10.834	225	16781	0.40	ng	# 98
12) 2-Methylnaphthalene	12.154	142	57468	0.40	ng	# 89
16) Acenaphthylene	14.054	152	64581	0.37	ng	98
17) Acenaphthene	14.409	154	48030	0.39	ng	99
18) Fluorene	15.398	166	58553	0.39	ng	99
20) 4,6-Dinitro-2-methylph...	15.475	198	233	0.36	ng	94
21) 4-Bromophenyl-phenylether	16.288	248	18180	0.39	ng	# 88
22) Hexachlorobenzene	16.397	284	21114	0.40	ng	# 91
23) Atrazine	16.556	200	9592	0.41	ng	92
24) Pentachlorophenol	16.750	266	1730	0.44	ng	99
25) Phenanthrene	17.140	178	93576	0.39	ng	99
26) Anthracene	17.225	178	76619	0.38	ng	99
28) Fluoranthene	19.168	202	102022	0.40	ng	# 97
30) Pyrene	19.530	202	100085	0.40	ng	99
32) Benzo(a)anthracene	21.292	228	85728	0.38	ng	98
33) Chrysene	21.345	228	97478	0.40	ng	97
34) Bis(2-ethylhexyl)phtha...	21.239	149	20901	0.41	ng	# 87
36) Indeno(1,2,3-cd)pyrene	25.826	276	84224	0.39	ng	# 89
37) Benzo(b)fluoranthene	22.889	252	92370	0.39	ng	# 94
38) Benzo(k)fluoranthene	22.934	252	99536	0.39	ng	# 94
39) Benzo(a)pyrene	23.468	252	85291	0.39	ng	# 86
40) Dibenzo(a,h)anthracene	25.847	278	65330	0.38	ng	# 91
41) Benzo(g,h,i)perylene	26.514	276	71979	0.38	ng	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063021\
 Data File : BN015224.D
 Acq On : 30 Jun 2021 16:10
 Operator : CG/JU
 Sample : SSTDICV0.4
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 ICVBN063021

Quant Time: Jul 01 09:32:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 01 09:06:31 2021
 Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.722 min Scan# 482
 Delta R.T. -0.010 min
 Lab File: BN015224.D
 Acq: 30 Jun 2021 16:10




Instrument :
 BNA_N
 ClientSampleId :
 ICVBN063021

Tgt Ion:152 Resp: 17660
 Ion Ratio Lower Upper
 152 100
 150 156.7 119.0 178.6
 115 61.3 62.2 93.4#



#2
 1,4-Dioxane
 Concen: 0.41 ng
 RT: 3.342 min Scan# 7
 Delta R.T. -0.010 min
 Lab File: BN015224.D
 Acq: 30 Jun 2021 16:10

Tgt Ion: 88 Resp: 3391
 Ion Ratio Lower Upper
 88 100
 43 28.3 12.9 19.3#
 58 78.8 38.1 57.1#









#3
n-Nitrosodimethylamine
Concen: 0.39 ng
RT: 3.684 min Scan# 44
Delta R.T. -0.010 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021


Tgt Ion: 42 Resp: 6124
Ion Ratio Lower Upper
42 100
74 148.8 149.5 224.3#
44 11.0 4.2 6.2#

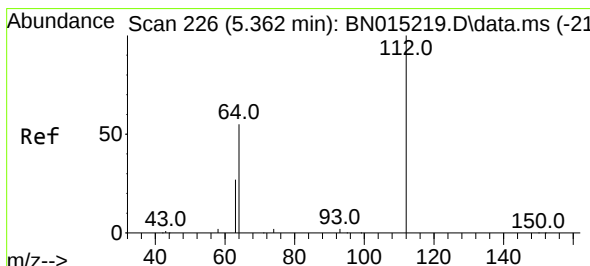

#4
2-Fluorophenol
Concen: 0.41 ng
RT: 5.343 min Scan# 224
Delta R.T. -0.019 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion: 112 Resp: 18390
Ion Ratio Lower Upper
112 100
64 56.1 39.0 58.6
63 28.5 20.6 30.8







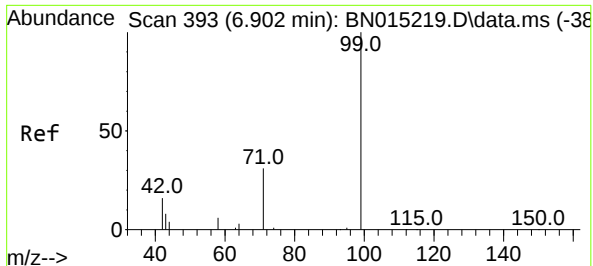

#5
Phenol-d6
Concen: 0.40 ng
RT: 6.892 min Scan# 392
Delta R.T. -0.010 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021

Tgt Ion: 99 Resp: 22845
Ion Ratio Lower Upper
99 100
42 17.1 8.9 13.3#
71 30.3 35.6 53.4#

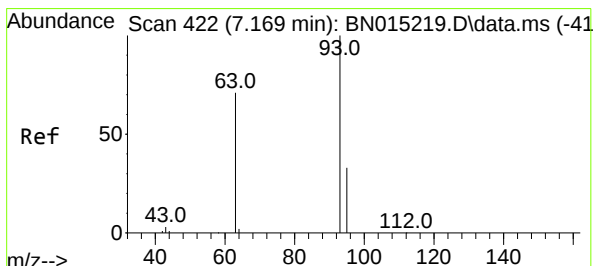

#6
bis(2-Chloroethyl)ether
Concen: 0.41 ng
RT: 7.160 min Scan# 421
Delta R.T. -0.010 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion: 93 Resp: 22928
Ion Ratio Lower Upper
93 100
63 74.4 46.6 70.0#
95 32.7 28.6 42.8









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.492 min Scan# 718
Delta R.T. -0.000 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021

Tgt Ion:	136	Resp:	77539
Ion Ratio	Lower	Upper	
136	100		
137	10.9	9.8	14.8
54	6.3	5.4	8.2
68	5.5	4.9	7.3



#8
Nitrobenzene-d5
Concen: 0.41 ng
RT: 8.857 min Scan# 589
Delta R.T. -0.013 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:	82	Resp:	17656
Ion Ratio	Lower	Upper	
82	100		
128	33.9	31.6	47.4
54	52.7	29.0	43.4









#9
Naphthalene
Concen: 0.40 ng
RT: 10.543 min Scan# 722
Delta R.T. -0.000 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021

Tgt Ion:128 Resp: 88891
Ion Ratio Lower Upper
128 100
129 11.0 9.1 13.7
127 12.7 11.8 17.6



#10
Hexachlorobutadiene
Concen: 0.40 ng
RT: 10.834 min Scan# 745
Delta R.T. -0.000 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:225 Resp: 16781
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.1 50.2 75.2









#11
2-Methylnaphthalene-d10
Concen: 0.39 ng
RT: 12.083 min Scan# 926
Delta R.T. -0.005 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021


Tgt Ion:152 Resp: 49776
Ion Ratio Lower Upper
152 100
151 20.3 16.7 25.1

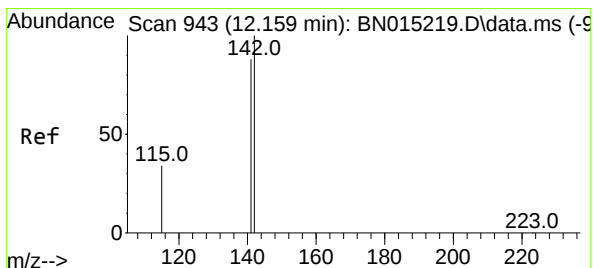

#12
2-Methylnaphthalene
Concen: 0.40 ng
RT: 12.154 min Scan# 942
Delta R.T. -0.005 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:142 Resp: 57468
Ion Ratio Lower Upper
142 100
141 88.0 72.3 108.5
115 33.5 40.7 61.1#









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.345 min Scan# 1166
Delta R.T. -0.001 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021

Tgt Ion:164 Resp: 39472
Ion Ratio Lower Upper
164 100
162 98.7 83.8 125.6
160 44.6 37.4 56.0



#14
2,4,6-Tribromophenol
Concen: 0.42 ng
RT: 15.843 min Scan# 1284
Delta R.T. -0.000 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:330 Resp: 3335
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 36.8 22.4 33.6#









#15
2-Fluorobiphenyl
Concen: 0.40 ng
RT: 12.962 min Scan# 1057
Delta R.T. -0.001 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021

Tgt Ion:172	Resp: 64133
Ion Ratio	Lower Upper
172	100
171	34.5 30.6 45.8
170	22.9 20.2 30.4



#16
Acenaphthylene
Concen: 0.37 ng
RT: 14.054 min Scan# 1143
Delta R.T. -0.013 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:152	Resp: 64581
Ion Ratio	Lower Upper
152	100
151	19.5 16.7 25.1
153	13.0 10.5 15.7









#17
Acenaphthene
Concen: 0.39 ng
RT: 14.409 min Scan# 1171
Delta R.T. -0.000 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021


Tgt Ion:154 Resp: 48030
Ion Ratio Lower Upper
154 100
153 112.9 90.9 136.3
152 56.4 45.8 68.8



#18
Fluorene
Concen: 0.39 ng
RT: 15.398 min Scan# 1249
Delta R.T. -0.001 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:166 Resp: 58553
Ion Ratio Lower Upper
166 100
165 97.5 79.2 118.8
167 13.5 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.091 min Scan# 1386
Delta R.T. 0.000 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021


Tgt Ion:188 Resp: 73849
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.4 9.0 13.4



#20
4,6-Dinitro-2-methylphenol
Concen: 0.36 ng
RT: 15.475 min Scan# 1255
Delta R.T. -0.013 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:198 Resp: 233
Ion Ratio Lower Upper
198 100
182 39.3 34.5 51.7
77 0.0 0.0 0.0







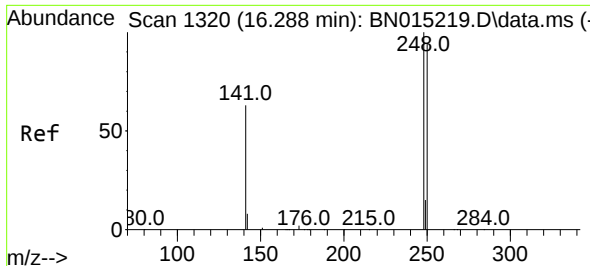

#21
4-Bromophenyl-phenylether
Concen: 0.39 ng
RT: 16.288 min Scan# 1320
Delta R.T. -0.000 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021


Tgt Ion:248 Resp: 18180
Ion Ratio Lower Upper
248 100
250 97.1 86.2 129.4
141 55.7 36.2 54.2#



#22
Hexachlorobenzene
Concen: 0.40 ng
RT: 16.397 min Scan# 1329
Delta R.T. -0.013 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:284 Resp: 21114
Ion Ratio Lower Upper
284 100
142 35.1 22.2 33.2#
249 30.6 26.6 39.8









#23
 Atrazine
 Concen: 0.41 ng
 RT: 16.556 min Scan# 1342
 Delta R.T. -0.000 min
 Lab File: BN015224.D
 Acq: 30 Jun 2021 16:10




Instrument :
 BNA_N
 ClientSampleId :
 ICVBN063021


Tgt Ion:	200	Resp:	9592
Ion Ratio	Lower	Upper	
200	100		
173	28.7	21.7	32.5
215	46.7	43.1	64.7



#24
 Pentachlorophenol
 Concen: 0.44 ng
 RT: 16.750 min Scan# 1358
 Delta R.T. -0.001 min
 Lab File: BN015224.D
 Acq: 30 Jun 2021 16:10

Tgt Ion:	266	Resp:	1730
Ion Ratio	Lower	Upper	
266	100		
264	63.1	51.0	76.4
268	64.0	50.6	76.0









#25
Phenanthrene
Concen: 0.39 ng
RT: 17.140 min Scan# 1390
Delta R.T. 0.012 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021


Tgt Ion:178 Resp: 93576
Ion Ratio Lower Upper
178 100
176 18.9 15.6 23.4
179 15.4 12.1 18.1



#26
Anthracene
Concen: 0.38 ng
RT: 17.225 min Scan# 1397
Delta R.T. 0.000 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:178 Resp: 76619
Ion Ratio Lower Upper
178 100
176 18.4 15.1 22.7
179 15.3 12.2 18.2









#27
Fluoranthene-d10
Concen: 0.38 ng
RT: 19.138 min Scan# 1688
Delta R.T. 0.005 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021


Tgt Ion:212 Resp: 81892
Ion Ratio Lower Upper
212 100
106 14.3 7.0 10.6#
104 7.8 4.1 6.1#



#28
Fluoranthene
Concen: 0.40 ng
RT: 19.168 min Scan# 1694
Delta R.T. 0.005 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:202 Resp: 102022
Ion Ratio Lower Upper
202 100
101 11.8 6.6 10.0#
203 17.4 13.9 20.9









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.313 min Scan# 1986
Delta R.T. 0.010 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021


Tgt Ion:240 Resp: 65526
Ion Ratio Lower Upper
240 100
120 7.0 4.2 6.4#
236 25.6 21.4 32.2



#30
Pyrene
Concen: 0.40 ng
RT: 19.530 min Scan# 1767
Delta R.T. 0.000 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:202 Resp: 100085
Ion Ratio Lower Upper
202 100
200 20.6 16.9 25.3
203 17.4 13.9 20.9









#31
Terphenyl-d14
Concen: 0.40 ng
RT: 19.744 min Scan# 1810
Delta R.T. 0.005 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021

Tgt Ion:244 Resp: 62043
Ion Ratio Lower Upper
244 100
212 7.8 6.3 9.5
122 12.7 6.2 9.2#



#32
Benzo(a)anthracene
Concen: 0.38 ng
RT: 21.292 min Scan# 1984
Delta R.T. 0.011 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:228 Resp: 85728
Ion Ratio Lower Upper
228 100
226 26.8 23.0 34.6
229 19.4 15.7 23.5









#33
Chrysene
Concen: 0.40 ng
RT: 21.345 min Scan# 1989
Delta R.T. 0.010 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021


Tgt Ion:228	Resp:	97478
Ion Ratio	Lower	Upper
228	100	
226	29.4	25.0 37.6
229	19.3	15.9 23.9

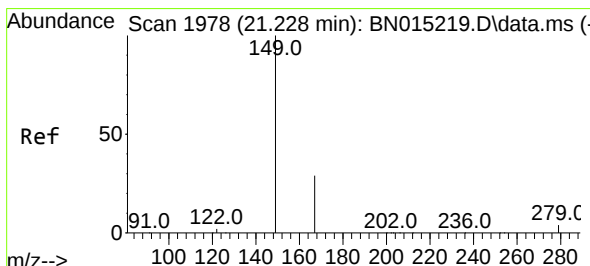

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.41 ng
RT: 21.239 min Scan# 1979
Delta R.T. 0.011 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:149	Resp:	20901
Ion Ratio	Lower	Upper
149	100	
167	27.8	28.9 43.3#
279	3.4	4.9 7.3#





#35

Perylene-d12

Concen: 0.40 ng

RT: 23.564 min Scan# 2427

Delta R.T. 0.014 min

Lab File: BN015224.D

Acq: 30 Jun 2021 16:10





Tgt Ion:264 Resp: 60693

Ion Ratio Lower Upper

264 100

260 25.0 20.6 31.0

265 23.7 21.4 32.2



#36

Indeno(1,2,3-cd)pyrene

Concen: 0.39 ng

RT: 25.826 min Scan# 3088

Delta R.T. 0.013 min

Lab File: BN015224.D

Acq: 30 Jun 2021 16:10




Tgt Ion:276 Resp: 84224

Ion Ratio Lower Upper

276 100

138 25.1 10.0 15.0#

277 24.9 20.4 30.6









#37
Benzo(b)fluoranthene
Concen: 0.39 ng
RT: 22.889 min Scan# 2230
Delta R.T. 0.013 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021

Tgt Ion:252 Resp: 92370
Ion Ratio Lower Upper
252 100
253 22.1 18.5 27.7
125 13.4 5.8 8.6#



#38
Benzo(k)fluoranthene
Concen: 0.39 ng
RT: 22.934 min Scan# 2243
Delta R.T. 0.013 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:252 Resp: 99536
Ion Ratio Lower Upper
252 100
253 22.1 19.1 28.7
125 11.1 5.4 8.0#









#39
Benzo(a)pyrene
Concen: 0.39 ng
RT: 23.468 min Scan# 2399
Delta R.T. 0.013 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10




Instrument :
BNA_N
ClientSampleId :
ICVBN063021


Tgt Ion:252 Resp: 85291
Ion Ratio Lower Upper
252 100
253 23.5 19.4 29.2
125 26.9 7.4 11.2#



#40
Dibenzo(a,h)anthracene
Concen: 0.38 ng
RT: 25.847 min Scan# 3094
Delta R.T. 0.020 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Tgt Ion:278 Resp: 65330
Ion Ratio Lower Upper
278 100
139 18.4 9.0 13.4#
279 23.7 21.0 31.4





#41
Benzo(g,h,i)perylene
Concen: 0.38 ng
RT: 26.514 min Scan# 3289
Delta R.T. 0.017 min
Lab File: BN015224.D
Acq: 30 Jun 2021 16:10

Instrument :
BNA_N
ClientSampleId :
ICVBN063021

Tgt Ion:	276	Resp:	71979
Ion Ratio	Lower	Upper	
276	100		
277	23.8	19.7	29.5
138	24.0	9.8	14.6#

