

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063021\
 Data File : BN015246.D
 Acq On : 01 Jul 2021 06:40
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Jul 01 09:32:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 01 09:06:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.732	152	25006	0.40	ng	# 0.00
7) Naphthalene-d8	10.493	136	110695	0.40	ng	# 0.00
13) Acenaphthene-d10	14.346	164	58326	0.40	ng	0.00
19) Phenanthrene-d10	17.092	188	111392	0.40	ng	0.00
29) Chrysene-d12	21.292	240	97374	0.40	ng	#-0.01
35) Perylene-d12	23.540	264	86371	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.353	112	27252	0.43	ng	0.00
5) Phenol-d6	6.902	99	33562	0.42	ng	0.00
8) Nitrobenzene-d5	8.870	82	26936	0.43	ng	0.00
11) 2-Methylnaphthalene-d10	12.084	152	71653	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.843	330	6633	0.48	ng	0.00
15) 2-Fluorobiphenyl	12.963	172	92330	0.39	ng	0.00
27) Fluoranthene-d10	19.128	212	125417	0.38	ng	0.00
31) Terphenyl-d14	19.734	244	93617	0.41	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.352	88	4723	0.40	ng	# 57
3) n-Nitrosodimethylamine	3.693	42	8625	0.39	ng	# 76
6) bis(2-Chloroethyl)ether	7.169	93	32741	0.41	ng	# 85
9) Naphthalene	10.543	128	126090	0.40	ng	97
10) Hexachlorobutadiene	10.835	225	23892	0.40	ng	# 98
12) 2-Methylnaphthalene	12.159	142	82954	0.41	ng	# 89
16) Acenaphthylene	14.067	152	101055	0.39	ng	98
17) Acenaphthene	14.409	154	71090	0.39	ng	98
18) Fluorene	15.399	166	87352	0.40	ng	99
20) 4,6-Dinitro-2-methylph...	15.475	198	659	0.50	ng	# 68
21) 4-Bromophenyl-phenylether	16.288	248	27175	0.38	ng	# 87
22) Hexachlorobenzene	16.398	284	31283	0.39	ng	# 92
23) Atrazine	16.556	200	16589	0.44	ng	94
24) Pentachlorophenol	16.751	266	4608	0.58	ng	99
25) Phenanthrene	17.128	178	141573	0.39	ng	99
26) Anthracene	17.225	178	117595	0.38	ng	99
28) Fluoranthene	19.158	202	155942	0.40	ng	# 97
30) Pyrene	19.526	202	152797	0.41	ng	99
32) Benzo(a)anthracene	21.271	228	128970	0.39	ng	98
33) Chrysene	21.324	228	144616	0.40	ng	98
34) Bis(2-ethylhexyl)phtha...	21.218	149	46008	0.53	ng	# 87
36) Indeno(1,2,3-cd)pyrene	25.792	276	112944	0.37	ng	# 88
37) Benzo(b)fluoranthene	22.866	252	134789	0.40	ng	# 93
38) Benzo(k)fluoranthene	22.907	252	140797	0.39	ng	# 94
39) Benzo(a)pyrene	23.441	252	120116	0.39	ng	# 83
40) Dibenzo(a,h)anthracene	25.810	278	86352	0.36	ng	# 91
41) Benzo(g,h,i)perylene	26.484	276	96287	0.36	ng	# 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063021\
Data File : BN015246.D
Acq On : 01 Jul 2021 06:40
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Jul 01 09:32:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 01 09:06:31 2021
Response via : Initial Calibration



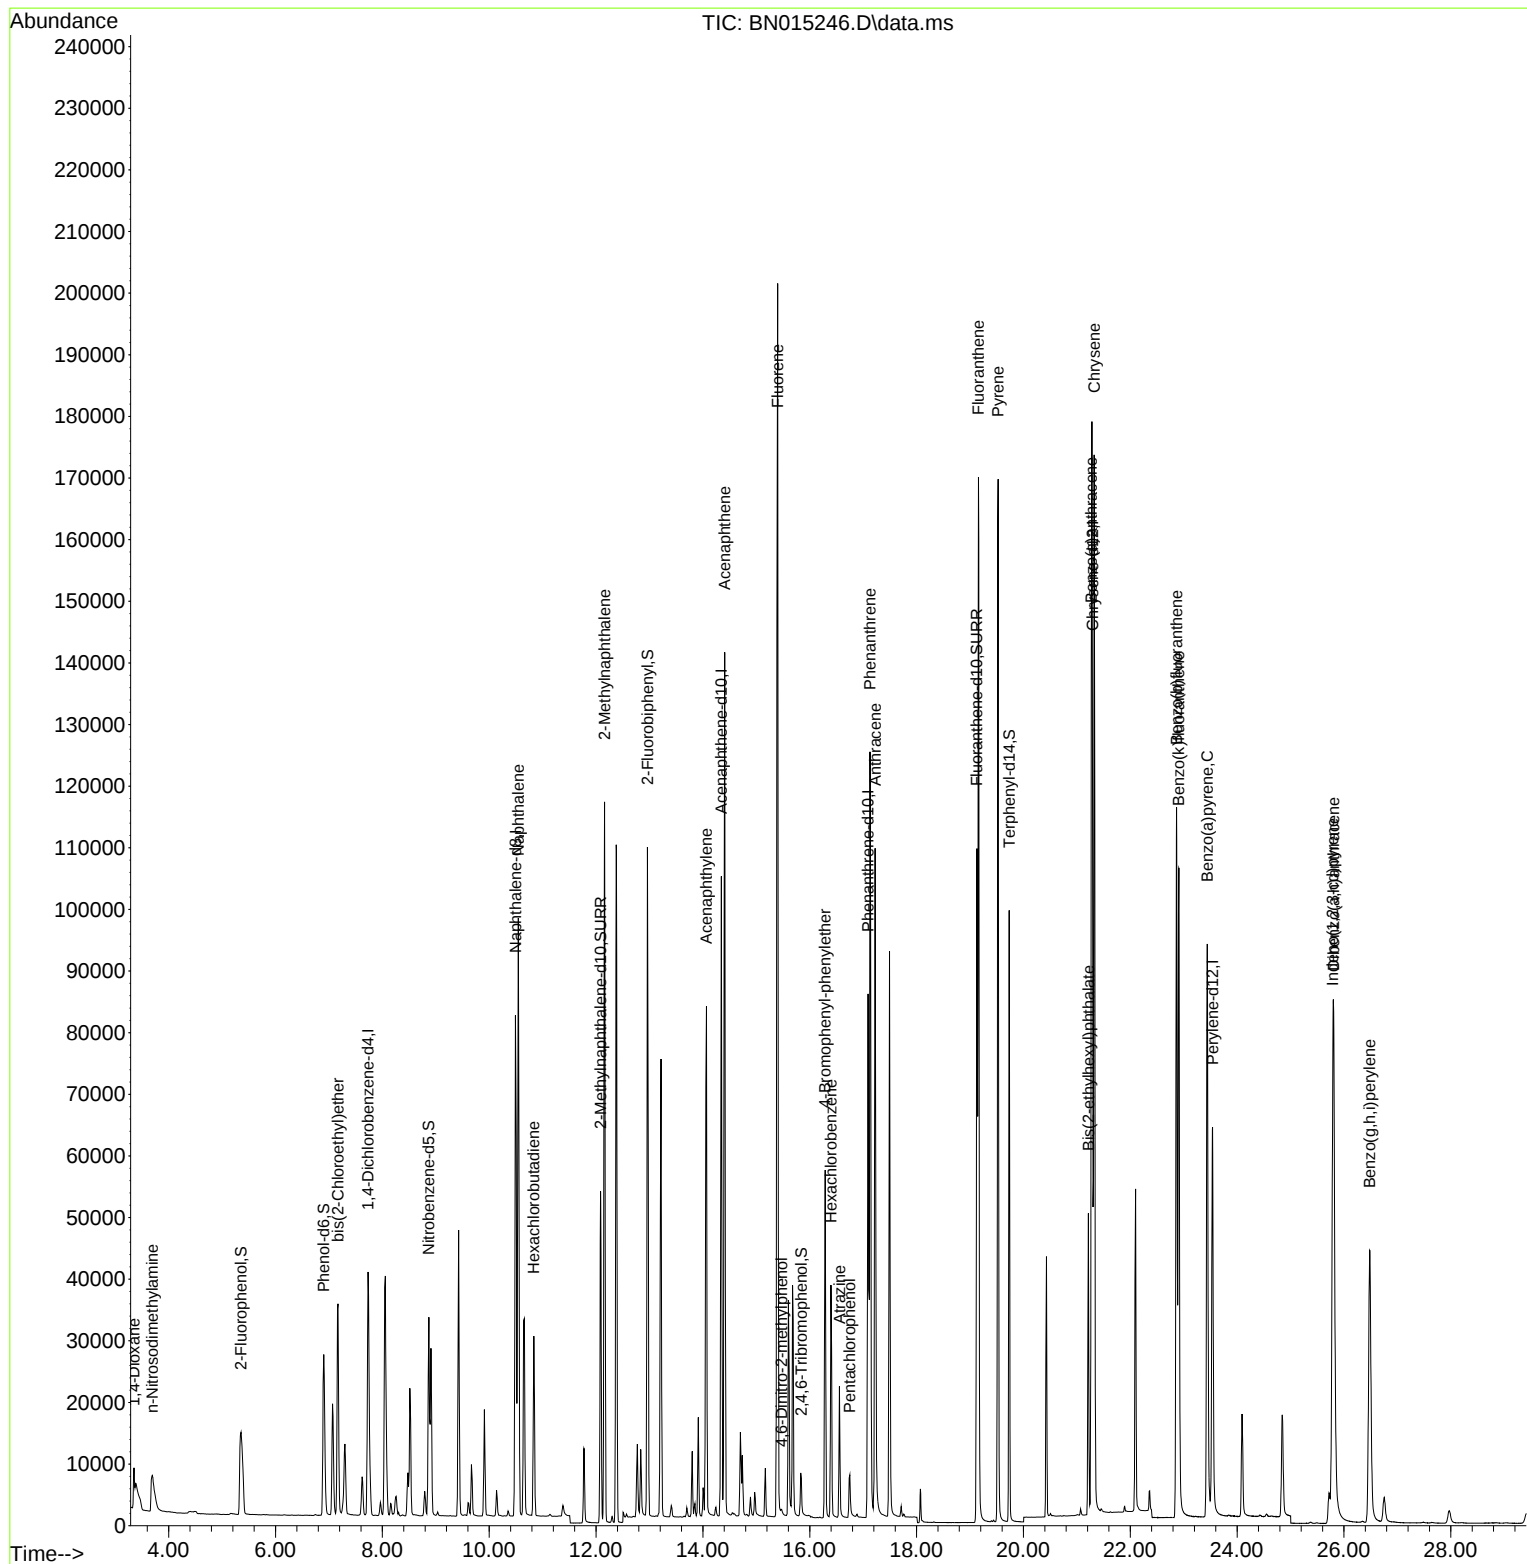




#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.732 min Scan# 483
Delta R.T. -0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampled :
SSTDCCC0.4

Tgt Ion:152 Resp: 25006
Ion Ratio Lower Upper
152 100
150 156.7 119.0 178.6
115 60.6 62.2 93.4#

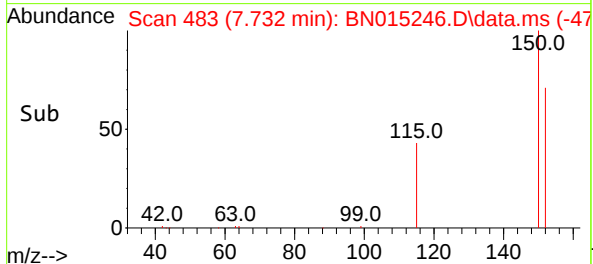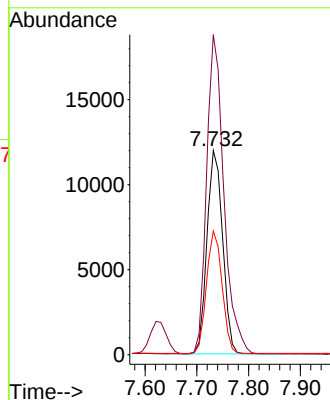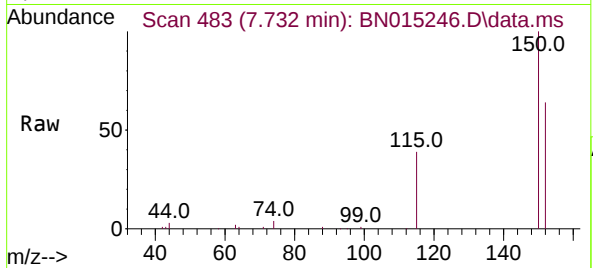

#2
1,4-Dioxane
Concen: 0.40 ng
RT: 3.352 min Scan# 8
Delta R.T. 0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion: 88 Resp: 4723
Ion Ratio Lower Upper
88 100
43 28.1 12.9 19.3#
58 79.5 38.1 57.1#


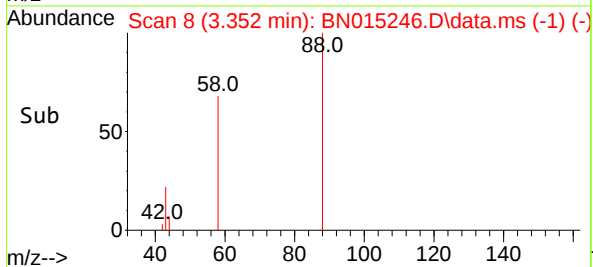
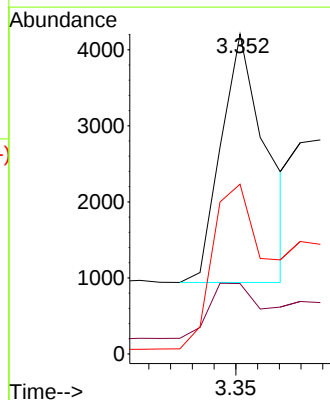
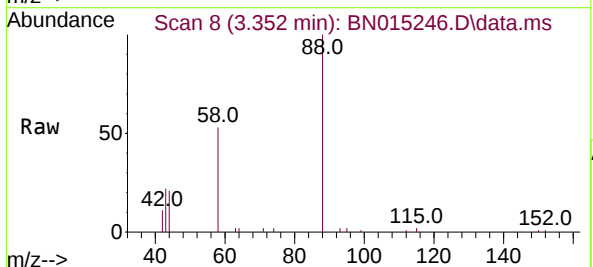




#3
n-Nitrosodimethylamine
Concen: 0.39 ng
RT: 3.693 min Scan# 45
Delta R.T. 0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion: 42 Resp: 8625
Ion Ratio Lower Upper
42 100
74 151.6 149.5 224.3
44 7.6 4.2 6.2#

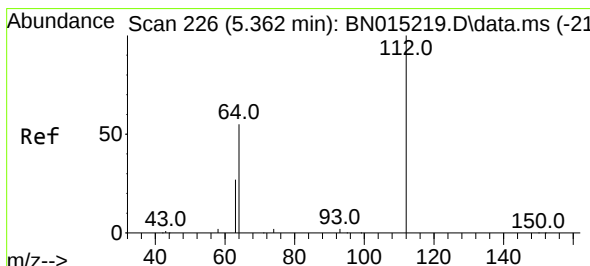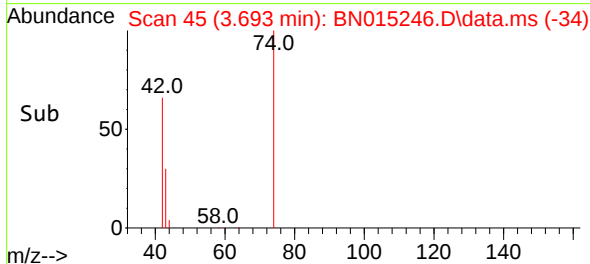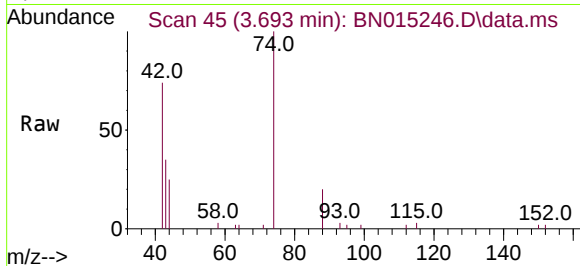

#4
2-Fluorophenol
Concen: 0.43 ng
RT: 5.353 min Scan# 225
Delta R.T. -0.009 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion: 112 Resp: 27252
Ion Ratio Lower Upper
112 100
64 56.0 39.0 58.6
63 27.7 20.6 30.8


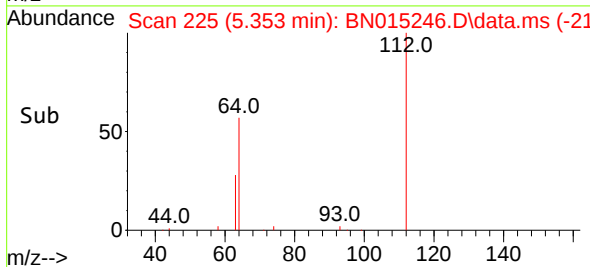

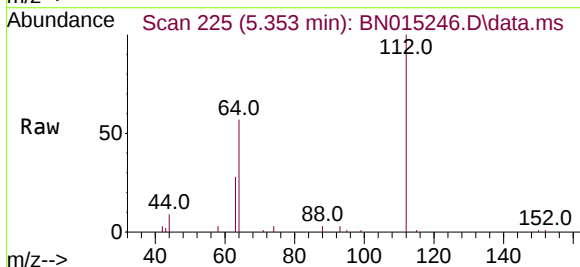




#5
Phenol-d6
Concen: 0.42 ng
RT: 6.902 min Scan# 393
Delta R.T. 0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion: 99 Resp: 33562
Ion Ratio Lower Upper
99 100
42 16.9 8.9 13.3#
71 30.0 35.6 53.4#

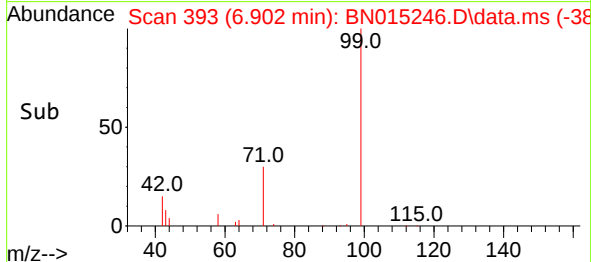

#6
bis(2-Chloroethyl)ether
Concen: 0.41 ng
RT: 7.169 min Scan# 422
Delta R.T. 0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion: 93 Resp: 32741
Ion Ratio Lower Upper
93 100
63 74.5 46.6 70.0#
95 32.8 28.6 42.8


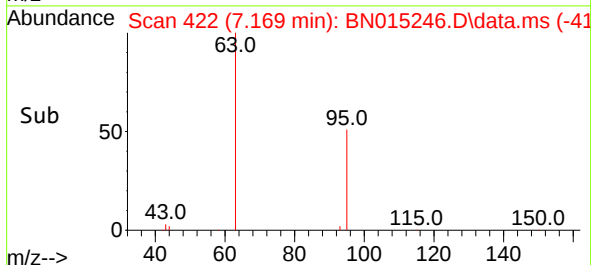

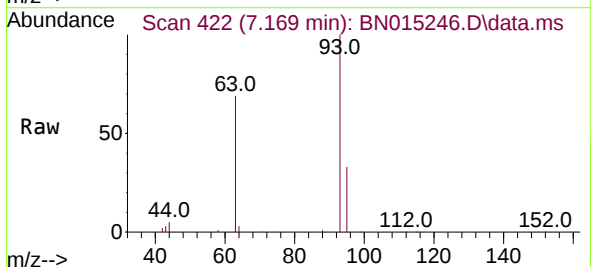




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.493 min Scan# 718
Delta R.T. 0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	110695
Ion Ratio	Lower	Upper	
136	100		
137	10.9	9.8	14.8
54	8.3	5.4	8.2#
68	6.9	4.9	7.3

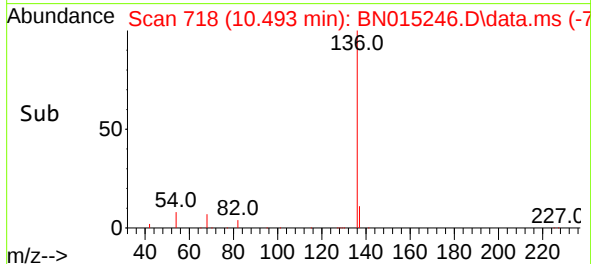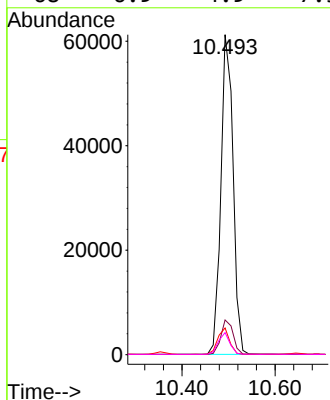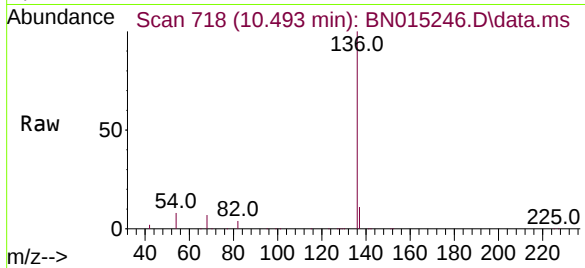

#8
Nitrobenzene-d5
Concen: 0.43 ng
RT: 8.870 min Scan# 590
Delta R.T. 0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:	82	Resp:	26936
Ion Ratio	Lower	Upper	
82	100		
128	40.9	31.6	47.4
54	46.8	29.0	43.4#



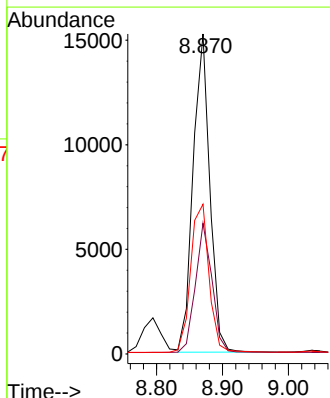
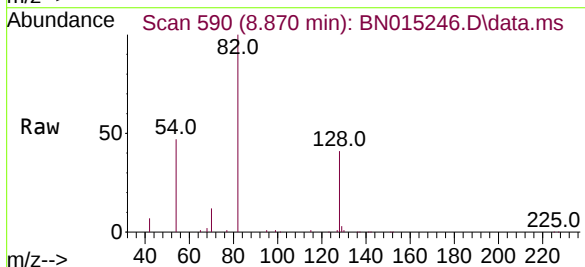


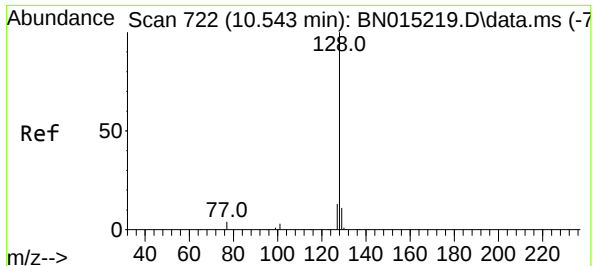

#9
Naphthalene
Concen: 0.40 ng
RT: 10.543 min Scan# 722
Delta R.T. 0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:128 Resp: 126090
Ion Ratio Lower Upper
128 100
129 11.0 9.1 13.7
127 13.0 11.8 17.6

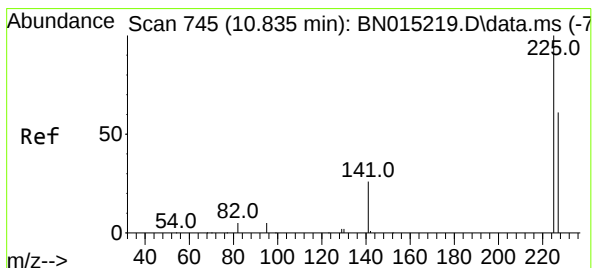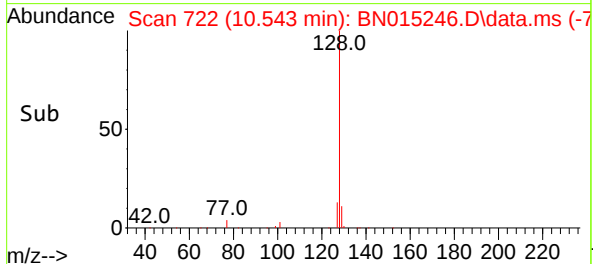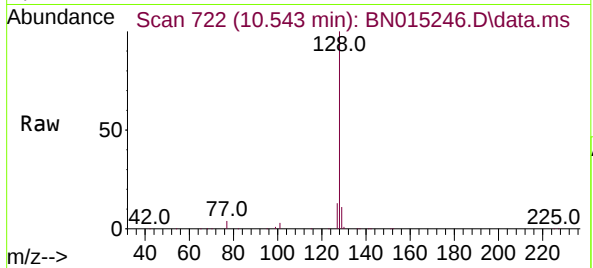

#10
Hexachlorobutadiene
Concen: 0.40 ng
RT: 10.835 min Scan# 745
Delta R.T. 0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:225 Resp: 23892
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.0 50.2 75.2


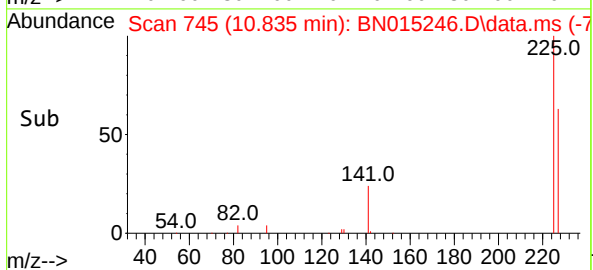

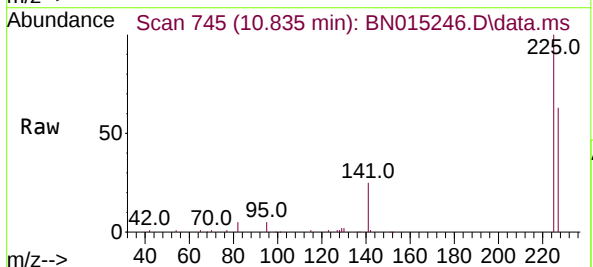




#11
2-Methylnaphthalene-d10
Concen: 0.39 ng
RT: 12.084 min Scan# 926
Delta R.T. -0.004 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 71653
Ion Ratio Lower Upper
152 100
151 20.4 16.7 25.1

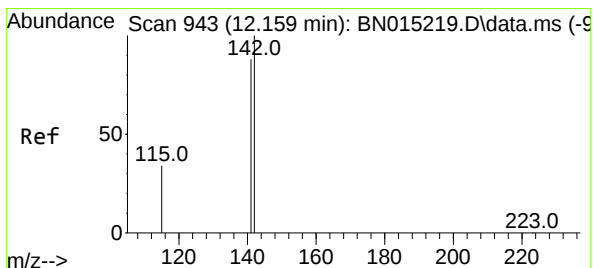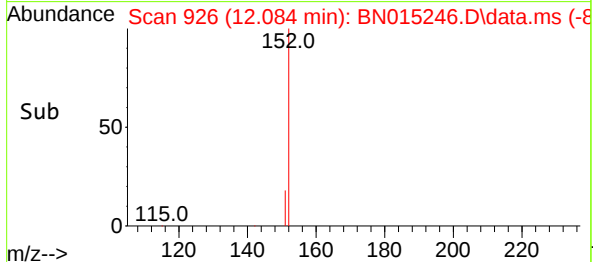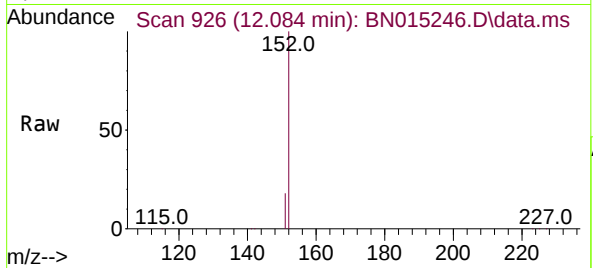

#12
2-Methylnaphthalene
Concen: 0.41 ng
RT: 12.159 min Scan# 943
Delta R.T. 0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:142 Resp: 82954
Ion Ratio Lower Upper
142 100
141 87.7 72.3 108.5
115 33.0 40.7 61.1#


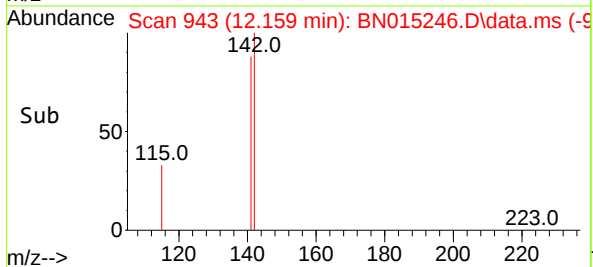

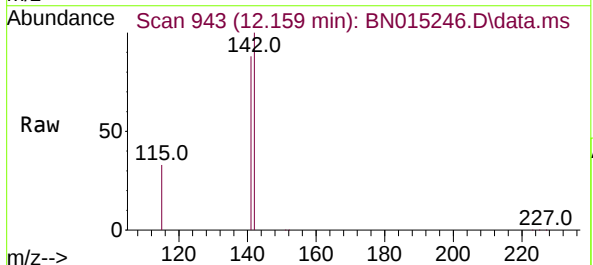




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.346 min Scan# 1166
Delta R.T. -0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:164 Resp: 58326
Ion Ratio Lower Upper
164 100
162 100.3 83.8 125.6
160 45.3 37.4 56.0

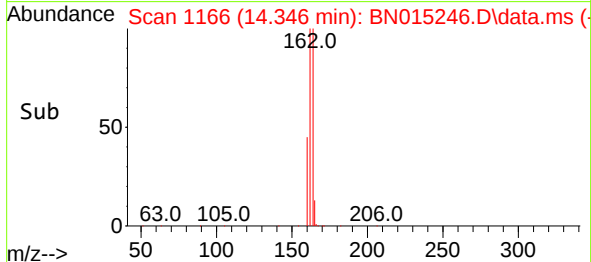

#14
2,4,6-Tribromophenol
Concen: 0.48 ng
RT: 15.843 min Scan# 1284
Delta R.T. -0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:330 Resp: 6633
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 36.1 22.4 33.6#


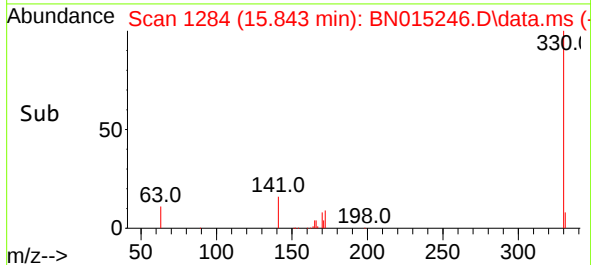

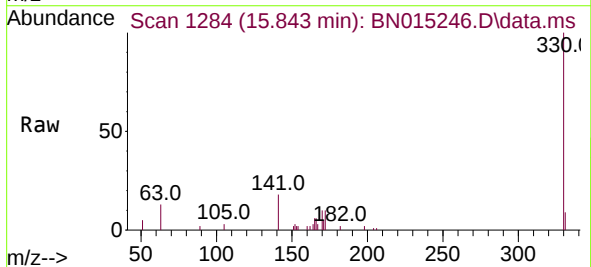




#15
2-Fluorobiphenyl
Concen: 0.39 ng
RT: 12.963 min Scan# 1057
Delta R.T. -0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:172	Resp:	92330
Ion Ratio	Lower	Upper
172	100	
171	34.6	30.6 45.8
170	23.4	20.2 30.4

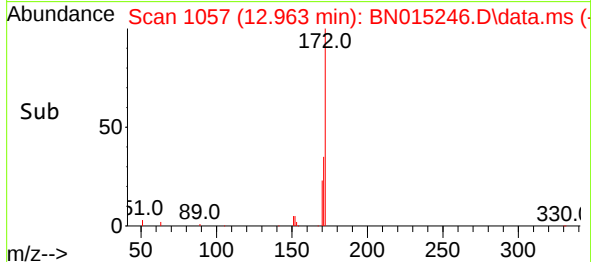

#16
Acenaphthylene
Concen: 0.39 ng
RT: 14.067 min Scan# 1144
Delta R.T. -0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:152	Resp:	101055
Ion Ratio	Lower	Upper
152	100	
151	19.4	16.7 25.1
153	13.1	10.5 15.7


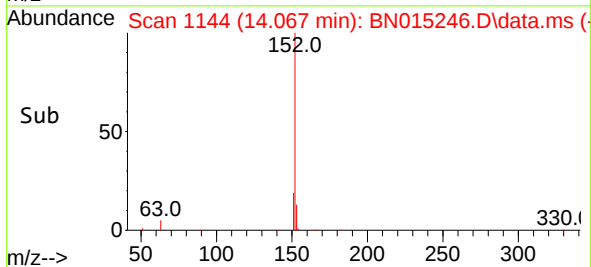

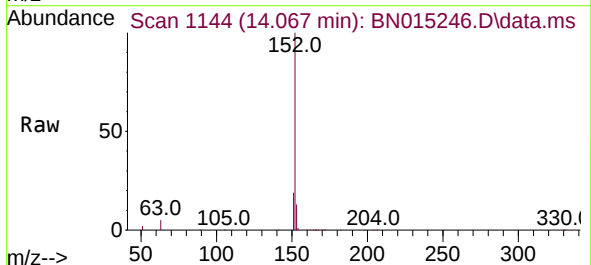




#17
Acenaphthene
Concen: 0.39 ng
RT: 14.409 min Scan# 1171
Delta R.T. 0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 71090
Ion Ratio Lower Upper
154 100
153 112.4 90.9 136.3
152 55.5 45.8 68.8

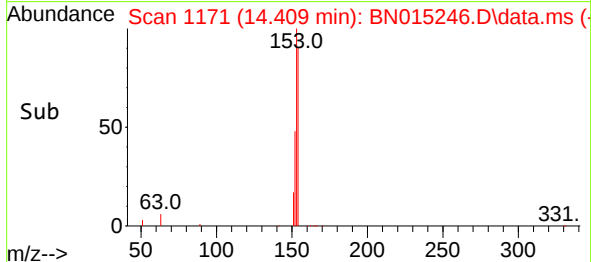

#18
Fluorene
Concen: 0.40 ng
RT: 15.399 min Scan# 1249
Delta R.T. -0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:166 Resp: 87352
Ion Ratio Lower Upper
166 100
165 97.6 79.2 118.8
167 13.5 10.7 16.1


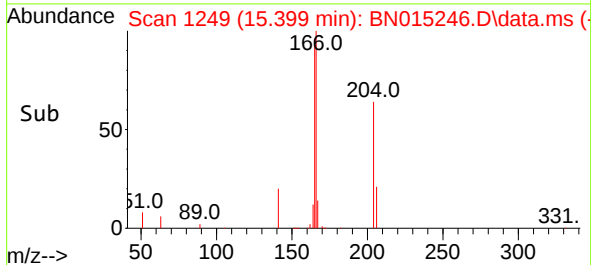

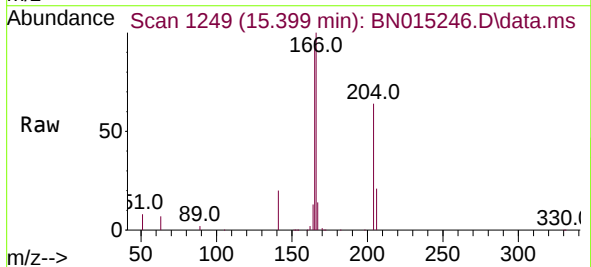




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.092 min Scan# 1386
Delta R.T. 0.001 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188 Resp: 111392
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.9 9.0 13.4

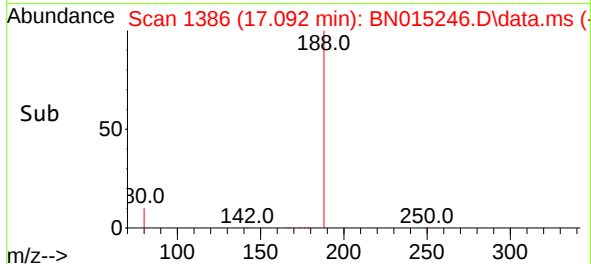

#20
4,6-Dinitro-2-methylphenol
Concen: 0.50 ng
RT: 15.475 min Scan# 1255
Delta R.T. -0.013 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:198 Resp: 659
Ion Ratio Lower Upper
198 100
182 22.5 34.5 51.7#
77 0.0 0.0 0.0


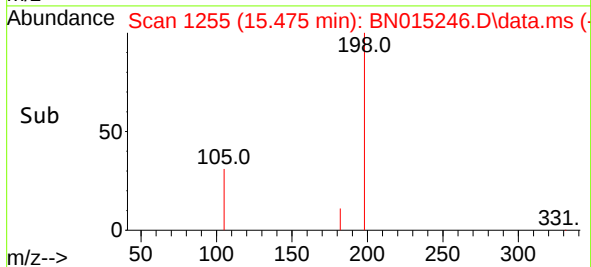

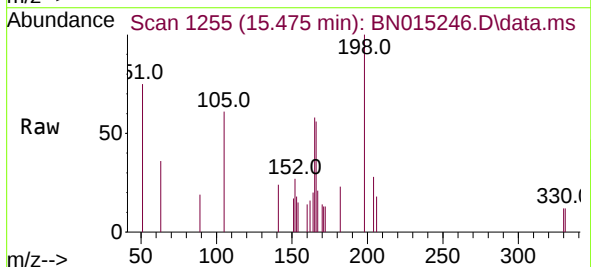


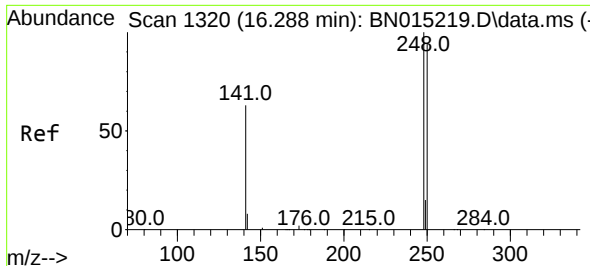

#21
4-Bromophenyl-phenylether
Concen: 0.38 ng
RT: 16.288 min Scan# 1320
Delta R.T. 0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:248 Resp: 27175
Ion Ratio Lower Upper
248 100
250 96.3 86.2 129.4
141 57.3 36.2 54.2#

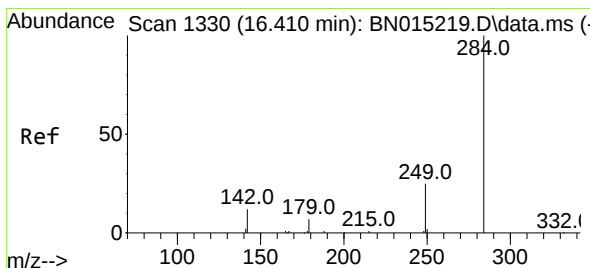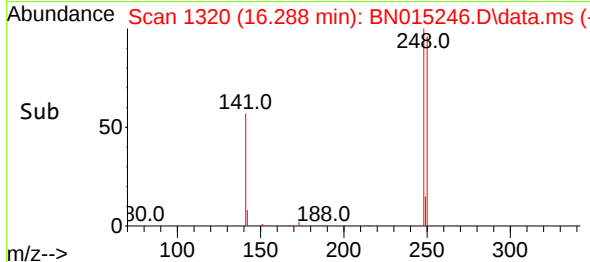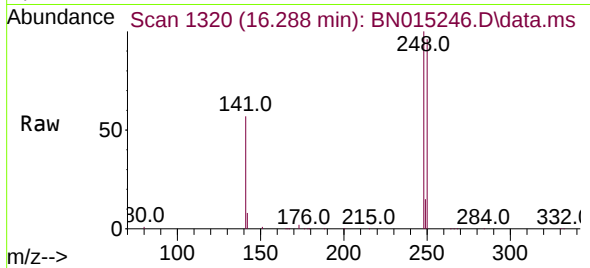

#22
Hexachlorobenzene
Concen: 0.39 ng
RT: 16.398 min Scan# 1329
Delta R.T. -0.012 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:284 Resp: 31283
Ion Ratio Lower Upper
284 100
142 34.6 22.2 33.2#
249 30.8 26.6 39.8


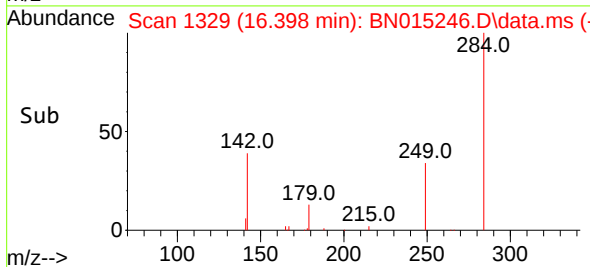

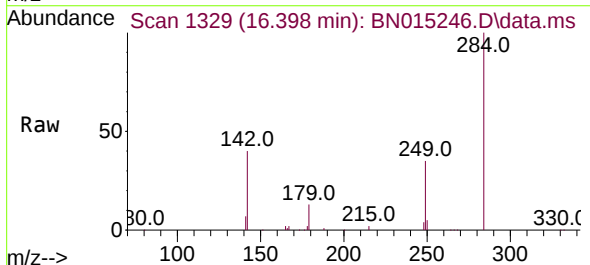




#23
Atrazine
Concen: 0.44 ng
RT: 16.556 min Scan# 1342
Delta R.T. 0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:200 Resp: 16589
Ion Ratio Lower Upper
200 100
173 27.0 21.7 32.5
215 47.7 43.1 64.7

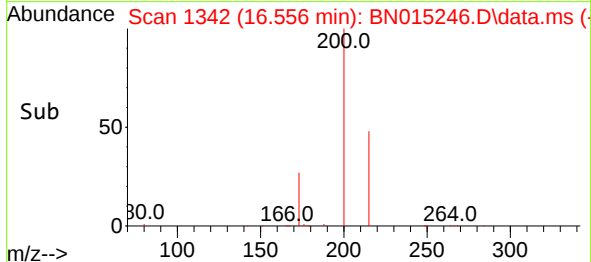

#24
Pentachlorophenol
Concen: 0.58 ng
RT: 16.751 min Scan# 1358
Delta R.T. -0.000 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:266 Resp: 4608
Ion Ratio Lower Upper
266 100
264 63.3 51.0 76.4
268 64.1 50.6 76.0


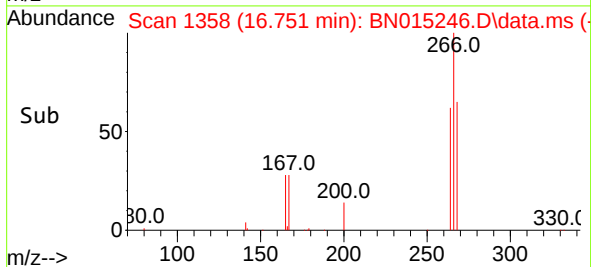

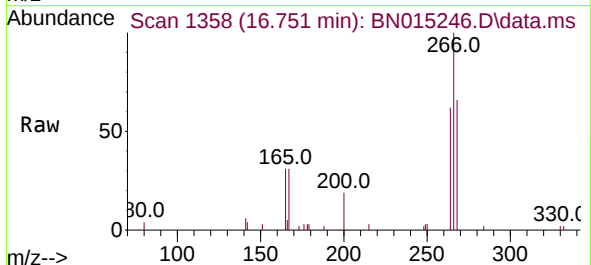


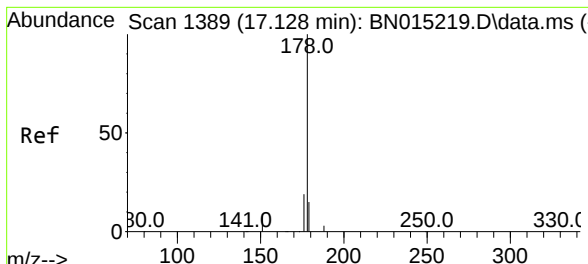

#25
 Phenanthrene
 Concen: 0.39 ng
 RT: 17.128 min Scan# 1389
 Delta R.T. 0.000 min
 Lab File: BN015246.D
 Acq: 01 Jul 2021 06:40




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion:	178	Resp:	141573
Ion Ratio	Lower	Upper	
178	100		
176	18.8	15.6	23.4
179	15.4	12.1	18.1

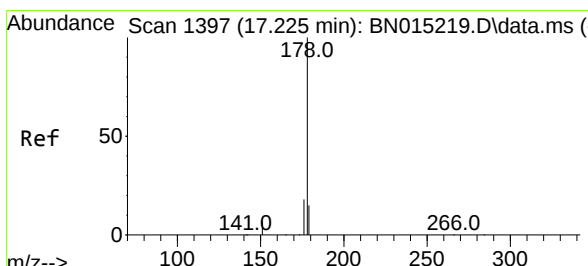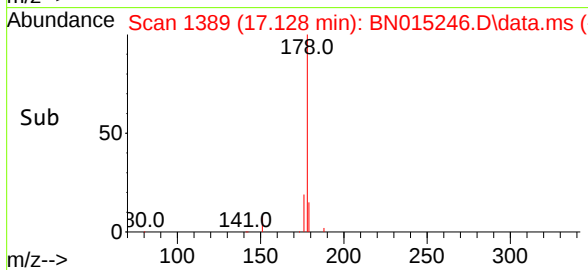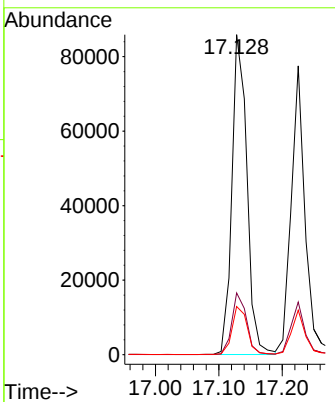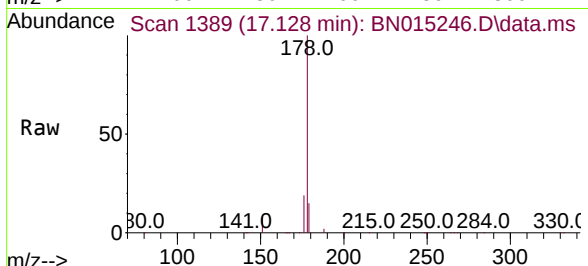

#26
 Anthracene
 Concen: 0.38 ng
 RT: 17.225 min Scan# 1397
 Delta R.T. 0.000 min
 Lab File: BN015246.D
 Acq: 01 Jul 2021 06:40

Tgt Ion:	178	Resp:	117595
Ion Ratio	Lower	Upper	
178	100		
176	18.3	15.1	22.7
179	15.3	12.2	18.2


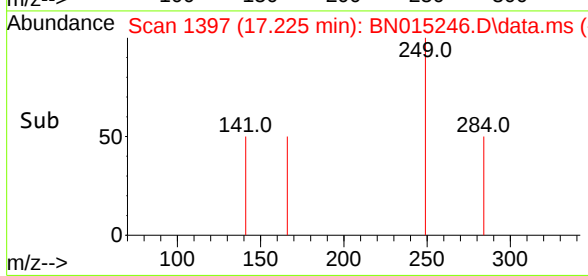
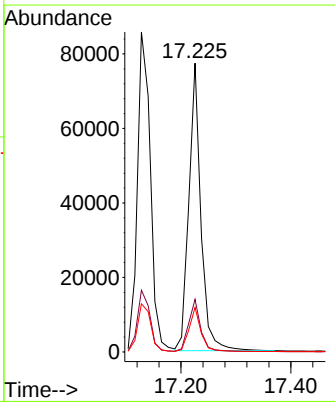
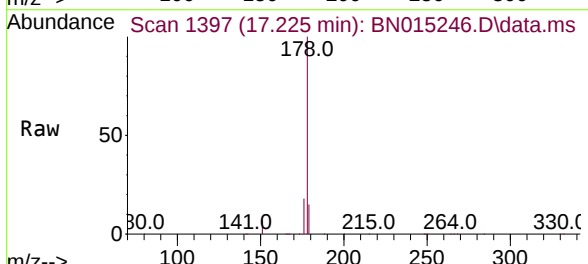


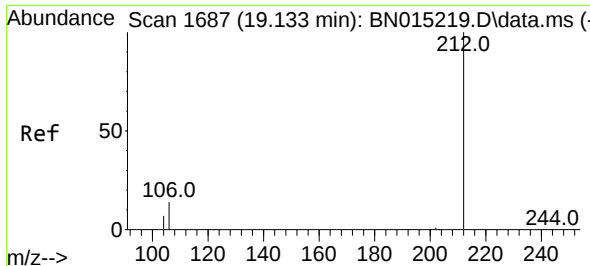

#27
Fluoranthene-d10
Concen: 0.38 ng
RT: 19.128 min Scan# 1686
Delta R.T. -0.005 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 125417
Ion Ratio Lower Upper
212 100
106 14.3 7.0 10.6#
104 7.8 4.1 6.1#

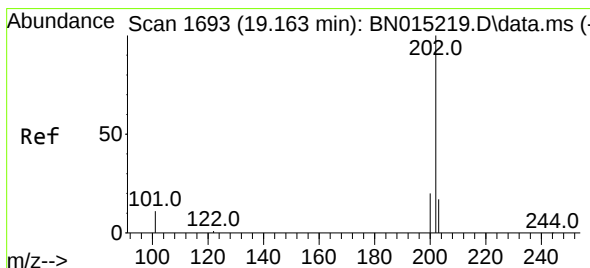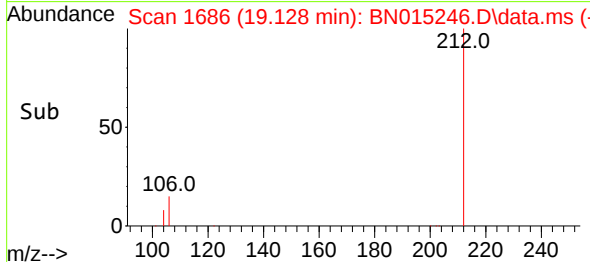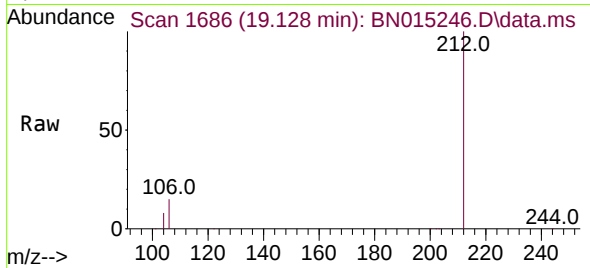

#28
Fluoranthene
Concen: 0.40 ng
RT: 19.158 min Scan# 1692
Delta R.T. -0.005 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:202 Resp: 155942
Ion Ratio Lower Upper
202 100
101 11.8 6.6 10.0#
203 17.3 13.9 20.9


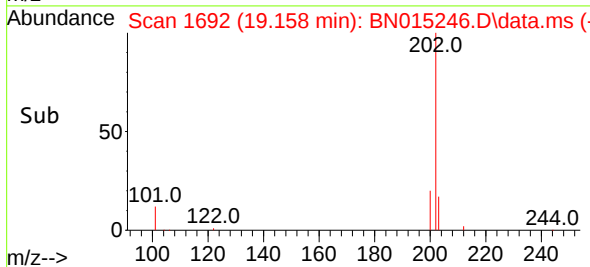

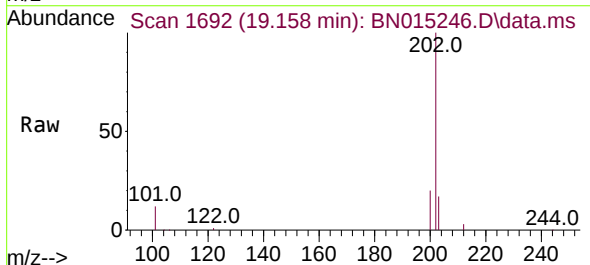




#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.292 min Scan# 1984
Delta R.T. -0.011 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:240 Resp: 97374
Ion Ratio Lower Upper
240 100
120 9.1 4.2 6.4#
236 26.5 21.4 32.2

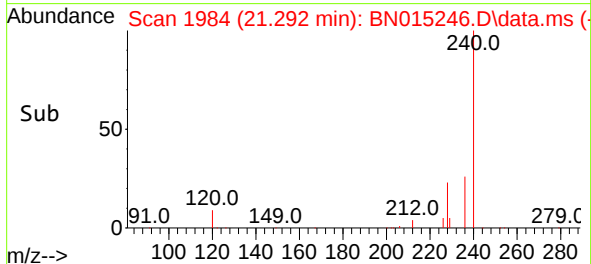

#30
Pyrene
Concen: 0.41 ng
RT: 19.526 min Scan# 1766
Delta R.T. -0.004 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:202 Resp: 152797
Ion Ratio Lower Upper
202 100
200 20.5 16.9 25.3
203 17.4 13.9 20.9


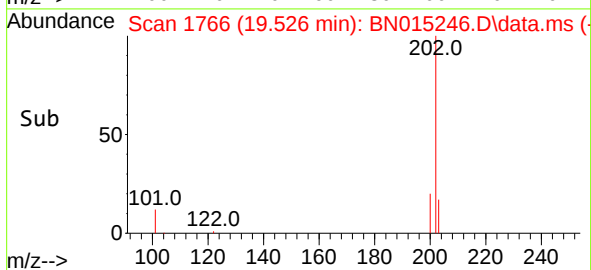

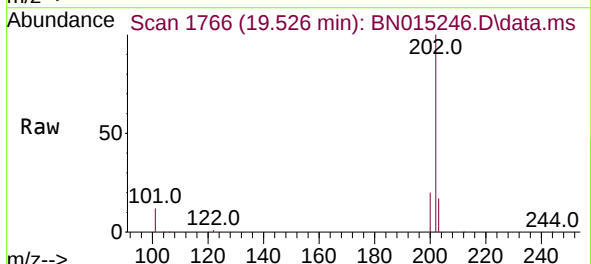




#31
Terphenyl-d14
Concen: 0.41 ng
RT: 19.734 min Scan# 1808
Delta R.T. -0.005 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:244 Resp: 93617
Ion Ratio Lower Upper
244 100
212 7.6 6.3 9.5
122 12.6 6.2 9.2#

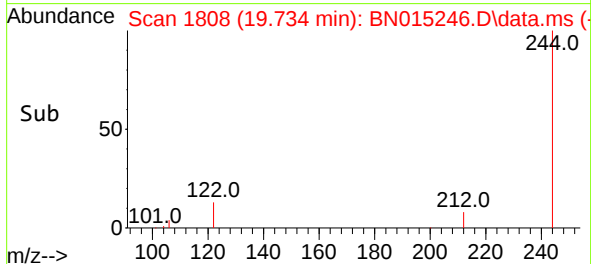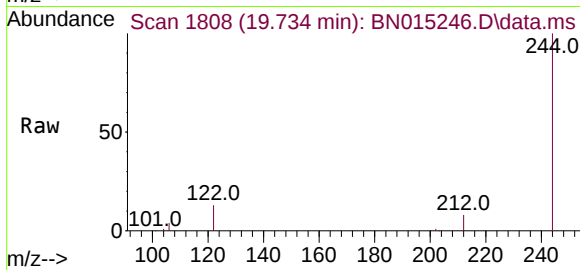

#32
Benzo(a)anthracene
Concen: 0.39 ng
RT: 21.271 min Scan# 1982
Delta R.T. -0.010 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:228 Resp: 128970
Ion Ratio Lower Upper
228 100
226 27.9 23.0 34.6
229 19.0 15.7 23.5


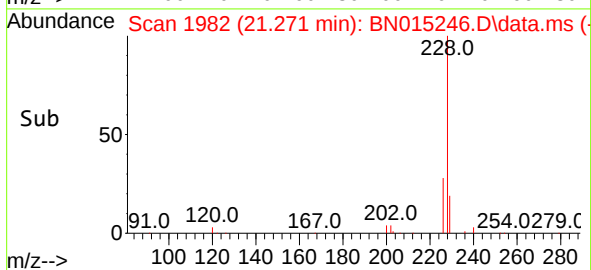

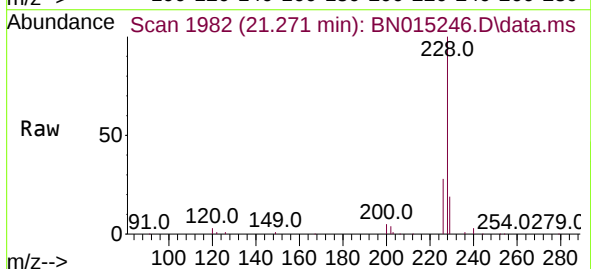




#33
Chrysene
Concen: 0.40 ng
RT: 21.324 min Scan# 1987
Delta R.T. -0.011 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:228	Resp: 144616
Ion Ratio	Lower Upper
228	100
226	29.8 25.0 37.6
229	19.1 15.9 23.9

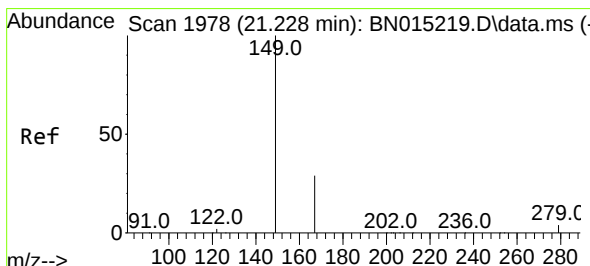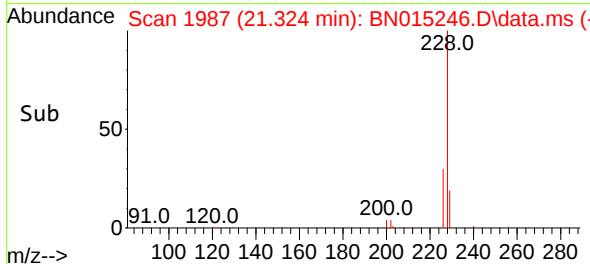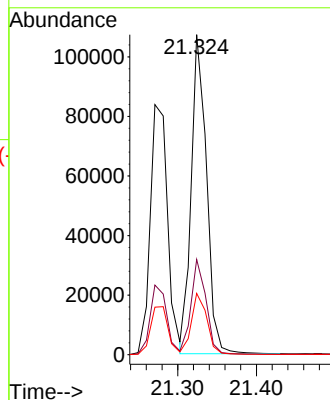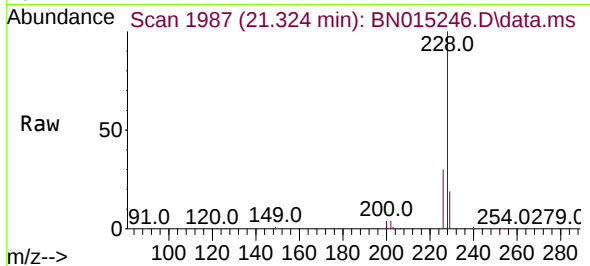

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.53 ng
RT: 21.218 min Scan# 1977
Delta R.T. -0.010 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40


Tgt Ion:149	Resp: 46008
Ion Ratio	Lower Upper
149	100
167	27.8 28.9 43.3#
279	3.5 4.9 7.3#

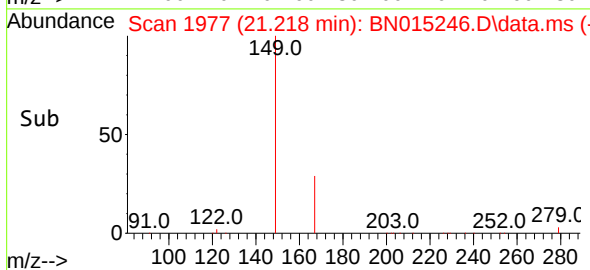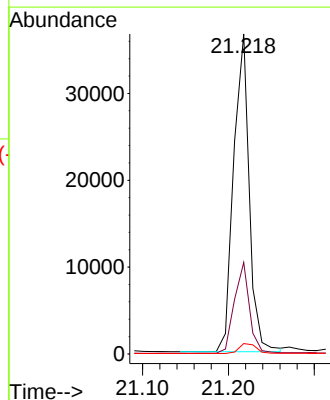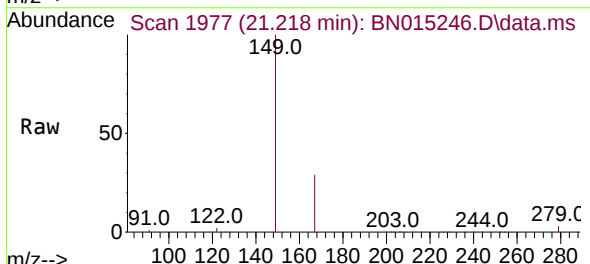






#35
Perylene-d12
Concen: 0.40 ng
RT: 23.540 min Scan# 2420
Delta R.T. -0.010 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4






Tgt Ion:	264	Resp:	86371
Ion Ratio	Lower	Upper	
264	100		
260	24.9	20.6	31.0
265	22.7	21.4	32.2

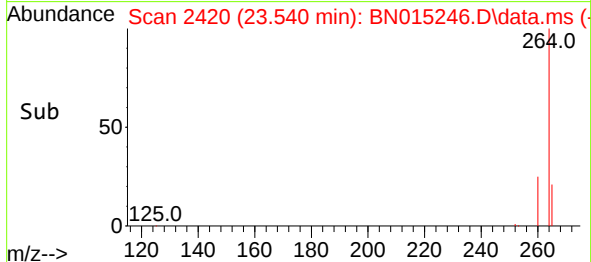

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.37 ng
RT: 25.792 min Scan# 3078
Delta R.T. -0.020 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:	276	Resp:	112944
Ion Ratio	Lower	Upper	
276	100		
138	25.8	10.0	15.0#
277	24.9	20.4	30.6


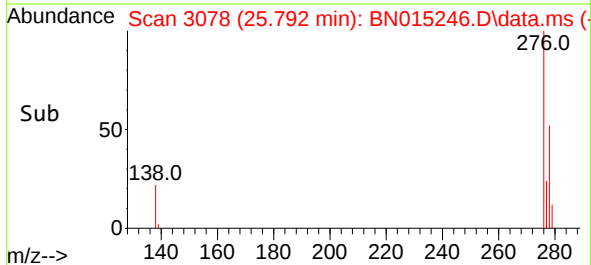
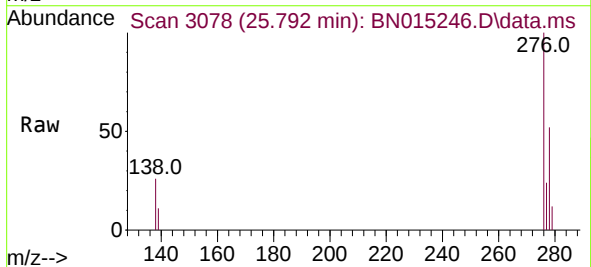





#37
Benzo(b)fluoranthene
Concen: 0.40 ng
RT: 22.866 min Scan# 2223
Delta R.T. -0.010 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:252 Resp: 134789
Ion Ratio Lower Upper
252 100
253 22.5 18.5 27.7
125 16.8 5.8 8.6#

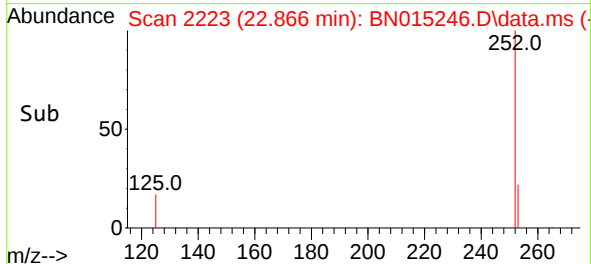

#38
Benzo(k)fluoranthene
Concen: 0.39 ng
RT: 22.907 min Scan# 2235
Delta R.T. -0.014 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Tgt Ion:252 Resp: 140797
Ion Ratio Lower Upper
252 100
253 21.8 19.1 28.7
125 11.0 5.4 8.0#

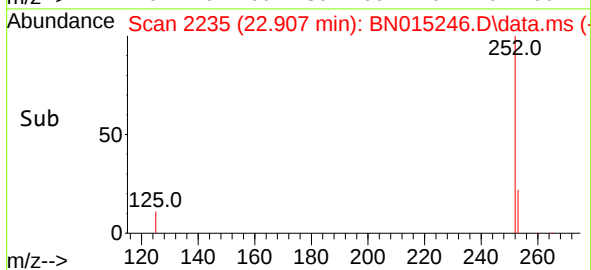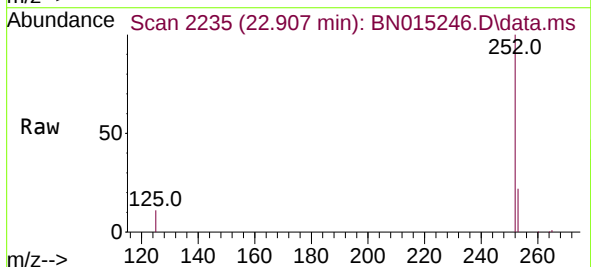



#39

Benzo(a)pyrene

Concen: 0.39 ng

RT: 23.441 min Scan# 2391

Delta R.T. -0.014 min

Lab File: BN015246.D

Acq: 01 Jul 2021 06:40





Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4

Tgt Ion:252	Resp:	120116
Ion Ratio	Lower	Upper
252	100	
253	24.3	19.4 29.2
125	31.3	7.4 11.2#

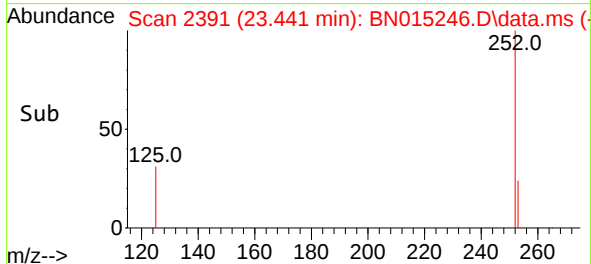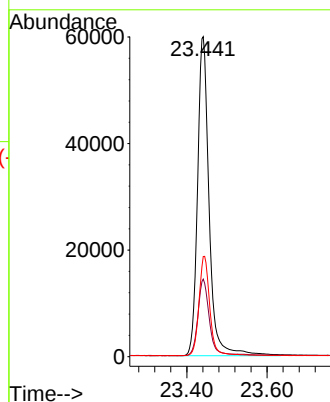

#40

Dibenzo(a,h)anthracene

Concen: 0.36 ng




RT: 25.810 min Scan# 3083


Delta R.T. -0.017 min

Lab File: BN015246.D

Acq: 01 Jul 2021 06:40

Tgt Ion:278	Resp:	86352
Ion Ratio	Lower	Upper
278	100	
139	18.7	9.0 13.4#
279	23.6	21.0 31.4

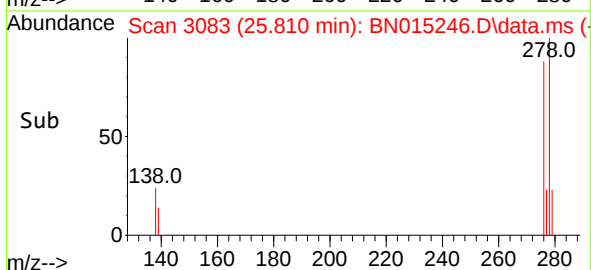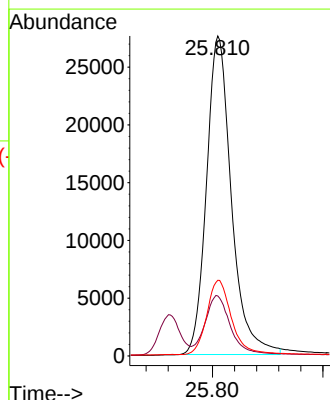

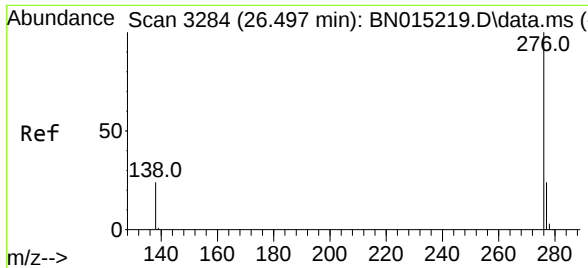

#41
Benzo(g,h,i)perylene
Concen: 0.36 ng
RT: 26.484 min Scan# 3280
Delta R.T. -0.014 min
Lab File: BN015246.D
Acq: 01 Jul 2021 06:40

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Tgt Ion:	276	Resp:	96287
Ion Ratio	Lower	Upper	
276	100		
277	23.6	19.7	29.5
138	23.8	9.8	14.6#

