
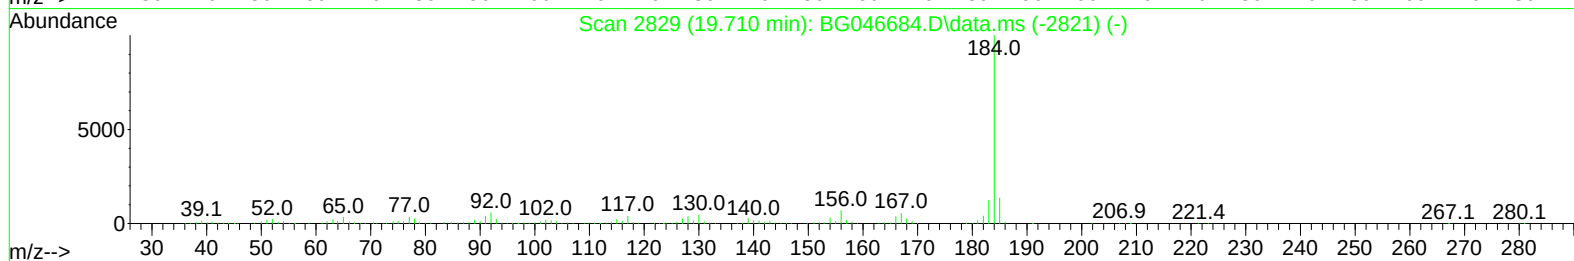
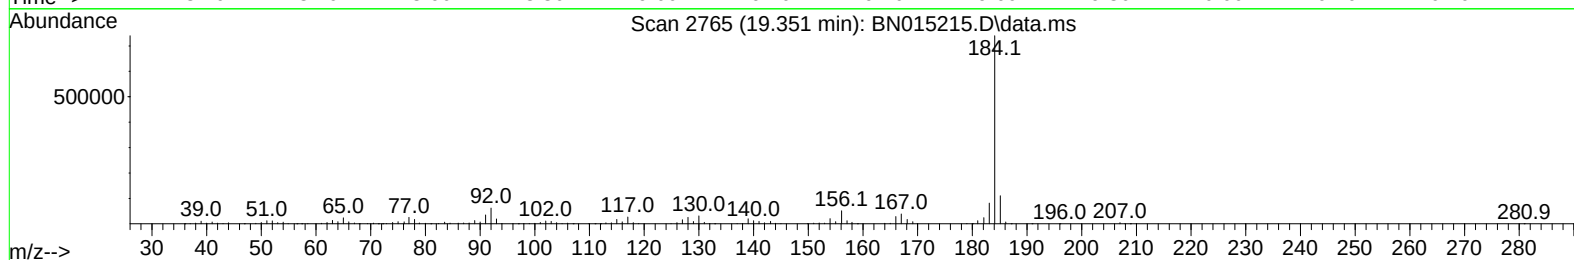


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063021\
 Data File : BN015215.D
 Acq On : 30 Jun 2021 09:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 10:42:33 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 23 10:10:58 2021
 Response via : Initial Calibration

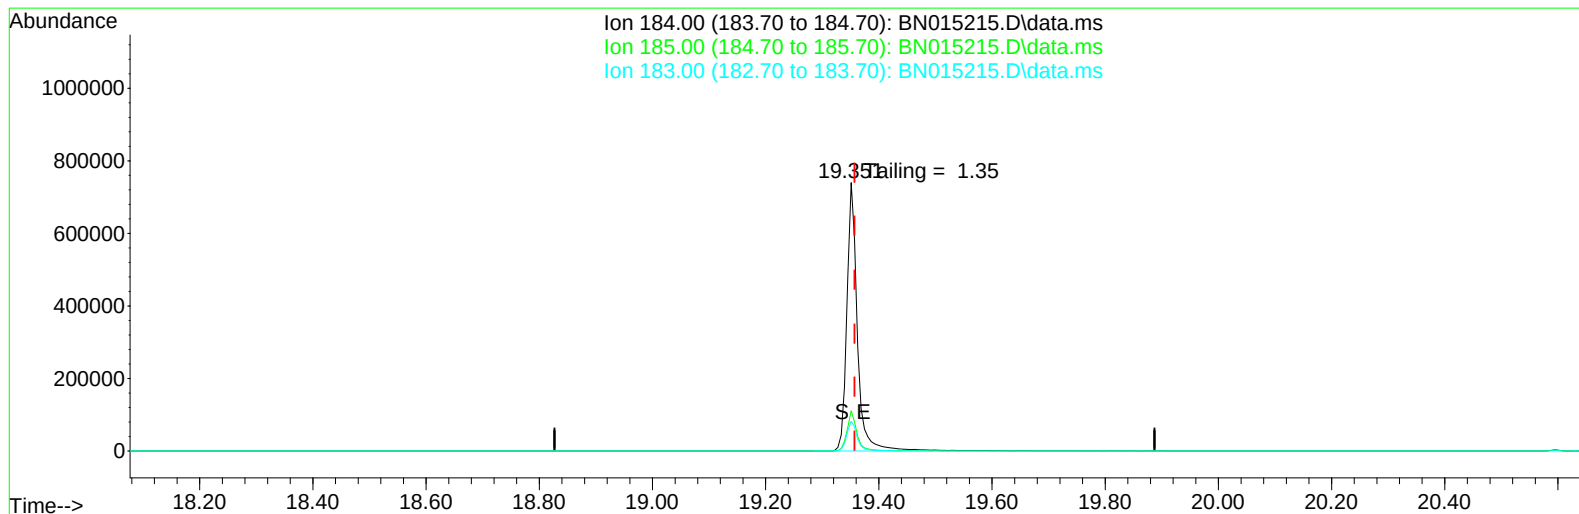

TIC: BN015215.D\data.ms

(77) Benzidine




19.351min (-0.006) 0.00 ng

response 956007

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.98
183.00	13.20	11.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063021\
Data File : BN015215.D
Acq On : 30 Jun 2021 09:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 10:42:33 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

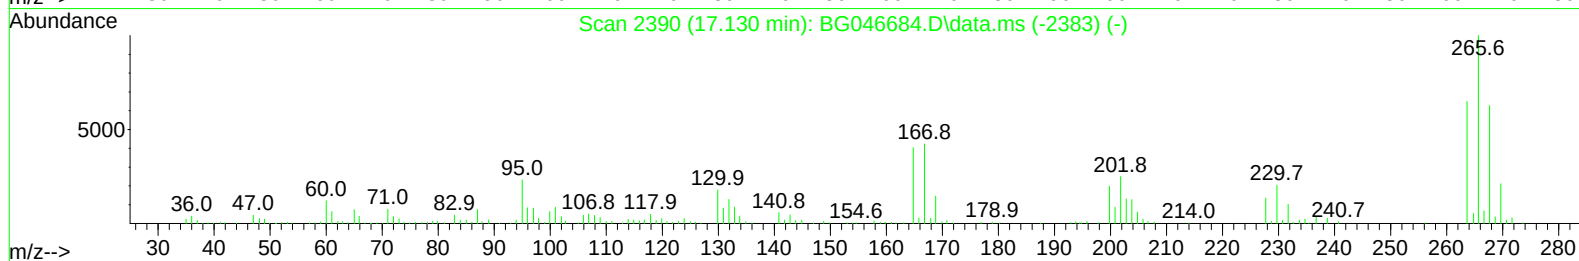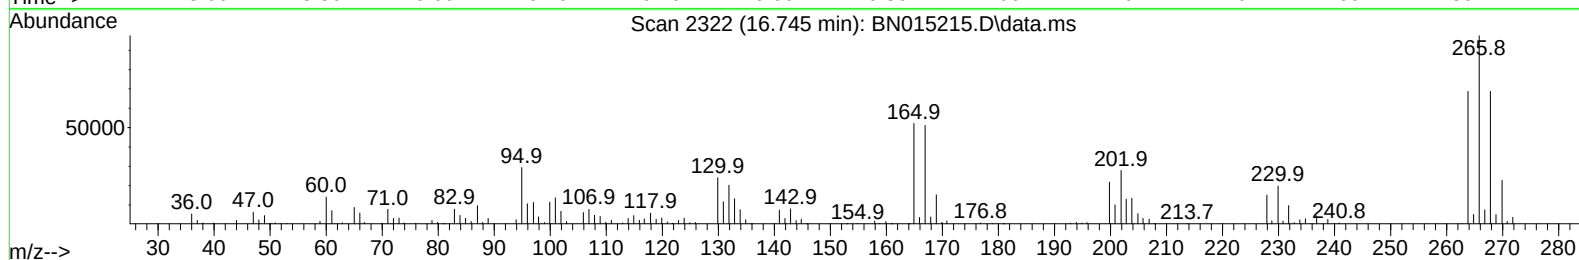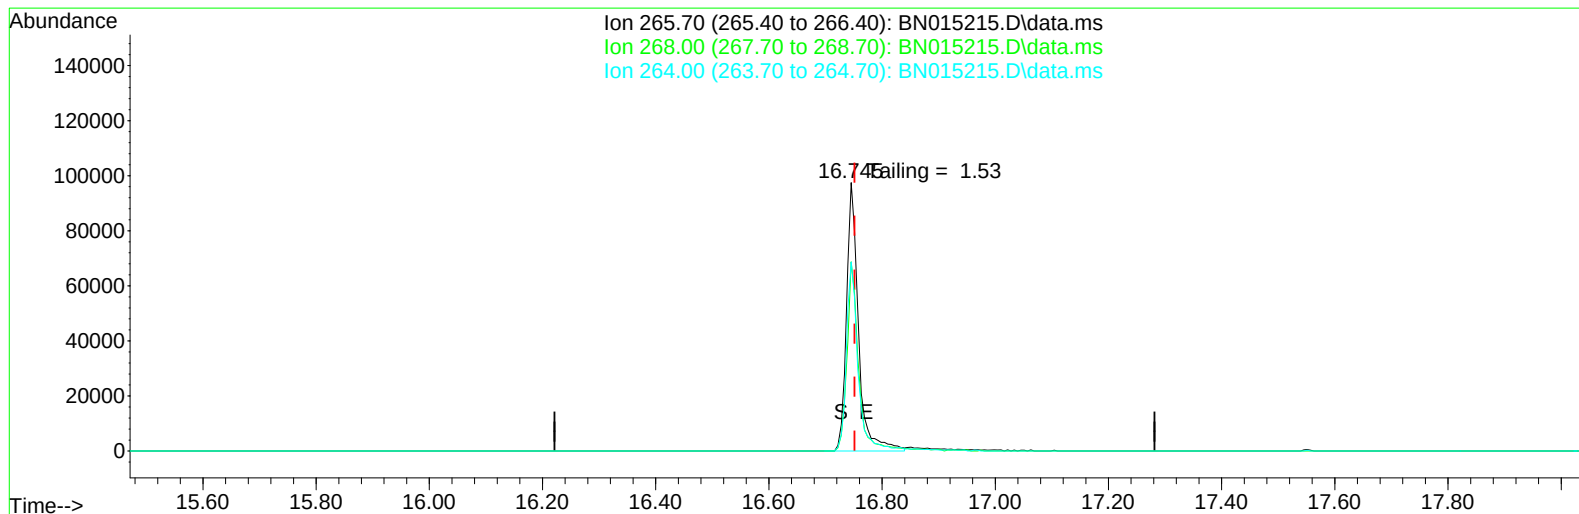

TIC: BN015215.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.006) 15167.50 ng

response 143432

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.46
264.00	61.60	70.44
0.00	0.00	0.00