

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063021\
 Data File : BN015218.D
 Acq On : 30 Jun 2021 12:07
 Operator : CG/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Manual Integrations
 APPROVED

mohammad
 7/1/2021 2:53:45 PM

Quant Time: Jun 30 13:23:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 30 13:21:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.732	152	20772	0.400	ng	# 0.00
7) Naphthalene-d8	10.493	136	90398	0.400	ng	# 0.00
13) Acenaphthene-d10	14.346	164	44390	0.400	ng	0.00
19) Phenanthrene-d10	17.092	188	84508	0.400	ng	0.00
29) Chrysene-d12	21.303	240	74187	0.400	ng	# 0.00
35) Perylene-d12	23.550	264	69311	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.362	112	10268	0.228	ng	0.00
5) Phenol-d6	6.902	99	12948	0.189	ng	0.00
8) Nitrobenzene-d5	8.870	82	8097	0.098	ng	0.00
11) 2-Methylnaphthalene-d10	12.088	152	31431	0.212	ng	0.00
14) 2,4,6-Tribromophenol	15.843	330	1440	0.104	ng	0.00
15) 2-Fluorobiphenyl	12.963	172	37802	0.203	ng	0.00
27) Fluoranthene-d10	19.133	212	50149	0.195	ng	0.00
31) Terphenyl-d14	19.739	244	34506	0.211	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.352	88	1855m	0.308	ng	
3) n-Nitrosodimethylamine	3.693	42	3262	0.267	ng	# 69
6) bis(2-Chloroethyl)ether	7.169	93	13386	0.203	ng	# 84
9) Naphthalene	10.543	128	52661	0.202	ng	97
10) Hexachlorobutadiene	10.835	225	9899	0.189	ng	# 98
12) 2-Methylnaphthalene	12.159	142	33485	0.202	ng	# 90
16) Acenaphthylene	14.067	152	33795	0.149	ng	98
17) Acenaphthene	14.409	154	27741	0.196	ng	100
18) Fluorene	15.399	166	32793	0.192	ng	99
20) 4,6-Dinitro-2-methylph...	15.488	198	90	0.043	ng	# 67
21) 4-Bromophenyl-phenylether	16.288	248	10103	0.173	ng	# 84
22) Hexachlorobenzene	16.410	284	12437	0.178	ng	# 90
23) Atrazine	16.556	200	3858	0.119	ng	93
24) Pentachlorophenol	16.751	266	661	0.085	ng	98
25) Phenanthrene	17.140	178	54207	0.188	ng	99
26) Anthracene	17.225	178	41680	0.166	ng	99
28) Fluoranthene	19.163	202	56725	0.182	ng	# 97
30) Pyrene	19.526	202	55464	0.206	ng	99
32) Benzo(a)anthracene	21.281	228	45935	0.180	ng	98
33) Chrysene	21.335	228	55634	0.199	ng	98
34) Bis(2-ethylhexyl)phtha...	21.218	149	9715	0.111	ng	# 85
36) Indeno(1,2,3-cd)pyrene	25.810	276	45687	0.161	ng	# 90
37) Benzo(b)fluoranthene	22.876	252	52372	0.191	ng	# 93
38) Benzo(k)fluoranthene	22.921	252	59104	0.203	ng	# 94
39) Benzo(a)pyrene	23.455	252	49450	0.194	ng	# 79
40) Dibenzo(a,h)anthracene	25.827	278	35160	0.154	ng	# 90
41) Benzo(g,h,i)perylene	26.501	276	40057	0.171	ng	# 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063021\
Data File : BN015218.D
Acq On : 30 Jun 2021 12:07
Operator : CG/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Manual Integrations
APPROVED

mohammad
7/1/2021 2:53:45 PM

Quant Time: Jun 30 13:23:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 30 13:21:47 2021
Response via : Initial Calibration

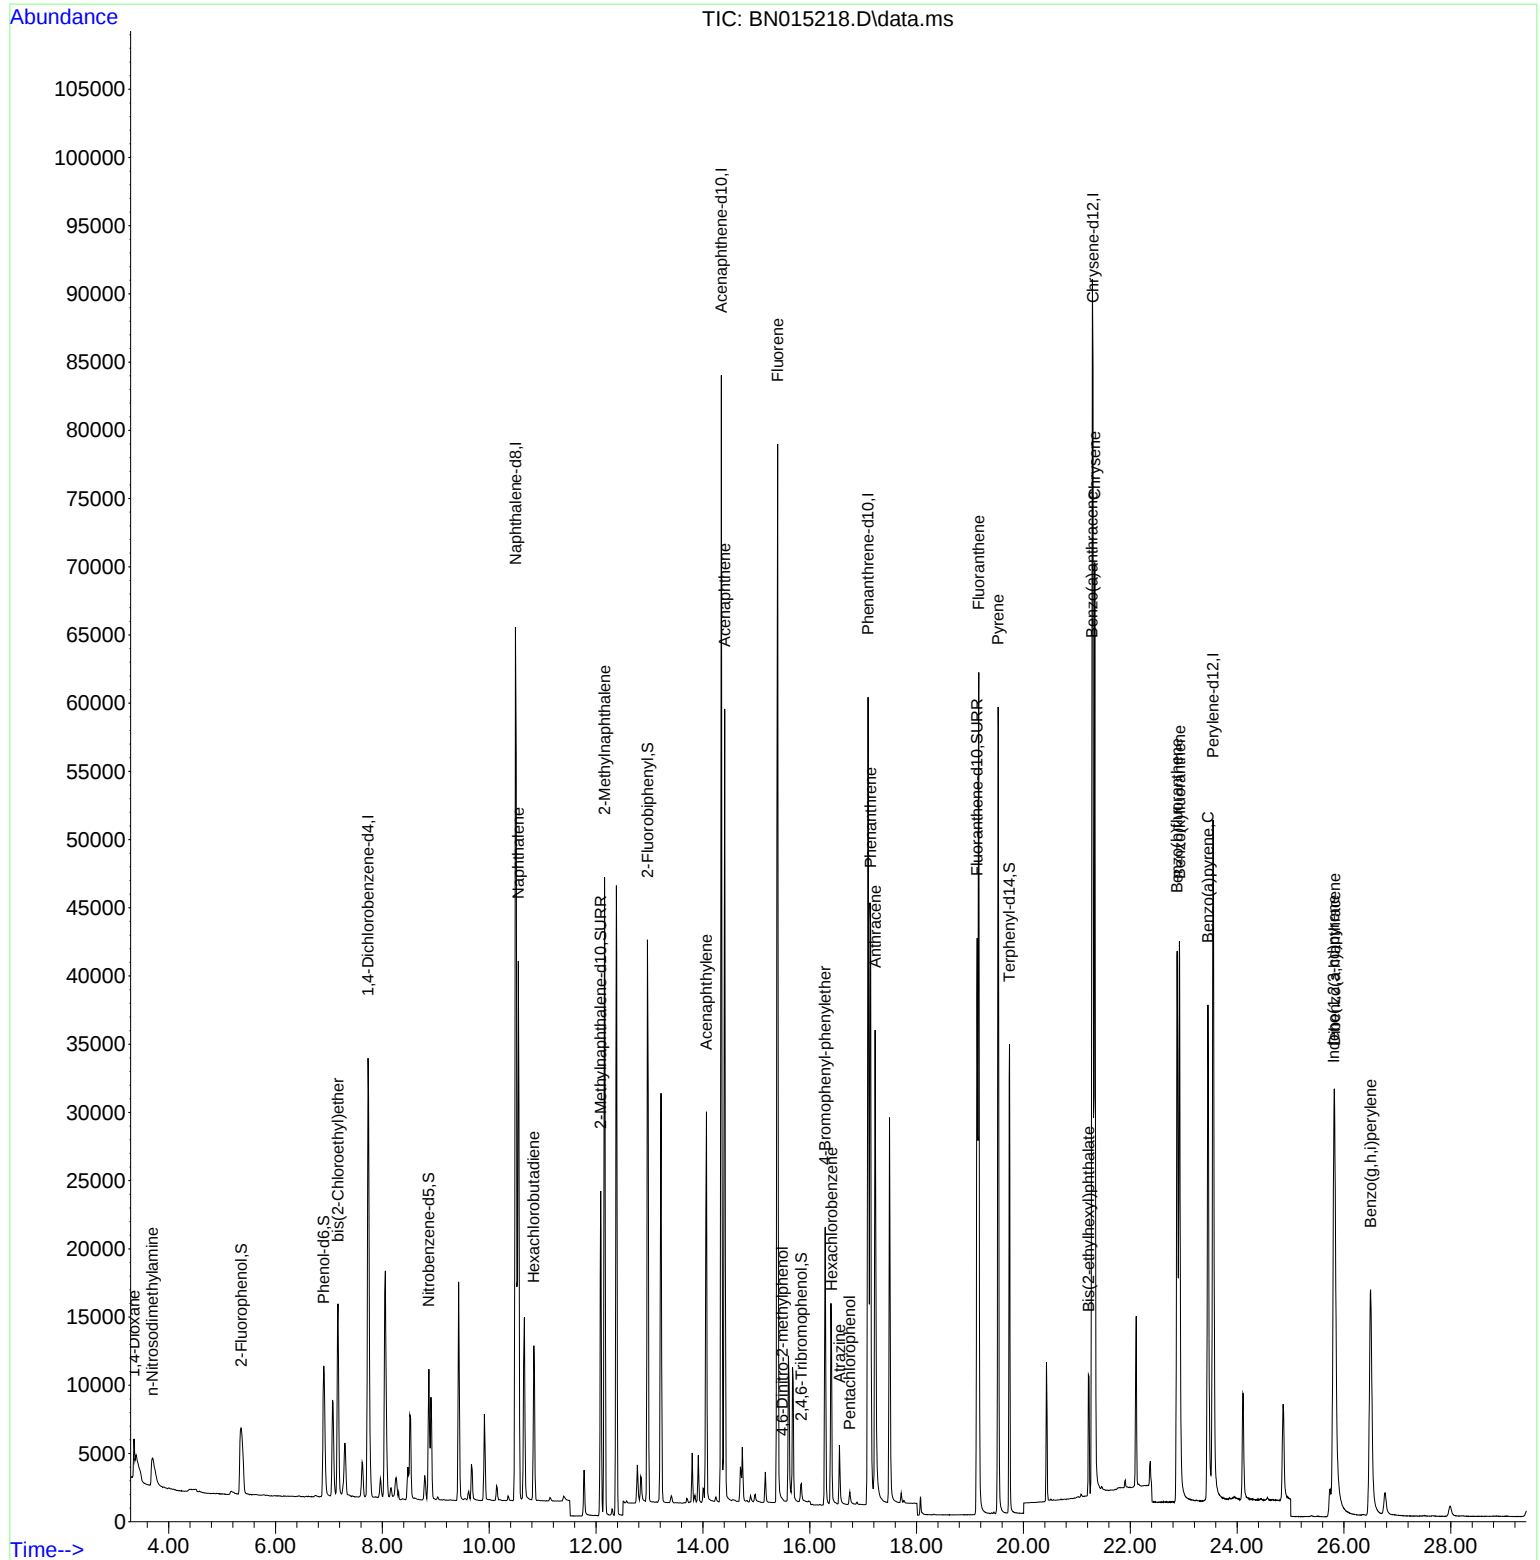







#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.732 min Scan# 483
Delta R.T. -0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion: 152 Resp: 20772
Ion Ratio Lower Upper
152 100
150 156.1 119.0 178.6
115 60.4 62.2 93.4#

Instrument :
BNA_N
ClientSampled :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:45 PM

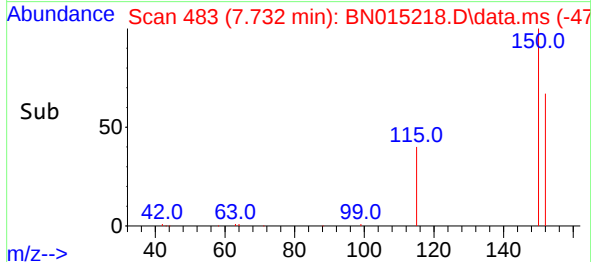

#2
1,4-Dioxane
Concen: 0.308 ng m
RT: 3.352 min Scan# 8
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion: 88 Resp: 1855
Ion Ratio Lower Upper
88 100
43 28.7 12.9 19.3#
58 81.3 38.1 57.1#

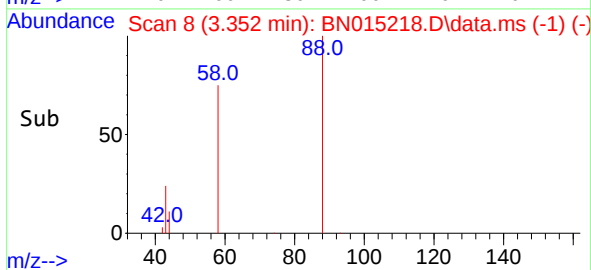

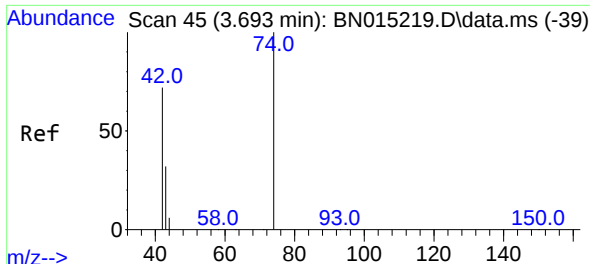





#3
n-Nitrosodimethylamine
Concen: 0.267 ng
RT: 3.693 min Scan# 45
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion: 42 Resp: 3262
Ion Ratio Lower Upper
42 100
74 141.1 149.5 224.3#
44 7.2 4.2 6.2#

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:45 PM

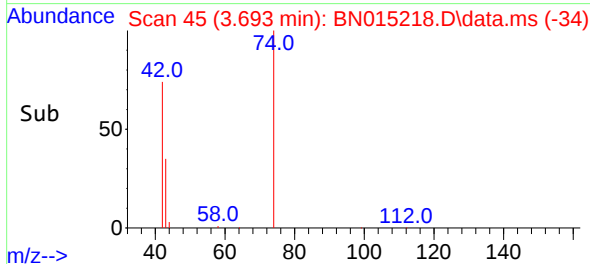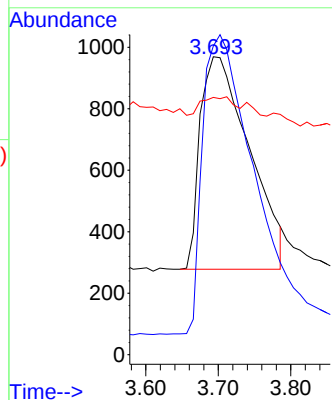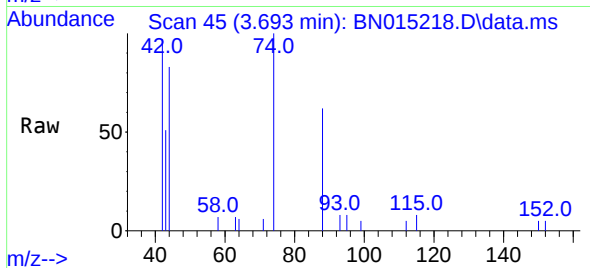

#4
2-Fluorophenol
Concen: 0.228 ng
RT: 5.362 min Scan# 226
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07


Tgt Ion: 112 Resp: 10268
Ion Ratio Lower Upper
112 100
64 56.3 39.0 58.6
63 28.5 20.6 30.8

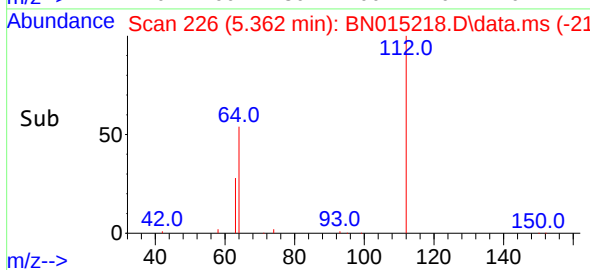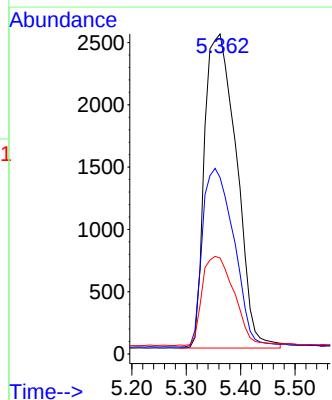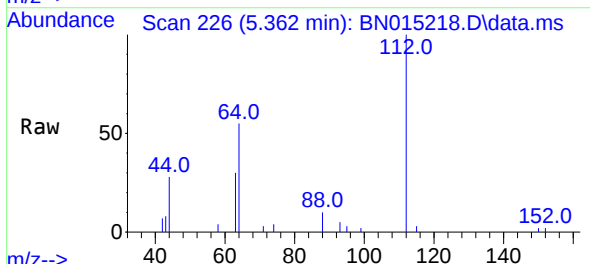



#5
Phenol-d6
Concen: 0.189 ng
RT: 6.902 min Scan# 393
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07



Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2




Tgt Ion: 99 Resp: 12948
Ion Ratio Lower Upper
99 100
42 17.1 8.9 13.3#
71 30.5 35.6 53.4#

Manual Integrations
APPROVED



mohammad
7/1/2021 2:53:45 PM

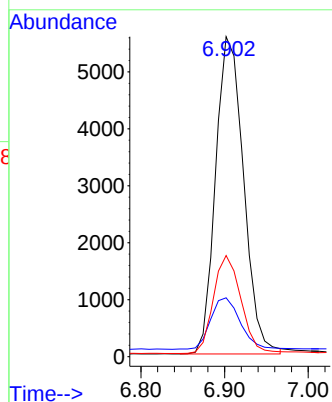


#6
bis(2-Chloroethyl)ether
Concen: 0.203 ng
RT: 7.169 min Scan# 422
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

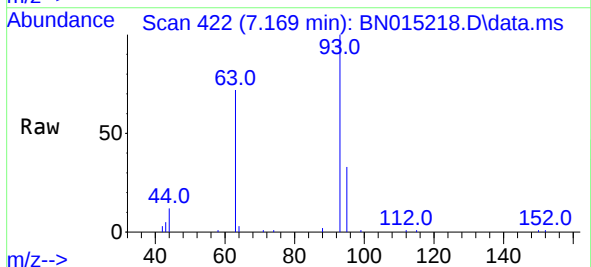


Tgt Ion: 93 Resp: 13386
Ion Ratio Lower Upper
93 100
63 74.9 46.6 70.0#
95 32.8 28.6 42.8

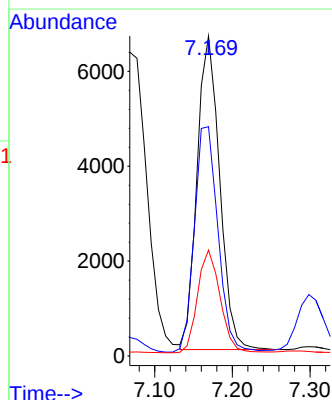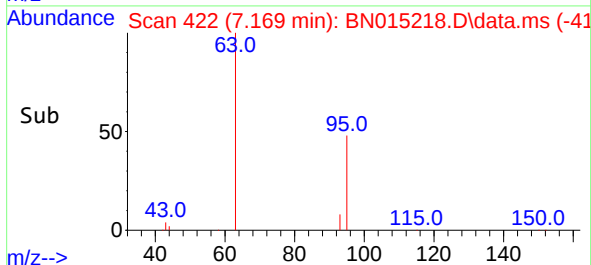



#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.493 min Scan# 718
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2



Tgt Ion:	136	Resp:	90398
Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.8	14.8
54	9.2	5.4	8.2#
68	7.4	4.9	7.3#




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:45 PM

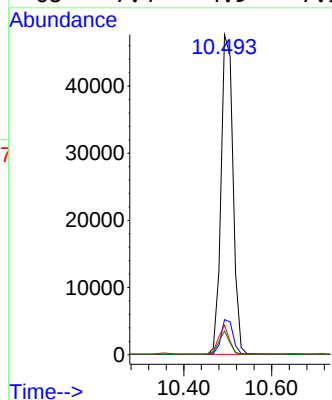

#8
Nitrobenzene-d5
Concen: 0.098 ng
RT: 8.870 min Scan# 590
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07


Tgt Ion:	82	Resp:	8097
Ion	Ratio	Lower	Upper
82	100		
128	36.7	31.6	47.4
54	50.8	29.0	43.4#

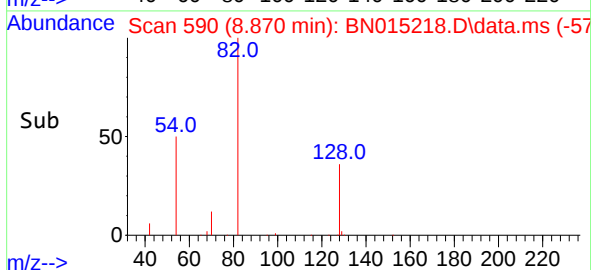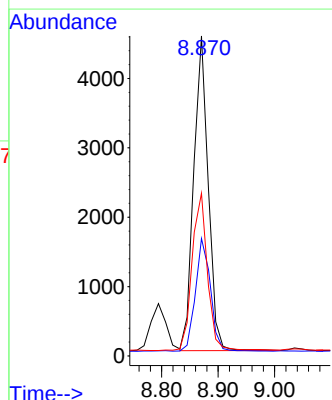



#9
Naphthalene
Concen: 0.202 ng
RT: 10.543 min Scan# 722
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07



Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Tgt Ion:	128	Resp:	52661
Ion	Ratio	Lower	Upper
128	100		
129	10.9	9.1	13.7
127	13.0	11.8	17.6

Manual Integrations
APPROVED



mohammad
7/1/2021 2:53:45 PM

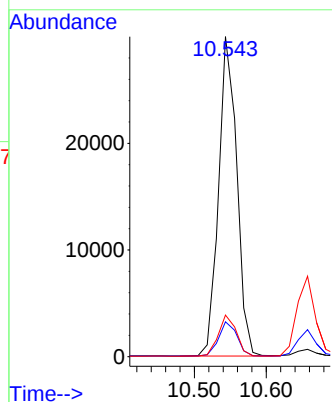


#10
Hexachlorobutadiene
Concen: 0.189 ng
RT: 10.835 min Scan# 745
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07



Tgt Ion:	225	Resp:	9899
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.9	50.2	75.2

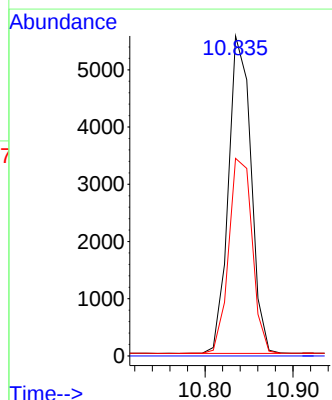

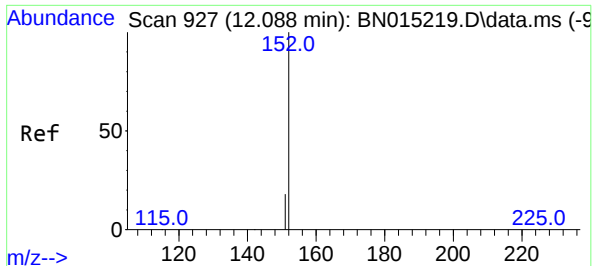





#11
2-Methylnaphthalene-d10
Concen: 0.212 ng
RT: 12.088 min Scan# 927
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion:152 Resp: 31431
Ion Ratio Lower Upper
152 100
151 20.5 16.7 25.1

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:45 PM

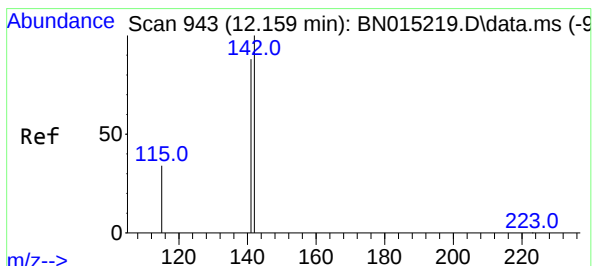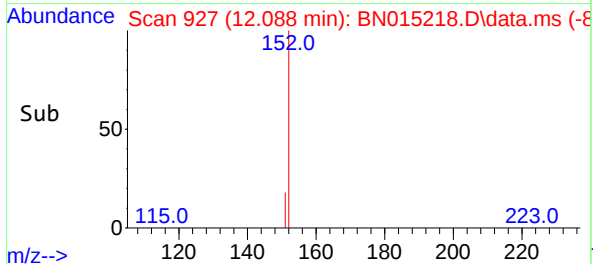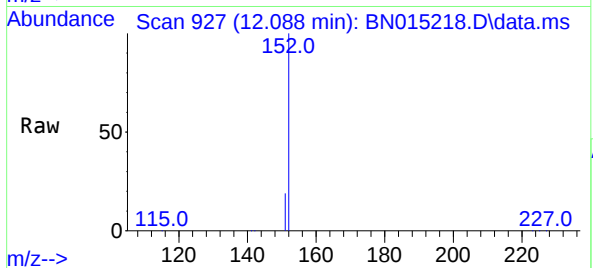


#12
2-Methylnaphthalene
Concen: 0.202 ng
RT: 12.159 min Scan# 943
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion:142 Resp: 33485
Ion Ratio Lower Upper
142 100
141 87.9 72.3 108.5
115 34.0 40.7 61.1#

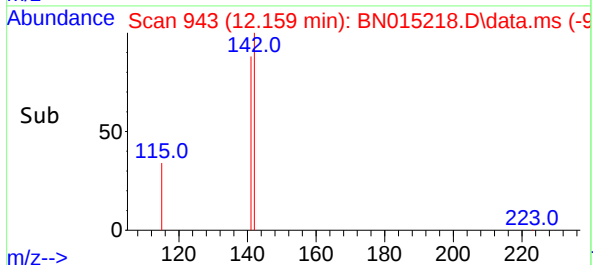
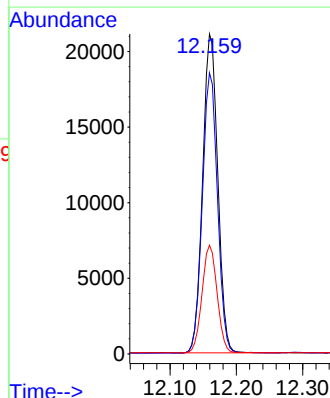
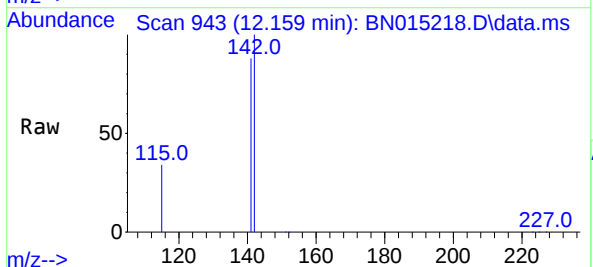





#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.346 min Scan# 1166
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07





Tgt Ion:164 Resp: 44390
Ion Ratio Lower Upper
164 100
162 100.4 83.8 125.6
160 46.2 37.4 56.0

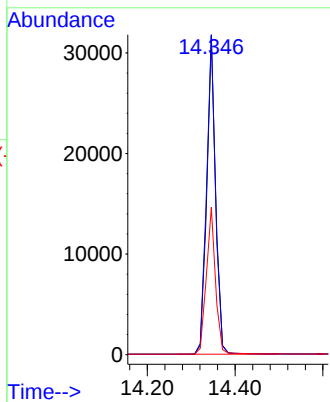

#14
2,4,6-Tribromophenol
Concen: 0.104 ng
RT: 15.843 min Scan# 1284
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

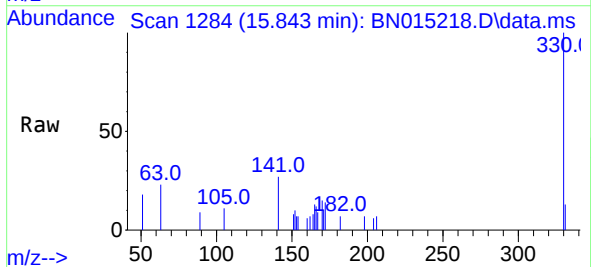


Tgt Ion:330 Resp: 1440
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 37.4 22.4 33.6#

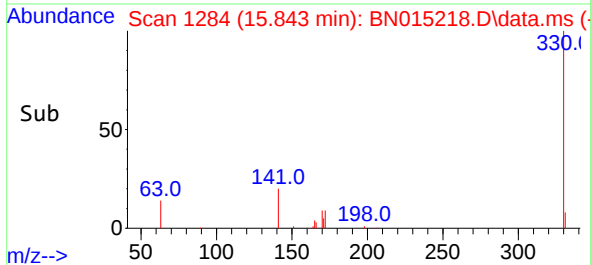

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED

mohammad
7/1/2021 2:53:45 PM



#15
2-Fluorobiphenyl
Concen: 0.203 ng
RT: 12.963 min Scan# 1057
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07





Tgt Ion:172 Resp: 37802

Ion	Ratio	Lower	Upper
172	100		
171	34.9	30.6	45.8
170	24.0	20.2	30.4

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED




mohammad
7/1/2021 2:53:45 PM




#16
Acenaphthylene
Concen: 0.149 ng
RT: 14.067 min Scan# 1144
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion:152 Resp: 33795


Ion	Ratio	Lower	Upper
152	100		
151	19.4	16.7	25.1
153	13.0	10.5	15.7





#17
Acenaphthene
Concen: 0.196 ng
RT: 14.409 min Scan# 1171
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2





Tgt Ion:154 Resp: 27741


Ion	Ratio	Lower	Upper
154	100		
153	113.4	90.9	136.3
152	58.0	45.8	68.8

Manual Integrations
APPROVED

mohammad
7/1/2021 2:53:45 PM


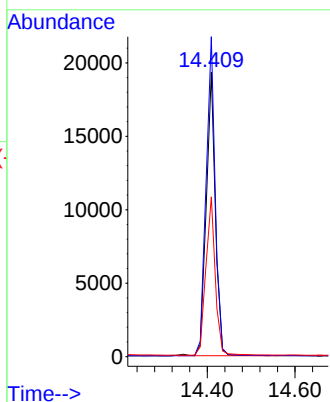



#18
Fluorene
Concen: 0.192 ng
RT: 15.399 min Scan# 1249
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

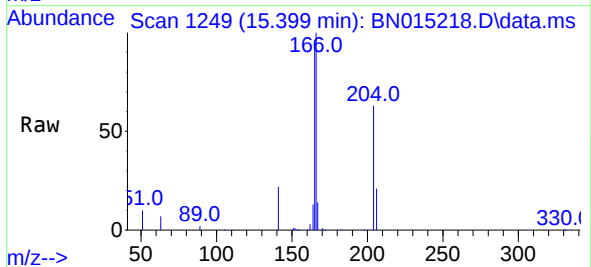

Tgt Ion:166 Resp: 32793

Ion	Ratio	Lower	Upper
166	100		
165	97.5	79.2	118.8
167	13.6	10.7	16.1

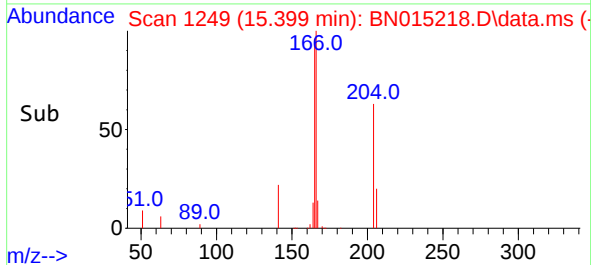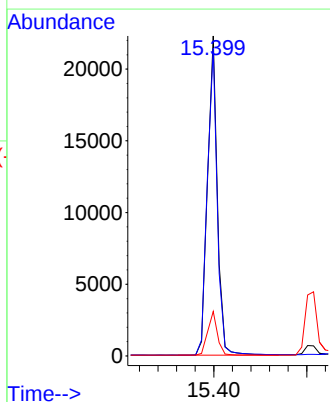







#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.092 min Scan# 1386
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion:188 Resp: 84508
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.5 9.0 13.4

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:45 PM



#20
4,6-Dinitro-2-methylphenol
Concen: 0.043 ng
RT: 15.488 min Scan# 1256
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07


Tgt Ion:198 Resp: 90
Ion Ratio Lower Upper
198 100
182 64.2 34.5 51.7#
77 0.0 0.0 0.0

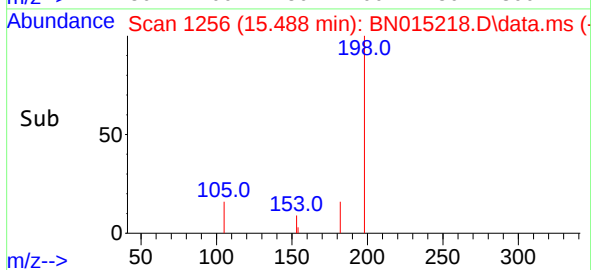



#21
4-Bromophenyl-phenylether
Concen: 0.173 ng
RT: 16.288 min Scan# 1320
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07



Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Tgt Ion:248 Resp: 10103
Ion Ratio Lower Upper
248 100
250 94.4 86.2 129.4
141 61.5 36.2 54.2#

Manual Integrations
APPROVED



mohammad
7/1/2021 2:53:45 PM




#22
Hexachlorobenzene
Concen: 0.178 ng
RT: 16.410 min Scan# 1330
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

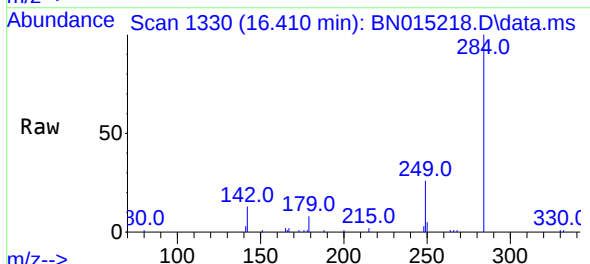


Tgt Ion:284 Resp: 12437
Ion Ratio Lower Upper
284 100
142 35.6 22.2 33.2#
249 30.4 26.6 39.8


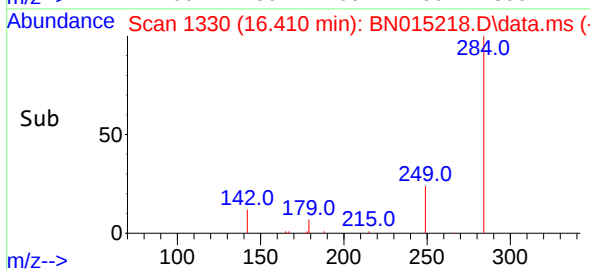






#23
Atrazine
Concen: 0.119 ng
RT: 16.556 min Scan# 1342
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07





Tgt Ion: 200 Resp: 3858
Ion Ratio Lower Upper
200 100
173 30.1 21.7 32.5
215 48.1 43.1 64.7

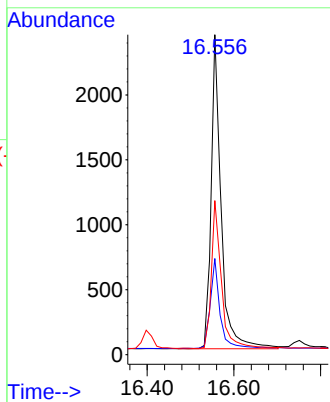

#24
Pentachlorophenol
Concen: 0.085 ng
RT: 16.751 min Scan# 1358
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

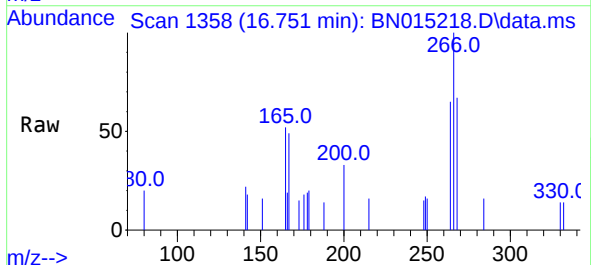


Tgt Ion: 266 Resp: 661
Ion Ratio Lower Upper
266 100
264 60.1 51.0 76.4
268 63.2 50.6 76.0

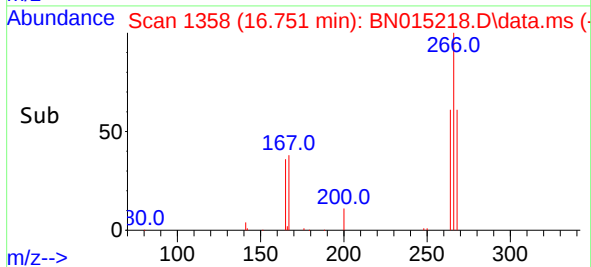


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED

mohammad
7/1/2021 2:53:45 PM






#25
Phenanthrene
Concen: 0.188 ng
RT: 17.140 min Scan# 1390
Delta R.T. 0.012 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07




Tgt Ion:178 Resp: 54207

Ion	Ratio	Lower	Upper
178	100		
176	18.8	15.6	23.4
179	15.7	12.1	18.1

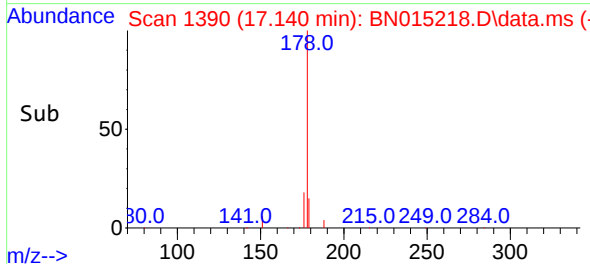
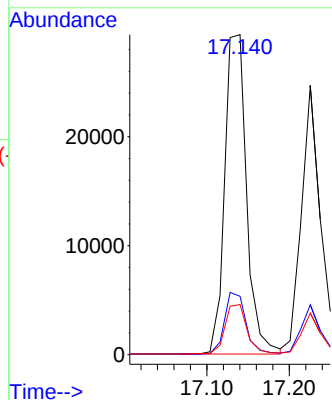


#26
Anthracene
Concen: 0.166 ng
RT: 17.225 min Scan# 1397
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

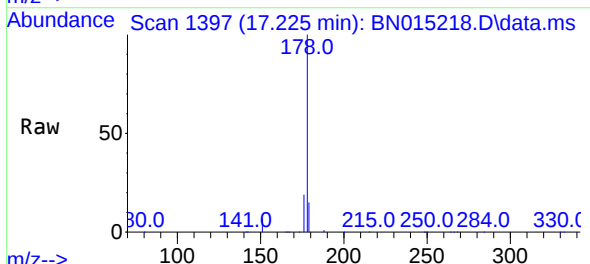

Tgt Ion:178 Resp: 41680


Ion	Ratio	Lower	Upper
178	100		
176	18.1	15.1	22.7
179	15.2	12.2	18.2

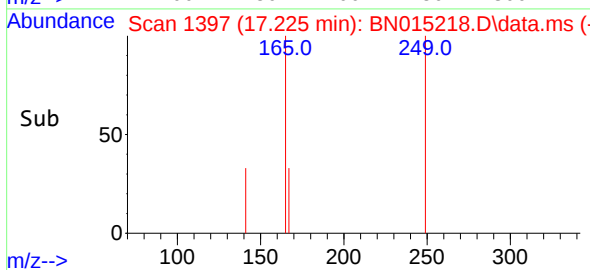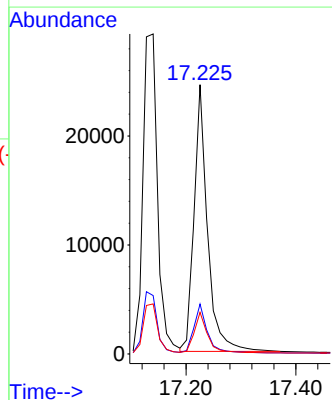

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED

mohammad
7/1/2021 2:53:45 PM







#27
Fluoranthene-d10
Concen: 0.195 ng
RT: 19.133 min Scan# 1687
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion:212 Resp: 50149
Ion Ratio Lower Upper
212 100
106 14.3 7.0 10.6#
104 7.8 4.1 6.1#

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:45 PM

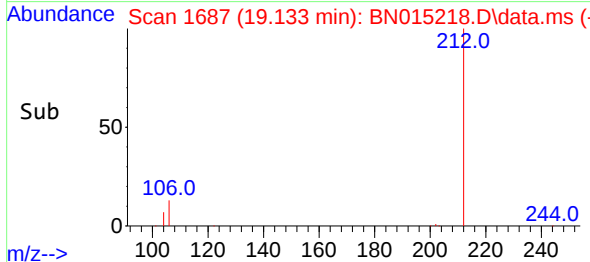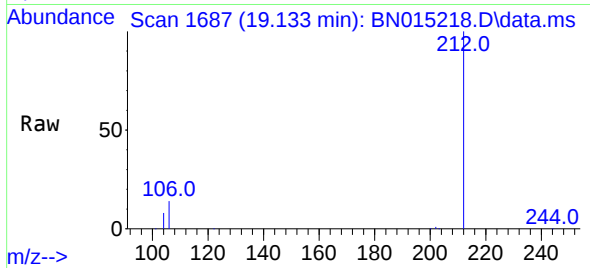

#28
Fluoranthene
Concen: 0.182 ng
RT: 19.163 min Scan# 1693
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion:202 Resp: 56725
Ion Ratio Lower Upper
202 100
101 11.8 6.6 10.0#
203 17.3 13.9 20.9

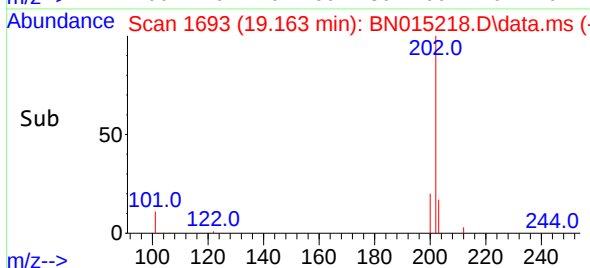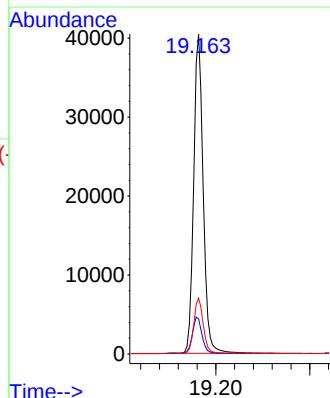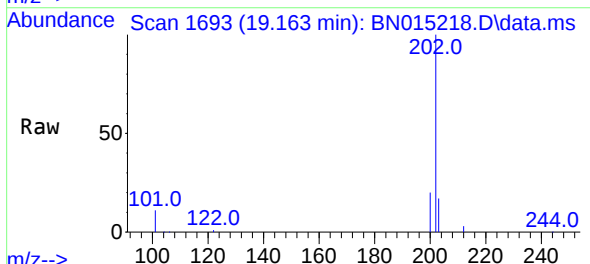







#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.303 min Scan# 1985
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion:240 Resp: 74187
Ion Ratio Lower Upper
240 100
120 7.8 4.2 6.4#
236 25.7 21.4 32.2

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:45 PM



#30
Pyrene
Concen: 0.206 ng
RT: 19.526 min Scan# 1766
Delta R.T. -0.005 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07


Tgt Ion:202 Resp: 55464
Ion Ratio Lower Upper
202 100
200 20.5 16.9 25.3
203 17.2 13.9 20.9

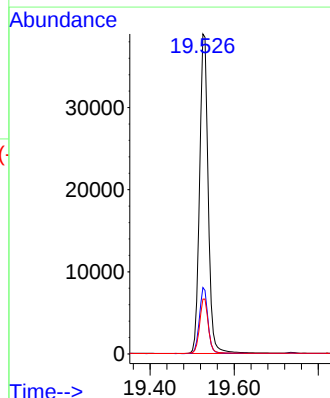

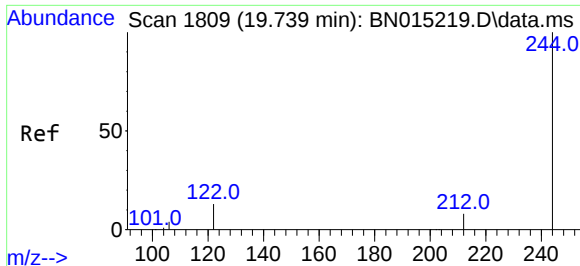

#31
Terphenyl-d14
Concen: 0.211 ng
RT: 19.739 min Scan# 1809
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

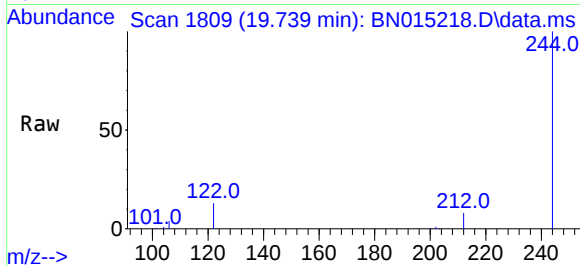

Tgt Ion:244 Resp: 34506
Ion Ratio Lower Upper
244 100
212 7.8 6.3 9.5
122 12.6 6.2 9.2#




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:45 PM

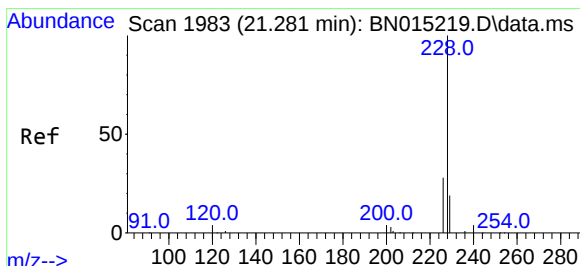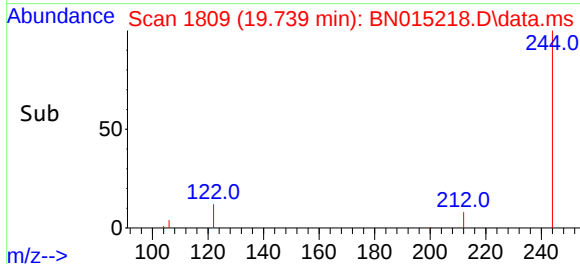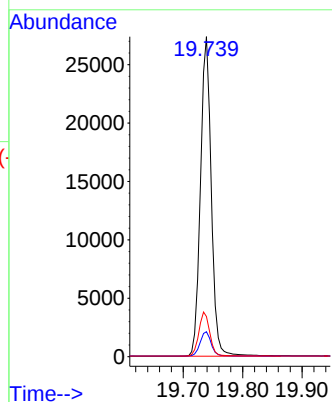

#32
Benzo(a)anthracene
Concen: 0.180 ng
RT: 21.281 min Scan# 1983
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion:228 Resp: 45935
Ion Ratio Lower Upper
228 100
226 27.6 23.0 34.6
229 19.2 15.7 23.5

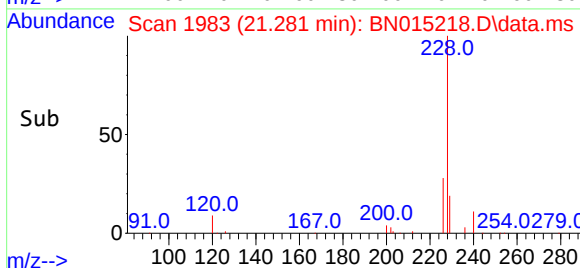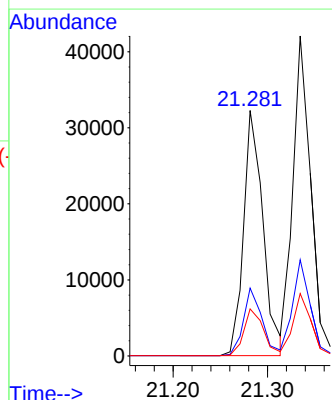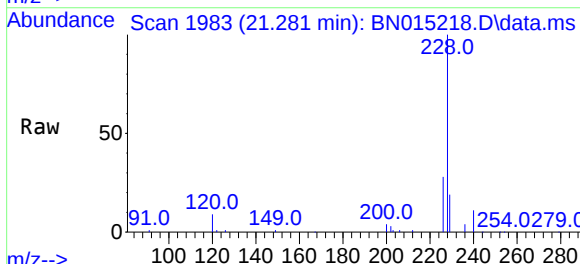







#33
Chrysene
Concen: 0.199 ng
RT: 21.335 min Scan# 1988
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion: 228 Resp: 55634
Ion Ratio Lower Upper
228 100
226 30.1 25.0 37.6
229 19.5 15.9 23.9

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:45 PM

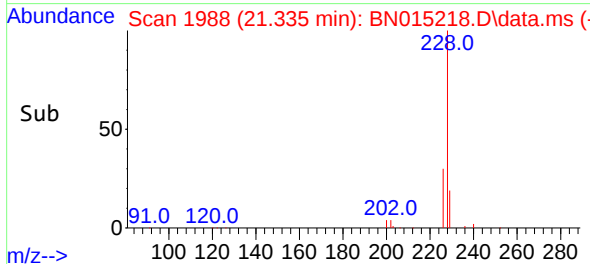


#34
Bis(2-ethylhexyl)phthalate
Concen: 0.111 ng
RT: 21.218 min Scan# 1977
Delta R.T. -0.011 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion: 149 Resp: 9715
Ion Ratio Lower Upper
149 100
167 26.8 28.9 43.3#
279 3.4 4.9 7.3#

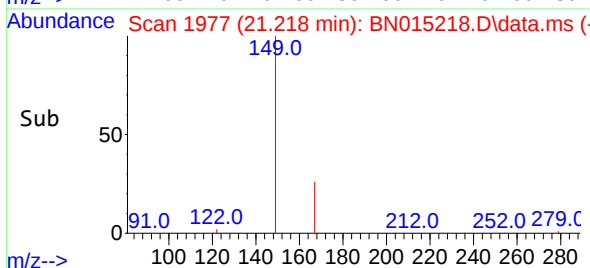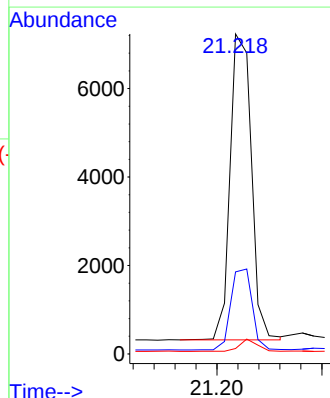
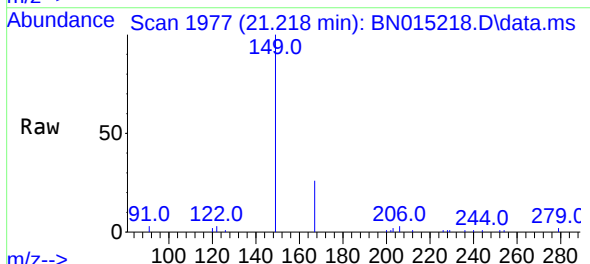




#35
Perylene-d12
Concen: 0.400 ng
RT: 23.550 min Scan# 2423
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07




Tgt Ion:264 Resp: 69311
Ion Ratio Lower Upper
264 100
260 25.2 20.6 31.0
265 23.3 21.4 32.2

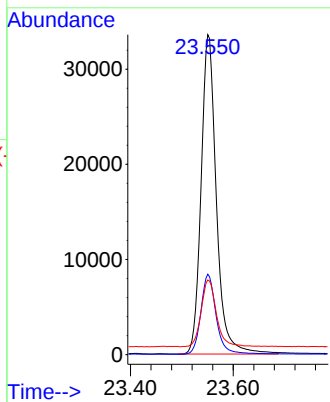


Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED



mohammad
7/1/2021 2:53:45 PM




#36
Indeno(1,2,3-cd)pyrene
Concen: 0.161 ng
RT: 25.810 min Scan# 3083
Delta R.T. -0.003 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07







Tgt Ion:276 Resp: 45687
Ion Ratio Lower Upper
276 100
138 24.0 10.0 15.0#
277 24.9 20.4 30.6

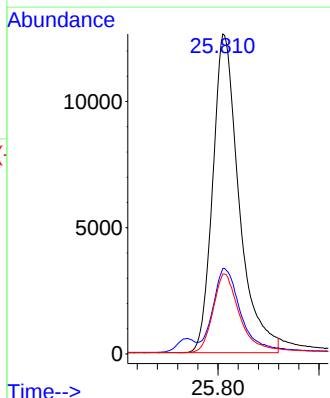






#37
Benzo(b)fluoranthene
Concen: 0.191 ng
RT: 22.876 min Scan# 2226
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion:252 Resp: 52372
Ion Ratio Lower Upper
252 100
253 22.8 18.5 27.7
125 16.0 5.8 8.6#

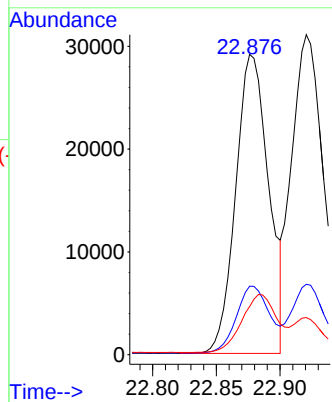

#38
Benzo(k)fluoranthene
Concen: 0.203 ng
RT: 22.921 min Scan# 2239
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07


Tgt Ion:252 Resp: 59104
Ion Ratio Lower Upper
252 100
253 22.0 19.1 28.7
125 11.6 5.4 8.0#

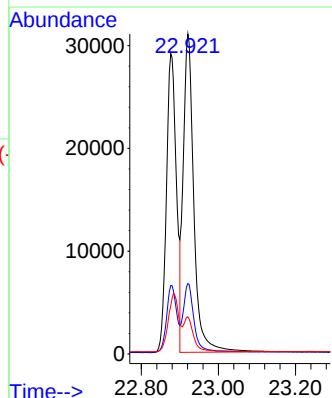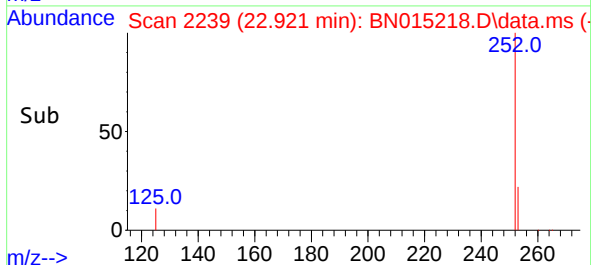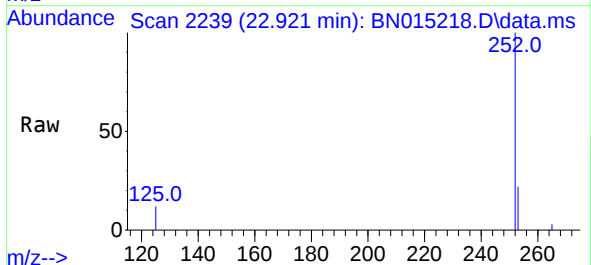

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED

mohammad
7/1/2021 2:53:45 PM







#39
Benzo(a)pyrene
Concen: 0.194 ng
RT: 23.455 min Scan# 2395
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion:252 Resp: 49450
Ion Ratio Lower Upper
252 100
253 24.7 19.4 29.2
125 36.3 7.4 11.2#

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2




Manual Integrations
APPROVED


mohammad
7/1/2021 2:53:45 PM

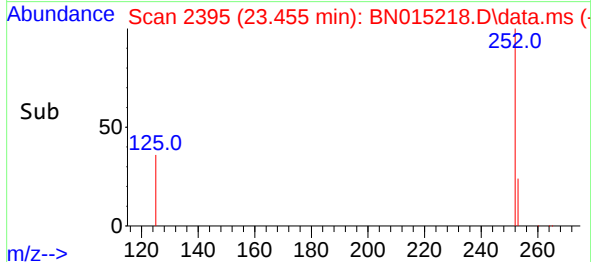


#40
Dibenzo(a,h)anthracene
Concen: 0.154 ng
RT: 25.827 min Scan# 3088
Delta R.T. 0.000 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

Tgt Ion:278 Resp: 35160
Ion Ratio Lower Upper
278 100
139 19.3 9.0 13.4#
279 23.3 21.0 31.4


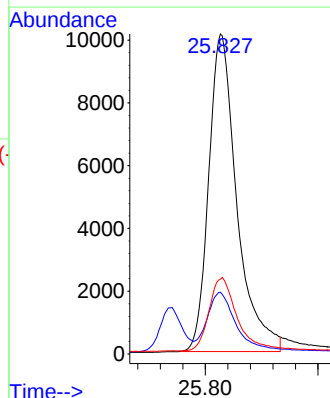


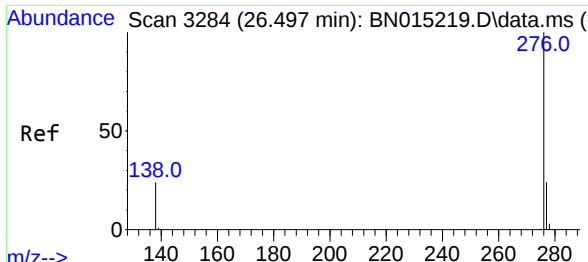

#41
Benzo(g,h,i)perylene
Concen: 0.171 ng
RT: 26.501 min Scan# 3285
Delta R.T. 0.003 min
Lab File: BN015218.D
Acq: 30 Jun 2021 12:07

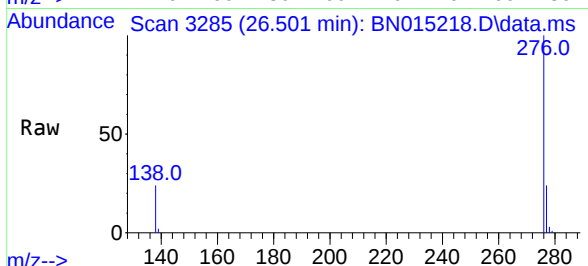

Tgt Ion: 276 Resp: 40057
Ion Ratio Lower Upper
276 100
277 24.2 19.7 29.5
138 24.2 9.8 14.6#

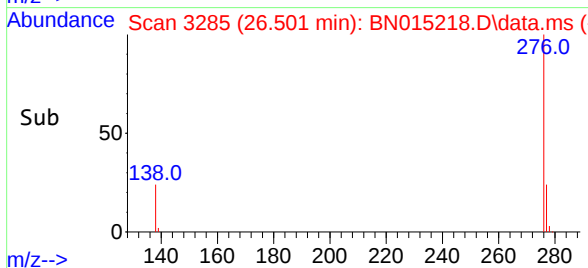

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2

Manual Integrations
APPROVED

mohammad
7/1/2021 2:53:45 PM