


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063021\
 Data File : BN015245.D
 Acq On : 01 Jul 2021 06:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 01 09:06:31 2021

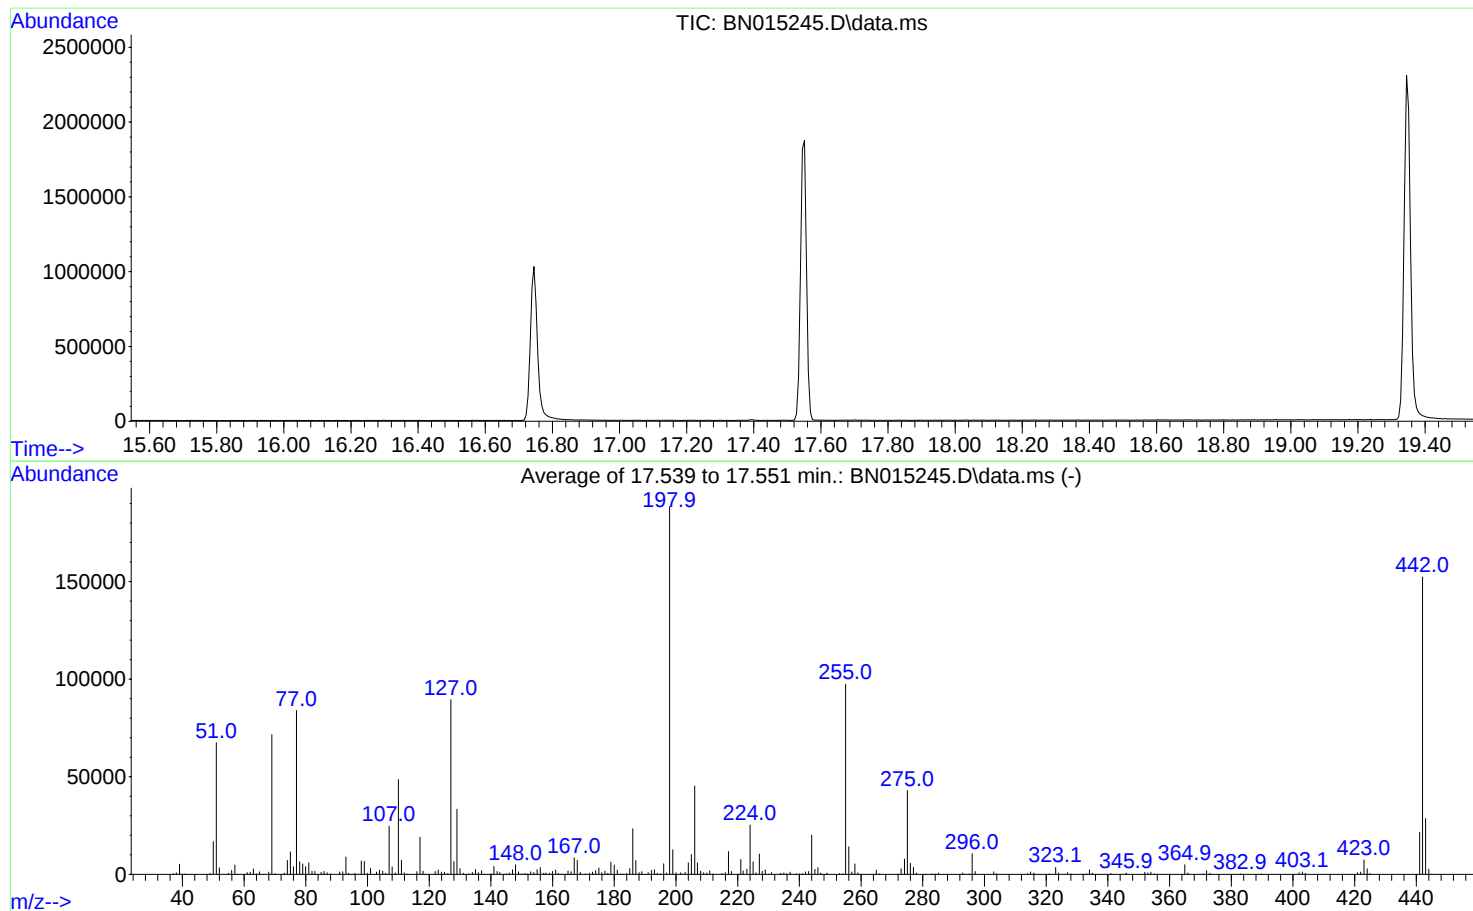




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	67445	PASS
68	69	0.00	2	1.6	1145	PASS
69	198	0.00	100	38.0	71581	PASS
70	69	0.00	2	0.6	426	PASS
127	198	10	80	47.5	89523	PASS
197	198	0.00	2	0.4	739	PASS
198	198	100	100	100.0	188424	PASS
199	198	5	9	6.7	12588	PASS
275	198	10	60	22.8	42987	PASS
365	198	1	100	2.6	4897	PASS
441	198	0.01	100	11.5	21584	PASS
442	442	50	100	100.0	152293	PASS
443	442	15	24	18.8	28571	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063021\
Data File : BN015245.D
Acq On : 01 Jul 2021 06:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 01 08:02:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

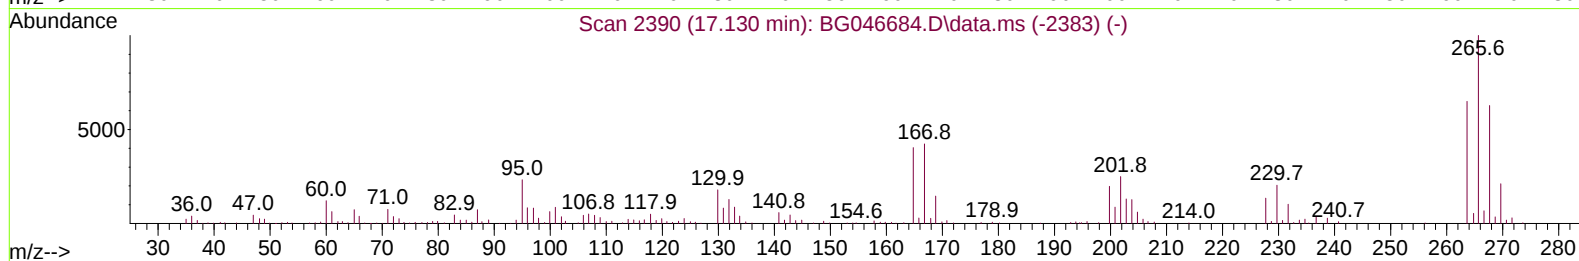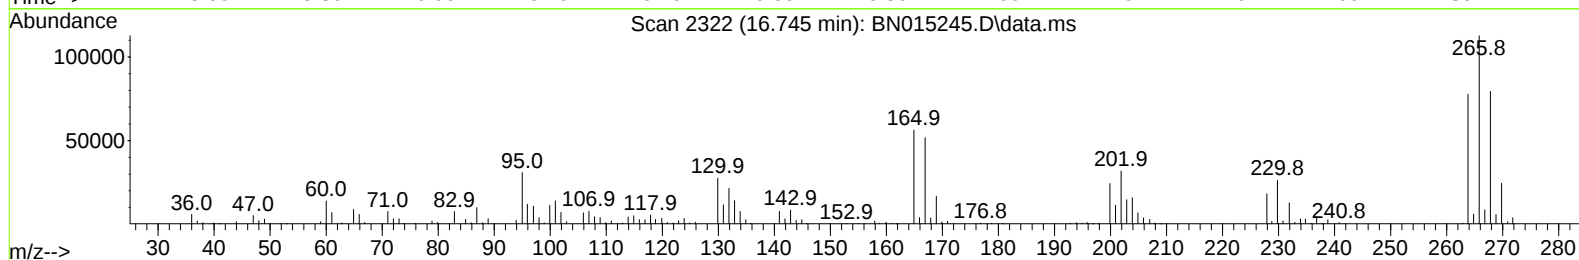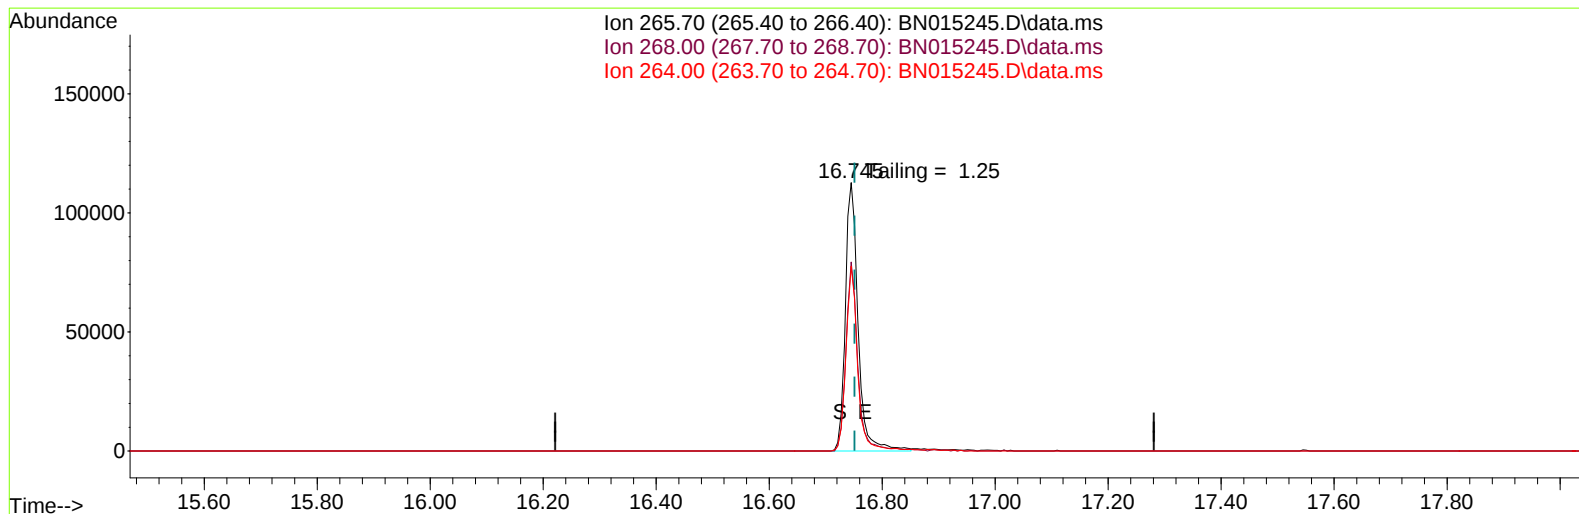

TIC: BN015245.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.006) 20397.47 ng




response 178963

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	70.43
264.00	61.60	68.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN063021\
Data File : BN015245.D
Acq On : 01 Jul 2021 06:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 01 08:02:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 23 10:10:58 2021
Response via : Initial Calibration

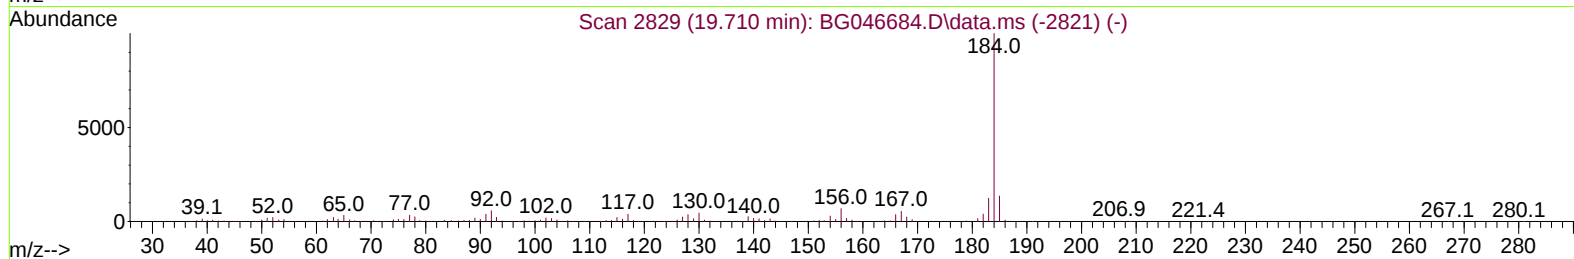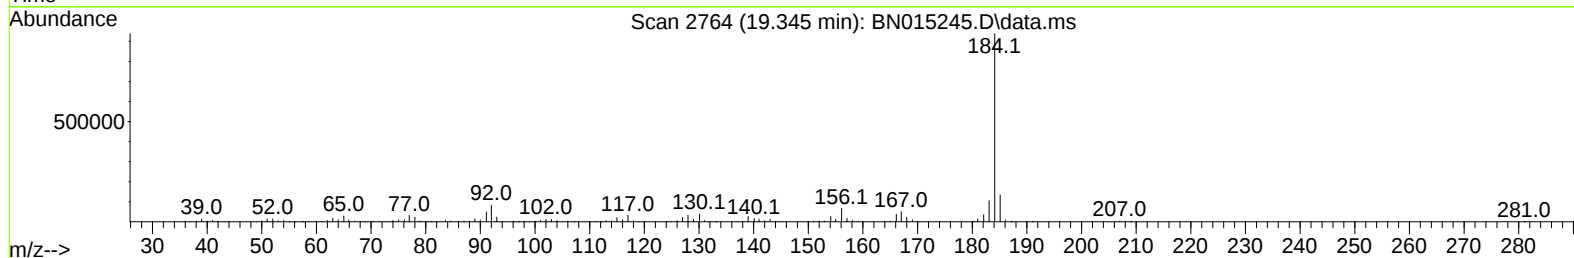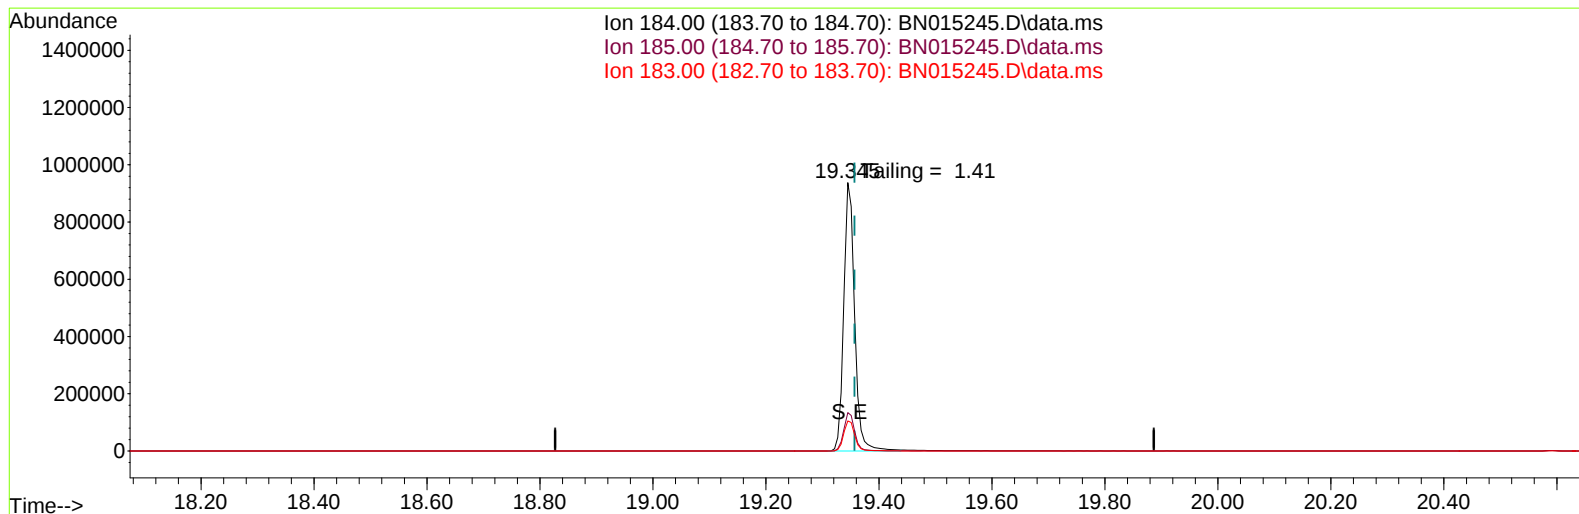

TIC: BN015245.D\data.ms

(77) Benzidine

19.345min (-0.012) 0.00 ng

response 1261430

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.35
183.00	13.20	11.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/30/2021	BNA_N	<u>BN015245.D</u>
Compound Name	Response	Retention Time
DDT	492013	20.592
DDD	11516	20.151
DDE	1190	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12706	504719	2.52