

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
 Data File : BN032367.D
 Acq On : 01 Jul 2024 18:19
 Operator : MA/JU
 Sample : PB161603BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK603

Quant Time: Jul 01 23:45:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 27 13:23:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.607	152	8653	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.382	136	27698	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.253	164	14908	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.109	188	1396602	0.400	ng/ul	0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.23
23) Perylene-d12	23.436	264	23551	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	44572	4.634	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.988	152	10408	0.251	ng/ul	-0.01
18) Fluoranthene-d10	19.050	212	14564	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.181	88	346	0.032	ng/ul#	29
26) Benzo(a)pyrene	23.289	252	4740	0.067	ng/ul#	19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032367.D
Acq On : 01 Jul 2024 18:19
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Quant Time: Jul 01 23:45:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration




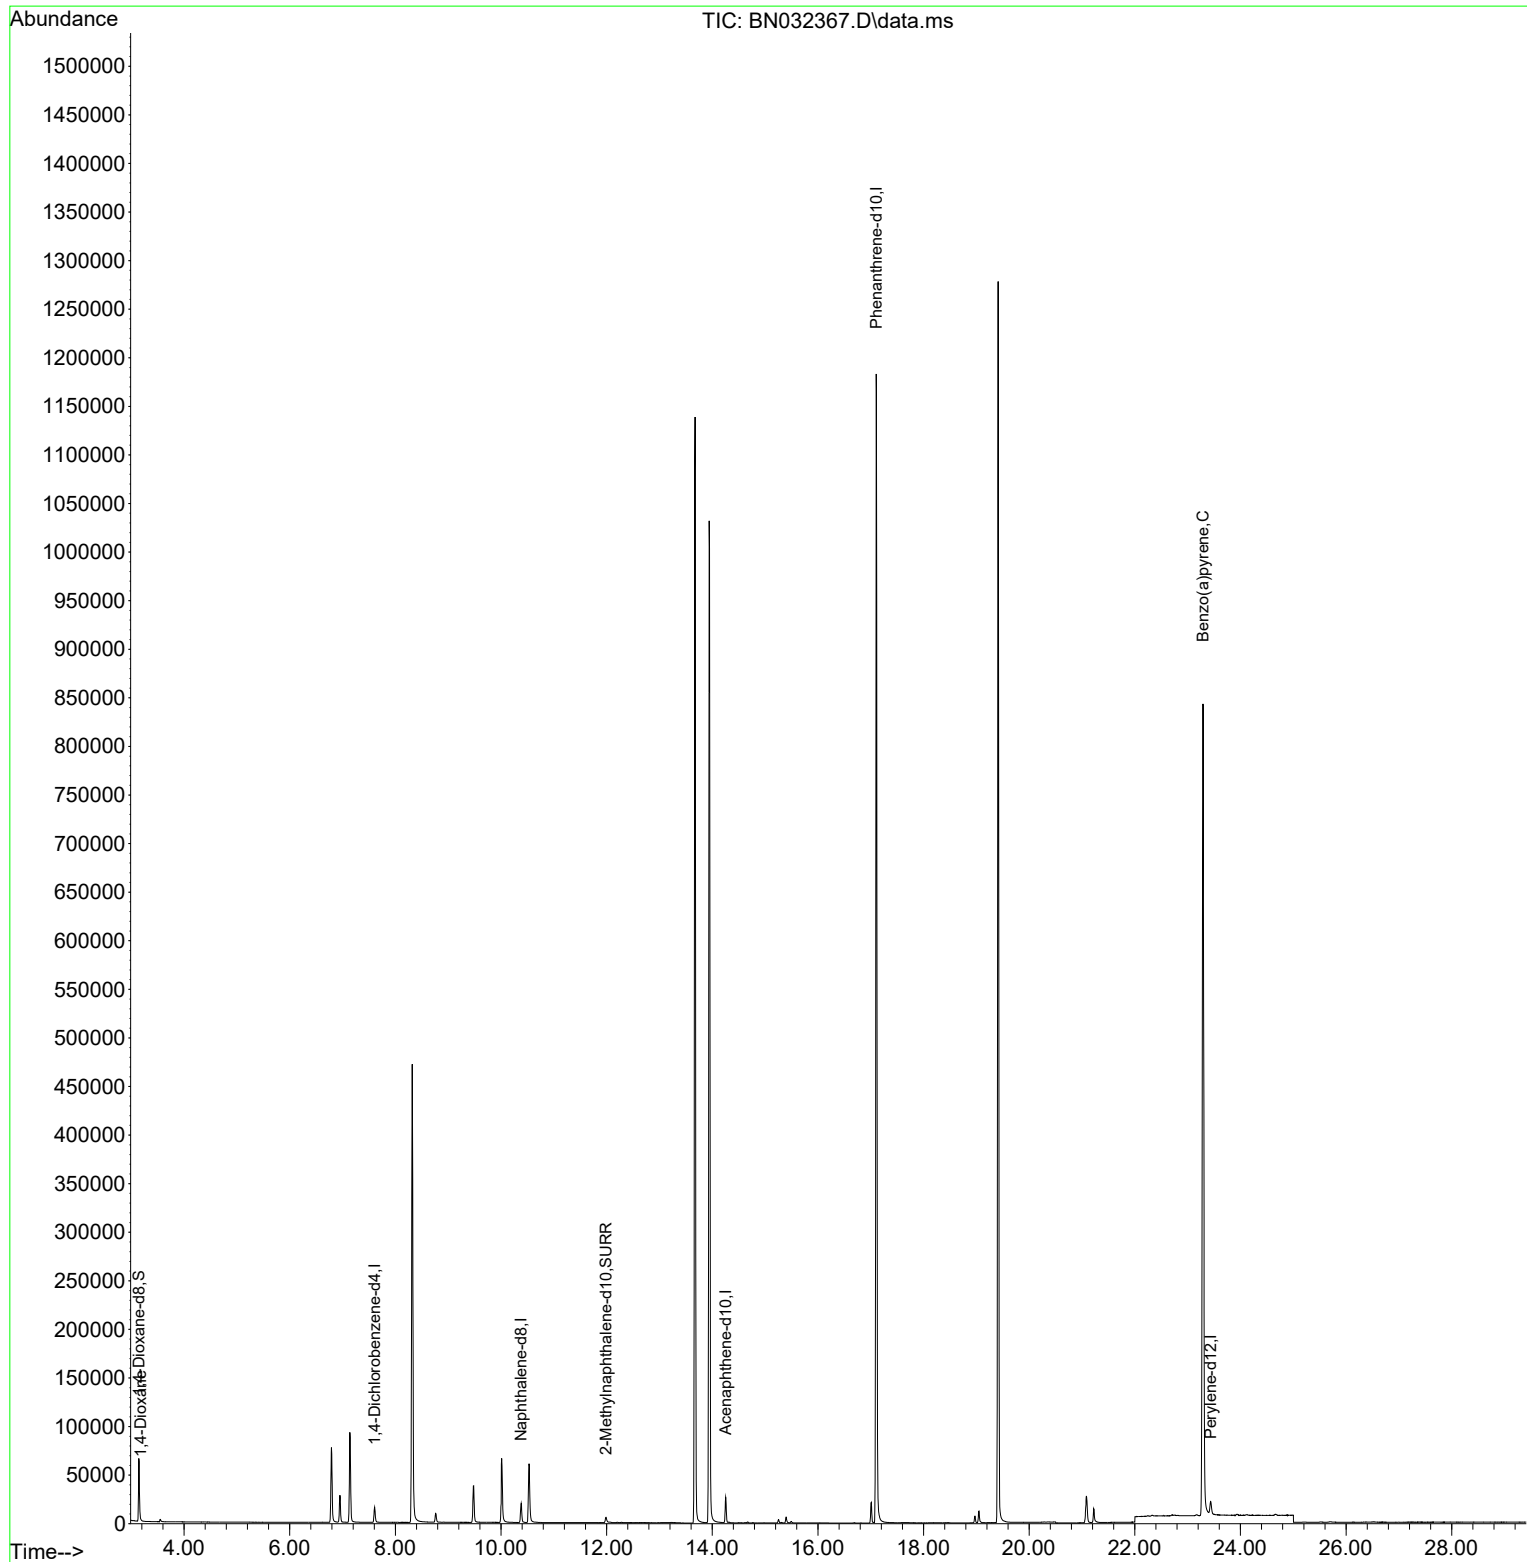


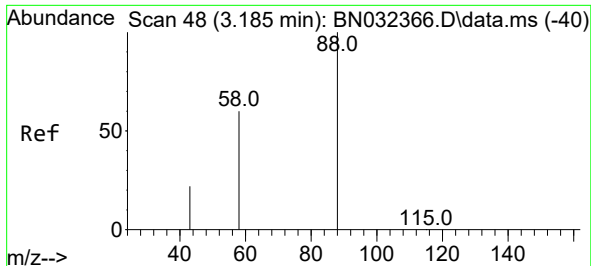

#2
 1,4-Dioxane
 Concen: 0.032 ng/ul
 RT: 3.181 min Scan# 41
 Delta R.T. -0.004 min
 Lab File: BN032367.D
 Acq: 01 Jul 2024 18:19

Instrument :
 BNA_N
 ClientSampleId :
 SBLK603

Tgt Ion: 88 Resp: 346
 Ion Ratio Lower Upper
 88 100
 43 122.4 28.4 42.6#
 58 40.3 43.3 64.9#

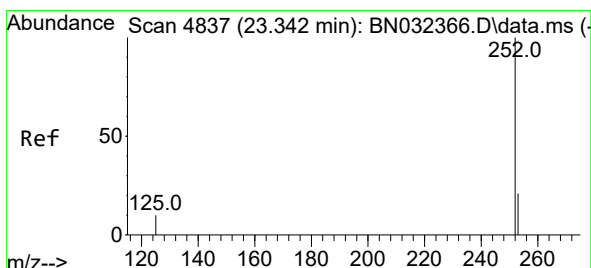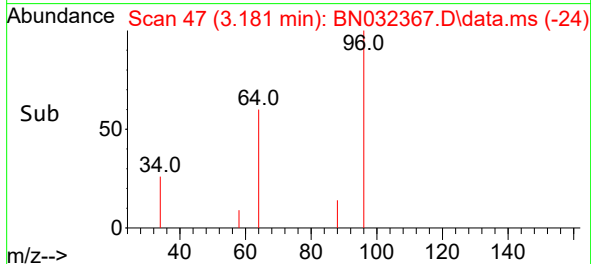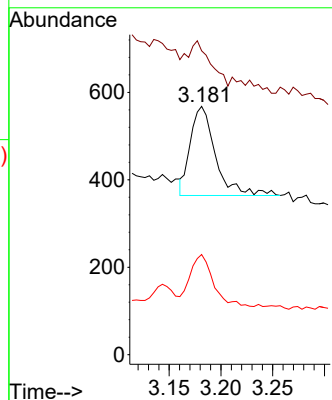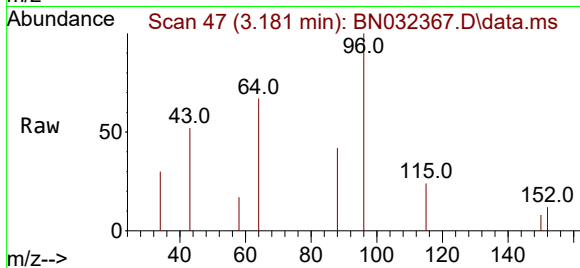

#26
 Benzo(a)pyrene
 Concen: 0.067 ng/ul
 RT: 23.289 min Scan# 4819
 Delta R.T. -0.070 min
 Lab File: BN032367.D
 Acq: 01 Jul 2024 18:19

Tgt Ion: 252 Resp: 4740
 Ion Ratio Lower Upper
 252 100
 253 55.2 22.2 33.2#
 125 75.7 16.4 24.6#

