




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032357.D
Acq On : 01 Jul 2024 11:35
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

Quant Time: Jul 01 12:24:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration

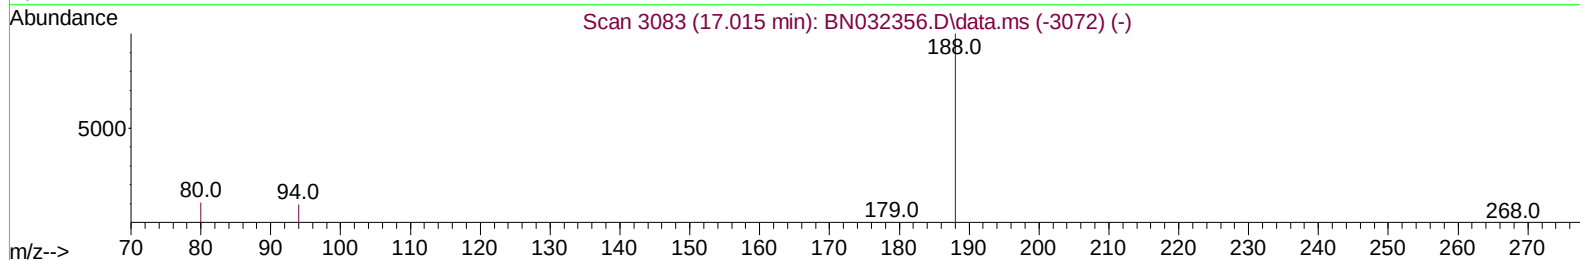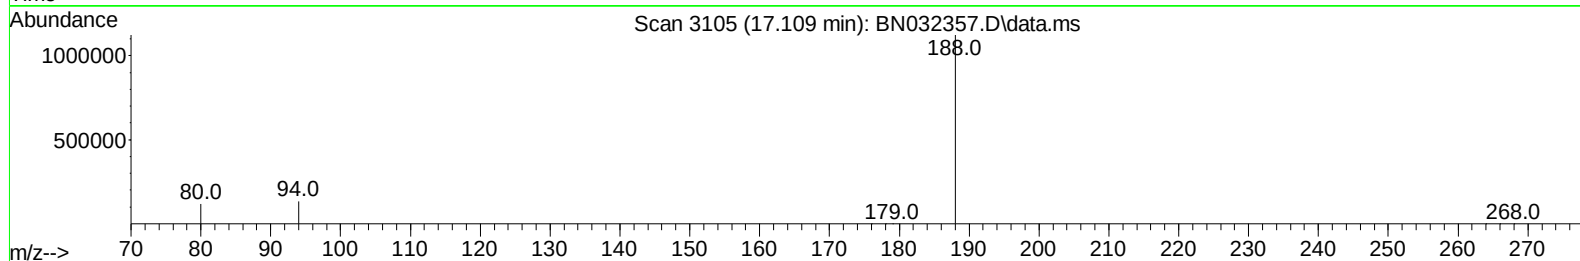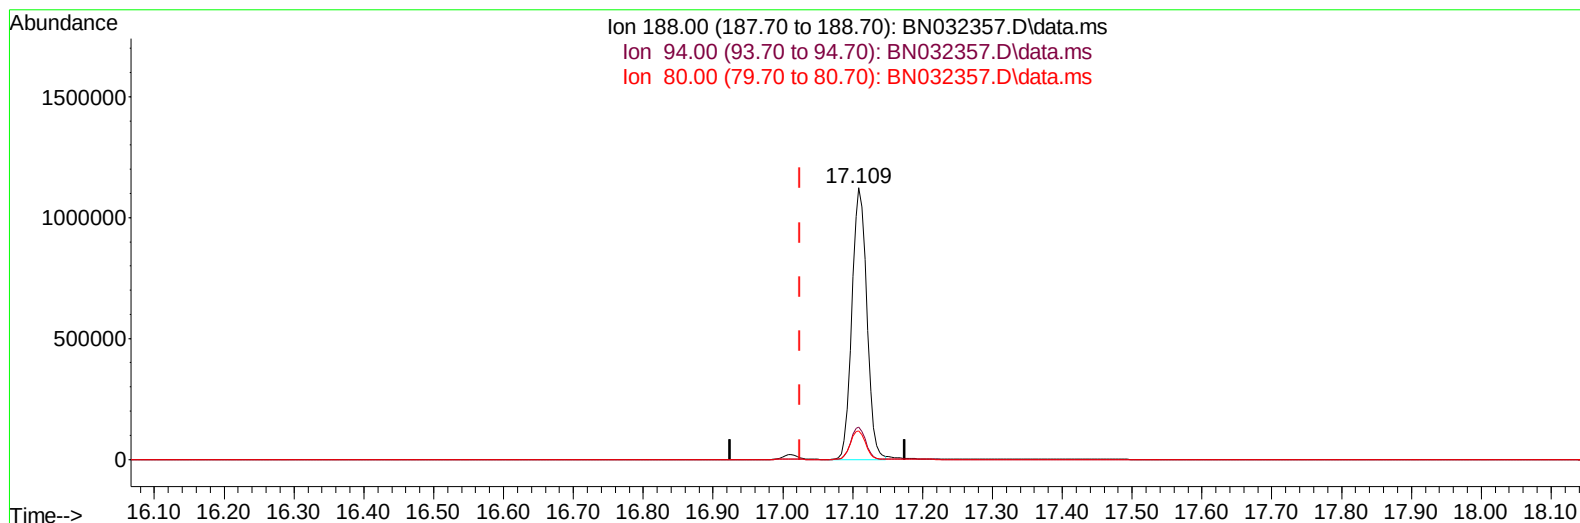

TIC: BN032357.D\data.ms

(13) Phenanthrene-d10 (I)

17.109min (+ 0.084) 0.40 ng/u1

response 1669500

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	11.94
80.00	10.50	10.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032357.D
Acq On : 01 Jul 2024 11:35
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Quant Time: Jul 01 12:24:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

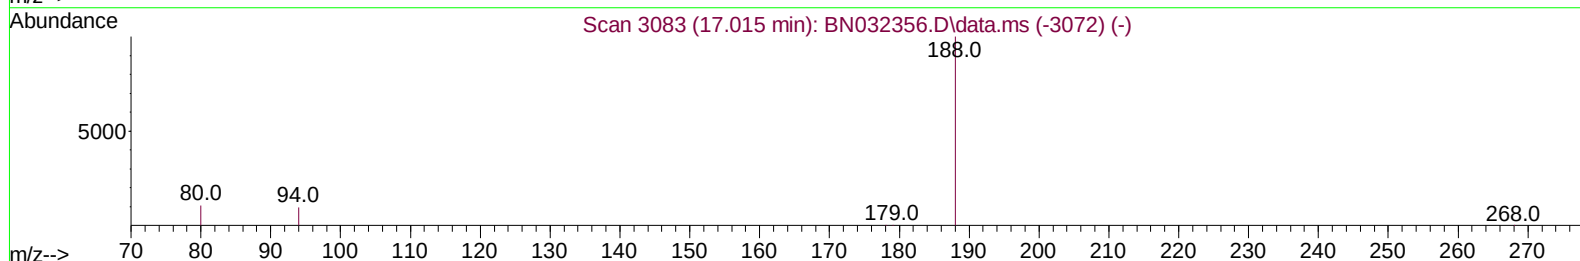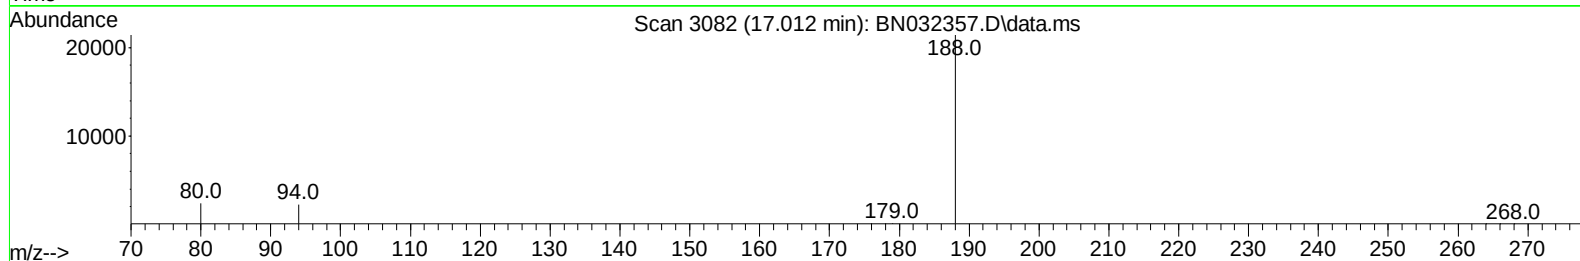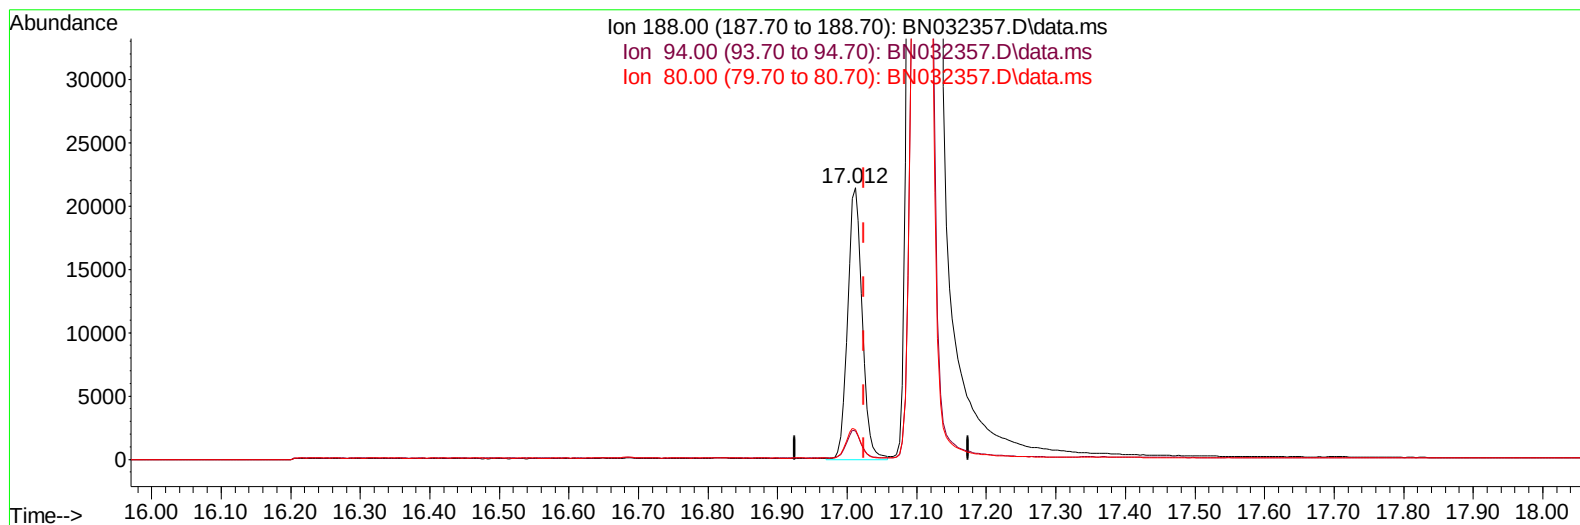

TIC: BN032357.D\data.ms

(13) Phenanthrene-d10 (I)

17.012min (-0.013) 0.40 ng/ul m

response 30921

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	10.46
80.00	10.50	11.09
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032357.D
Acq On : 01 Jul 2024 11:35
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Quant Time: Jul 01 12:24:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

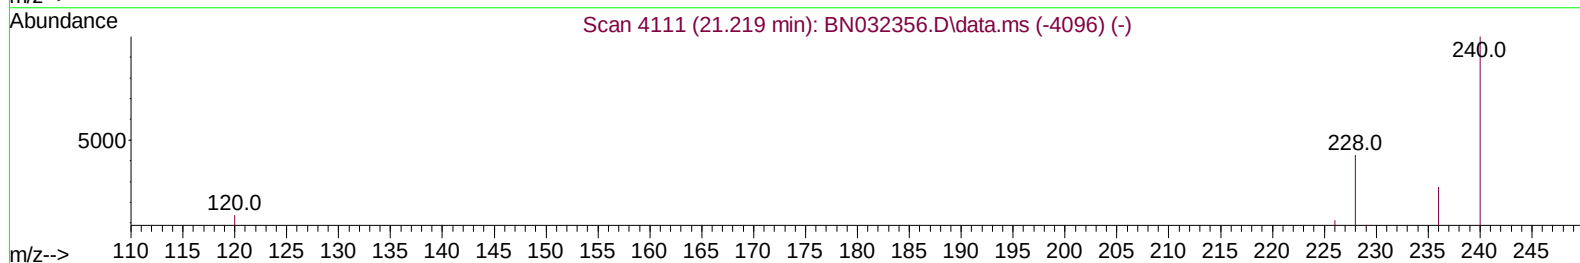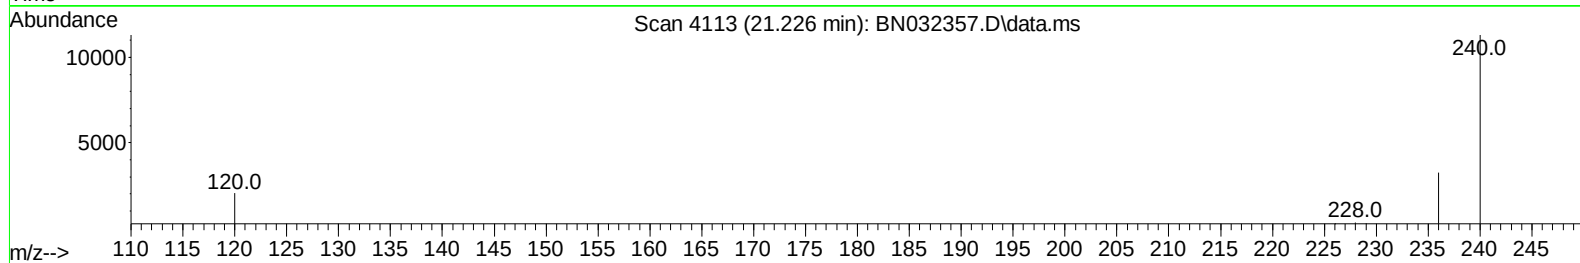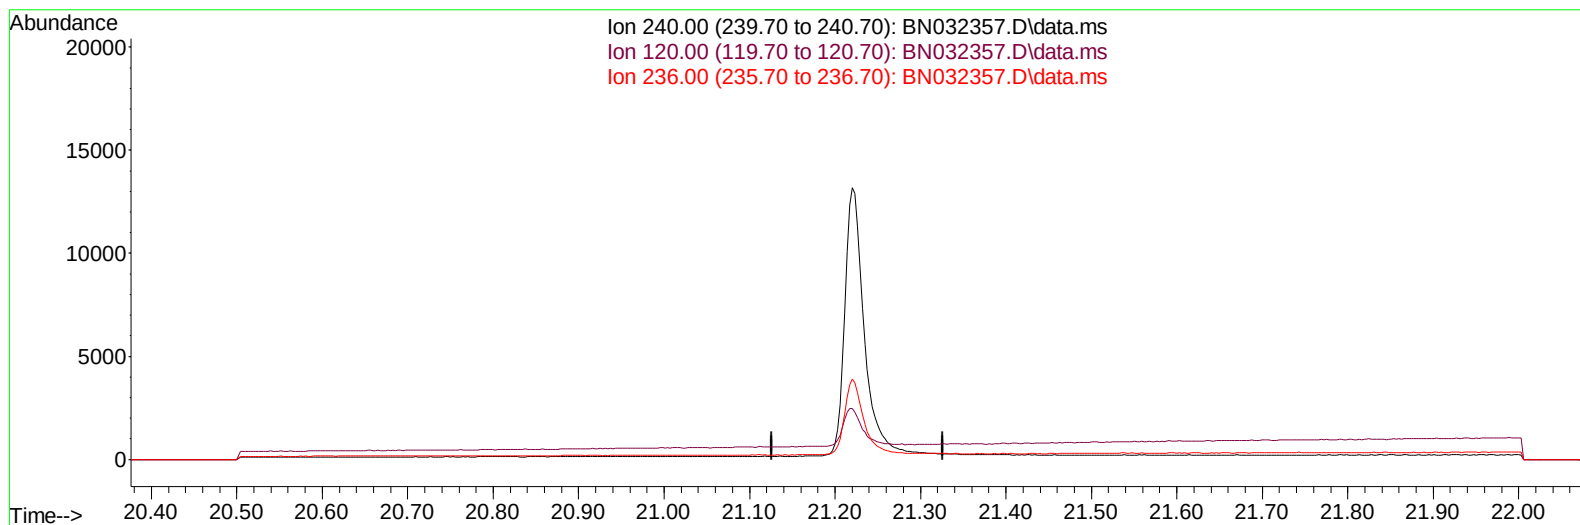

TIC: BN032357.D\data.ms

(17) Chrysene-d12

21.226min (-21.226) 0.00 ng/ul

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.80	0.00#
236.00	28.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032357.D
Acq On : 01 Jul 2024 11:35
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Quant Time: Jul 01 12:24:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

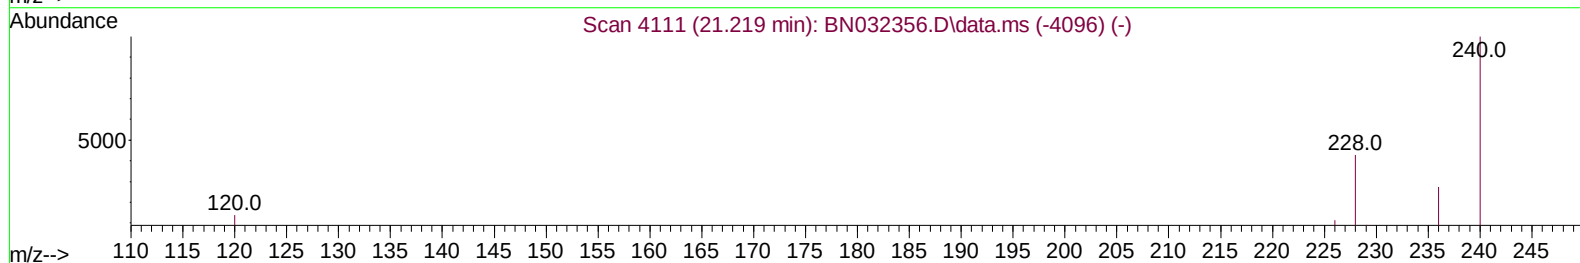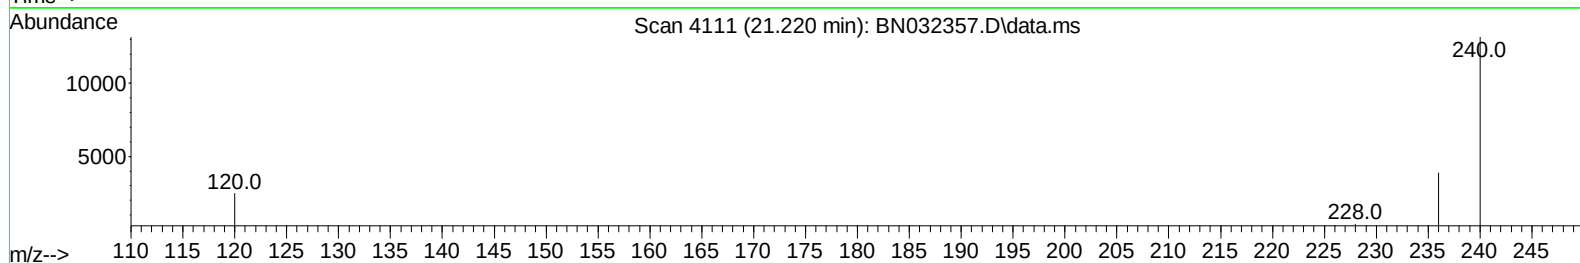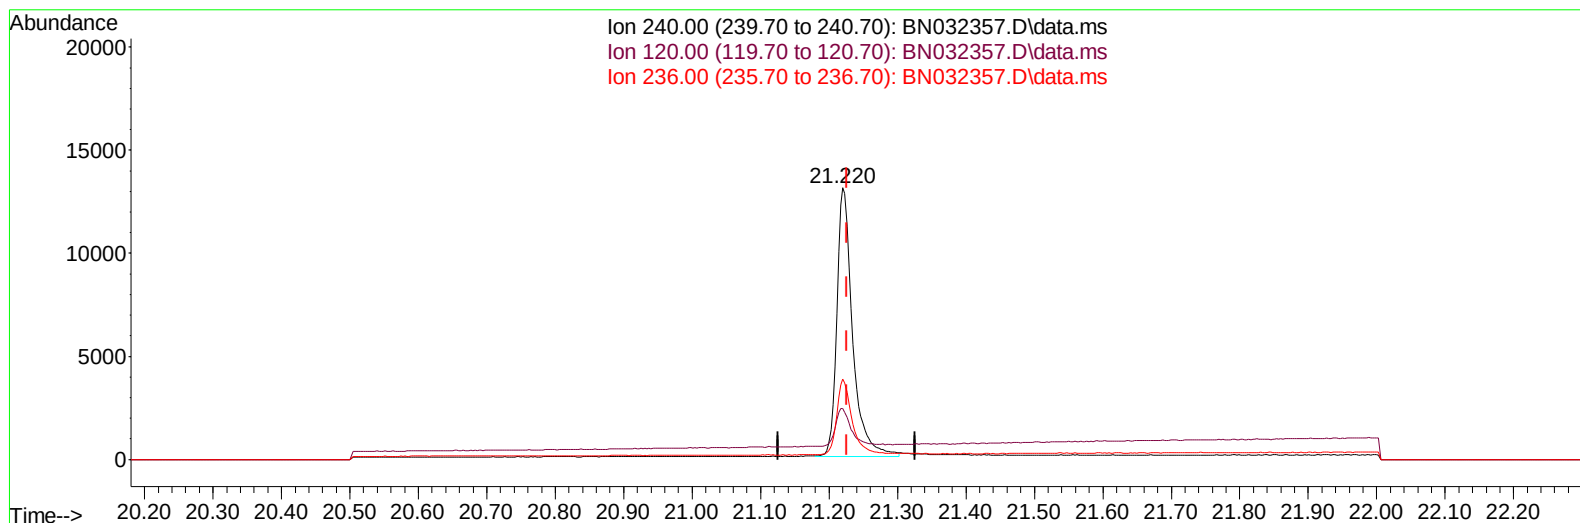

TIC: BN032357.D\data.ms

(17) Chrysene-d12

21.220min (-0.006) 0.40 ng/ul m

response 20835

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	18.85
236.00	28.40	29.52
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032357.D
Acq On : 01 Jul 2024 11:35
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Quant Time: Jul 01 12:24:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

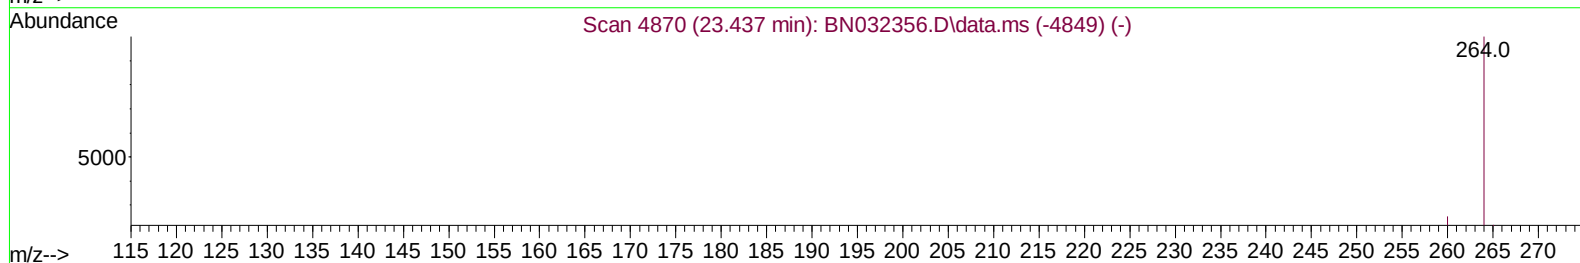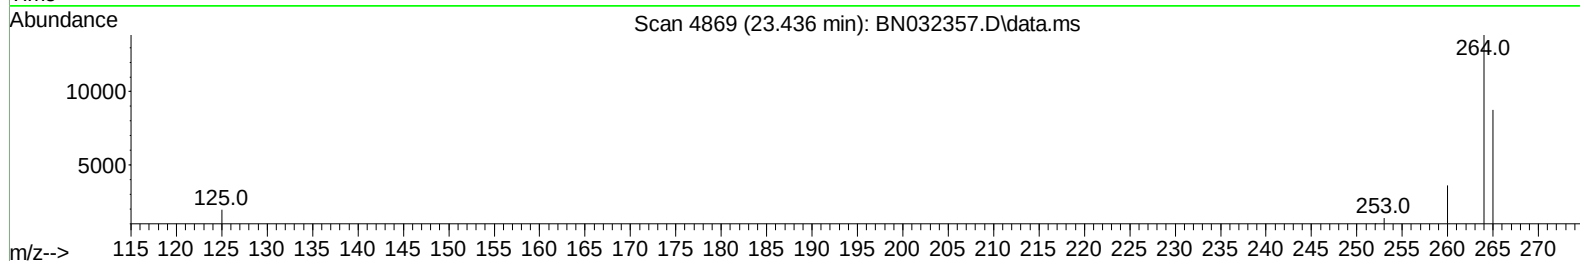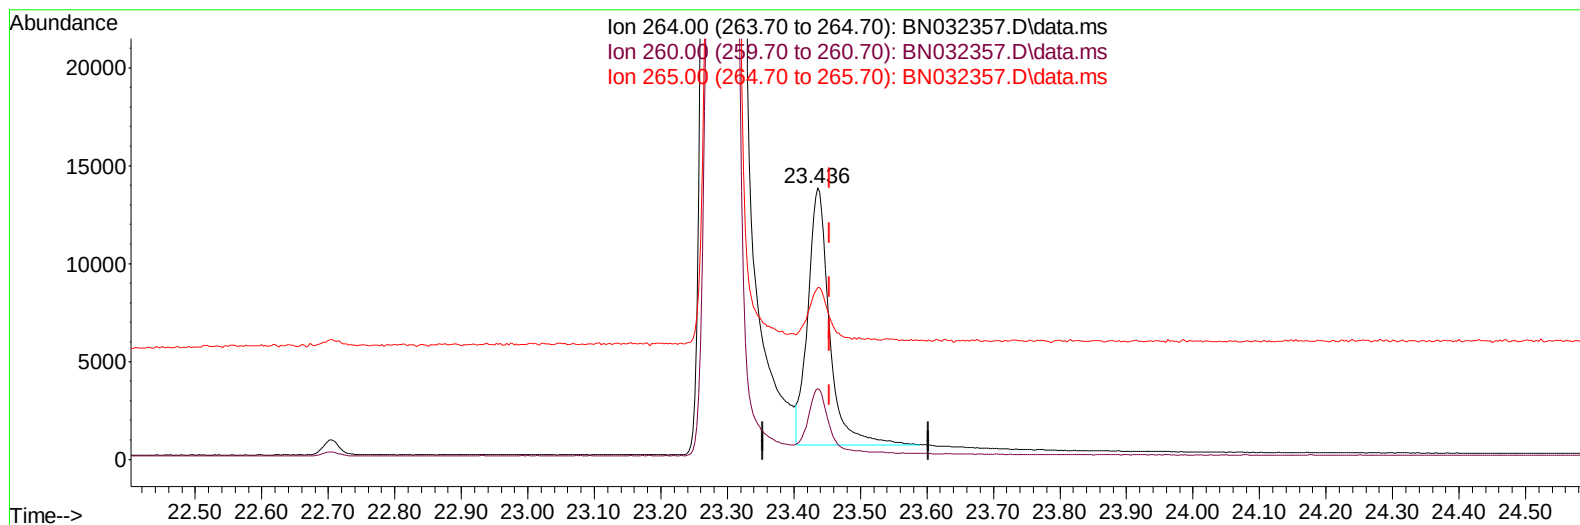

TIC: BN032357.D\data.ms

(23) Perylene-d12 (I)

23.436min (-0.018) 0.40 ng/u1

response 29585

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	26.14
265.00	67.20	63.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032357.D
Acq On : 01 Jul 2024 11:35
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

Quant Time: Jul 01 12:24:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration

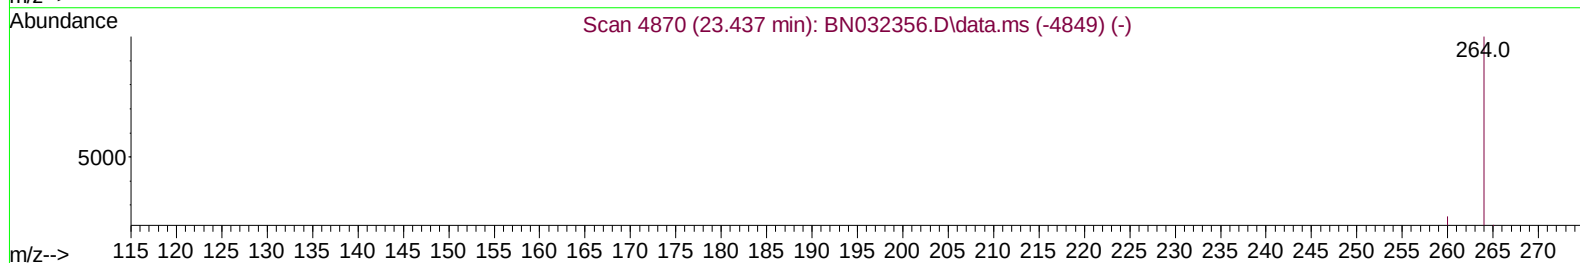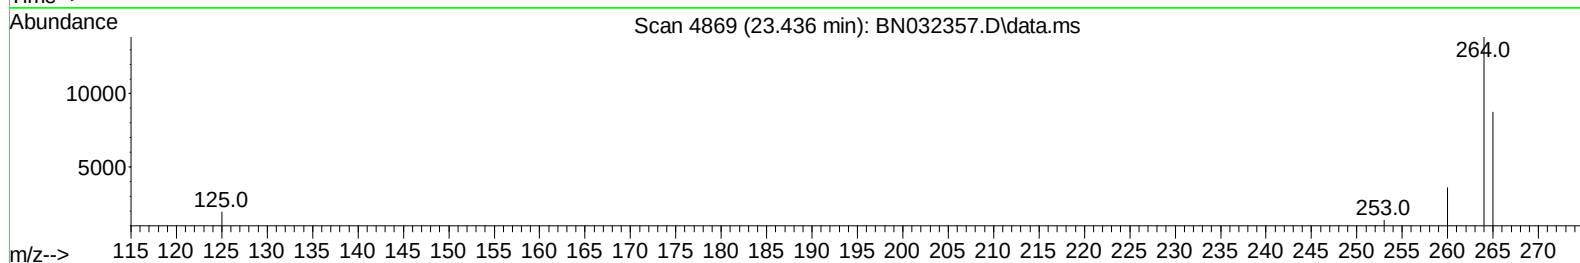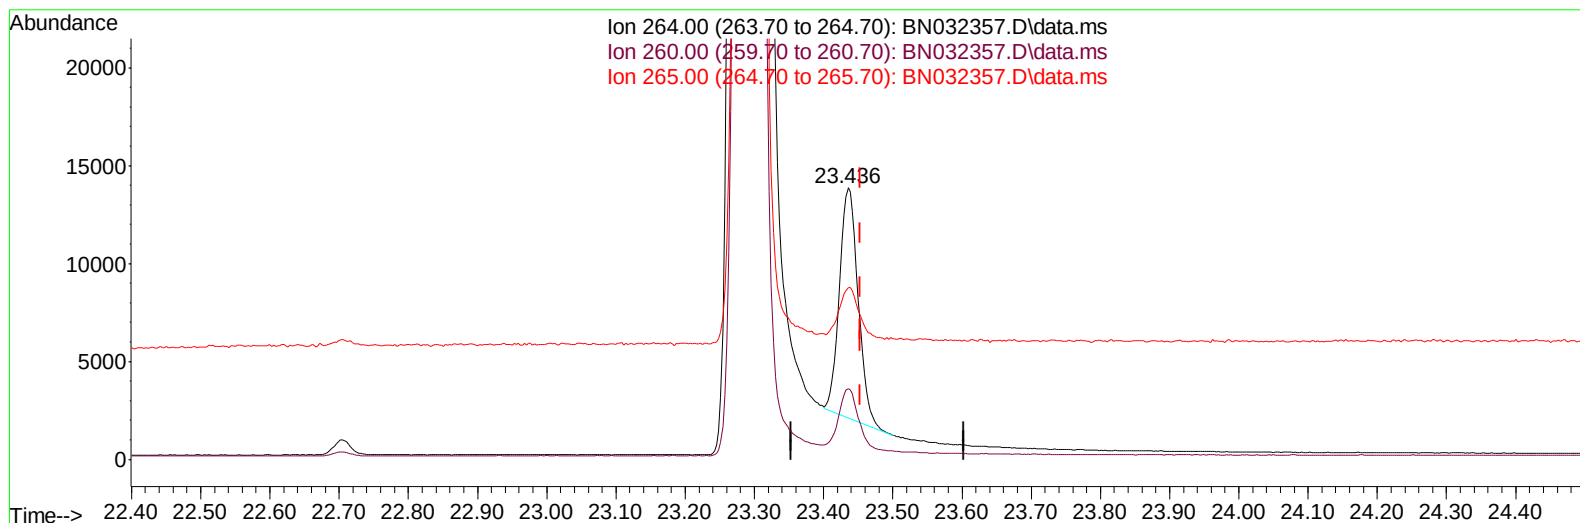

TIC: BN032357.D\data.ms

(23) Perylene-d12 (I)

23.436min (-0.018) 0.40 ng/ul m

response 22061

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	26.14
265.00	67.20	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
 Data File : BN032357.D
 Acq On : 01 Jul 2024 11:35
 Operator : MA/JU
 Sample : PB161603BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK603

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/02/2024
 Supervised By :mohammad ahmed 07/04/2024

Quant Time: Jul 01 12:24:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 27 13:23:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.612	152	9458	0.400	ng/ul	0.00
4) Naphthalene-d8	10.387	136	31071	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.258	164	17919	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.012	188	30921m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.220	240	20835m	0.400	ng/ul	0.00
23) Perylene-d12	23.436	264	22061m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.148	96	47265	4.496	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.988	152	12013	0.258	ng/ul	-0.01
18) Fluoranthene-d10	19.050	212	18662	0.298	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032357.D
Acq On : 01 Jul 2024 11:35
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Quant Time: Jul 01 12:24:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/02/2024
Supervised By :mohammad ahmed 07/04/2024

