




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032418.D
Acq On : 03 Jul 2024 02:11
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Quant Time: Jul 03 03:31:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

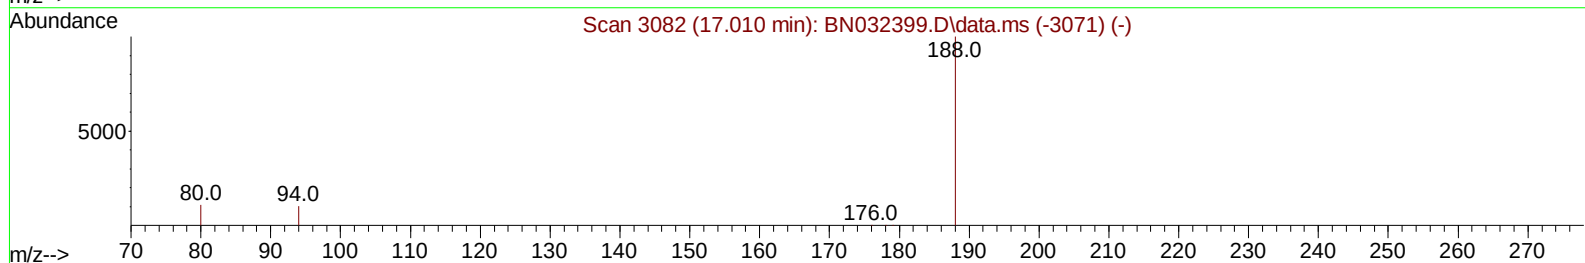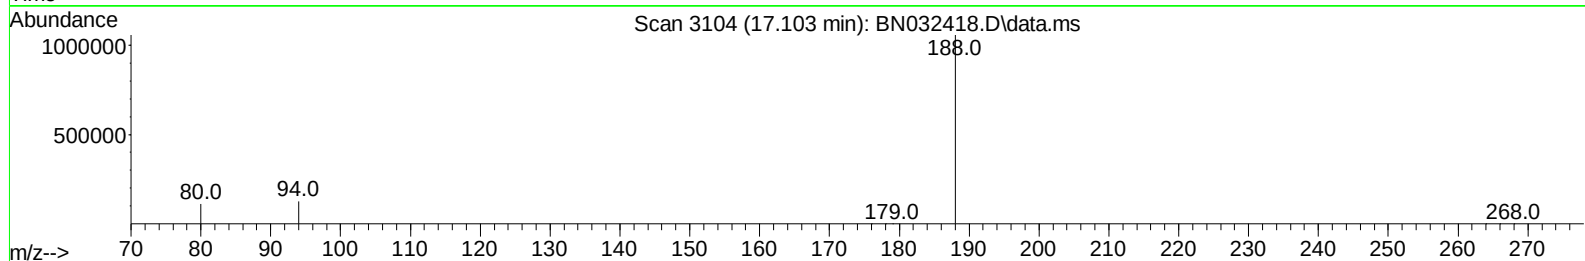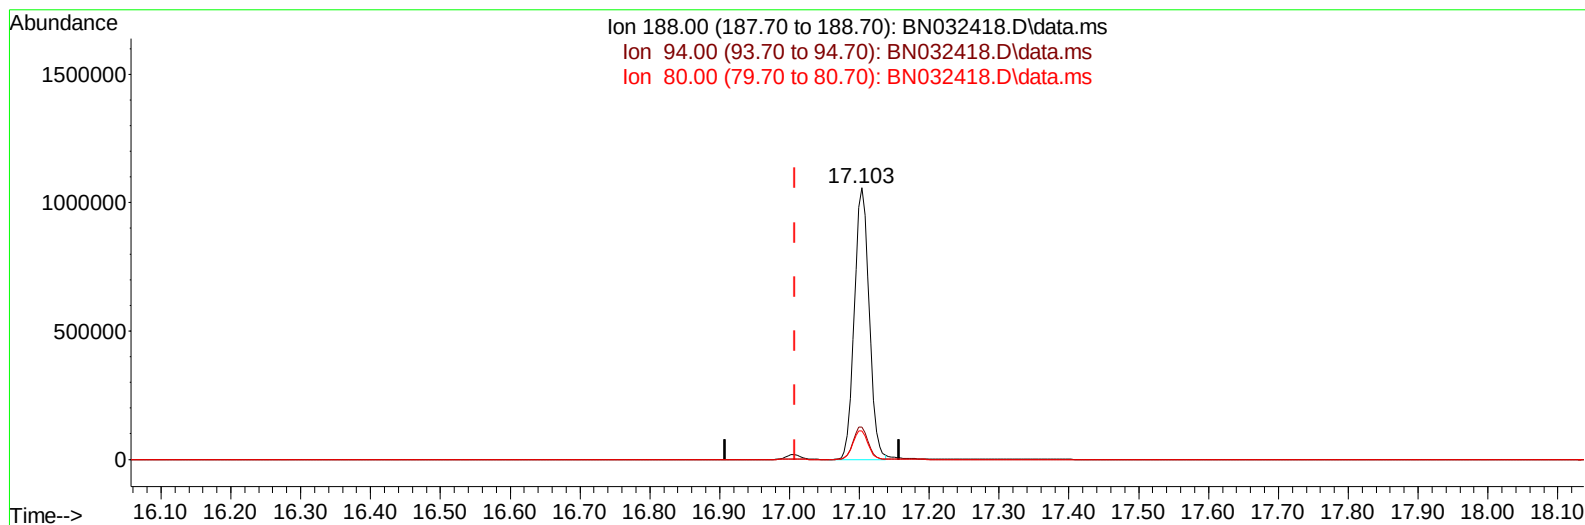

TIC: BN032418.D\data.ms

(13) Phenanthrene-d10 (I)

17.103min (+ 0.096) 0.40 ng/u1

response 1559622

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	11.89
80.00	10.50	10.52
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032418.D
Acq On : 03 Jul 2024 02:11
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Quant Time: Jul 03 03:31:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

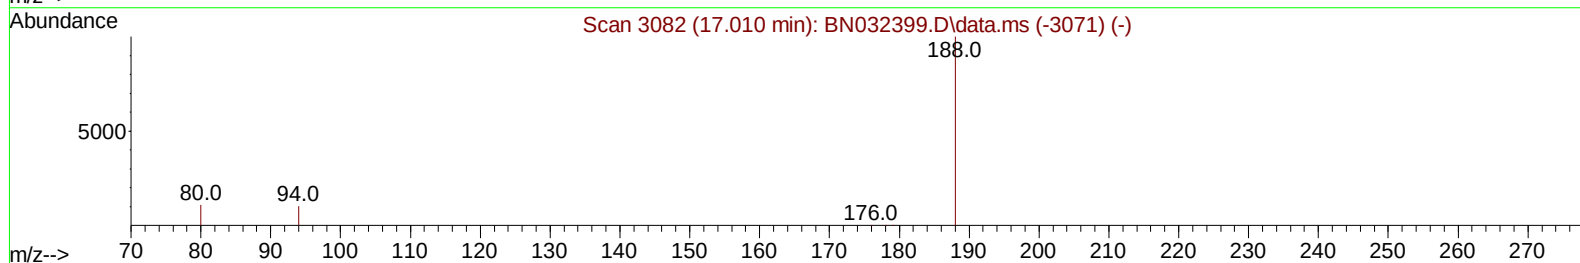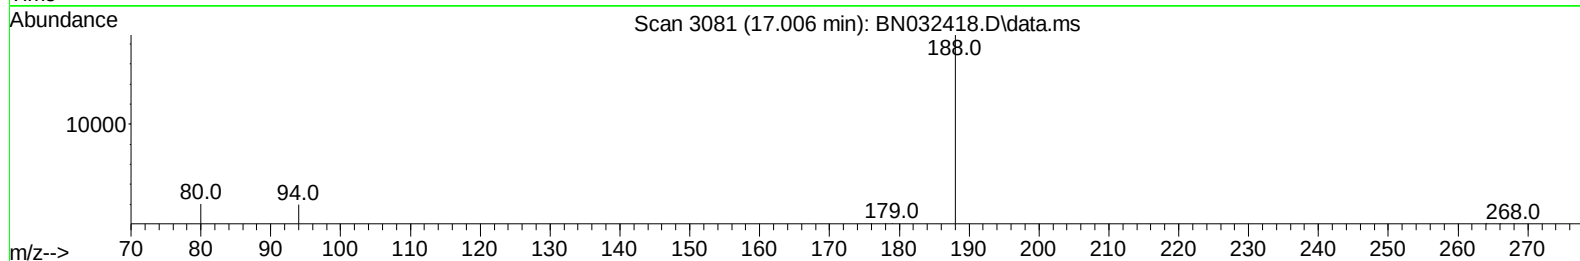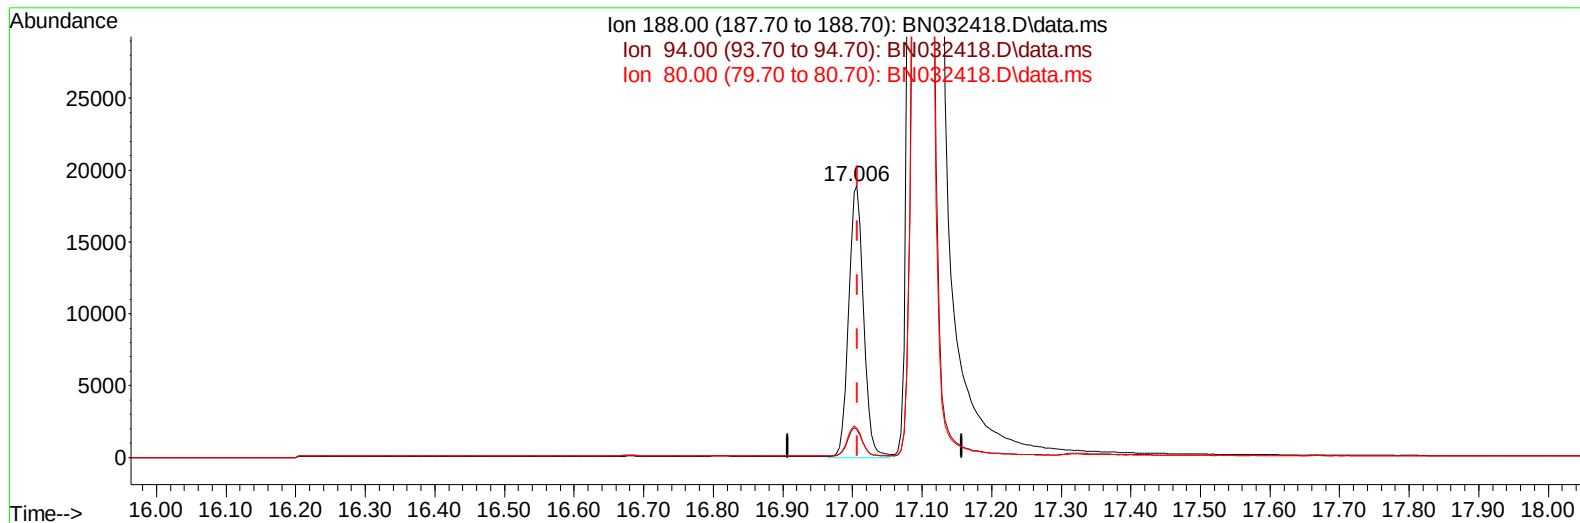

TIC: BN032418.D\data.ms

(13) Phenanthrene-d10 (I)

17.006min (-0.001) 0.40 ng/ul m

response 27934

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	10.39
80.00	10.50	10.85
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032418.D
Acq On : 03 Jul 2024 02:11
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Quant Time: Jul 03 03:31:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

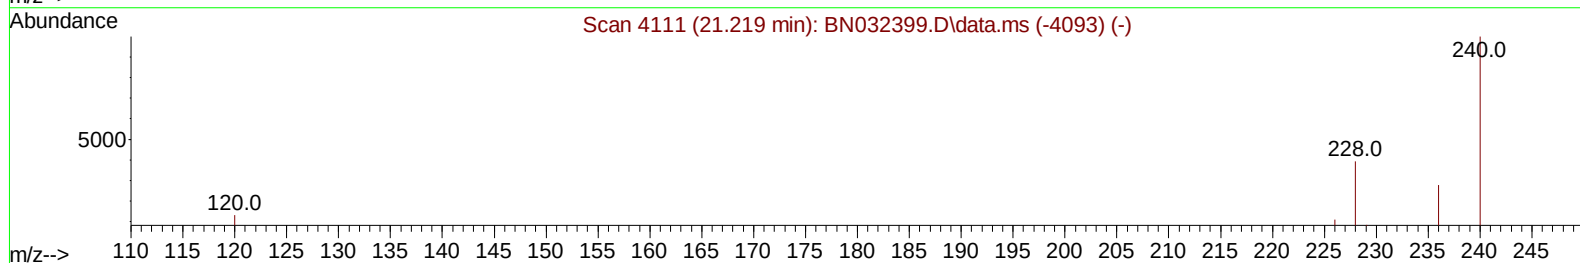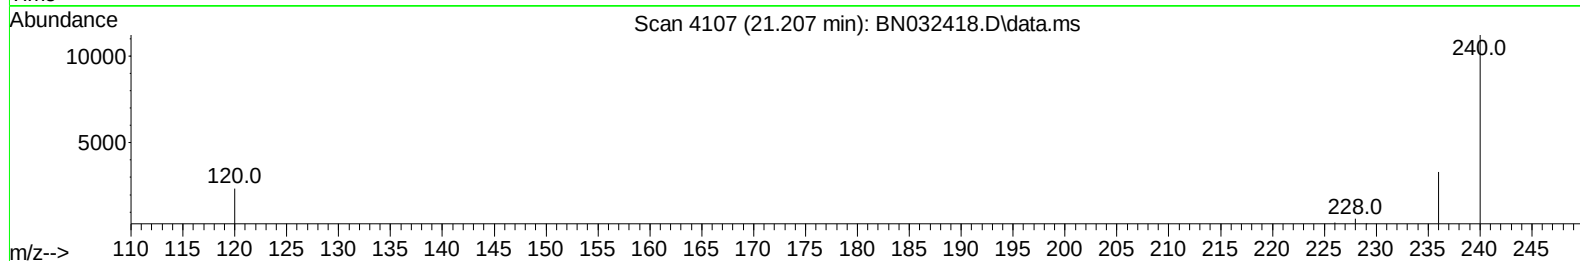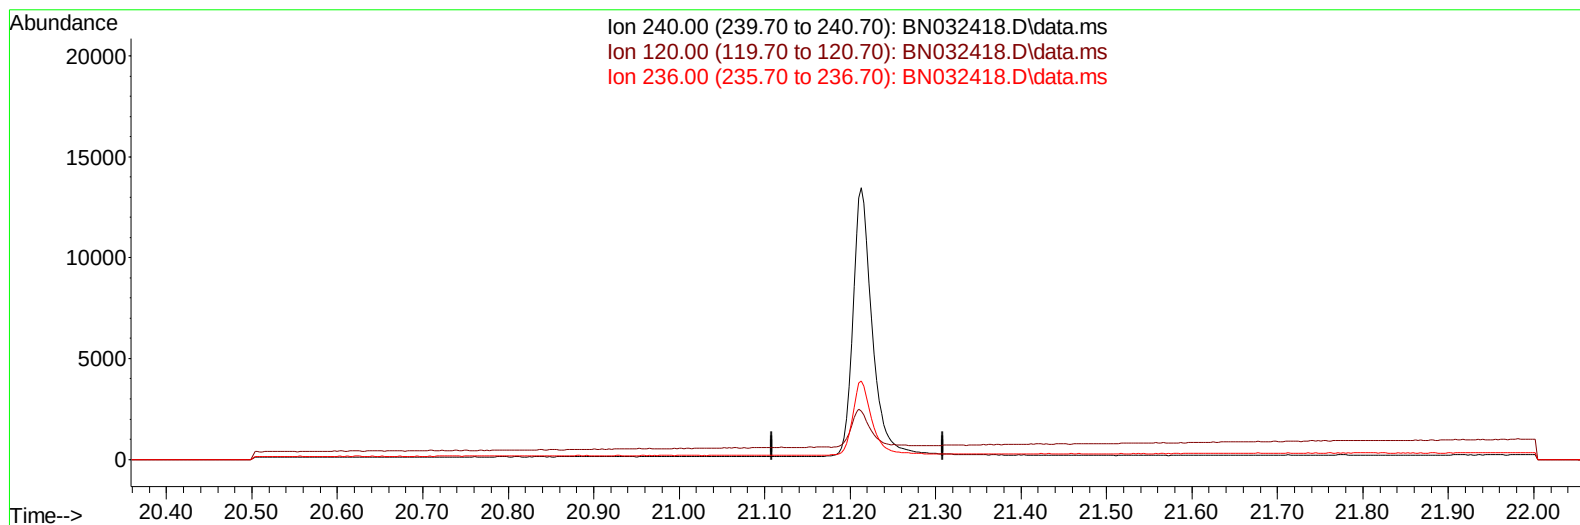

TIC: BN032418.D\data.ms

(17) Chrysene-d12

21.209min (-21.209) 0.00 ng/ul

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.80	0.00#
236.00	28.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032418.D
Acq On : 03 Jul 2024 02:11
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Quant Time: Jul 03 03:31:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

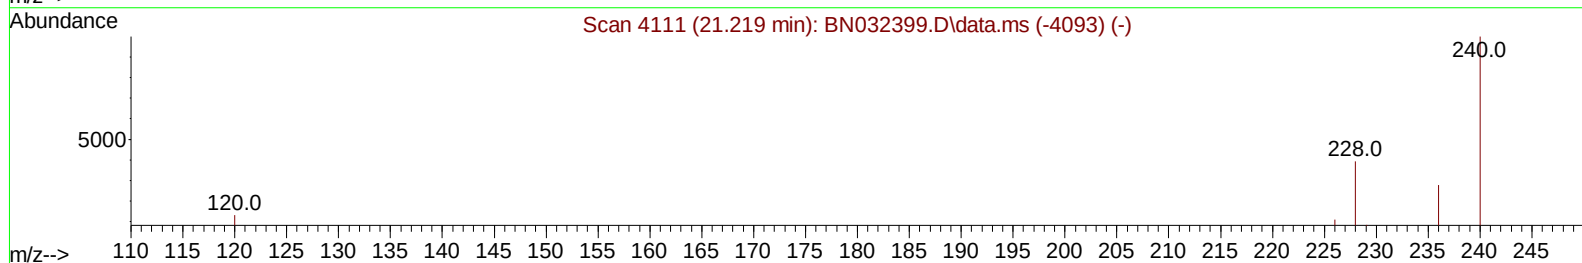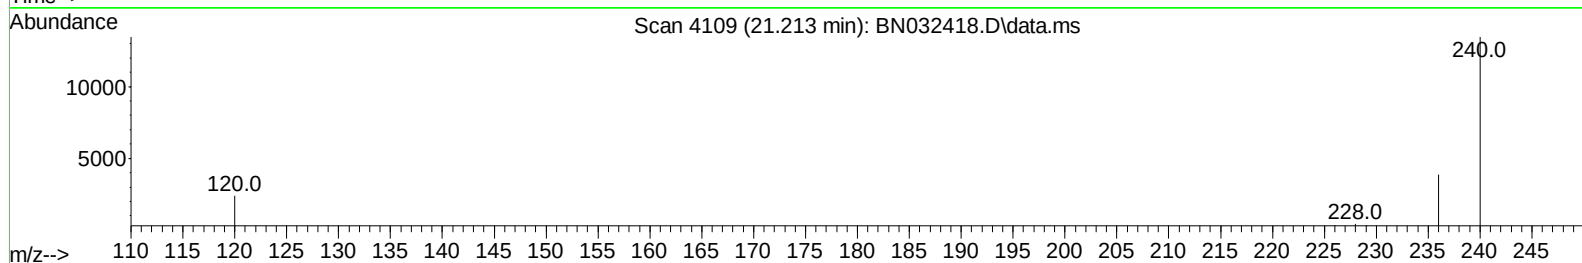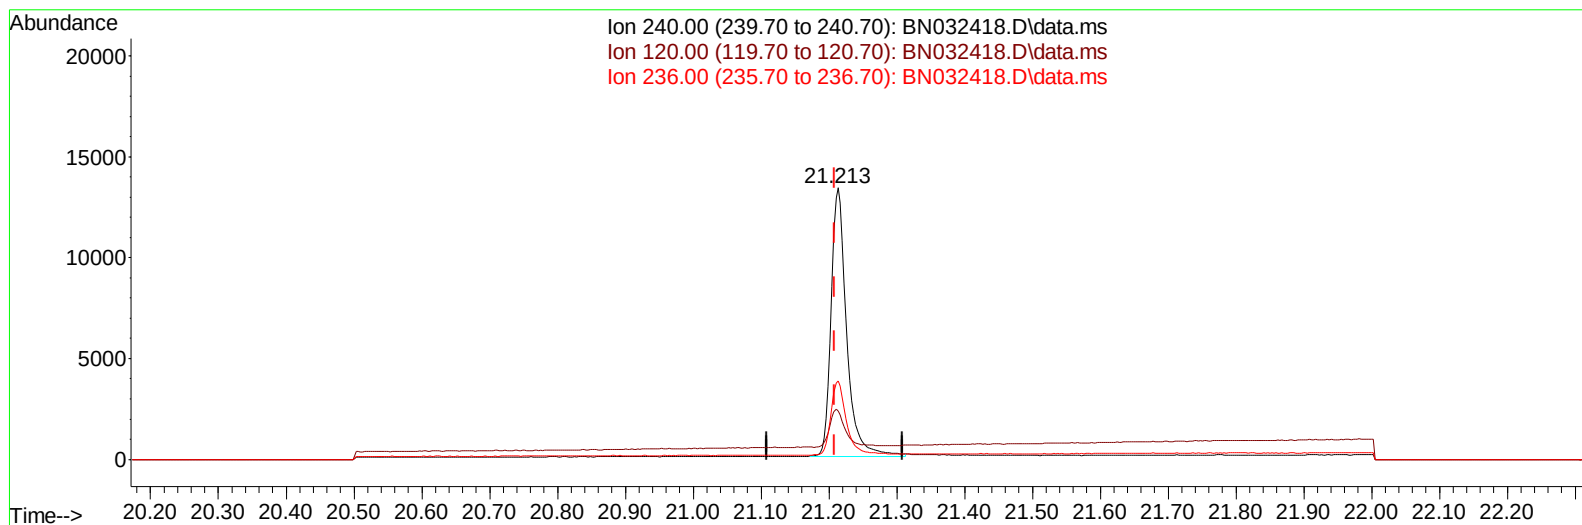

TIC: BN032418.D\data.ms

(17) Chrysene-d12

21.213min (+ 0.005) 0.40 ng/ul m

response 21199

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	17.80
236.00	28.40	28.81
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032418.D
Acq On : 03 Jul 2024 02:11
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Quant Time: Jul 03 03:31:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

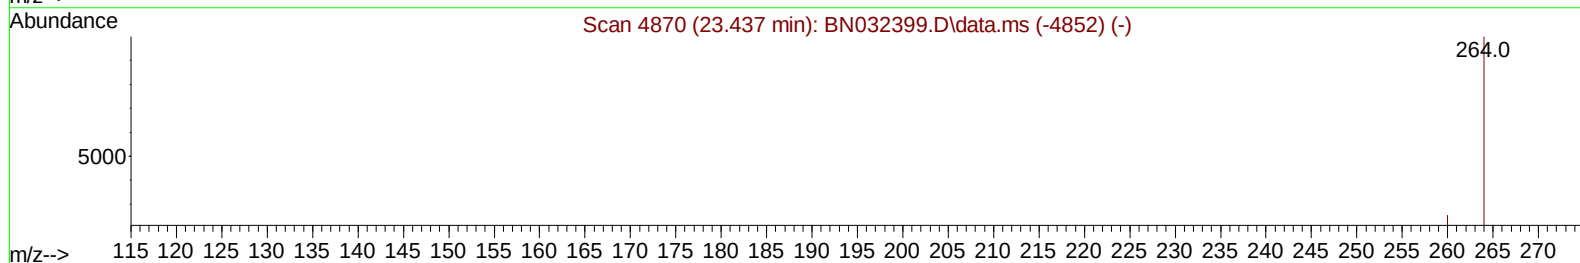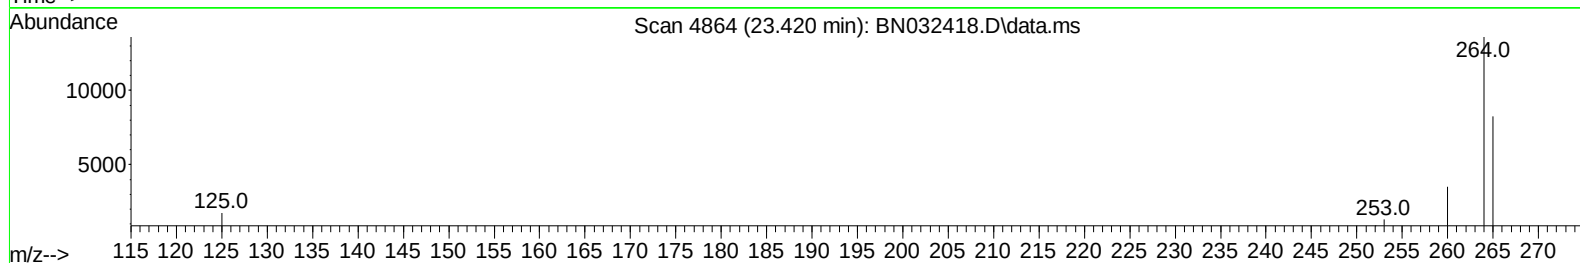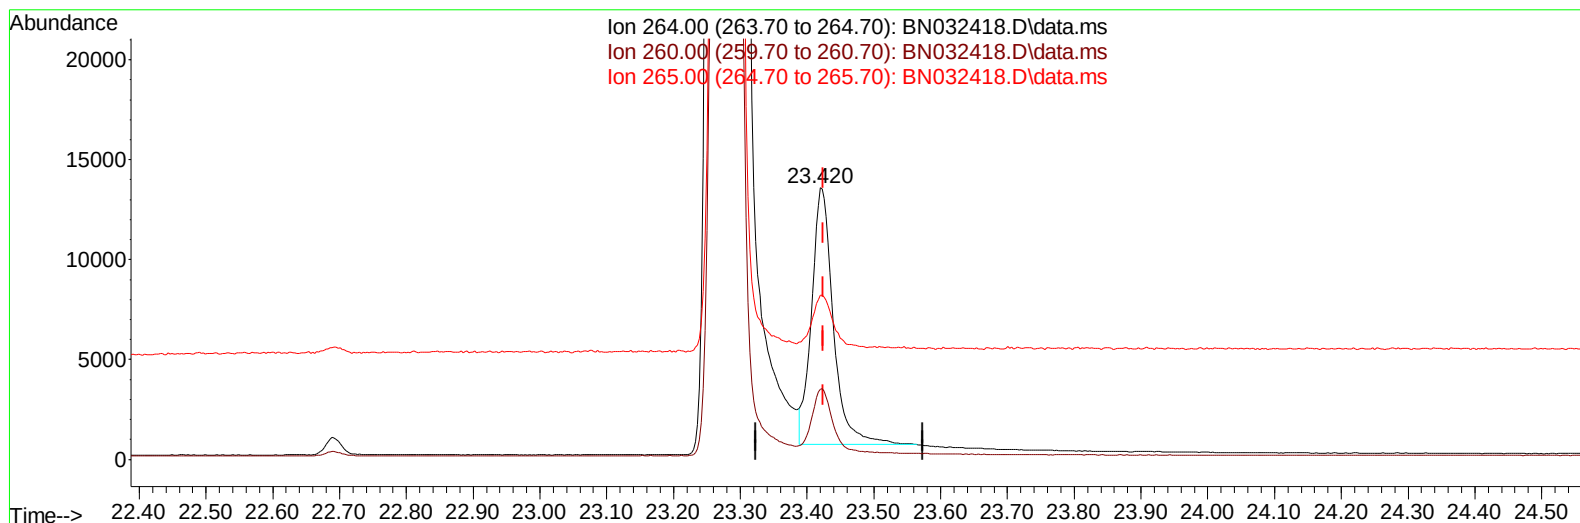

TIC: BN032418.D\data.ms

(23) Perylene-d12 (I)

23.420min (-0.004) 0.40 ng/u1

response 29421

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	25.88
265.00	67.20	60.60
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032418.D
Acq On : 03 Jul 2024 02:11
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Quant Time: Jul 03 03:31:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

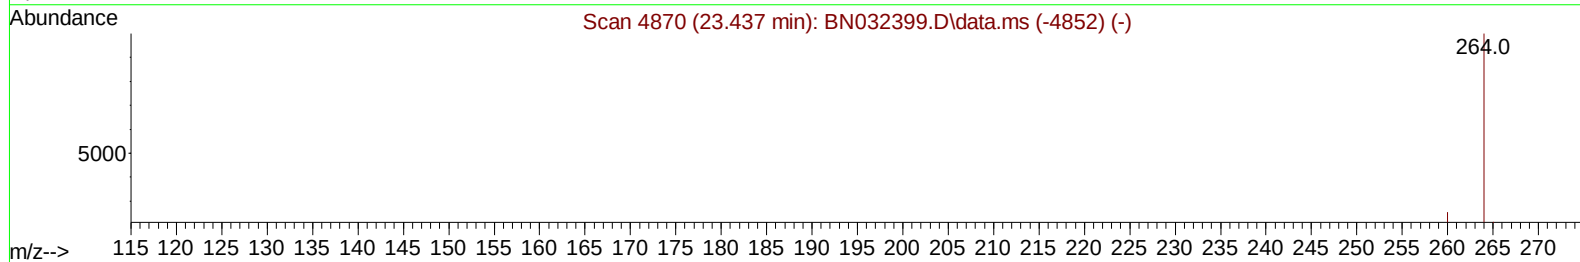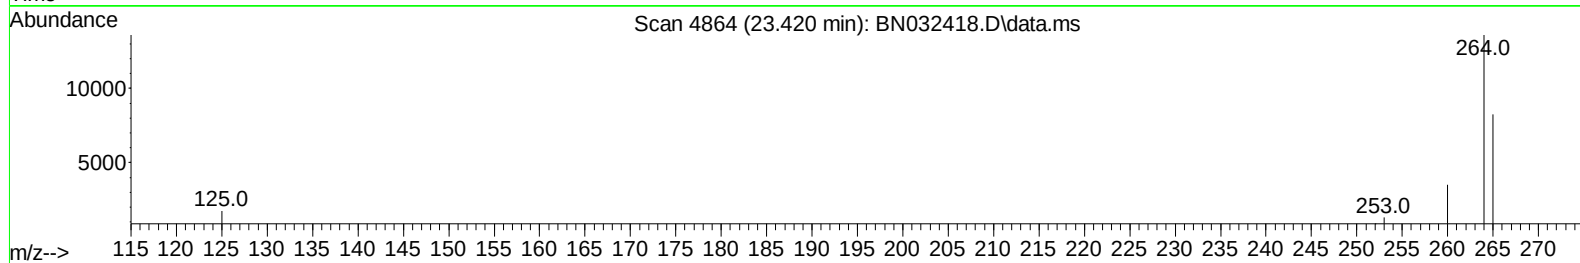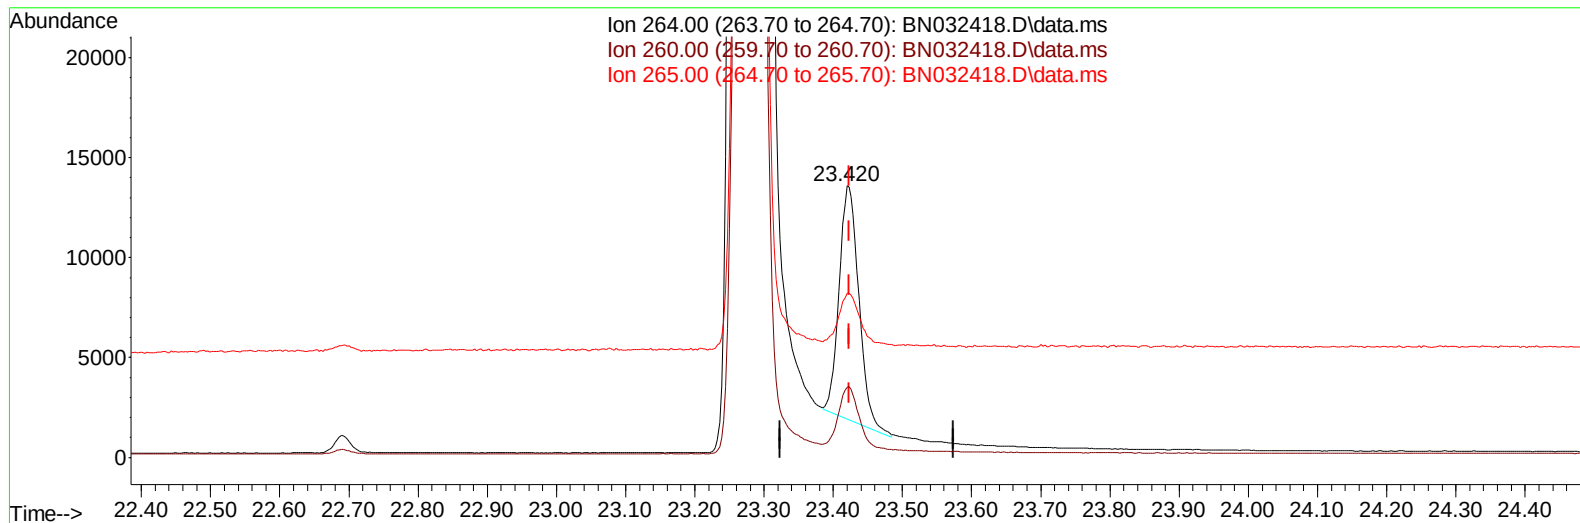

TIC: BN032418.D\data.ms

(23) Perylene-d12 (I)

23.420min (-0.004) 0.40 ng/ul m

response 23110

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	25.88
265.00	67.20	60.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
 Data File : BN032418.D
 Acq On : 03 Jul 2024 02:11
 Operator : MA/JU
 Sample : PB161603BL
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK603

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/03/2024
 Supervised By :mohammad ahmed 07/04/2024

Quant Time: Jul 03 03:31:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 03 03:26:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.603	152	9621	0.400	ng/ul	0.00
4) Naphthalene-d8	10.375	136	30334	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.252	164	16519	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.006	188	27934m	0.400	ng/ul	0.00
17) Chrysene-d12	21.213	240	21199m	0.400	ng/ul	0.00
23) Perylene-d12	23.420	264	23110m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.144	96	48810	4.564	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.981	152	11829	0.260	ng/ul	0.00
18) Fluoranthene-d10	19.044	212	18241	0.286	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032418.D
Acq On : 03 Jul 2024 02:11
Operator : MA/JU
Sample : PB161603BL
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK603

Manual IntegrationsAPPROVED

Quant Time: Jul 03 03:31:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

