

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
 Data File : BN032414.D
 Acq On : 02 Jul 2024 23:12
 Operator : MA/JU
 Sample : P2871-23DL 5X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4B54DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/03/2024
 Supervised By :mohammad ahmed 07/04/2024

Quant Time: Jul 02 23:57:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 27 13:23:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.603	152	8219	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.382	136	26733	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.248	164	15805	0.400	ng/ul	-0.02
13) Phenanthrene-d10	17.003	188	32329	0.400	ng/ul	-0.02
17) Chrysene-d12	21.206	240	19536	0.400	ng/ul	-0.02
23) Perylene-d12	23.421	264	22624	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	8326	0.911	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.977	152	2662	0.066	ng/ul	-0.02
18) Fluoranthene-d10	19.041	212	4876	0.083	ng/ul	-0.02
Target Compounds					Qvalue	
5) Naphthalene	10.426	128	20980	0.297	ng/ul	99
7) 2-Methylnaphthalene	12.054	142	7442	0.159	ng/ul	98
8) 1-Methylnaphthalene	12.274	142	6142	0.126	ng/ul	100
10) Acenaphthylene	13.971	152	6126	0.093	ng/ul#	90
11) Acenaphthene	14.313	153	24584	0.482	ng/ul	99
12) Fluorene	15.308	166	35815	0.589	ng/ul	98
15) Phenanthrene	17.046	178	497444	5.612	ng/ul	99
16) Anthracene	17.138	178	120756	1.527	ng/ul	99
19) Fluoranthene	19.073	202	534451	7.184	ng/ul	100
20) Pyrene	19.436	202	352319	4.532	ng/ul	99
21) Benzo(a)anthracene	21.191	228	193908	2.750	ng/ul	99
22) Chrysene	21.244	228	169800	2.194	ng/ul	97
24) Benzo(b)fluoranthene	22.757	252	201107m	2.046	ng/ul	
25) Benzo(k)fluoranthene	22.795	252	84832m	0.888	ng/ul	
26) Benzo(a)pyrene	23.325	252	81593	1.193	ng/ul	94
27) Indeno(1,2,3-cd)pyrene	25.656	276	64543	0.603	ng/ul#	94
28) Dibenzo(a,h)anthracene	25.656	278	23821	0.299	ng/ul#	84
29) Benzo(g,h,i)perylene	26.340	276	8576	0.101	ng/ul#	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070124\
Data File : BN032414.D
Acq On : 02 Jul 2024 23:12
Operator : MA/JU
Sample : P2871-23DL 5X
Misc :
ALS Vial : 61 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
A4B54DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024


Quant Time: Jul 02 23:57:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:23:38 2024
Response via : Initial Calibration

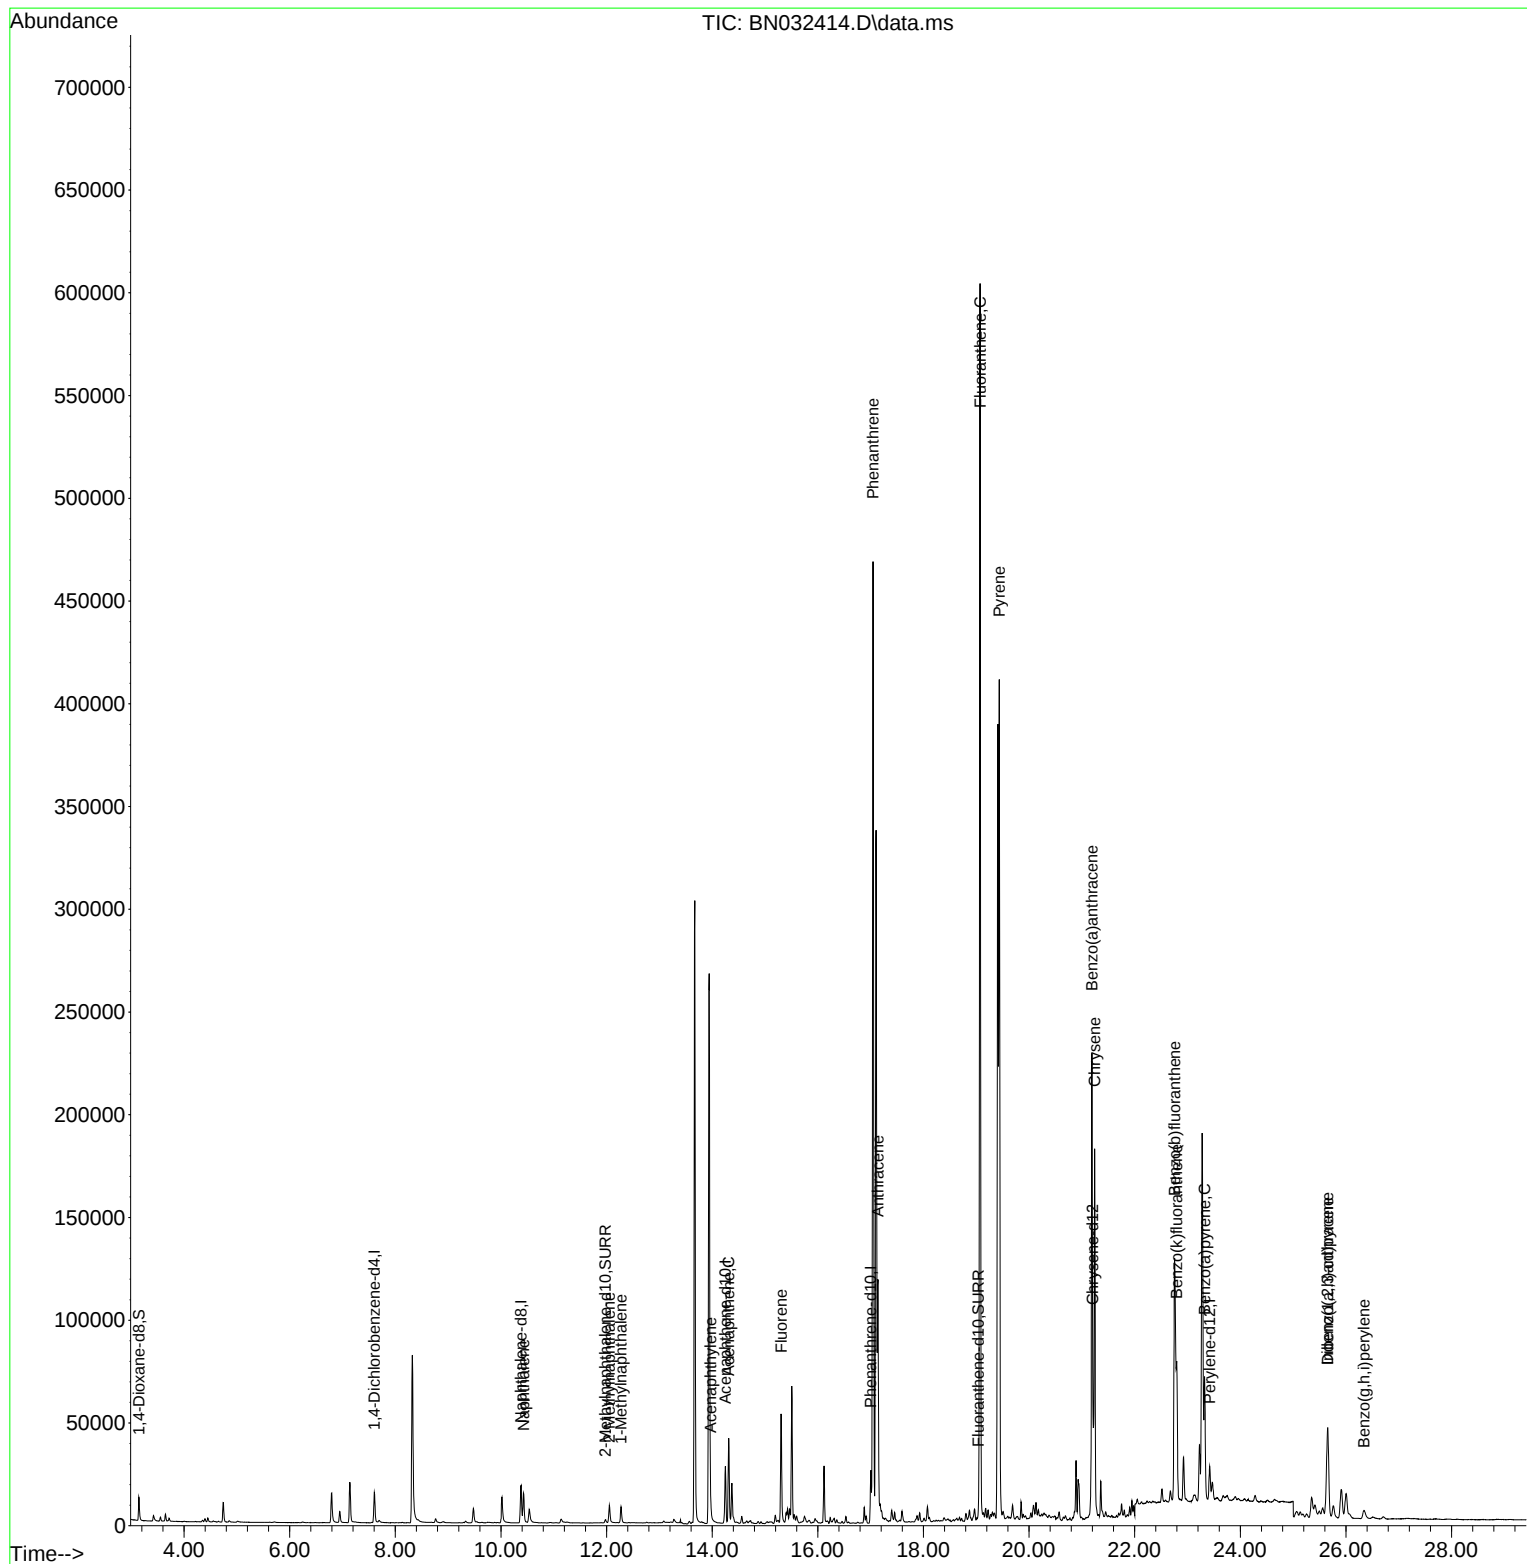

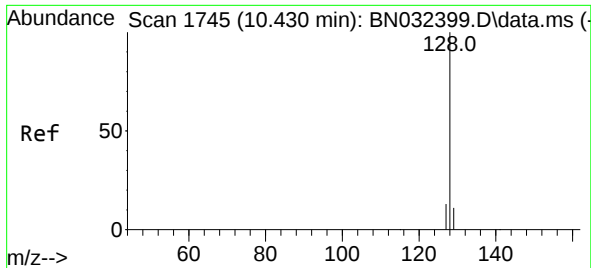

#5
Naphthalene
Concen: 0.297 ng/ul
RT: 10.426 min Scan# 1744
Delta R.T. -0.022 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12




Instrument :
BNA_N
ClientSampleId :
A4B54DL

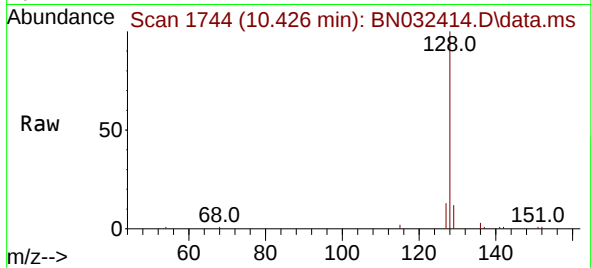

Tgt Ion:128 Resp: 20980
Ion Ratio Lower Upper
128 100
129 11.9 9.2 13.8
127 13.4 10.8 16.2




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

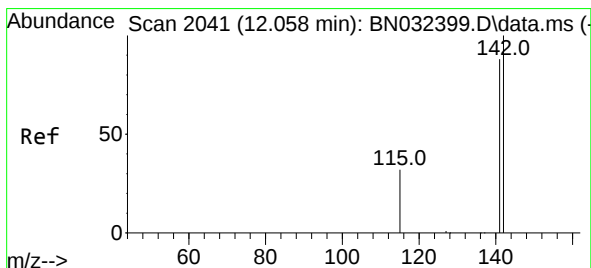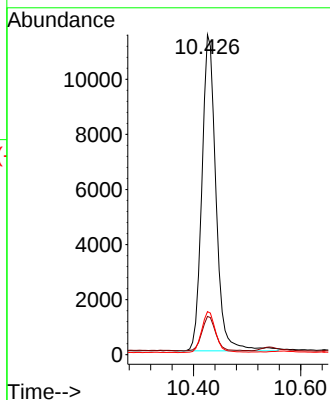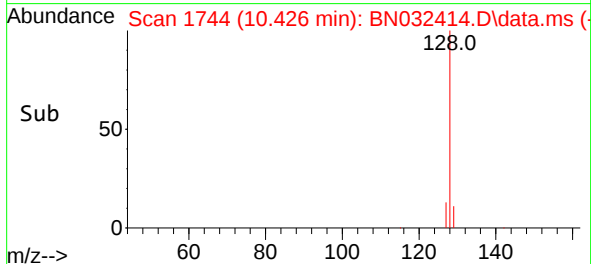

#7
2-Methylnaphthalene
Concen: 0.159 ng/ul
RT: 12.054 min Scan# 2040
Delta R.T. -0.022 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12


Tgt Ion:142 Resp: 7442
Ion Ratio Lower Upper
142 100
141 88.8 72.2 108.2

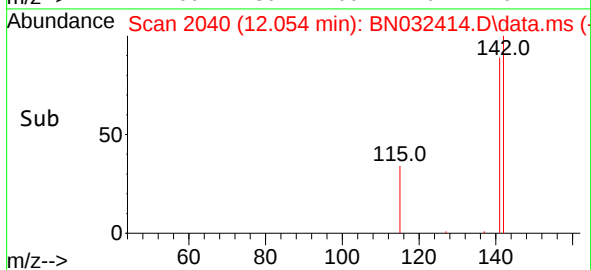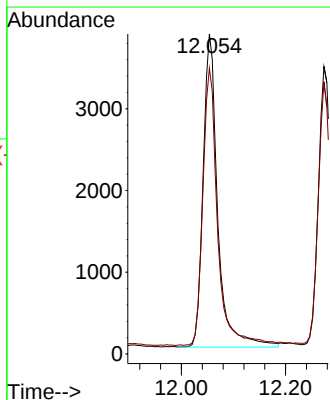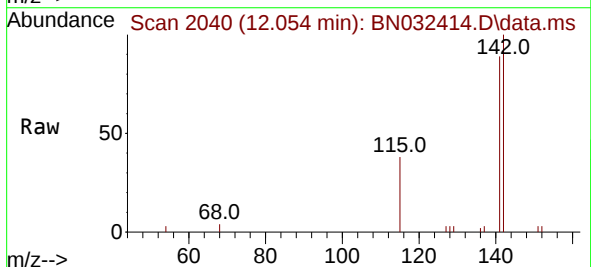

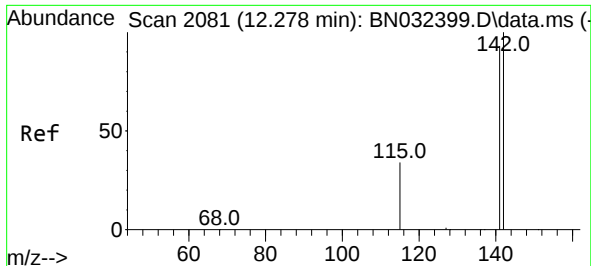

#8
1-Methylnaphthalene
Concen: 0.126 ng/ul
RT: 12.274 min Scan# 2081
Delta R.T. -0.022 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12




Instrument :
BNA_N
ClientSampleId :
A4B54DL

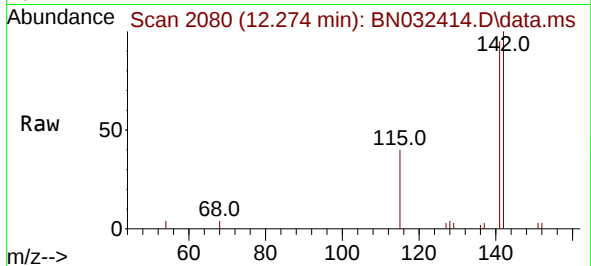

Tgt Ion:142 Resp: 6142
Ion Ratio Lower Upper
142 100
141 92.1 73.4 110.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

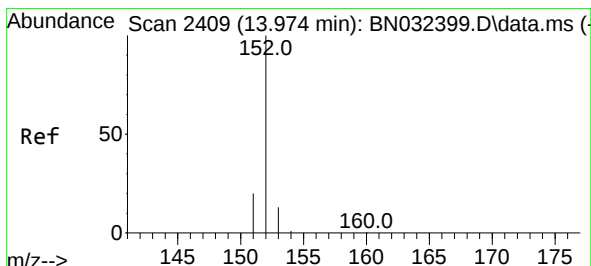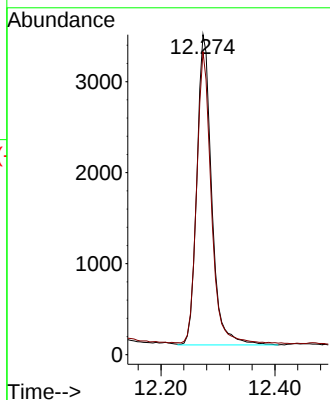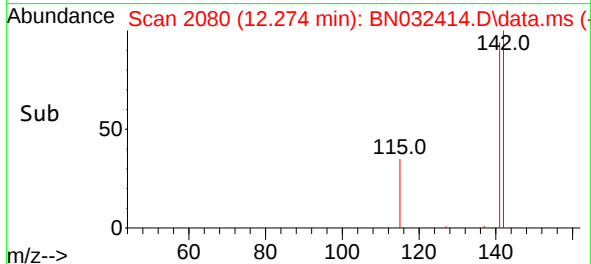

#10
Acenaphthylene
Concen: 0.093 ng/ul
RT: 13.971 min Scan# 2408
Delta R.T. -0.019 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12


Tgt Ion:152 Resp: 6126
Ion Ratio Lower Upper
152 100
151 23.1 15.7 23.5
153 19.2 10.9 16.3#

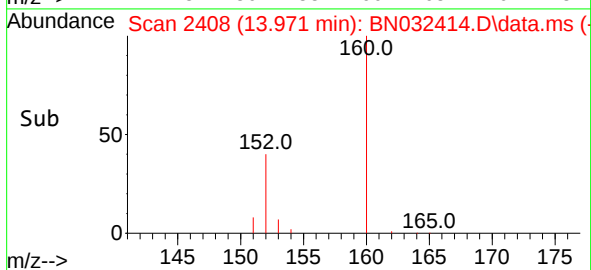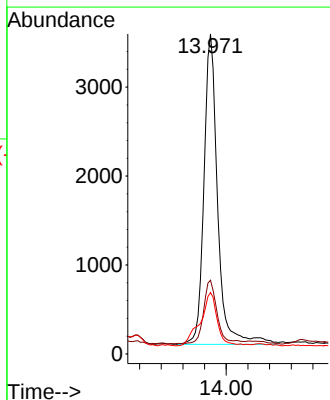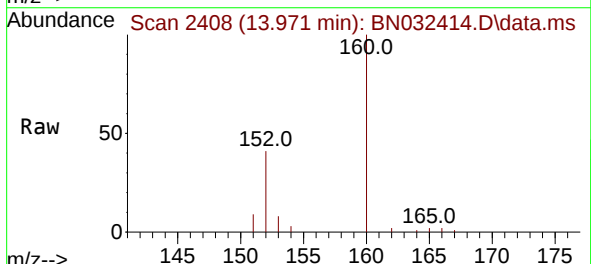

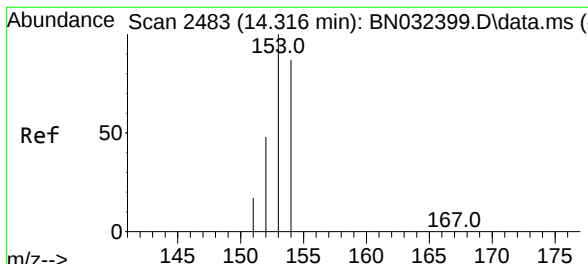

#11
 Acenaphthene
 Concen: 0.482 ng/ul
 RT: 14.313 min Scan# 2482
 Delta R.T. -0.019 min
 Lab File: BN032414.D
 Acq: 02 Jul 2024 23:12

Instrument :
 BNA_N
 ClientSampleId :
 A4B54DL



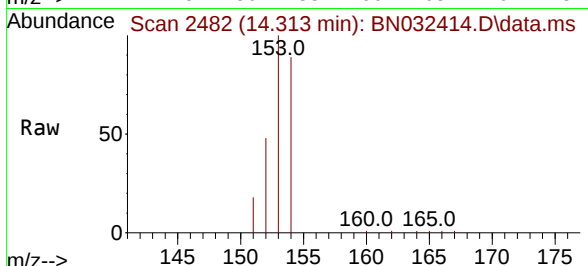


Tgt Ion:153 Resp: 24584

Ion	Ratio	Lower	Upper
153	100		
152	48.3	39.5	59.3
154	89.0	71.7	107.5

Manual Integrations
 APPROVED




Reviewed By :Yogesh Patel 07/03/2024
 Supervised By :mohammad ahmed 07/04/2024

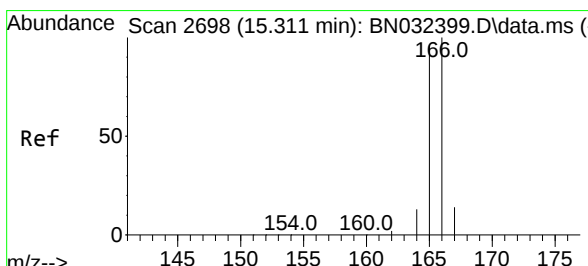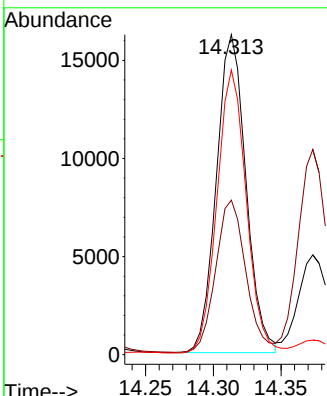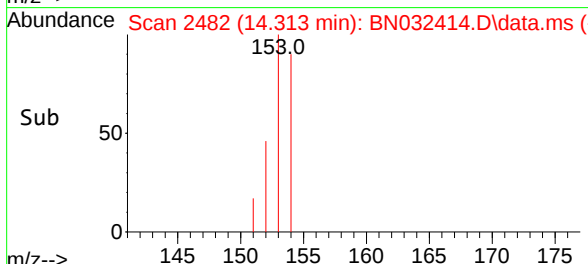


#12
 Fluorene
 Concen: 0.589 ng/ul
 RT: 15.308 min Scan# 2697
 Delta R.T. -0.019 min
 Lab File: BN032414.D
 Acq: 02 Jul 2024 23:12

Tgt Ion:166 Resp: 35815


Ion	Ratio	Lower	Upper
166	100		
165	96.5	79.0	118.6
167	14.8	11.0	16.6

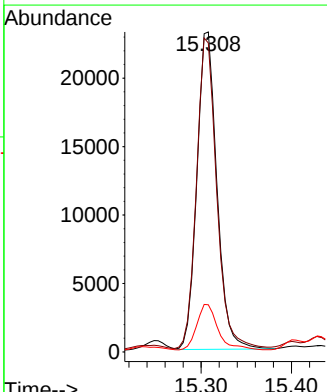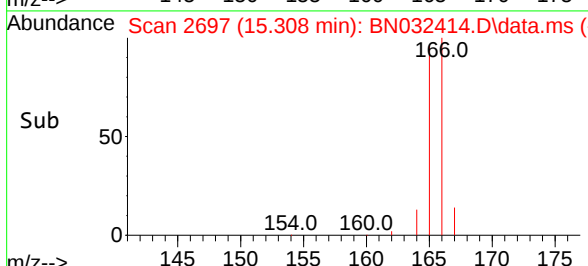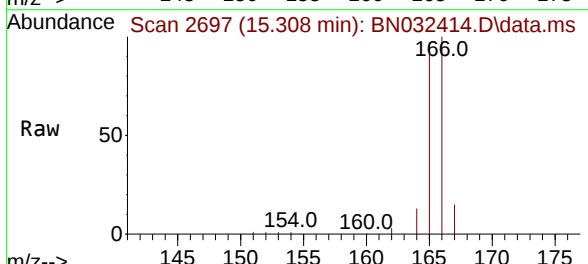

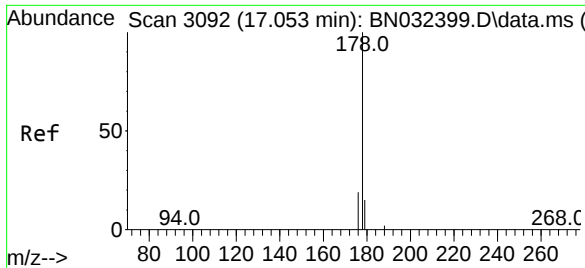

#15
Phenanthrene
Concen: 5.612 ng/u1
RT: 17.046 min Scan# 3092
Delta R.T. -0.021 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12




Instrument :
BNA_N
ClientSampleId :
A4B54DL

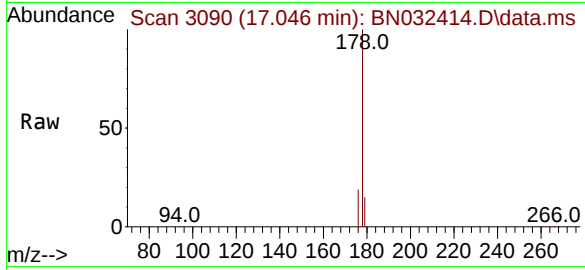

Tgt Ion:178 Resp: 49744
Ion Ratio Lower Upper
178 100
179 15.4 12.6 18.8
176 19.1 15.6 23.4




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

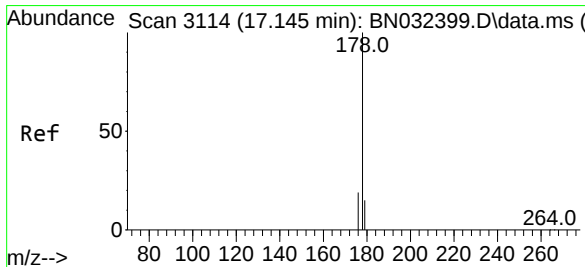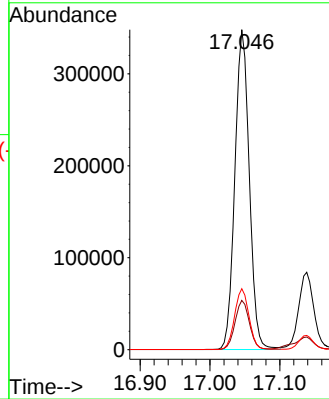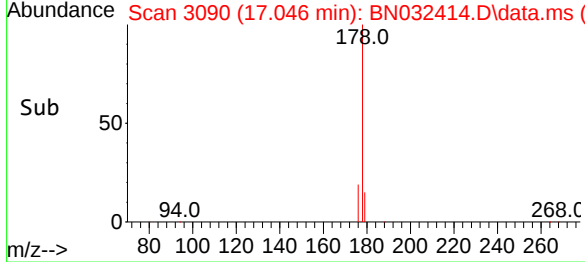

#16
Anthracene
Concen: 1.527 ng/u1
RT: 17.138 min Scan# 3112
Delta R.T. -0.021 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12


Tgt Ion:178 Resp: 120756
Ion Ratio Lower Upper
178 100
179 16.3 12.5 18.7
176 18.5 15.0 22.6

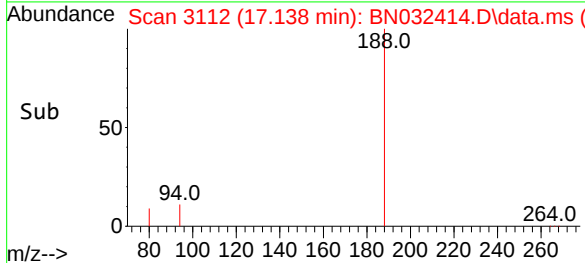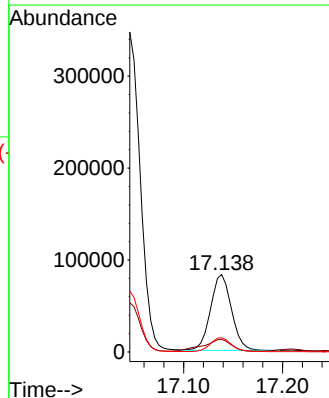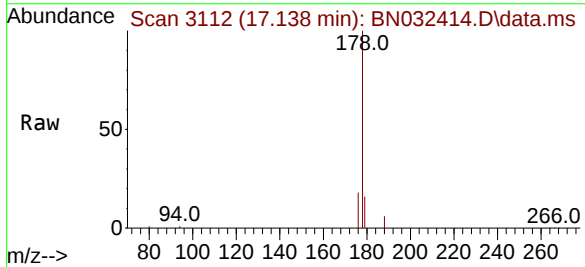

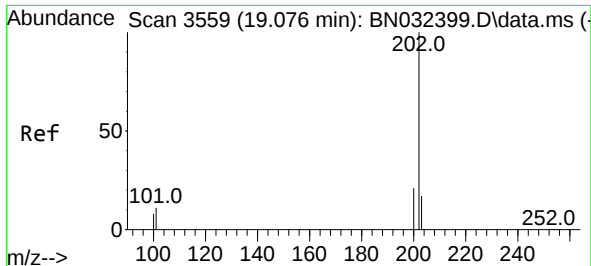

#19
Fluoranthene
Concen: 7.184 ng/u1
RT: 19.073 min Scan# 3559
Delta R.T. -0.019 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12




Instrument :
BNA_N
ClientSampleId :
A4B54DL

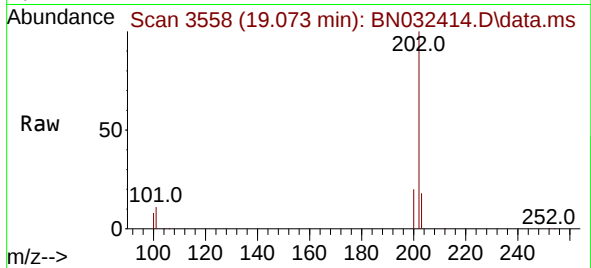

Tgt Ion:202 Resp: 53445
Ion Ratio Lower Upper
202 100
101 10.9 8.8 13.2
100 8.0 6.4 9.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

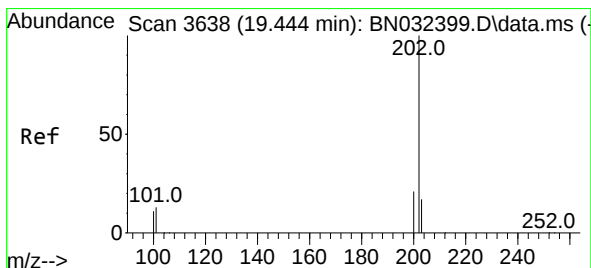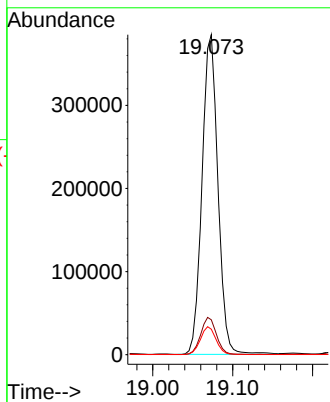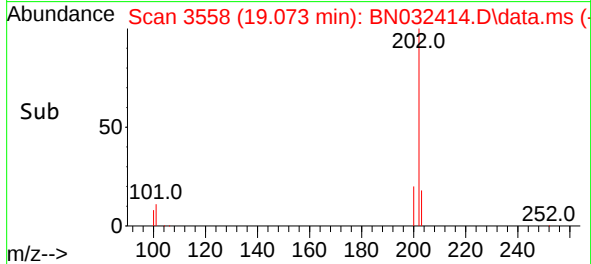

#20
Pyrene
Concen: 4.532 ng/u1
RT: 19.436 min Scan# 3636
Delta R.T. -0.019 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12


Tgt Ion:202 Resp: 352319
Ion Ratio Lower Upper
202 100
101 13.3 11.0 16.4
100 10.6 8.7 13.1

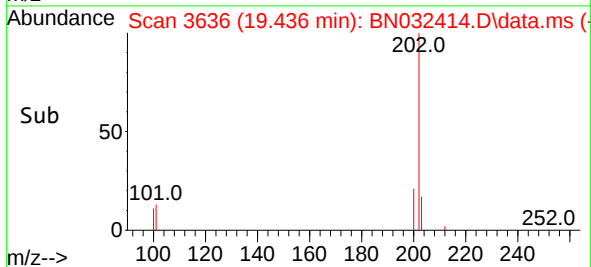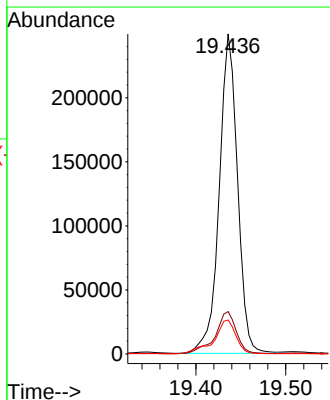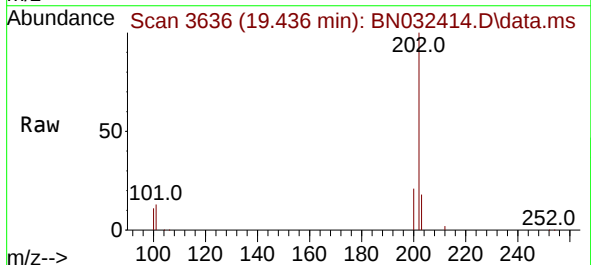

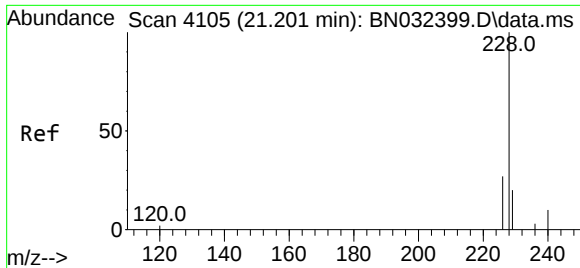

#21
Benzo(a)anthracene
Concen: 2.750 ng/ul
RT: 21.191 min Scan# 4110
Delta R.T. -0.023 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12




Instrument :
BNA_N
ClientSampleId :
A4B54DL

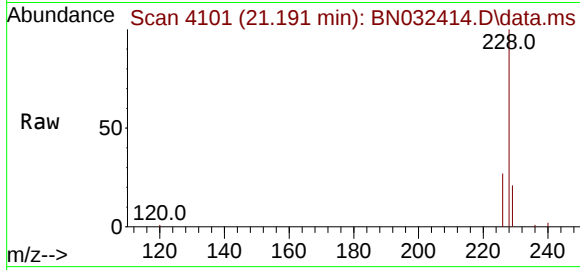

Tgt Ion:228 Resp: 193908
Ion Ratio Lower Upper
228 100
229 20.7 15.7 23.5
226 27.3 21.8 32.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

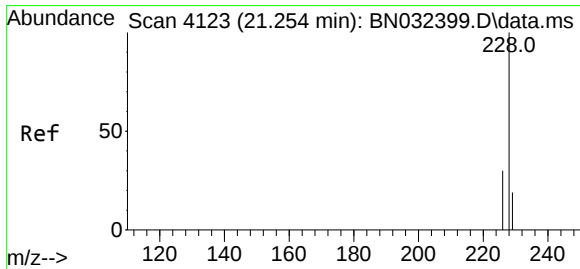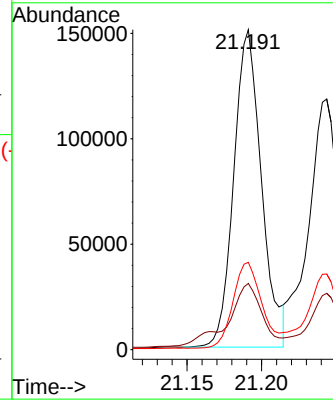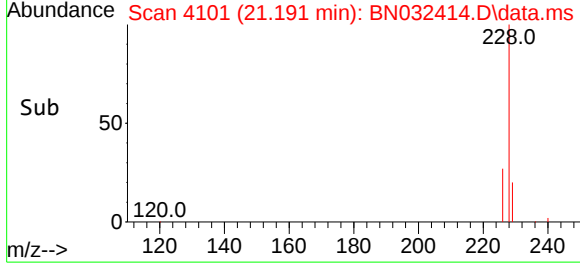

#22
Chrysene
Concen: 2.194 ng/ul
RT: 21.244 min Scan# 4119
Delta R.T. -0.023 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12


Tgt Ion:228 Resp: 169800
Ion Ratio Lower Upper
228 100
226 30.2 23.6 35.4
229 22.4 15.7 23.5

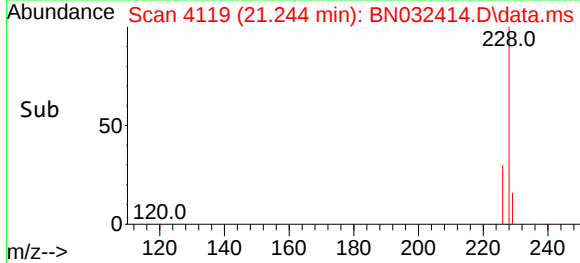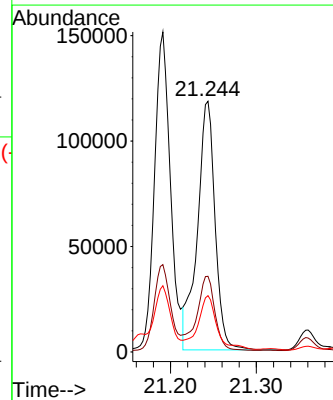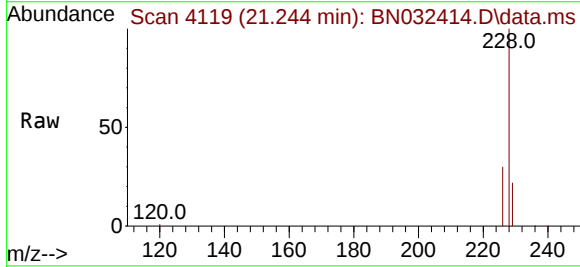

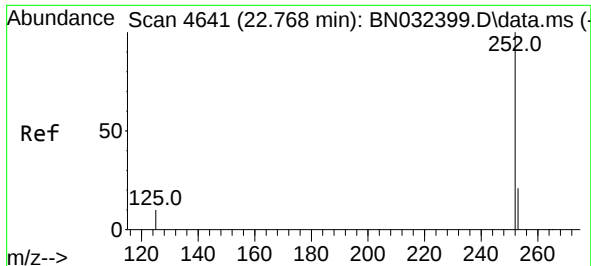

#24
Benzo(b)fluoranthene
Concen: 2.046 ng/ul m
RT: 22.757 min Scan# 4637
Delta R.T. -0.026 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12




Instrument :
BNA_N
ClientSampleId :
A4B54DL

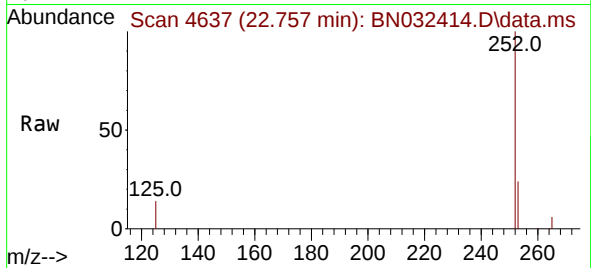

Tgt Ion:252 Resp: 20110
Ion Ratio Lower Upper
252 100
253 23.7 0.0 50.2
125 14.0 0.0 32.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

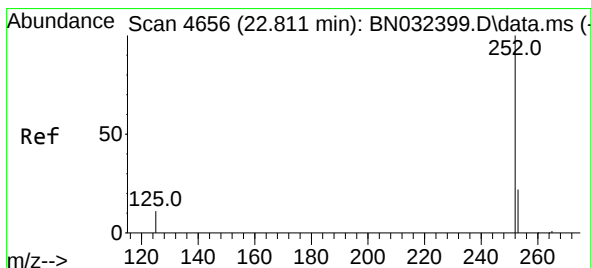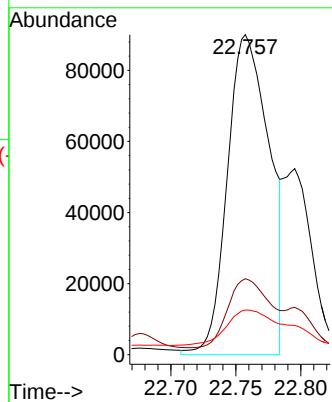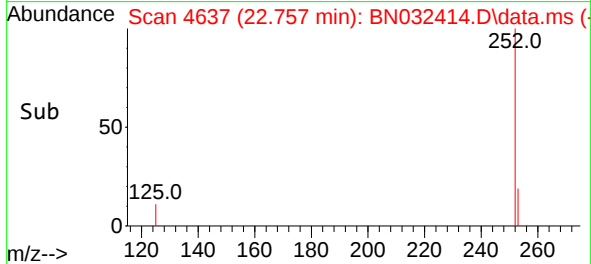

#25
Benzo(k)fluoranthene
Concen: 0.888 ng/ul m
RT: 22.795 min Scan# 4650
Delta R.T. -0.032 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12


Tgt Ion:252 Resp: 84832
Ion Ratio Lower Upper
252 100
253 25.5 20.3 30.5
125 15.7 12.8 19.2

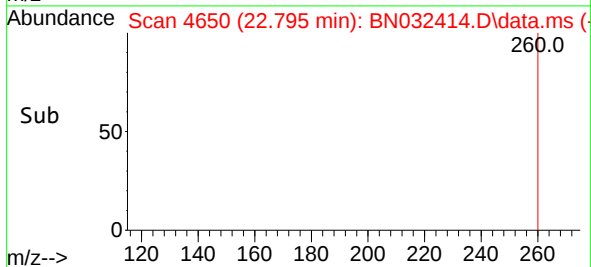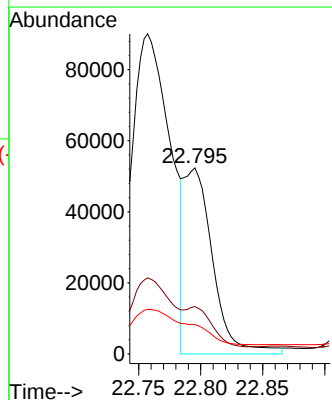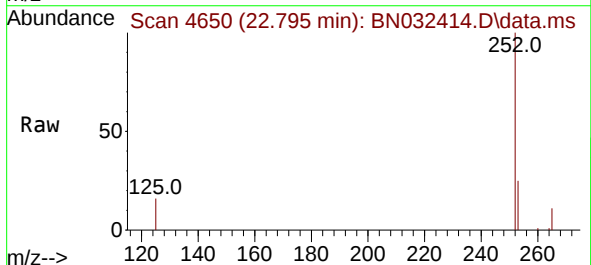

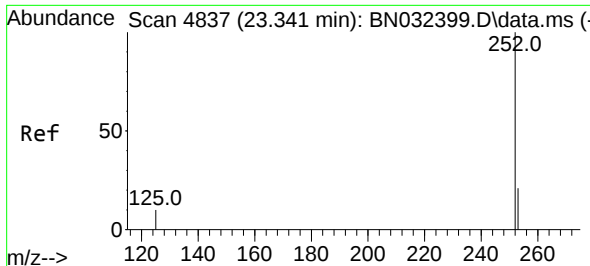

#26
Benzo(a)pyrene
Concen: 1.193 ng/ul
RT: 23.325 min Scan# 4831
Delta R.T. -0.035 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12




Instrument :
BNA_N
ClientSampleId :
A4B54DL

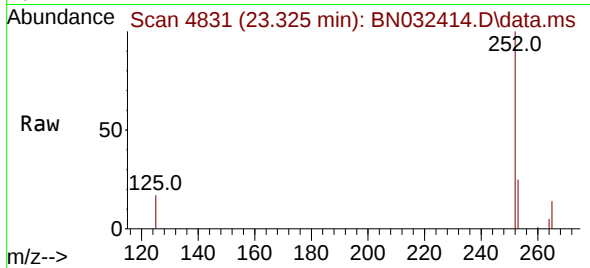

Tgt Ion:252 Resp: 8159
Ion Ratio Lower Upper
252 100
253 24.9 22.2 33.2
125 16.8 16.4 24.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/03/2024
Supervised By :mohammad ahmed 07/04/2024

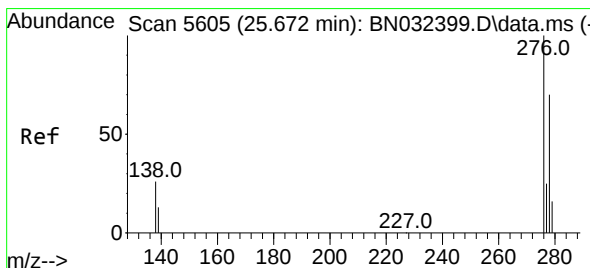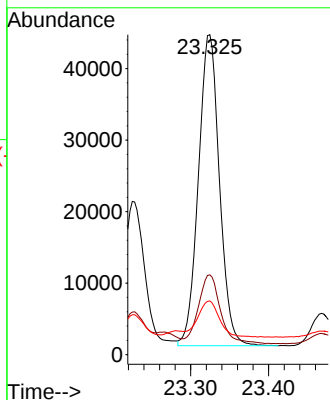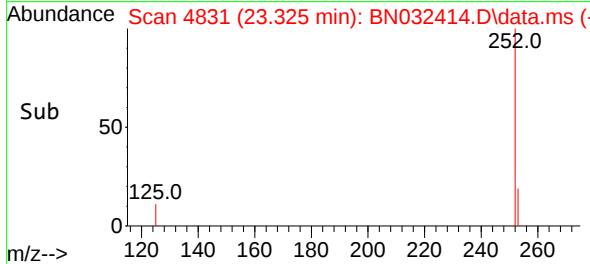

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.603 ng/ul
RT: 25.656 min Scan# 5600
Delta R.T. -0.044 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12

Tgt Ion:276 Resp: 64543
Ion Ratio Lower Upper
276 100
138 23.4 21.3 31.9
227 0.1 0.1 0.1#

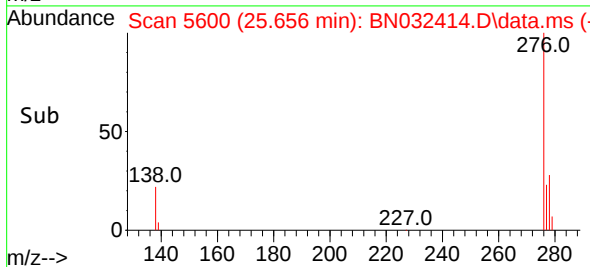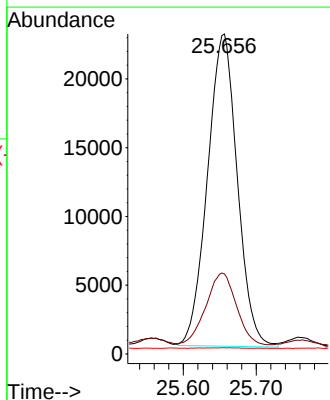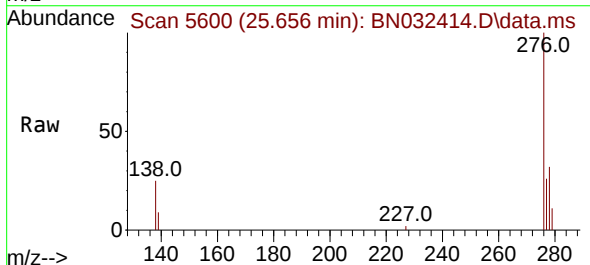

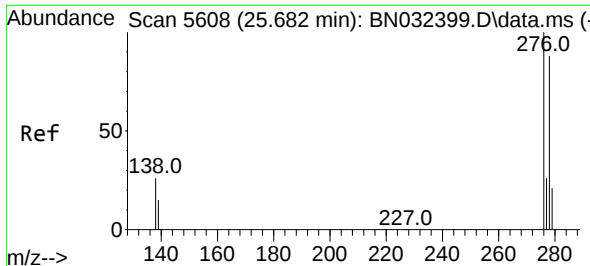


#28
Dibenzo(a,h)anthracene
Concen: 0.299 ng/ul
RT: 25.656 min Scan# 50
Delta R.T. -0.054 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12

Instrument :

BNA_N

ClientSampleId :

A4B54DL

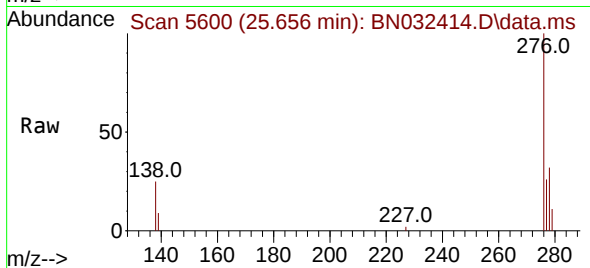




Tgt Ion:278 Resp: 2382
Ion Ratio Lower Upper
278 100
139 27.4 15.9 23.9#
279 34.6 21.1 31.7#

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 07/03/2024

Supervised By :mohammad ahmed 07/04/2024

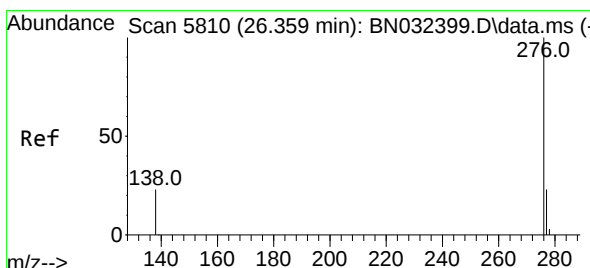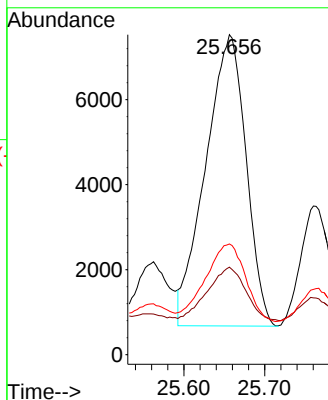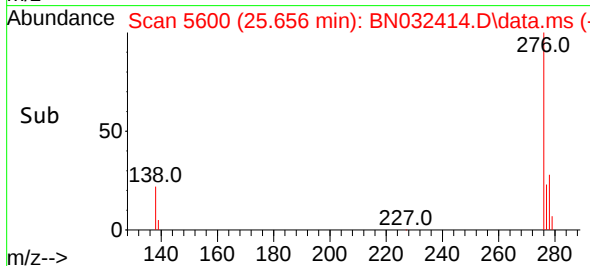

#29
Benzo(g,h,i)perylene
Concen: 0.101 ng/ul
RT: 26.340 min Scan# 5804
Delta R.T. -0.040 min
Lab File: BN032414.D
Acq: 02 Jul 2024 23:12

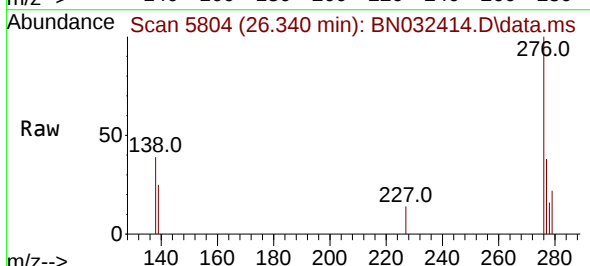

Tgt Ion:276 Resp: 8576
Ion Ratio Lower Upper
276 100
138 39.1 19.8 29.6#
277 37.5 19.8 29.6#

