
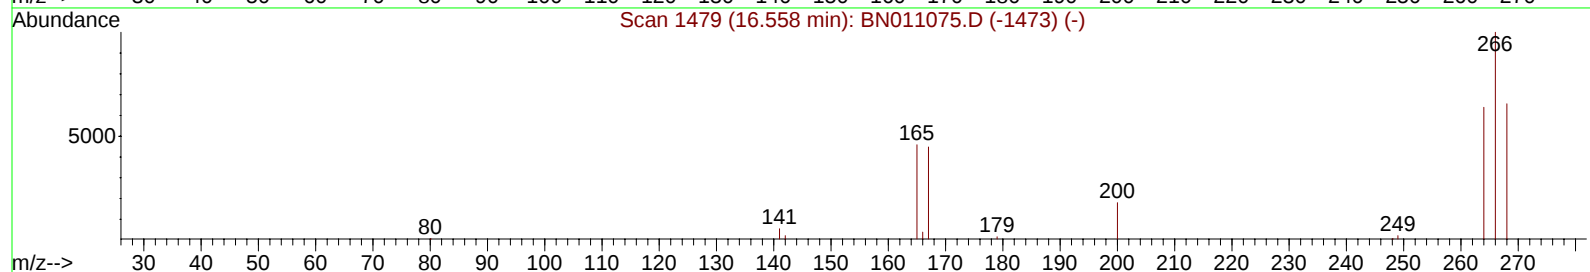
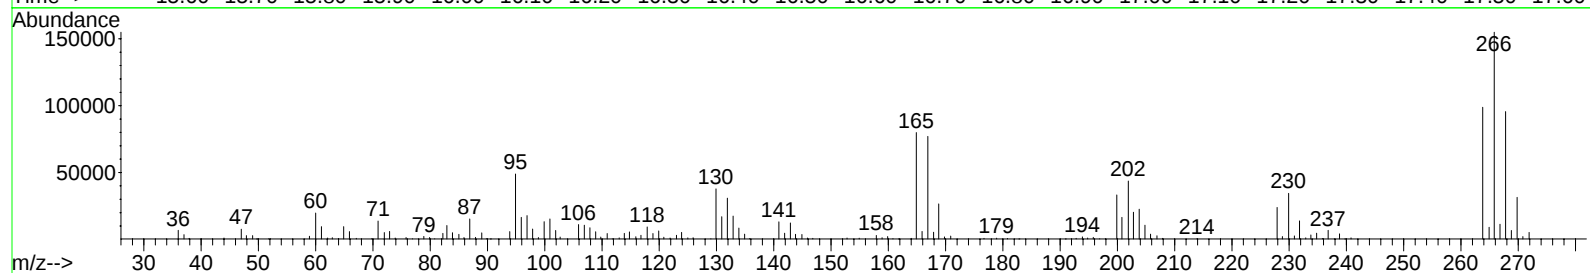


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN070220\
Data File : BN011081.D
Acq On : 02 Jul 2020 11:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 20:31:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN063020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 30 14:12:13 2020
Response via : Initial Calibration

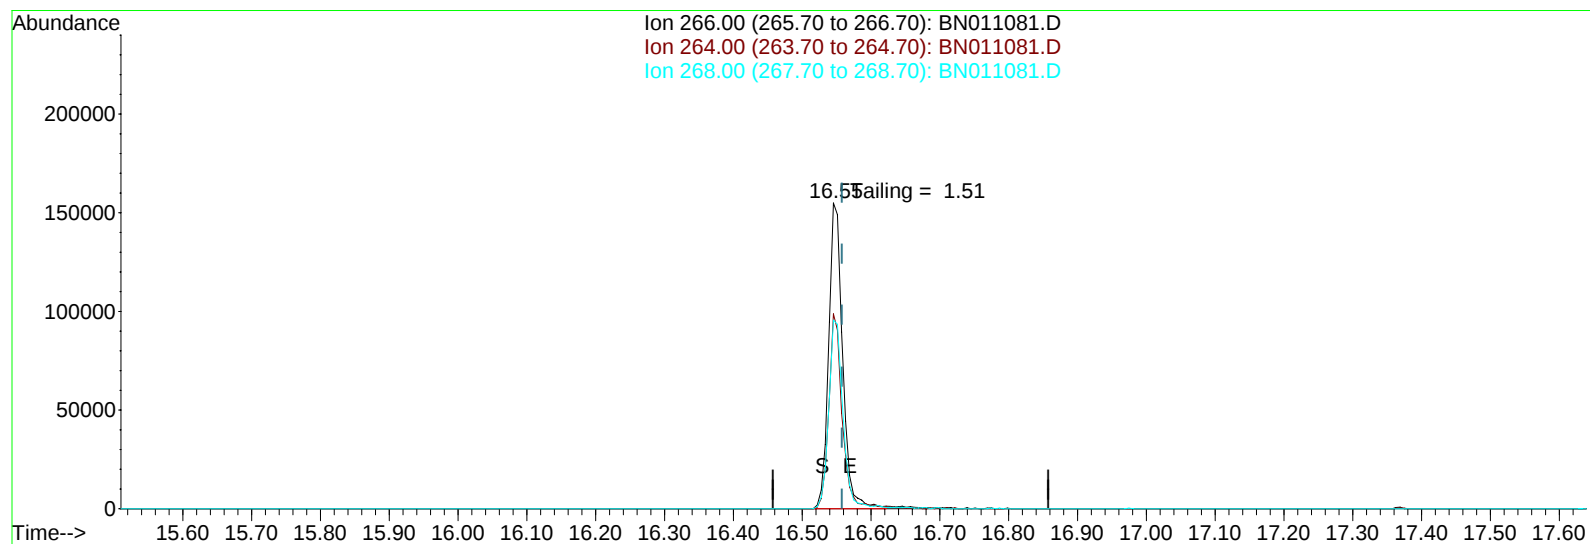

TIC: BN011081.D

(24) Pentachlorophenol

16.545min (-0.012) 0.00ng

response 220064

Ion	Exp%	Act%
266.00	100	100
264.00	59.20	61.54
268.00	68.70	62.83
0.00	0.00	0.00